


Data Path : Z:\HPCHEM1\BNA_M\Data\BM081715\
 Data File : BM002444.D
 Acq On : 17 Aug 2015 09:37
 Operator : UM/IZ
 Sample : DFTPP01
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP01

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Aug 18 03:02:54 2015

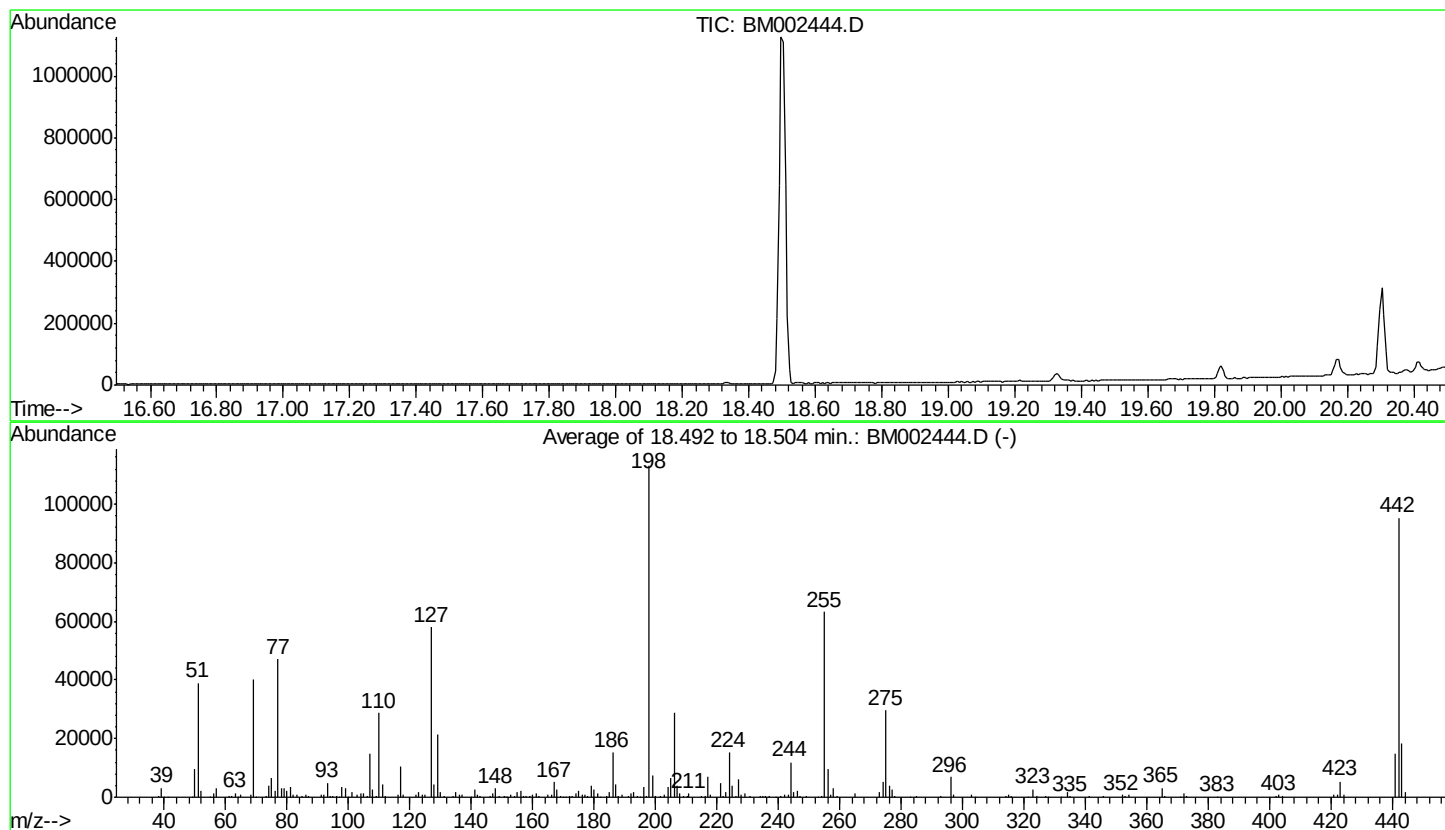

AutoFind: Scans 2619, 2620, 2621; Background Corrected with Scan 2614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	39032	PASS
68	69	0.00	2	1.8	707	PASS
69	198	0.00	100	35.6	40280	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	51.3	58056	PASS
197	198	0.00	2	0.6	661	PASS
198	198	100	100	100.0	113168	PASS
199	198	5	9	6.7	7626	PASS
275	198	10	60	26.2	29597	PASS
365	198	1	100	2.8	3216	PASS
441	443	0.01	100	79.2	14670	PASS
442	198	50	100	84.2	95301	PASS
443	442	15	24	19.4	18520	PASS

m/z	Abundance
38.00	383.0
39.10	2695.0
39.90	462.0
41.10	367.0
43.10	376.0
44.00	2799.0
50.00	7461.0
51.00	31280.0
52.00	1780.0
55.00	513.0
56.00	1034.0
57.00	2479.0
61.00	364.0
62.00	470.0
63.00	1265.0
65.00	618.0
68.10	687.0
69.00	31352.0
73.10	570.0
74.00	3245.0
75.00	5057.0
76.10	1610.0
77.10	36136.0
78.10	2562.0
79.00	2393.0
80.00	1800.0
81.00	2604.0
82.00	687.0
83.00	800.0
84.90	515.0
86.00	758.0
86.90	304.0
91.00	571.0
92.00	634.0
93.00	3881.0
93.90	354.0
96.10	358.0
98.00	2750.0
99.00	2369.0
101.00	1421.0
102.90	537.0
104.00	878.0
105.00	927.0
106.00	356.0
107.00	11300.0
108.00	1824.0
109.10	465.0
110.00	21776.0
111.00	3493.0
112.10	327.0
116.00	515.0
117.00	7972.0
118.00	823.0
121.90	851.0
123.00	1364.0
124.00	574.0
125.00	547.0
127.00	42104.0
128.00	3271.0
129.00	14987.0
129.90	1515.0
134.00	498.0
135.00	1341.0
136.00	566.0
137.00	551.0
141.00	1935.0
142.00	723.0
143.00	534.0
146.00	494.0
146.90	1050.0
148.00	2154.0
149.00	575.0
150.90	347.0
153.00	632.0
154.00	449.0
155.00	1087.0
156.00	1651.0
157.10	442.0
158.00	392.0
159.00	369.0
160.00	772.0
161.00	990.0
165.00	696.0
165.90	557.0
167.00	3697.0
168.00	2032.0
169.00	403.0
171.90	325.0
172.90	461.0
174.00	981.0
175.00	1385.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

176.00	581.0
176.90	817.0
179.00	2722.0
180.00	1870.0
180.90	972.0
185.00	1471.0
186.00	10261.0
187.00	3192.0
188.00	419.0
188.90	749.0
191.00	588.0
191.90	1033.0
193.00	1106.0
195.90	2141.0
197.10	533.0
197.90	75320.0
198.90	5300.0
199.90	373.0
201.50	427.0
203.00	612.0
204.10	2530.0
205.00	4452.0
206.00	19168.0
207.00	3600.0
208.00	827.0
208.90	304.0
210.10	342.0
211.00	745.0
217.00	4873.0
217.90	577.0
221.00	3167.0
223.00	1028.0
224.00	9833.0
225.00	2751.0
227.00	4001.0
228.00	597.0
229.00	872.0
231.10	354.0
235.00	382.0
237.00	301.0
241.90	495.0
243.10	538.0
244.00	7776.0
244.90	1015.0
246.00	1428.0
247.00	307.0
248.90	388.0
254.00	319.0
255.00	40136.0
256.00	5985.0
257.00	495.0
258.00	2086.0
258.90	362.0
264.90	824.0
272.90	1090.0
274.00	2959.0
275.00	18032.0
276.00	2670.0
277.00	1525.0
292.90	307.0
296.00	4120.0
297.00	586.0
303.00	568.0
314.90	469.0
323.00	1563.0
324.00	314.0
326.90	300.0
334.00	882.0
346.00	396.0
352.00	485.0
353.00	383.0
354.00	522.0
364.90	1744.0
366.00	383.0
372.00	970.0
402.10	316.0
403.00	378.0
421.00	379.0
422.00	372.0
423.00	2815.0
424.00	567.0
441.00	7020.0
442.00	47544.0
443.00	9865.0
444.00	842.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	578.0
39.10	3725.0
40.00	527.0
41.00	505.0
43.00	404.0
44.00	2923.0
49.10	315.0
50.00	11958.0
51.10	46472.0
52.00	2181.0
55.10	573.0
56.00	1418.0
57.00	3431.0
61.00	653.0
62.00	684.0
63.00	1792.0
64.00	321.0
65.00	961.0
68.00	712.0
69.00	47792.0
70.00	312.0
73.10	701.0
74.00	4756.0
75.00	7503.0
76.10	2581.0
77.10	56664.0
78.00	4017.0
79.00	3790.0
80.00	2648.0
81.00	4216.0
82.00	952.0
83.00	1155.0
85.00	752.0
86.00	1041.0
87.00	559.0
91.00	1121.0
92.00	1018.0
93.00	5899.0
94.00	436.0
95.00	380.0
96.00	399.0
97.00	317.0
98.00	4687.0
99.00	3651.0
99.90	391.0
101.00	2184.0
103.00	885.0
104.00	1419.0
105.00	1504.0
106.00	448.0
107.00	17528.0
108.00	2909.0
109.00	695.0
110.00	33560.0
111.00	5214.0
111.90	630.0
116.00	991.0
117.00	12031.0
118.00	905.0
121.90	1024.0
123.00	2010.0
124.00	877.0
125.00	941.0
127.00	69872.0
128.00	5198.0
129.00	25568.0
130.00	2109.0
130.90	463.0
134.00	742.0
135.00	2211.0
136.00	909.0
137.00	1081.0
140.00	305.0
141.00	3503.0
142.00	1143.0
143.00	742.0
145.90	536.0
147.00	1858.0
148.00	3421.0
149.00	730.0
151.20	417.0
151.70	381.0
152.90	930.0
154.00	758.0
155.00	1852.0
156.00	2737.0
157.10	605.0
158.00	590.0
159.00	498.0
160.00	1049.0
161.00	1609.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

162.00	464.0
164.90	1100.0
166.00	1056.0
167.00	5816.0
168.00	2701.0
169.00	575.0
169.90	327.0
171.90	594.0
172.90	679.0
174.00	1291.0
175.00	2987.0
176.00	802.0
176.90	1115.0
178.00	477.0
179.00	4471.0
180.00	3231.0
181.00	1369.0
184.00	417.0
185.00	2108.0
186.00	18544.0
187.00	5192.0
187.90	611.0
189.00	1049.0
190.90	648.0
192.00	1310.0
193.00	1754.0
194.00	431.0
196.00	4125.0
197.00	668.0
198.00	133248.0
198.90	9203.0
200.00	799.0
201.50	860.0
202.90	1118.0
204.00	4183.0
205.00	7635.0
206.00	34784.0
207.00	5171.0
208.00	1312.0
208.90	590.0
210.20	603.0
210.90	1263.0
215.00	377.0
216.00	526.0
217.00	8126.0
217.90	1167.0
221.00	6036.0
222.90	1867.0
224.00	17608.0
225.00	4437.0
226.00	560.0
227.00	7232.0
227.90	992.0
229.00	1547.0
230.90	595.0
234.00	384.0
235.00	557.0
235.90	417.0
237.00	616.0
239.00	311.0
240.80	340.0
242.00	898.0
243.00	1053.0
244.00	14310.0
245.00	2035.0
246.00	2407.0
247.00	508.0
248.90	503.0
253.00	324.0
254.10	694.0
255.00	73096.0
256.00	11292.0
257.00	782.0
258.00	3658.0
259.00	621.0
264.90	1683.0
273.00	2078.0
274.00	6172.0
275.00	34248.0
276.00	4552.0
276.90	2891.0
278.00	585.0
282.90	316.0
285.00	544.0
293.00	560.0
296.00	8179.0
297.00	1088.0
303.00	1080.0
303.90	329.0
313.90	415.0
315.00	1040.0
315.90	552.0
321.10	324.0
323.00	3188.0
324.00	493.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

327.00	615.0
332.00	344.0
334.00	1966.0
335.00	530.0
341.10	353.0
345.90	591.0
351.90	873.0
353.00	653.0
354.00	1056.0
365.00	3672.0
365.90	497.0
371.00	300.0
372.00	1481.0
373.00	443.0
402.00	735.0
403.00	956.0
403.90	413.0
421.00	854.0
422.00	845.0
423.00	5583.0
424.00	1208.0
441.00	16968.0
442.00	104536.0
443.00	20280.0
444.00	1992.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

m/z	Abundance
38.00	433.0
39.00	3087.0
40.00	718.0
41.00	477.0
44.00	2623.0
50.10	9738.0
51.10	39344.0
52.00	2042.0
55.00	511.0
56.00	1305.0
57.00	2930.0
61.00	530.0
62.00	523.0
63.00	1485.0
65.00	866.0
68.10	724.0
69.00	41696.0
73.00	744.0
74.00	4175.0
75.00	6522.0
76.00	2222.0
77.10	48720.0
78.00	3173.0
79.00	2896.0
80.00	2453.0
81.00	3657.0
82.00	903.0
83.00	836.0
85.00	641.0
86.00	948.0
87.00	590.0
91.00	937.0
91.90	927.0
93.00	5043.0
93.90	348.0
95.00	346.0
95.90	456.0
98.00	3701.0
99.00	3185.0
101.00	2047.0
102.90	738.0
104.00	1107.0
105.00	1278.0
106.00	520.0
107.00	15306.0
108.00	2592.0
109.10	778.0
110.00	30920.0
111.00	4693.0
112.00	512.0
116.00	1067.0
117.00	11259.0
118.00	834.0
122.00	957.0
123.00	1638.0
123.90	658.0
125.00	657.0
127.00	62192.0
128.00	4424.0
129.00	23472.0
130.00	1703.0
131.00	460.0
133.90	688.0
135.00	1961.0
136.00	747.0
137.00	1037.0
141.00	3001.0
142.00	1098.0
142.90	602.0
146.00	578.0
147.00	1672.0
148.00	3226.0
149.00	710.0
150.90	460.0
153.00	957.0
154.00	740.0
155.00	1781.0
156.00	2514.0
157.10	545.0
157.90	658.0
158.90	400.0
160.00	1021.0
161.00	1322.0
161.90	476.0
164.90	1132.0
166.00	1032.0
167.00	5879.0
168.00	2538.0
169.00	444.0
170.90	374.0
171.90	635.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

173.00	644.0
174.00	1309.0
175.00	2441.0
176.00	777.0
176.90	1142.0
178.00	468.0
178.90	4334.0
180.00	2945.0
180.90	1460.0
182.00	418.0
184.00	466.0
185.00	2281.0
186.00	16744.0
187.00	4945.0
188.00	492.0
189.00	1099.0
191.00	664.0
192.00	1354.0
193.00	1797.0
194.00	411.0
194.80	351.0
196.00	4069.0
197.10	782.0
197.90	130936.0
199.00	8375.0
199.90	664.0
201.30	619.0
202.90	821.0
204.00	4244.0
205.00	7455.0
206.00	32160.0
207.00	5068.0
208.00	1365.0
209.00	369.0
210.20	657.0
211.00	1391.0
214.90	367.0
216.00	611.0
217.00	7677.0
218.00	1081.0
221.00	5433.0
221.80	1312.0
223.00	1846.0
224.00	17904.0
225.00	4642.0
226.10	469.0
227.00	7489.0
228.00	1092.0
229.00	1573.0
231.00	726.0
234.00	475.0
234.90	513.0
236.00	386.0
237.00	614.0
239.00	306.0
240.90	394.0
242.10	820.0
243.00	987.0
244.00	13800.0
245.10	1850.0
246.00	2685.0
246.90	530.0
248.90	553.0
252.90	301.0
254.20	751.0
255.00	76224.0
256.00	11168.0
257.00	870.0
258.00	3765.0
259.00	809.0
265.00	1583.0
273.00	2345.0
274.00	6085.0
275.00	36512.0
276.00	4988.0
277.00	2919.0
277.90	532.0
282.90	389.0
285.00	532.0
292.90	649.0
296.00	8583.0
297.00	1268.0
303.00	1128.0
304.00	323.0
314.00	511.0
314.90	934.0
316.00	585.0
323.00	3359.0
324.00	597.0
326.90	582.0
328.00	345.0
334.00	1886.0
335.00	592.0
341.00	515.0
346.00	675.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

352.00	1096.0
353.00	689.0
354.10	1129.0
365.00	4233.0
366.00	553.0
372.00	1819.0
373.00	450.0
383.00	444.0
402.00	699.0
403.00	1106.0
404.00	420.0
420.90	1018.0
422.00	840.0
423.00	7403.0
424.00	1233.0
441.00	20024.0
442.00	133824.0
443.00	25416.0
444.00	2149.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01

Scan 2614 (18.463 min): BM002444.D
DFTPP01

m/z	Abundance
39.90	444.0
41.00	354.0
43.10	402.0
44.00	2834.0
55.10	372.0
73.00	348.0
207.10	790.0
281.00	316.0

Instrument :
BNA_M
ClientSampleId :
DFTPP01