

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
 Data File : BM007161.D
 Acq On : 17 Aug 2016 02:51
 Operator : UM/SJ
 Sample : H4445-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N34

Quant Time: Aug 17 03:53:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 03:20:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	265699	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1063541	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	634946	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1519692	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1932233	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2017585	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	30981	5.09	ng/uL	0.00
5) Phenol-d5	6.97	99	594367	27.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	352547	28.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	479182	27.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	474813	26.81	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	228179	29.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	257959	31.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	491845	28.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	611399	29.72	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1541827	29.39	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1848801	29.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	238220	25.33	ng/ul	0.00
57) Fluorene-d10	15.43	176	1322280	28.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	202227	24.08	ng/ul	0.00
70) Anthracene-d10	17.27	188	2123650	30.16	ng/ul	0.00
76) Pyrene-d10	19.57	212	2537922	31.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2869211	31.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.89	163	411755	7.85	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007161.D
Acq On : 17 Aug 2016 02:51
Operator : UM/SJ
Sample : H4445-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N34

Quant Time: Aug 17 03:53:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 03:20:37 2016
Response via : Initial Calibration

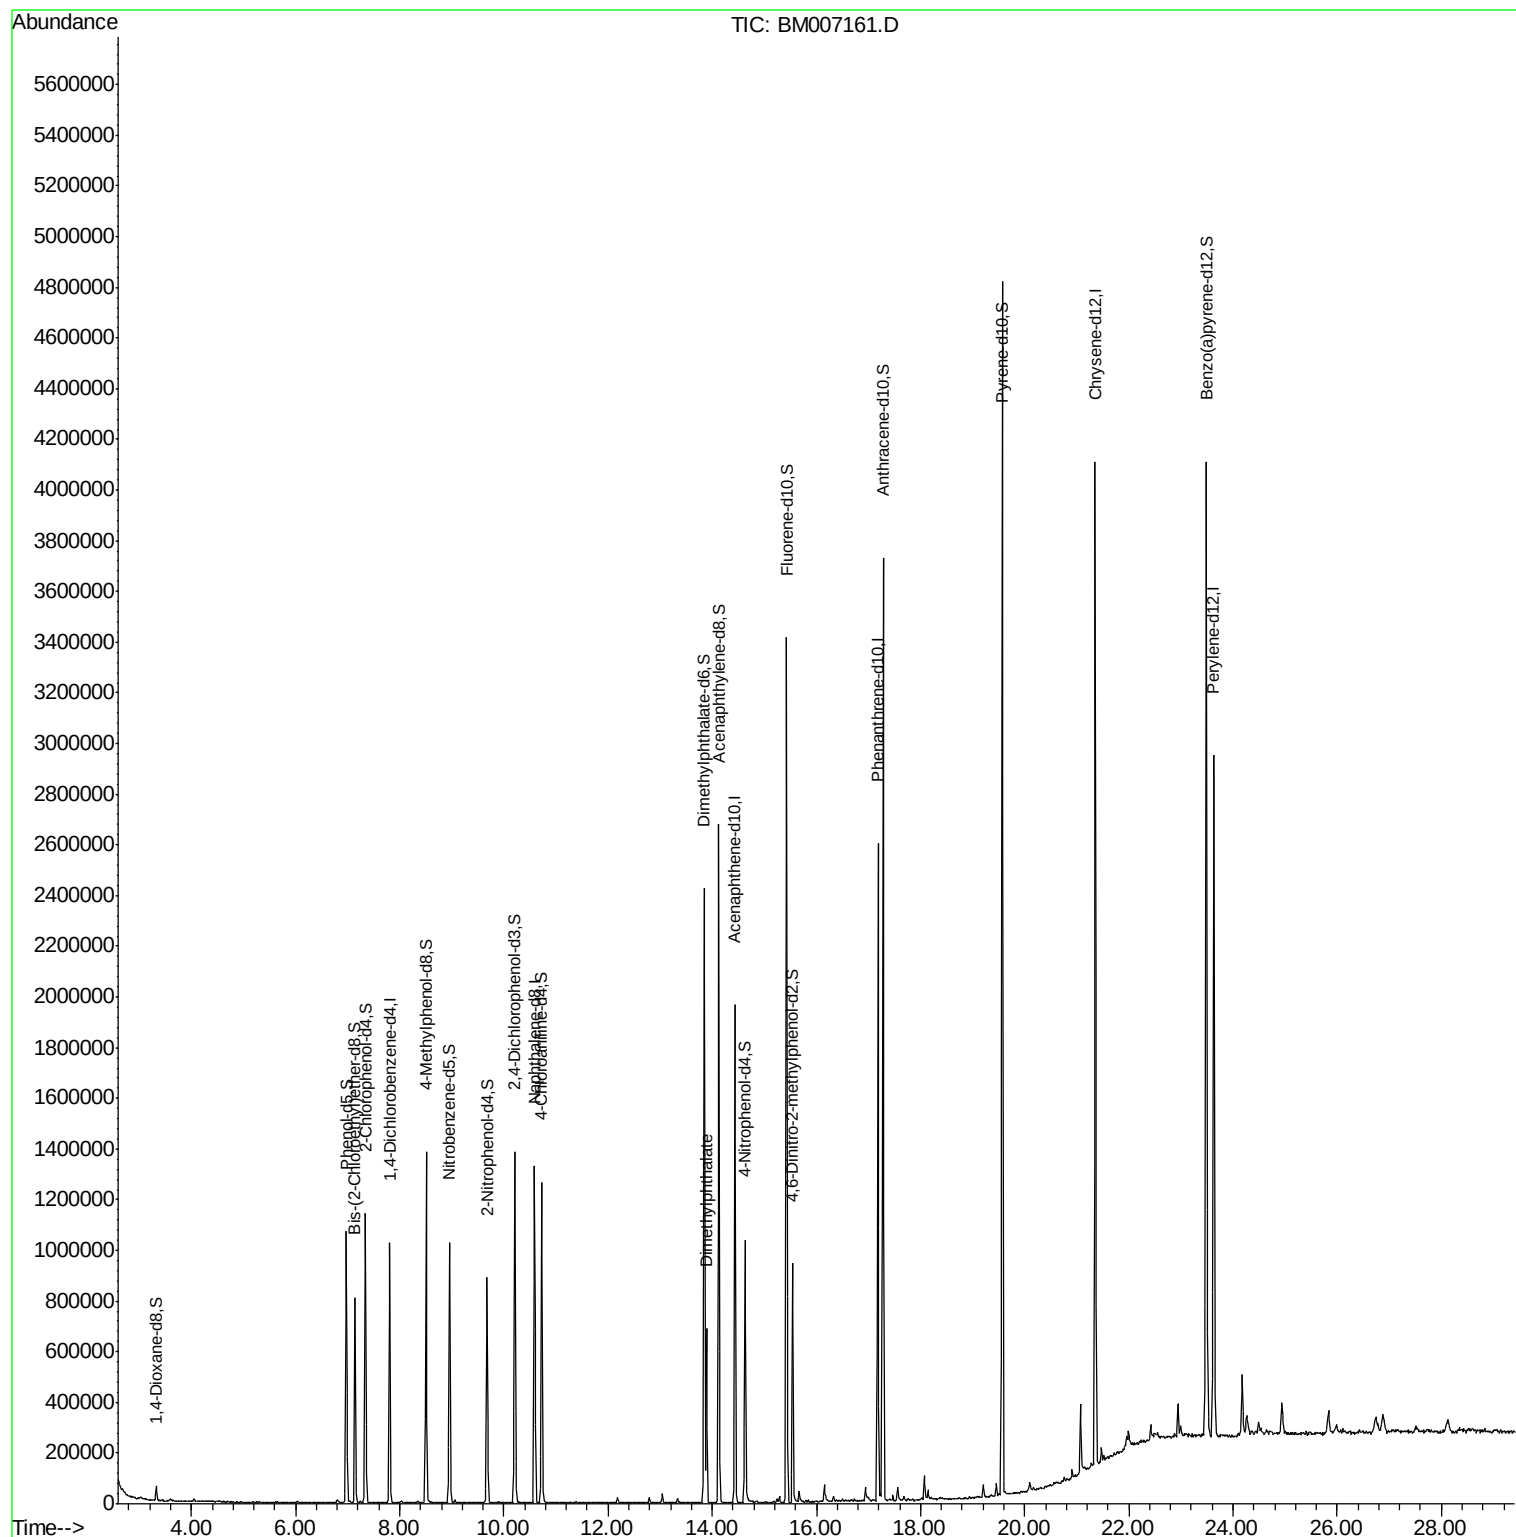

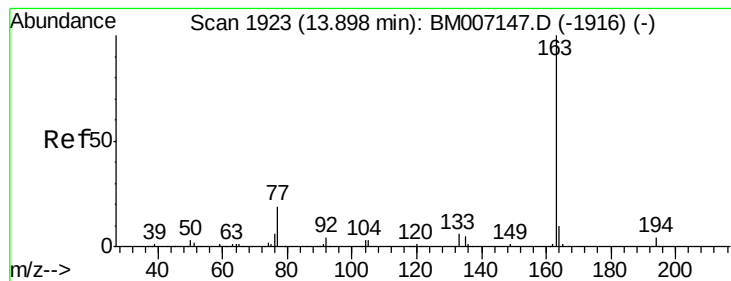

#44

Dimethylphthalate

Concen: 7.85 ng/ul

RT: 13.89 min Scan# 1922

Delta R.T. -0.01 min

Lab File: BM007161.D

Acq: 17 Aug 2016 02:51

Instrument :

BNA_M

ClientSampleId :

E5N34


Tgt Ion:163 Resp: 411755

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 9.9 7.8 11.8

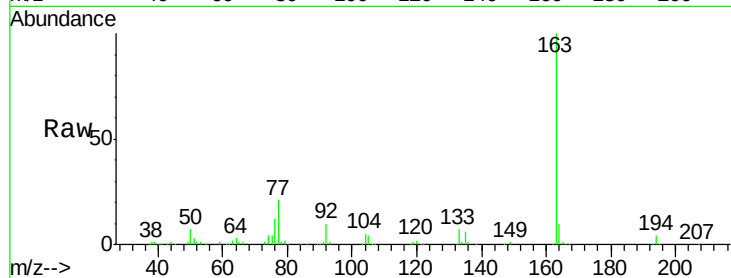

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

