

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
 Data File : BM007167.D
 Acq On : 17 Aug 2016 06:25
 Operator : UM/SJ
 Sample : H4423-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD2Q9

Quant Time: Aug 17 07:04:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 04:01:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	254614	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1002905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	570802	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1337636	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1803044	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1995071	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	29794	5.11	ng/uL	0.00
5) Phenol-d5	6.97	99	571577	27.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	342059	28.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	465226	28.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	440074	25.93	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	220111	30.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	245870	31.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	460548	28.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	580328	29.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1406290	29.82	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1697815	29.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	198009	23.42	ng/ul	0.00
57) Fluorene-d10	15.43	176	1217264	29.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	153291	20.74	ng/ul	0.00
70) Anthracene-d10	17.27	188	1930352	31.15	ng/ul	0.00
76) Pyrene-d10	19.57	212	2334598	30.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2904648	31.83	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.89	163	624317	13.24	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007167.D
Acq On : 17 Aug 2016 06:25
Operator : UM/SJ
Sample : H4423-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2Q9

Quant Time: Aug 17 07:04:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 04:01:43 2016
Response via : Initial Calibration

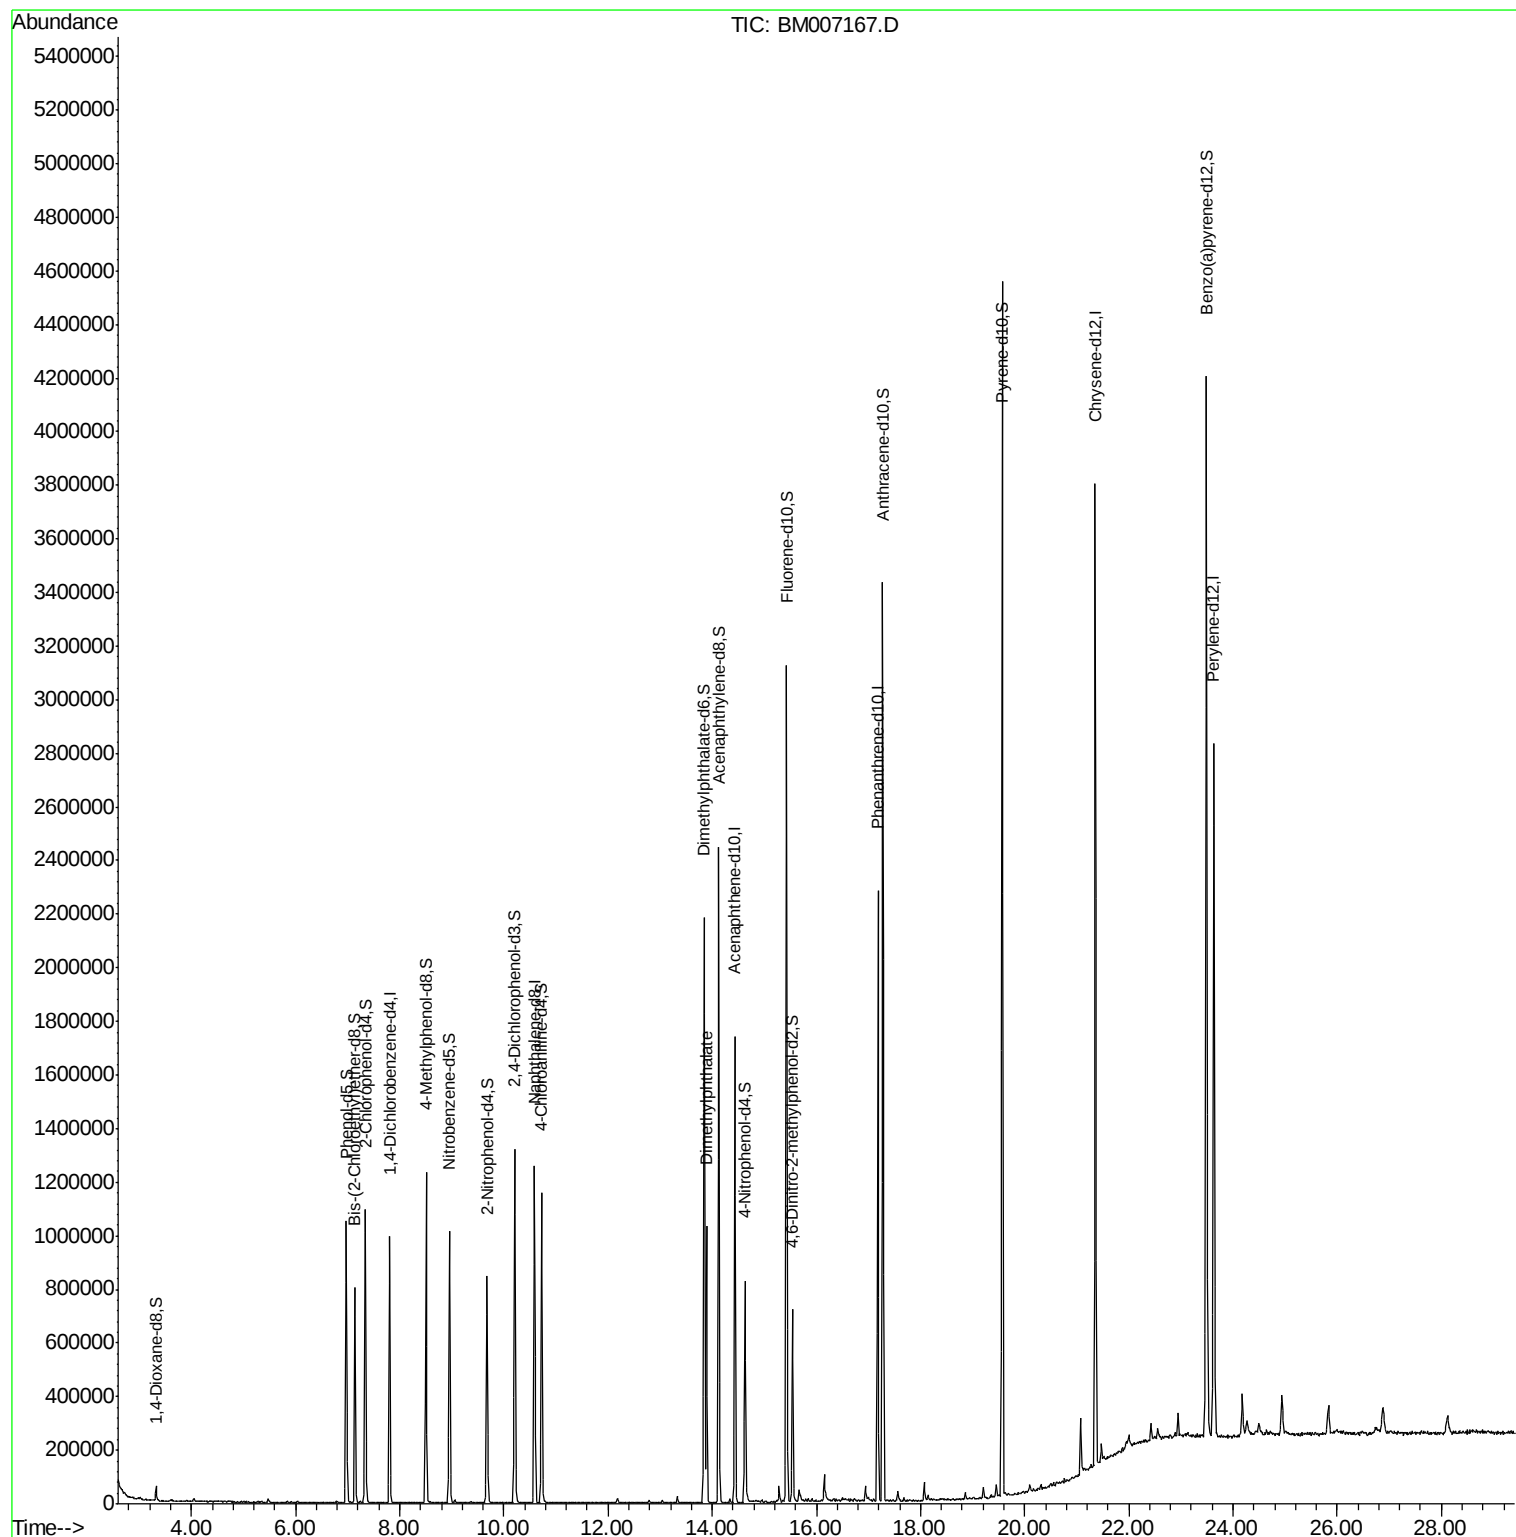

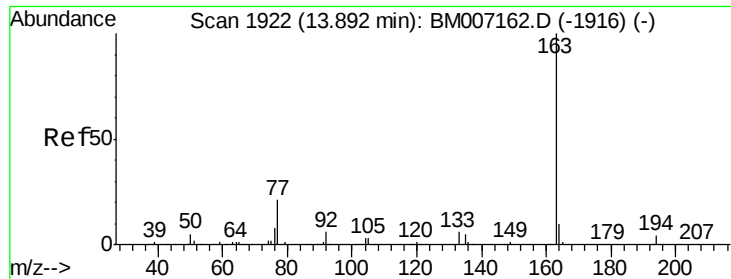

#44

Dimethylphthalate

Concen: 13.24 ng/ul

RT: 13.89 min Scan# 1922

Delta R.T. 0.00 min

Lab File: BM007167.D

Acq: 17 Aug 2016 06:25

Instrument :

BNA_M

ClientSampleId :

BD2Q9



Tgt Ion:163 Resp: 624317

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.4 7.8 11.8

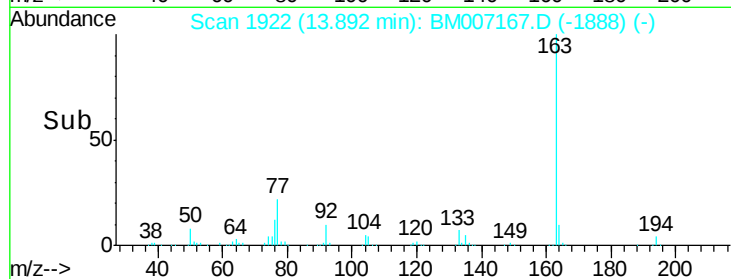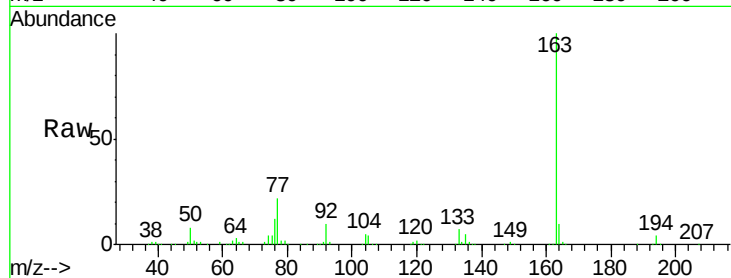

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

