

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
 Data File : BM007149.D
 Acq On : 16 Aug 2016 19:39
 Operator : UM/SJ
 Sample : H4436-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA204

Manual Integrations
 APPROVED

sohil
 8/17/2016 6:27:02 PM

Quant Time: Aug 17 03:26:24 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 03:20:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	200278	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	795049	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	473927	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1131209	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1495287	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1575251	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	3845	0.84	ng/uL	0.00
5) Phenol-d5	6.97	99	74473	4.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	219947	23.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	241796	18.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	147526	11.05	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	142888	24.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	159134	25.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	289670	22.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	15941	1.04	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1050351	26.82	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1240125	26.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	25194m	3.59	ng/ul	0.00
57) Fluorene-d10	15.43	176	924166	27.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	138695	22.19	ng/ul	0.00
70) Anthracene-d10	17.28	188	1447239	27.62	ng/ul	0.00
76) Pyrene-d10	19.57	212	1858322	29.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2112272	29.32	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	13.89	163	174830	4.47 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
Data File : BM007149.D
Acq On : 16 Aug 2016 19:39
Operator : UM/SJ
Sample : H4436-06
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
DA204

Manual Integrations
APPROVED

sohil
8/17/2016 6:27:02 PM

Quant Time: Aug 17 03:26:24 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 03:20:37 2016
Response via : Initial Calibration

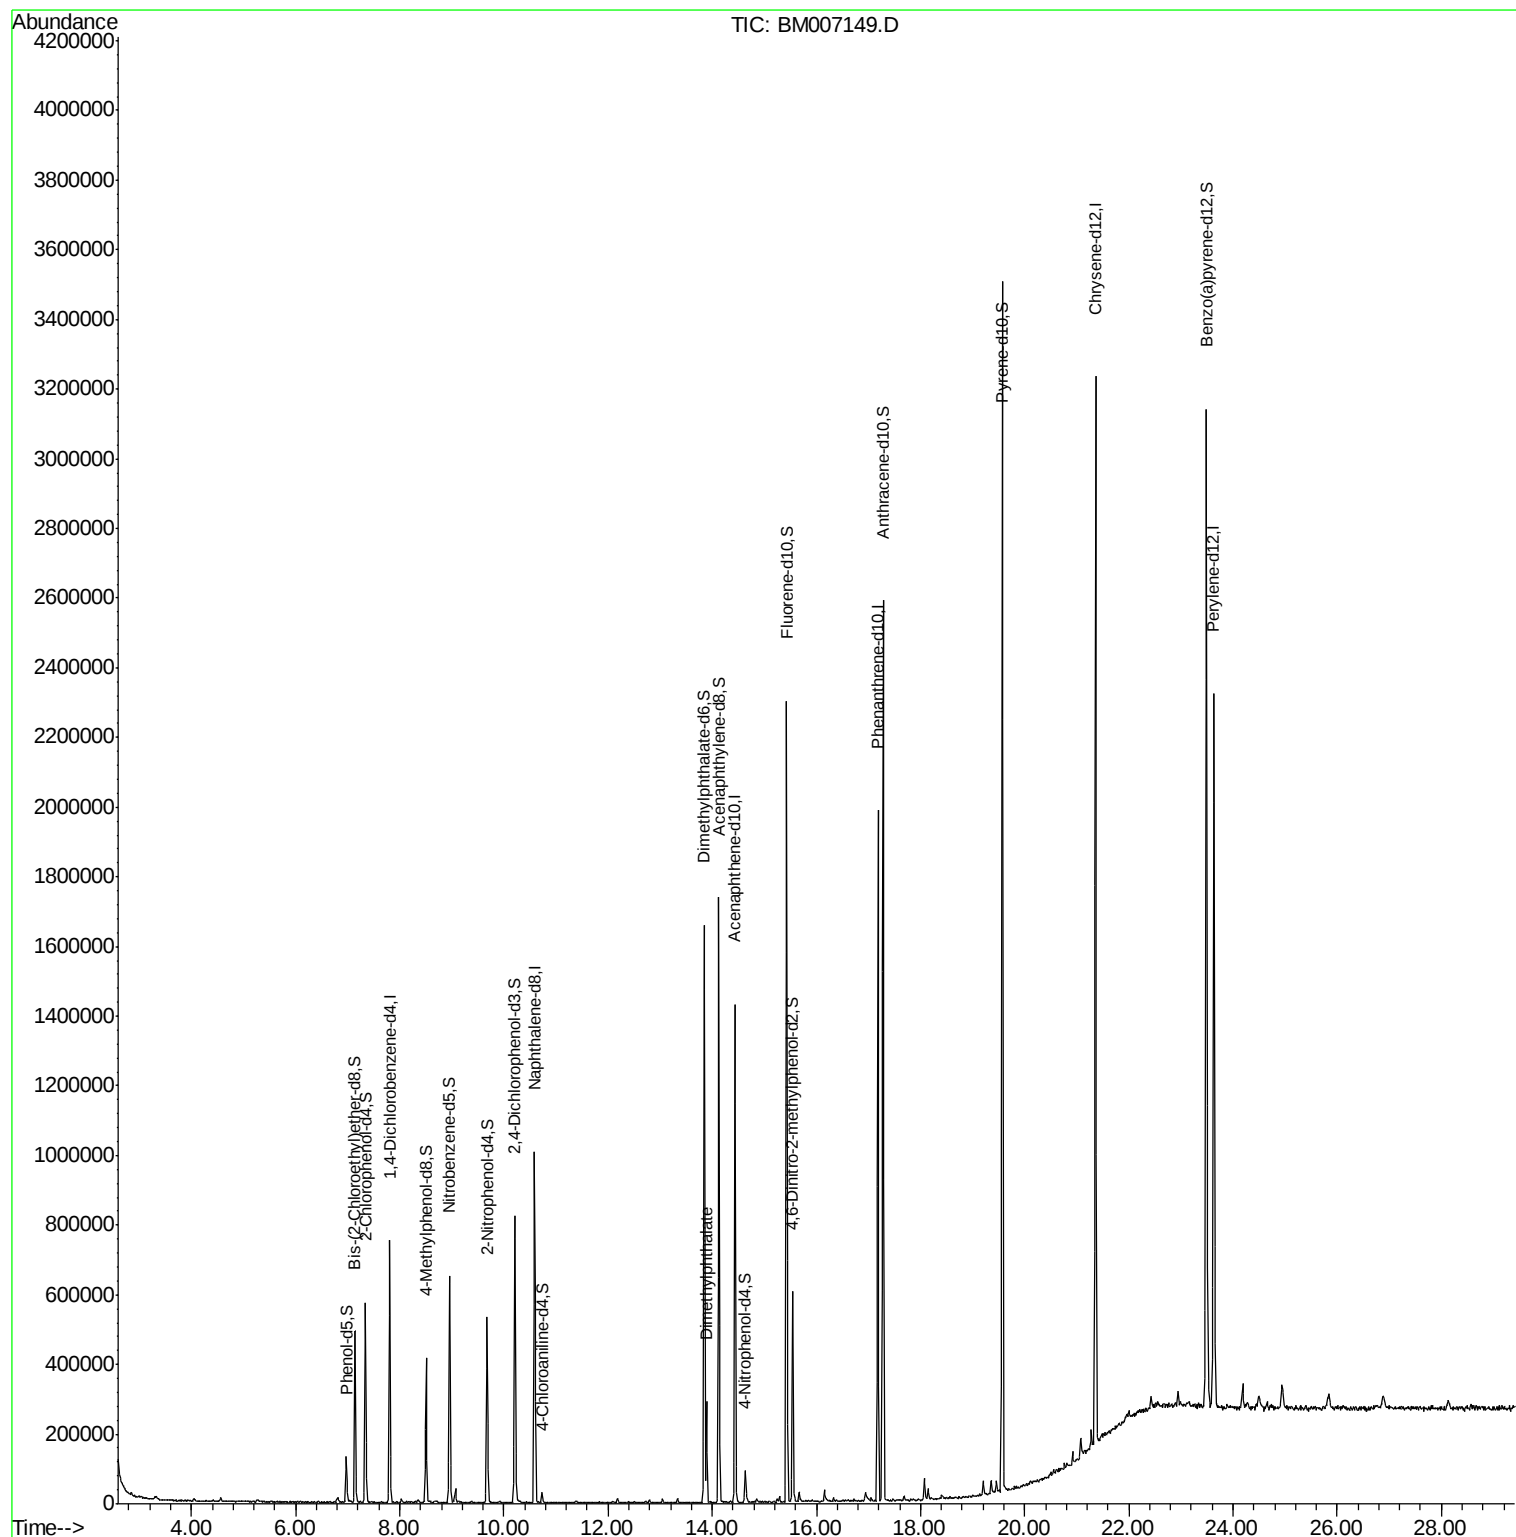

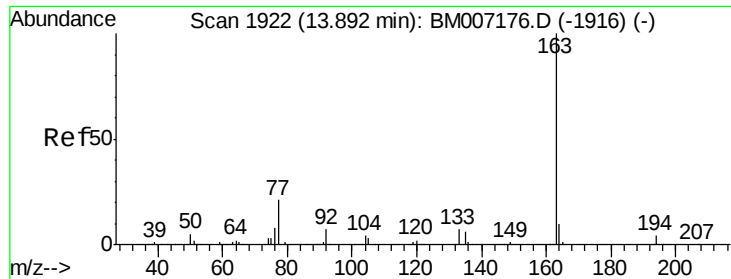

#44
 Dimethylphthalate
 Concen: 4.47 ng/ul
 RT: 13.89 min Scan# 1922
 Delta R.T. -0.01 min
 Lab File: BM007149.D
 Acq: 16 Aug 2016 19:39

Instrument :
 BNA_M
 ClientSampleId :
 DA204

Tot Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.3	3.4	5.2
164	10.5	7.8	11.8

Manual Integrations
 APPROVED

sohil
 8/17/2016 6:27:02 PM

