

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
 Data File : BM007171.D
 Acq On : 17 Aug 2016 09:40
 Operator : UM/SJ
 Sample : H4423-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD2R9

Quant Time: Aug 17 13:50:22 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 17 04:01:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	307337	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1218280	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	700935	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1658167	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	2149292	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2219623	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	39515	5.62	ng/uL	0.00
5) Phenol-d5	6.97	99	772712	31.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	454155	31.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	632976	31.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	608220	29.69	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	296078	33.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	329305	34.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	613955	31.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	778620	33.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1884090	32.53	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	2291796	32.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	249497	24.03	ng/ul	0.00
57) Fluorene-d10	15.43	176	1614670	31.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	202449	22.09	ng/ul	0.00
70) Anthracene-d10	17.27	188	2535392	33.01	ng/ul	0.00
76) Pyrene-d10	19.57	212	3025857	33.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	3451778	34.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.89	163	1058481	18.29	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
Data File : BM007171.D
Acq On : 17 Aug 2016 09:40
Operator : UM/SJ
Sample : H4423-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2R9

Quant Time: Aug 17 13:50:22 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 17 04:01:43 2016
Response via : Initial Calibration

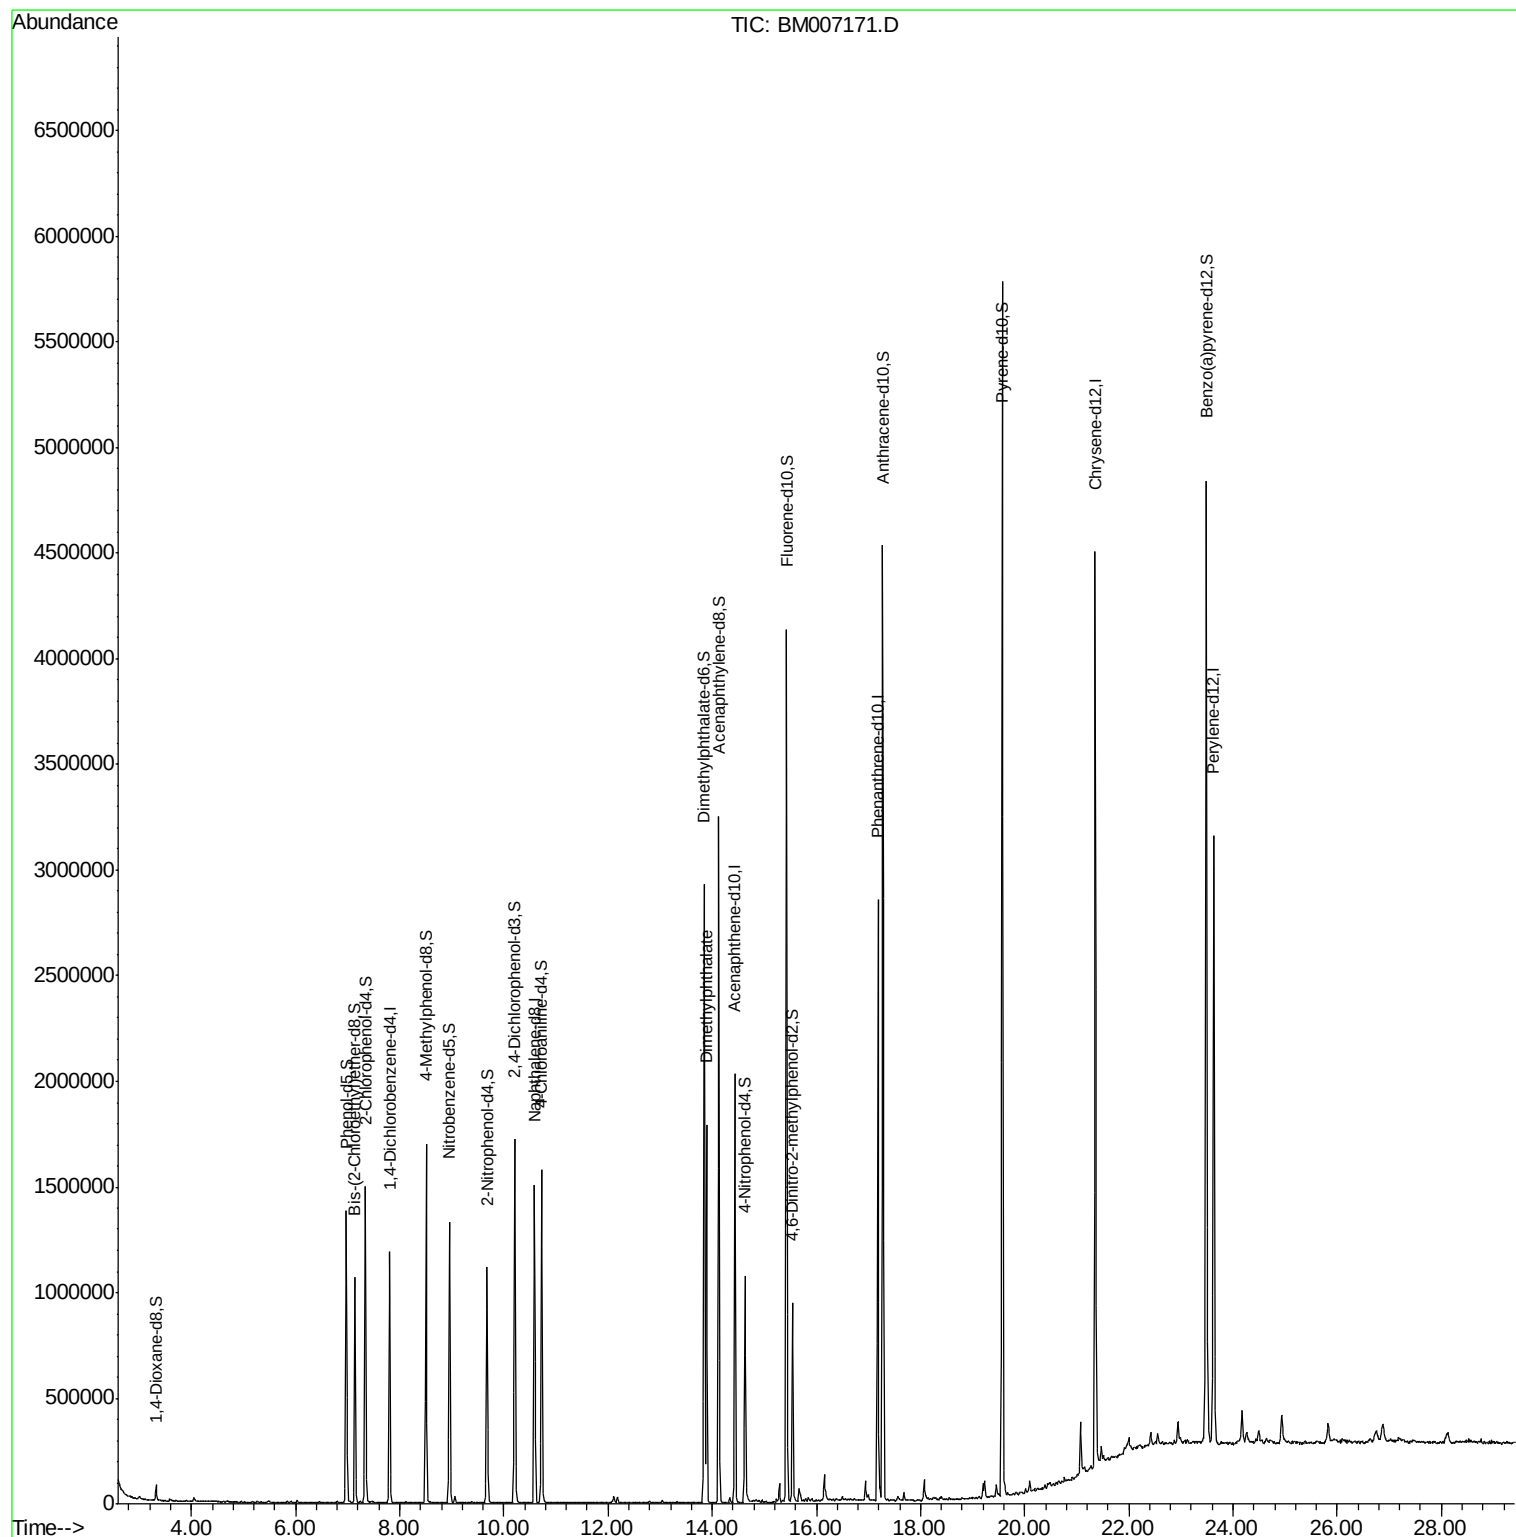


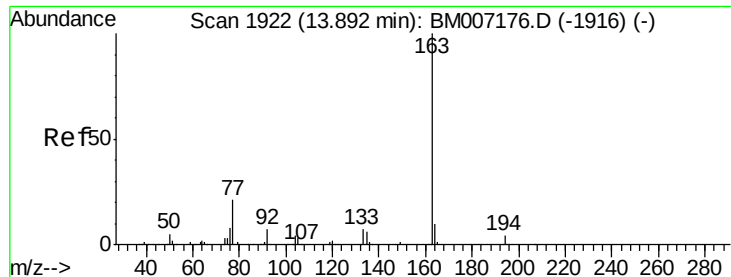

#44
 Dimethylphthalate
 Concen: 18.29 ng/ul
 RT: 13.89 min Scan# 1922
 Delta R.T. 0.00 min
 Lab File: BM007171.D
 Acq: 17 Aug 2016 09:40

Instrument :
 BNA_M
 ClientSampleId :
 BD2R9

Tot Ion:163 Resp: 1058481
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.2
 164 9.9 7.8 11.8

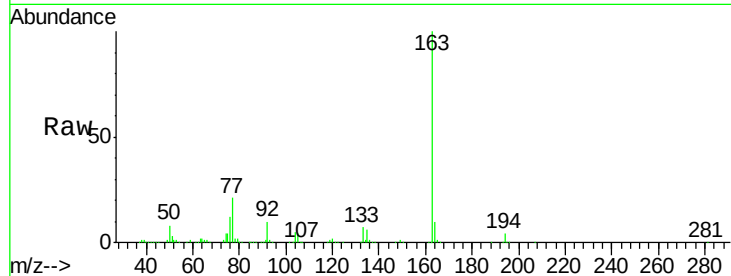

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

