

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
 Data File : BM007151.D
 Acq On : 16 Aug 2016 20:52
 Operator : UM/SJ
 Sample : H4436-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA206

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.975	738	746	753	rBV	163966	271770	5.04%	0.530%
2	7.145	768	775	785	rBV	577213	919198	17.04%	1.794%
3	7.340	801	808	819	rBV	662037	1070440	19.84%	2.089%
4	7.810	880	888	896	rBV	870415	1424929	26.41%	2.781%
5	8.504	995	1006	1015	rBV2	513197	820785	15.21%	1.602%
6	8.957	1075	1083	1095	rBV	737433	1257141	23.30%	2.454%
7	9.675	1198	1205	1214	rBV	616085	1050523	19.47%	2.050%
8	10.210	1289	1296	1306	rBV	931520	1583486	29.35%	3.091%
9	10.592	1353	1361	1371	rBV	1158908	1931601	35.81%	3.770%
10	10.728	1378	1384	1394	rBV	50850	89993	1.67%	0.176%
11	13.845	1908	1914	1919	rBV	1884915	2591746	48.04%	5.059%
12	13.892	1919	1922	1930	rVB	311508	414122	7.68%	0.808%
13	14.127	1955	1962	1973	rVB	1994891	2980629	55.25%	5.818%
14	14.439	2008	2015	2023	rBV2	1678127	2590831	48.03%	5.057%
15	14.633	2043	2048	2057	rBV	107556	189289	3.51%	0.369%
16	15.427	2177	2183	2192	rBV	2623763	3840673	71.19%	7.496%
17	15.545	2197	2203	2215	rBV	686813	995465	18.45%	1.943%
18	15.668	2220	2224	2234	rBV3	31452	57349	1.06%	0.112%
19	17.180	2475	2481	2490	rVV	2280713	3247094	60.19%	6.338%
20	17.280	2491	2498	2510	rVB2	2783941	4176573	77.42%	8.152%
21	18.074	2626	2633	2640	rBV3	51363	81984	1.52%	0.160%
22	18.151	2640	2646	2650	rVB	39205	54165	1.00%	0.106%
23	19.203	2821	2825	2834	rVB	38243	59136	1.10%	0.115%
24	19.568	2881	2887	2894	rBV	3633569	5133607	95.16%	10.020%
25	21.074	3139	3143	3149	rBV3	103491	158683	2.94%	0.310%
26	21.362	3186	3192	3199	rBV	3311805	4464301	82.75%	8.714%
27	23.486	3546	3553	3566	rVB2	2679789	5394604	100.00%	10.529%
28	23.633	3571	3578	3588	rVB	2279523	4383325	81.25%	8.556%


Sum of corrected areas: 51233442

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
Data File : BM007151.D
Acq On : 16 Aug 2016 20:52
Operator : UM/SJ
Sample : H4436-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA206

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

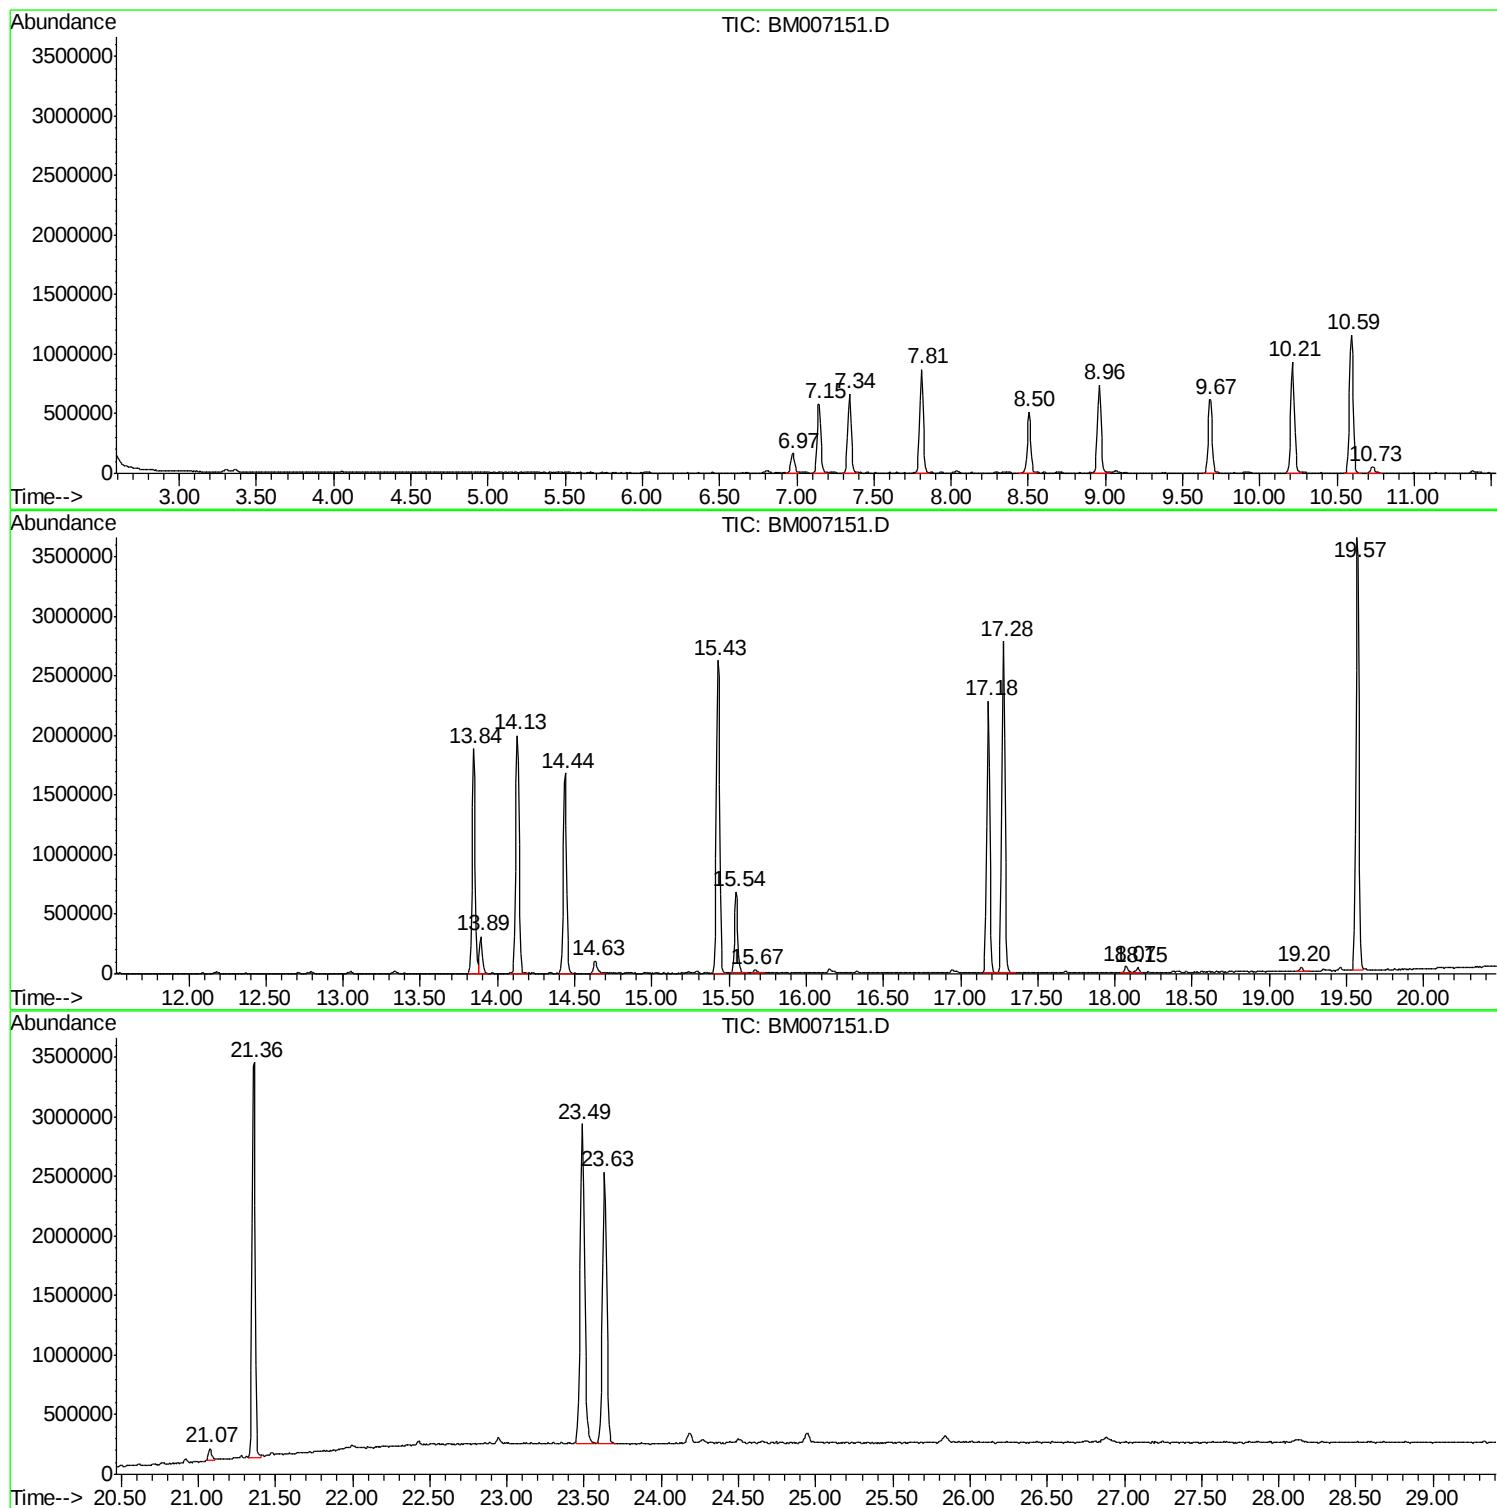

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007151.D
Acq On : 16 Aug 2016 20:52
Operator : UM/SJ
Sample : H4436-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA206

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007151.D
Acq On : 16 Aug 2016 20:52
Operator : UM/SJ
Sample : H4436-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA206

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc