

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
 Data File : BM007164.D
 Acq On : 17 Aug 2016 04:38
 Operator : UM/SJ
 Sample : H4423-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD2Q6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	121	126	134	rVB	59453	93251	1.16%	0.122%
2	6.975	738	746	757	rBV	1158732	1929695	24.07%	2.530%
3	7.139	765	774	783	rBV	883935	1388084	17.32%	1.820%
4	7.339	800	808	816	rBV	1238318	1977235	24.67%	2.593%
5	7.804	880	887	895	rBV	994694	1607592	20.05%	2.108%
6	8.504	996	1006	1018	rBV	1475140	2327084	29.03%	3.052%
7	8.957	1075	1083	1095	rBV	1127841	1858310	23.18%	2.437%
8	9.675	1198	1205	1215	rBV	960727	1598335	19.94%	2.096%
9	10.210	1288	1296	1305	rBV	1478034	2473874	30.86%	3.244%
10	10.592	1353	1361	1371	rBV	1263208	2188940	27.31%	2.870%
11	10.727	1375	1384	1397	rBV	1343342	2347996	29.29%	3.079%
12	13.845	1908	1914	1918	rBV	2527813	3562130	44.44%	4.671%
13	13.892	1918	1922	1932	rVB	1328630	1765336	22.02%	2.315%
14	14.127	1955	1962	1972	rVB	2893884	4212580	52.55%	5.524%
15	14.433	2007	2014	2022	rBV2	1834786	2921247	36.44%	3.831%
16	14.627	2041	2047	2066	rBV	848934	1386922	17.30%	1.819%
17	15.427	2177	2183	2190	rBV	3660733	5242945	65.40%	6.875%
18	15.545	2197	2203	2215	rBV	754256	1043479	13.02%	1.368%
19	15.668	2219	2224	2228	rBV2	50712	80296	1.00%	0.105%
20	16.151	2302	2306	2314	rBV	87519	155850	1.94%	0.204%
21	17.180	2474	2481	2486	rBV	2508174	3644474	45.46%	4.779%
22	17.221	2486	2488	2491	rVV	79193	92225	1.15%	0.121%
23	17.274	2491	2497	2508	rVB2	3942209	5780546	72.11%	7.580%
24	17.562	2540	2546	2556	rBV9	46196	86143	1.07%	0.113%
25	18.068	2623	2632	2636	rBV2	119442	175671	2.19%	0.230%
26	19.233	2827	2830	2838	rVB	126322	163593	2.04%	0.215%
27	19.568	2881	2887	2899	rBV	5074923	7340884	91.57%	9.626%
28	21.074	3139	3143	3149	rBV4	112617	164109	2.05%	0.215%
29	21.356	3185	3191	3197	rBV	3843881	5113539	63.79%	6.705%
30	22.944	3457	3461	3466	rBV3	117698	203862	2.54%	0.267%
31	23.491	3546	3554	3567	rVB2	4042470	8016284	100.00%	10.512%
32	23.633	3571	3578	3593	rVB	2611228	5064724	63.18%	6.641%
33	24.180	3667	3671	3677	rVB	135906	252756	3.15%	0.331%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
Data File : BM007164.D
Acq On : 17 Aug 2016 04:38
Operator : UM/SJ
Sample : H4423-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2Q6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Title : SVOA CALIBRATION


Sum of corrected areas: 76259991

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081716\
Data File : BM007164.D
Acq On : 17 Aug 2016 04:38
Operator : UM/SJ
Sample : H4423-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2Q6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

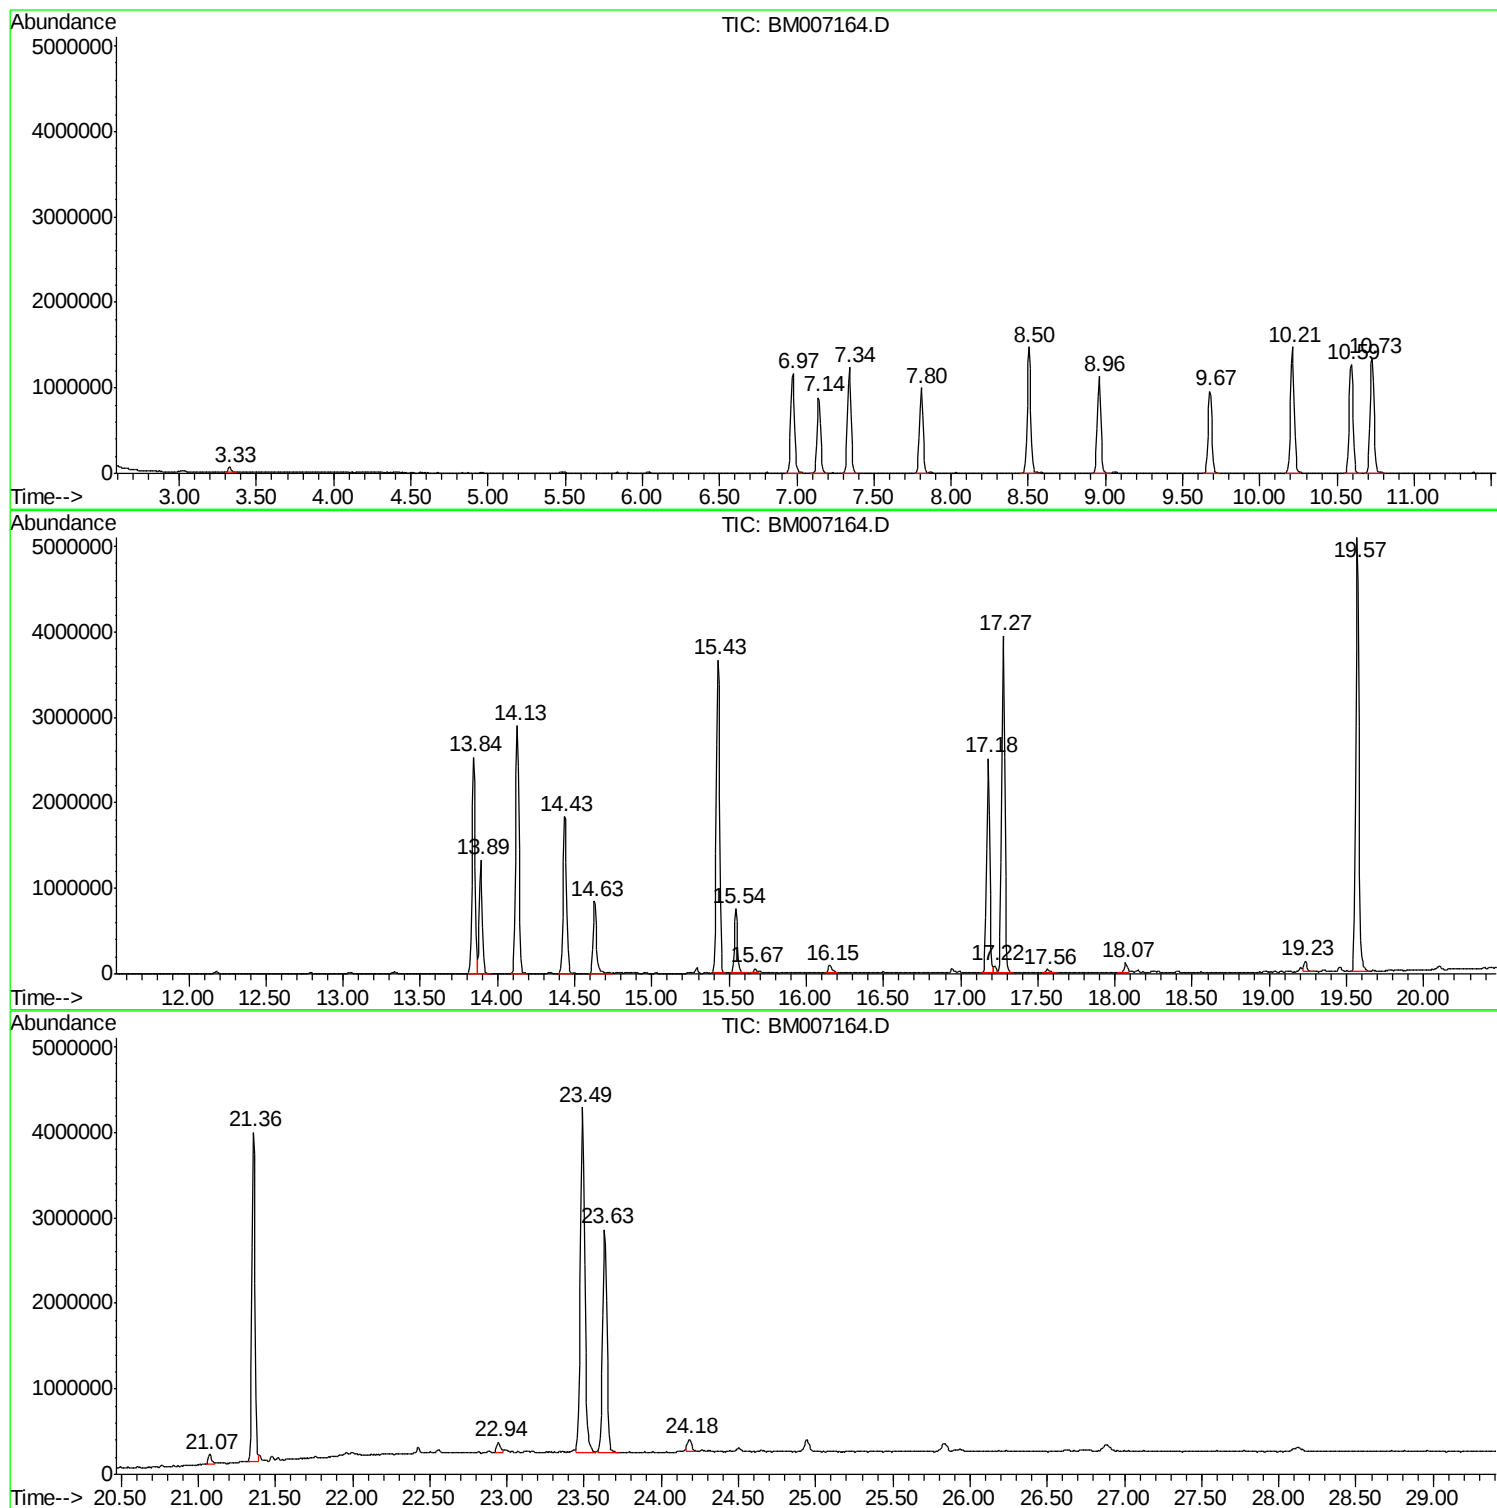

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007164.D
Acq On : 17 Aug 2016 04:38
Operator : UM/SJ
Sample : H4423-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2Q6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081716\
Data File : BM007164.D
Acq On : 17 Aug 2016 04:38
Operator : UM/SJ
Sample : H4423-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD2Q6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc