
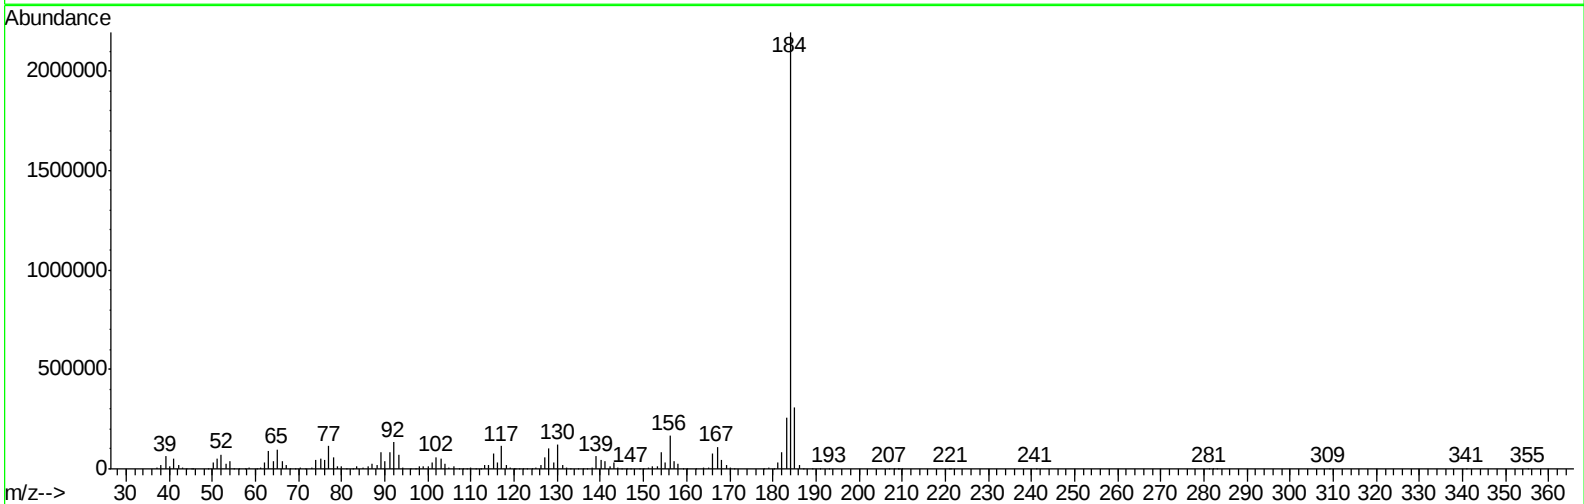


```
Data Path : Z:\HPCHEM1\BNA M\DATA\BM081717\  
Data File : BM011285.D  
Acq On    : 18 Aug 2017  03:12  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 18 06:36:56 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

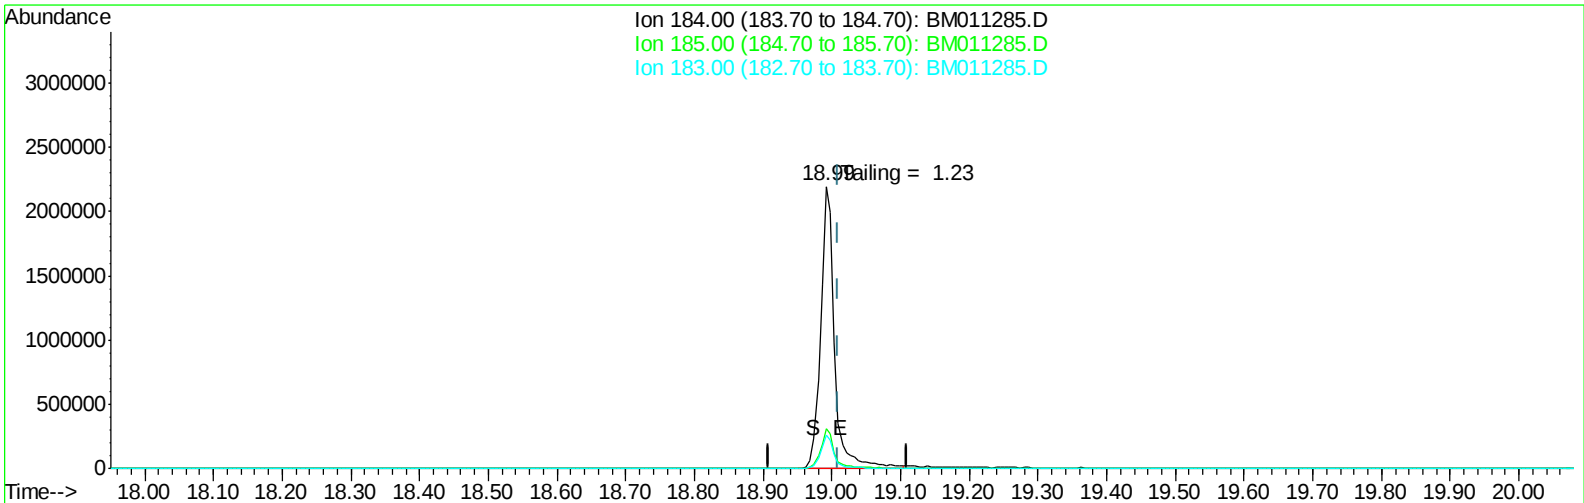

TIC: BM011285.D

(76) Benzidine



18.992min (-0.018) 3562.27ng

```
response 3086818
```

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.97
183.00	11.10	11.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081717\
Data File : BM011285.D
Acq On : 18 Aug 2017 03:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 06:36:56 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

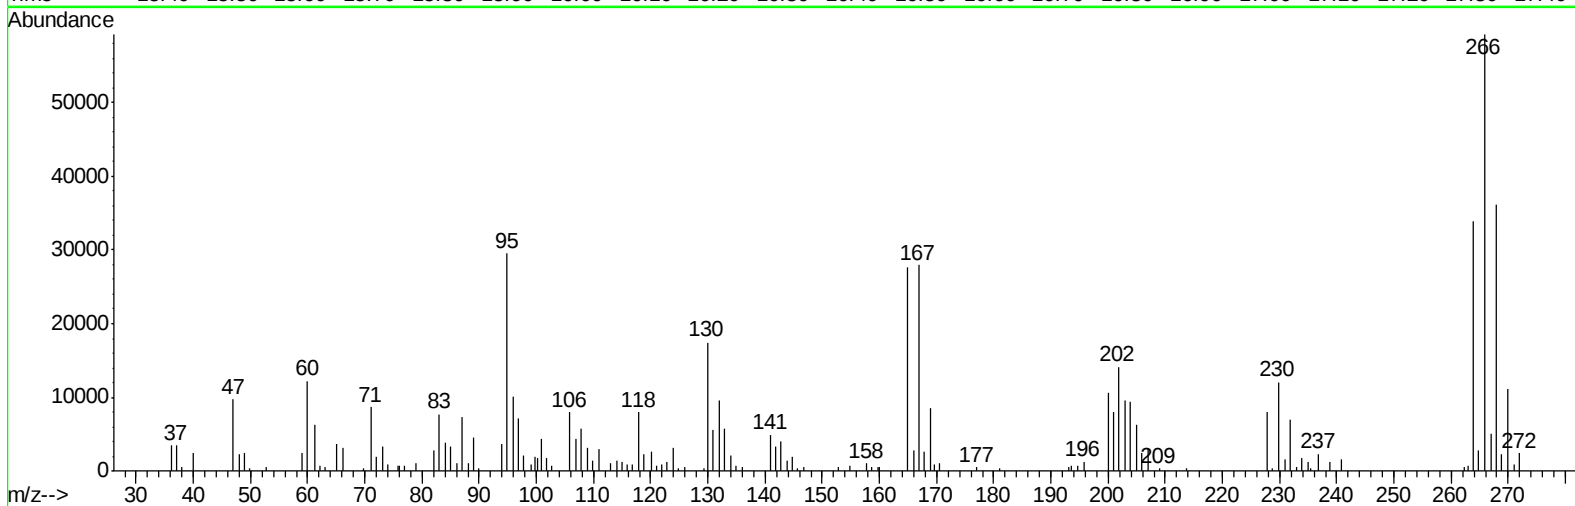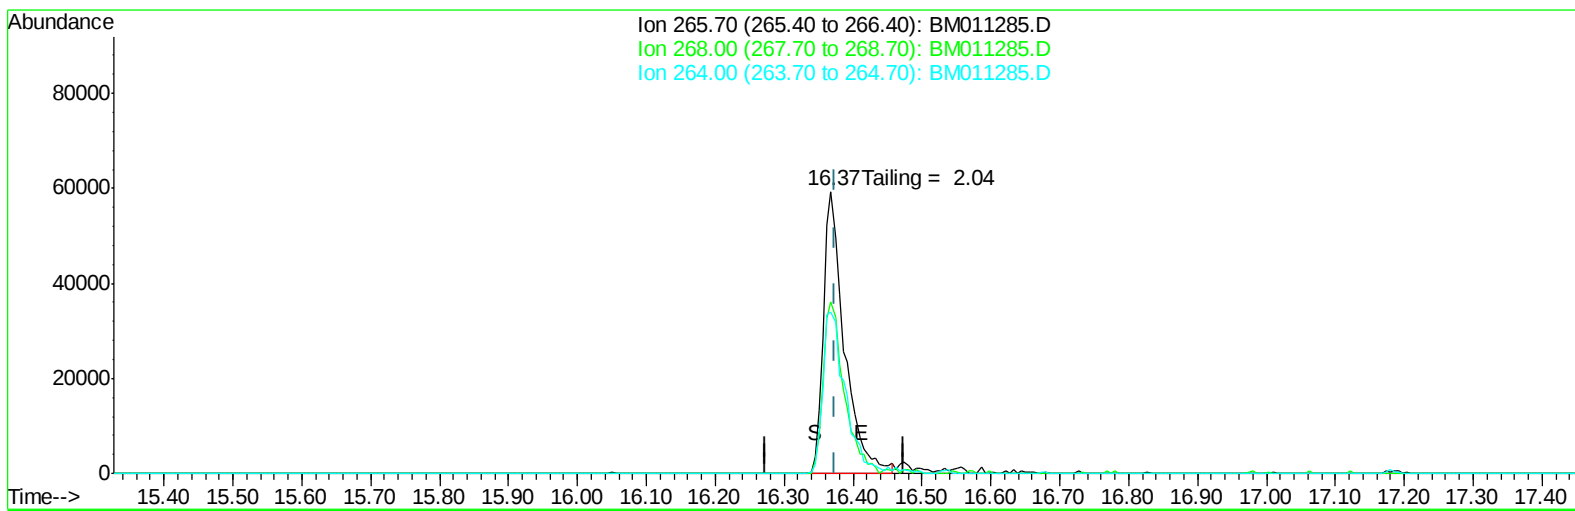

TIC: BM011285.D

(69) Pentachlorophenol (C)

16.368min (-0.006) 686.36ng

response 123809

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.91
264.00	61.20	57.10
0.00	0.00	0.00