
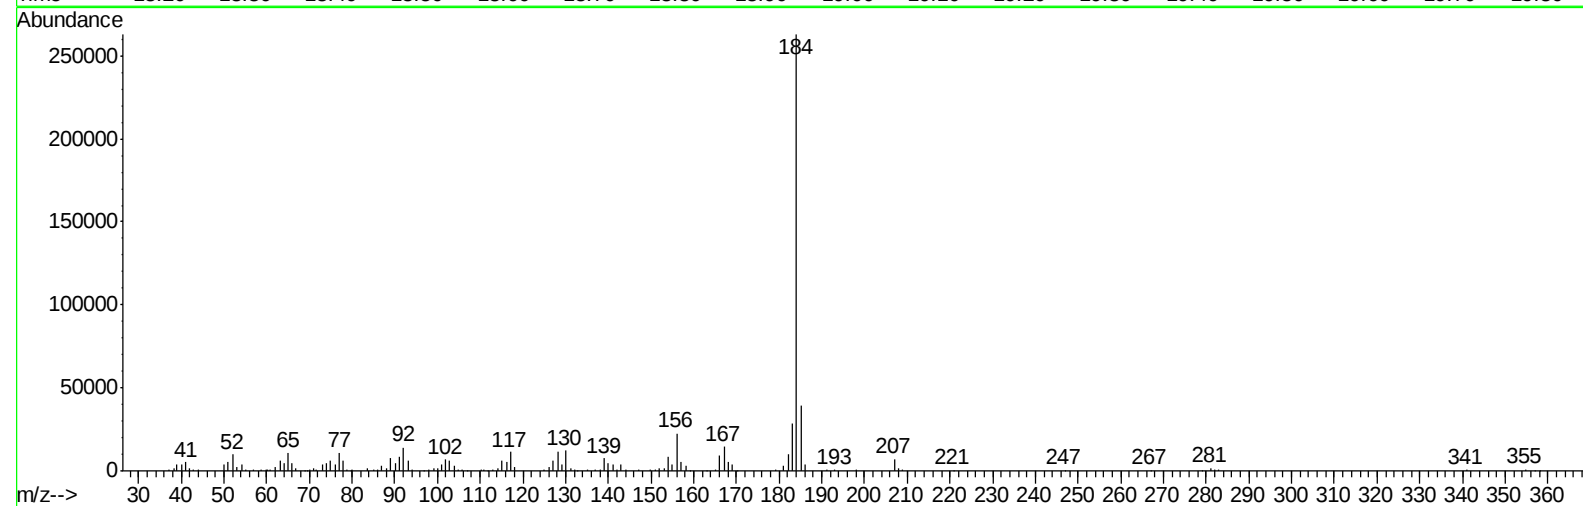


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081717\
 Data File : BM011266.D
 Acq On : 17 Aug 2017 14:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 06:38:12 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration

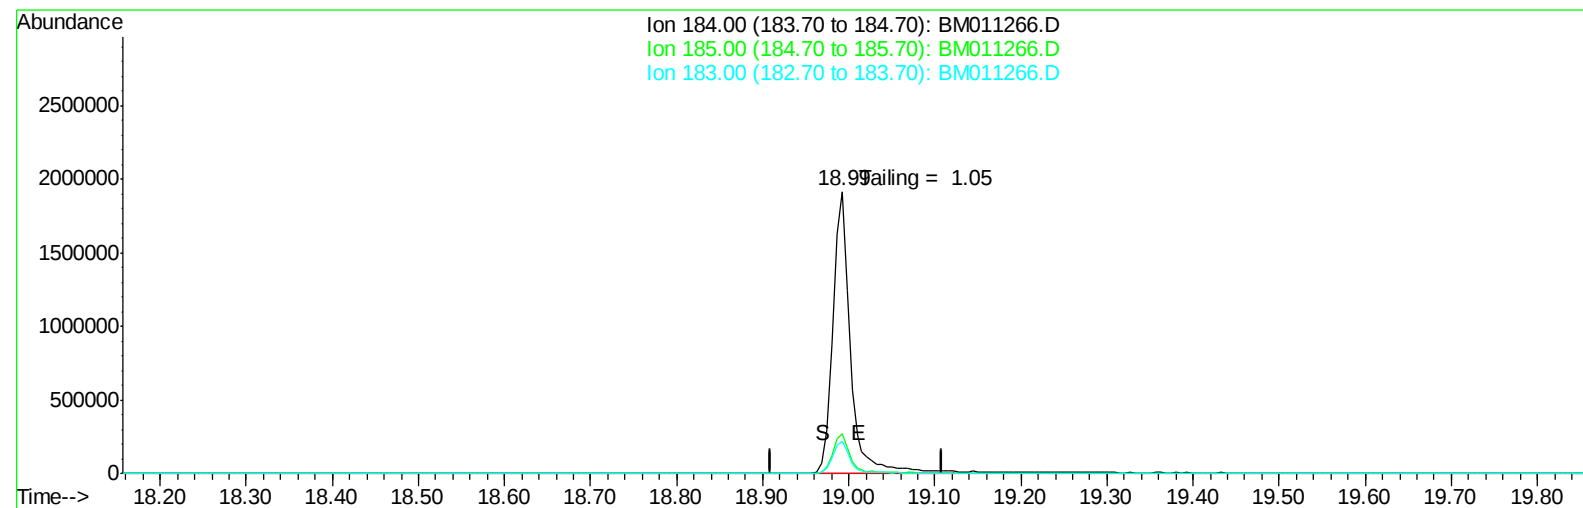

TIC: BM011266.D

(76) Benzidine



19.009min (-19.009) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.10	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081717\
Data File : BM011266.D
Acq On : 17 Aug 2017 14:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 06:38:12 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

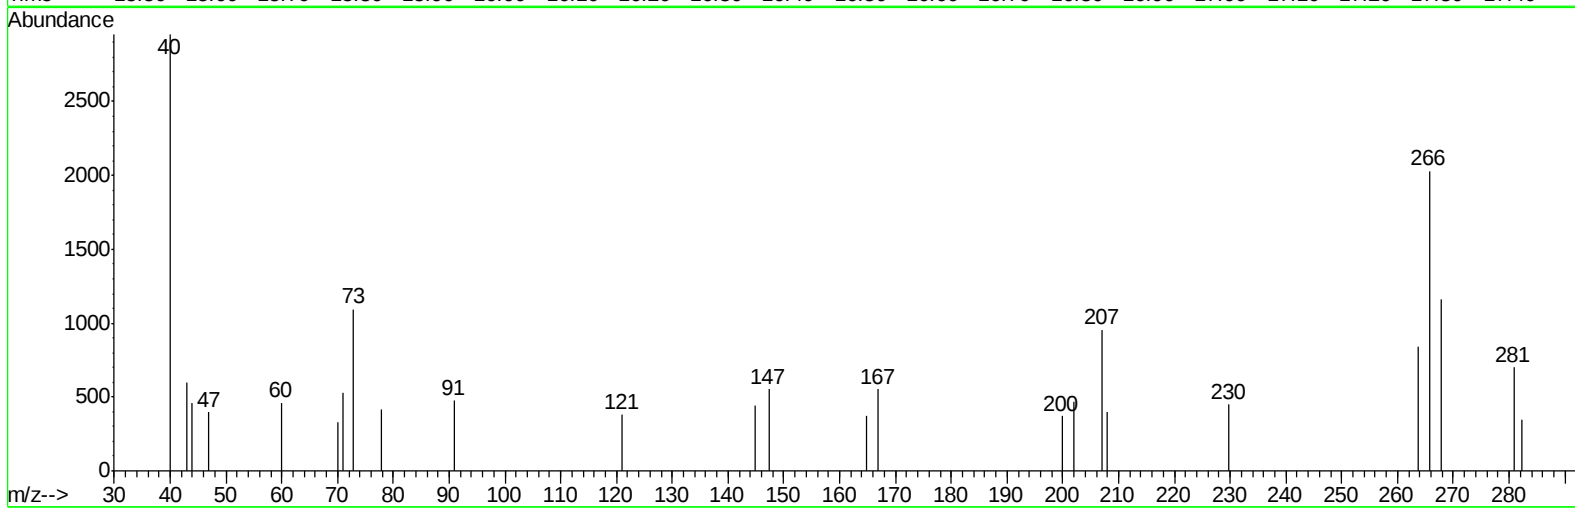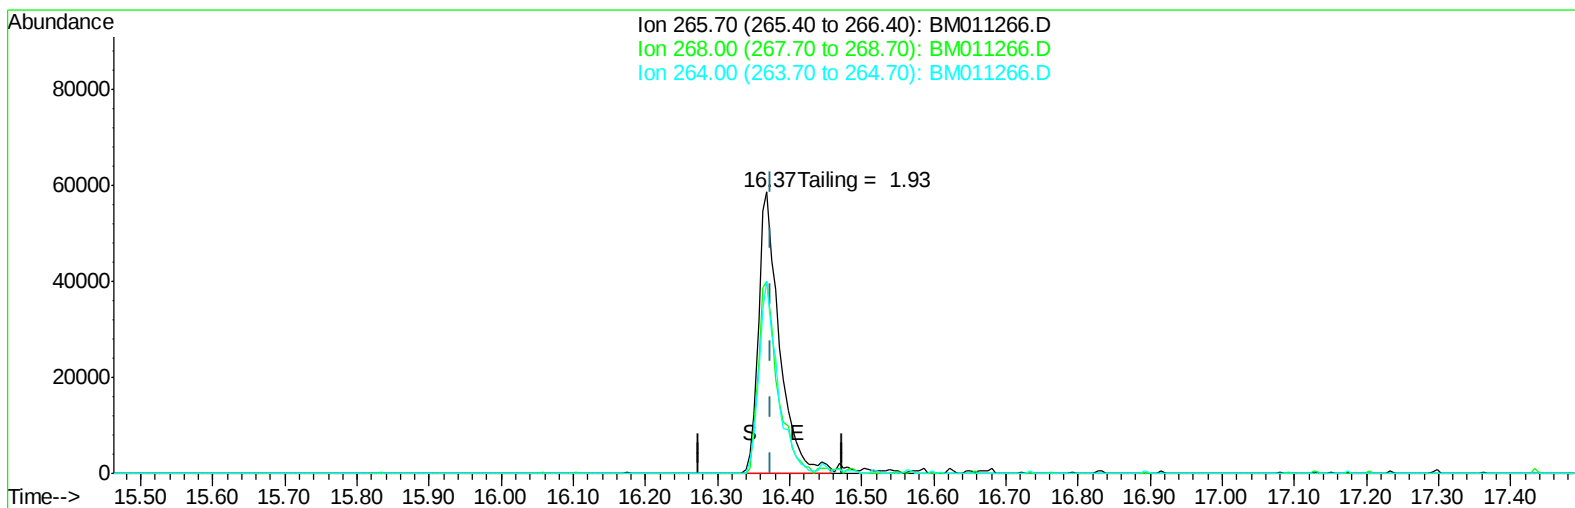

TIC: BM011266.D

(69) Pentachlorophenol (C)

16.468min (+0.094) 170.56ng

response 1326

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	57.45
264.00	61.20	41.32#
0.00	0.00	0.00