


Data Path : Z:\HPCHEM1\BNA M\Data\BM081717\
 Data File : BM011285.D
 Acq On : 18 Aug 2017 03:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

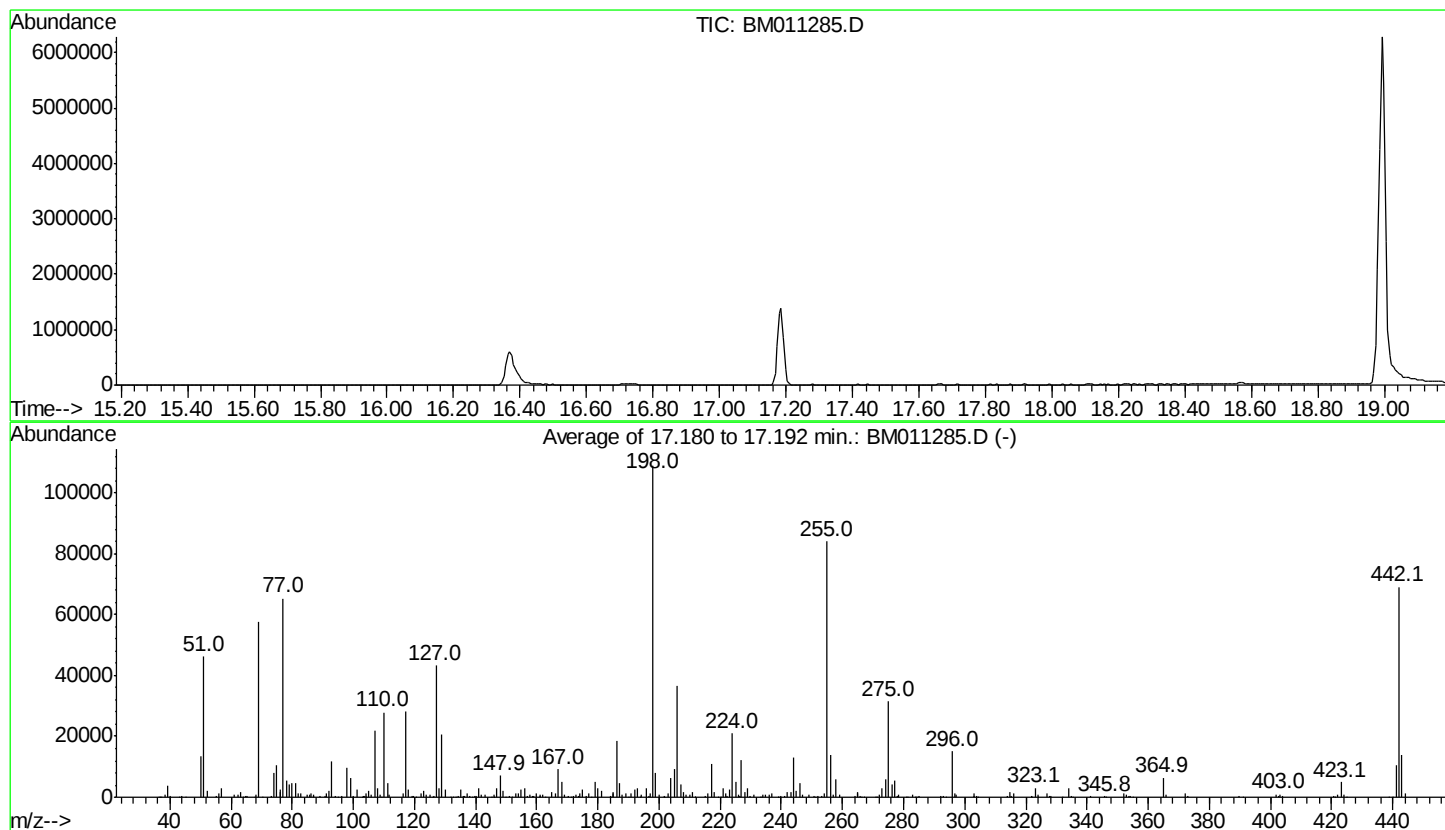

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	46266	PASS
68	69	0.00	2	1.6	903	PASS
69	198	0.00	100	52.8	57568	PASS
70	69	0.00	2	0.2	137	PASS
127	198	10	80	39.7	43274	PASS
197	198	0.00	2	1.0	1085	PASS
198	198	100	100	100.0	109000	PASS
199	198	5	9	7.5	8180	PASS
275	198	10	60	28.9	31498	PASS
365	198	1	100	5.8	6337	PASS
441	442	0.01	24	15.5	10699	PASS
442	198	50	100	63.3	69034	PASS
443	442	15	24	19.9	13710	PASS