

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081718\
 Data File : BM016448.D
 Acq On : 17 Aug 2018 21:42
 Operator : SJ/JU
 Sample : J4486-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ202RE

Quant Time: Aug 18 00:14:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 16:27:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	13277	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	48890	20.00	ng	0.00
38) Acenaphthene-d10	14.70	164	28354	20.00	ng	0.00
63) Phenanthrene-d10	17.44	188	75196	20.00	ng	0.00
75) Chrysene-d12	21.58	240	106414	20.00	ng	0.00
86) Perylene-d12	23.89	264	120427	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	119941	151.82	ng	0.00
7) Phenol-d6	7.23	99	131823	124.14	ng	0.00
23) Nitrobenzene-d5	9.25	82	130153	110.87	ng	0.00
41) 2,4,6-Tribromophenol	16.19	330	82513	192.68	ng	0.00
44) 2-Fluorobiphenyl	13.32	172	265282	97.29	ng	0.00
78) Terphenyl-d14	20.03	244	836298	118.78	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.37	79	2618	2.716	ng	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081718\
Data File : BM016448.D
Acq On : 17 Aug 2018 21:42
Operator : SJ/JU
Sample : J4486-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ202RE

Quant Time: Aug 18 00:14:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 16:27:00 2018
Response via : Initial Calibration

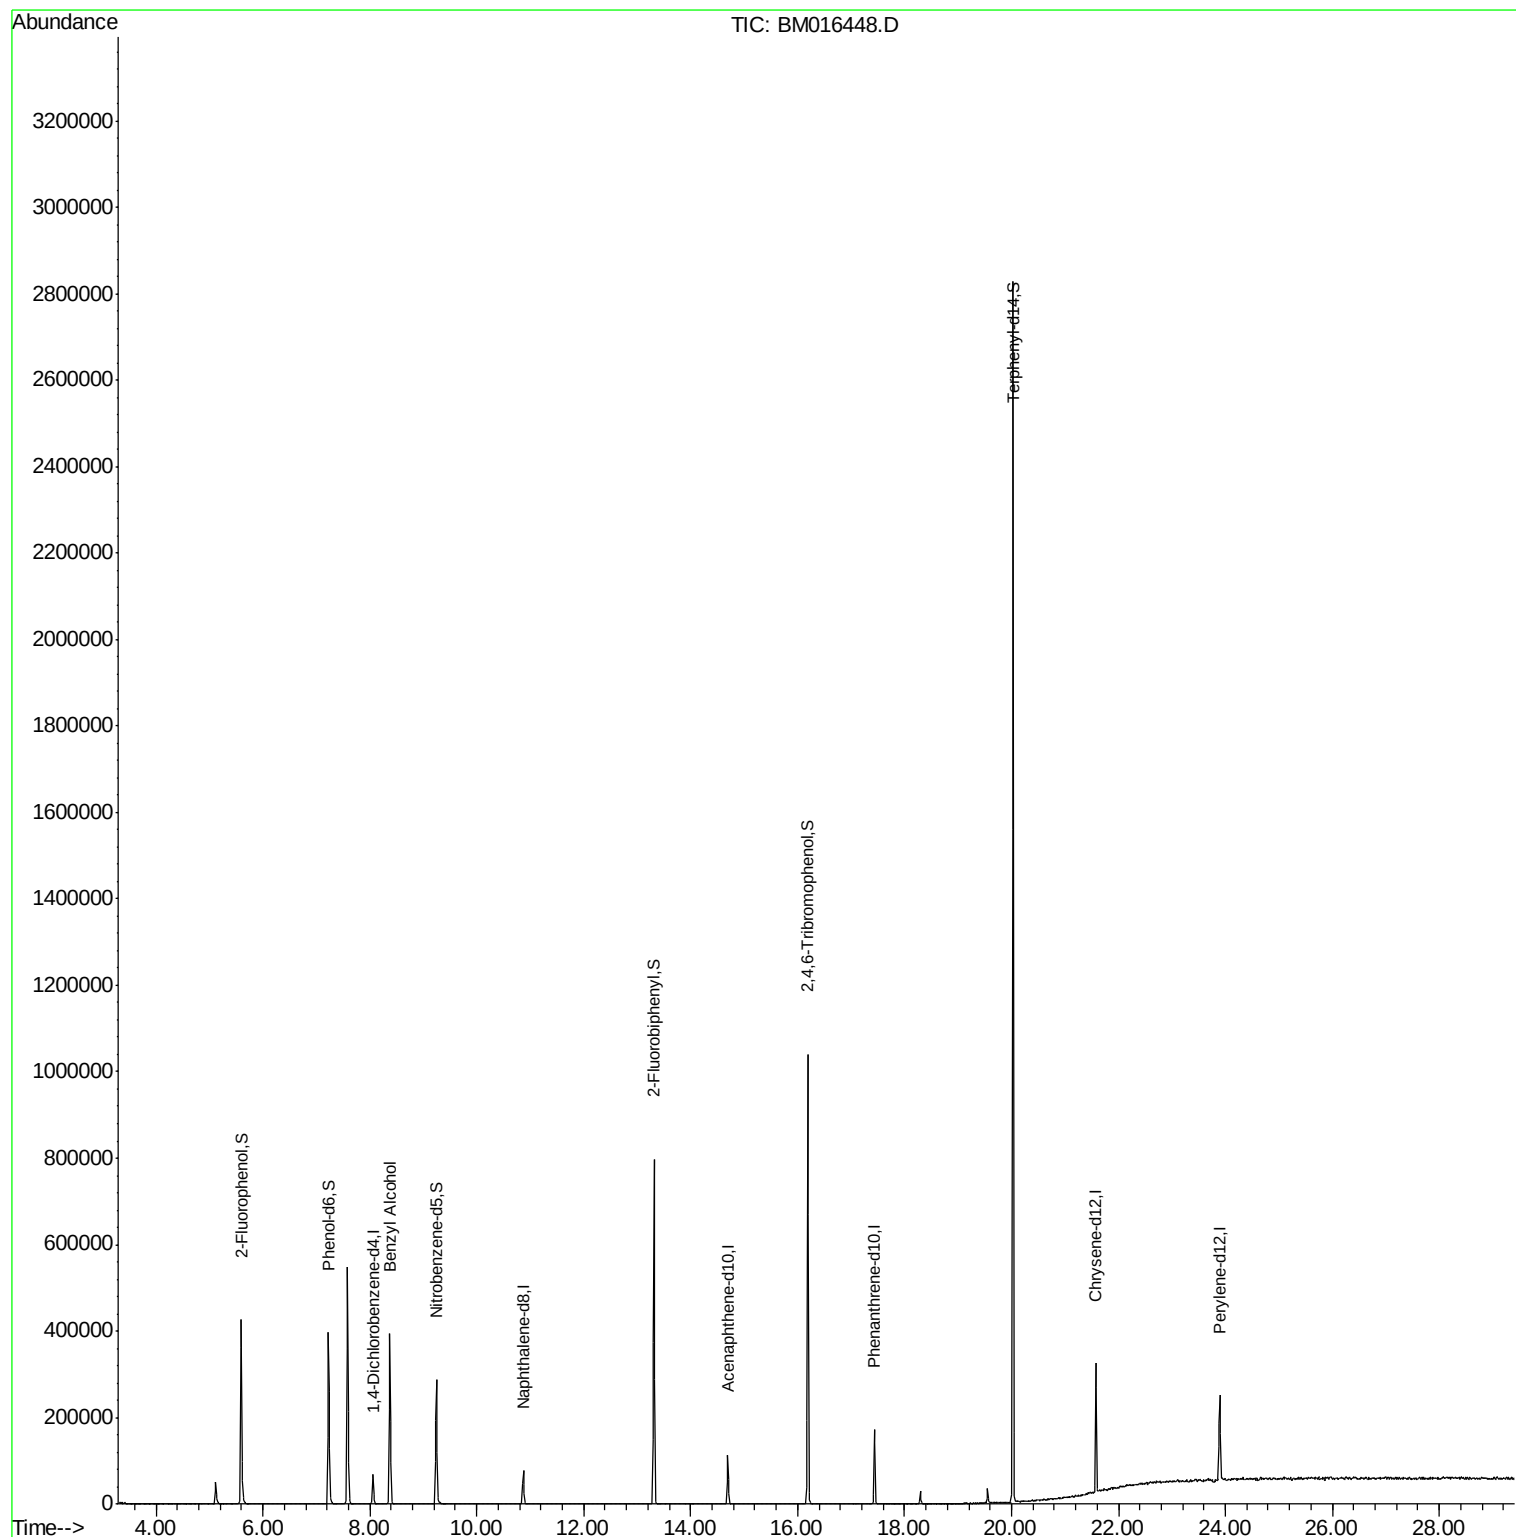

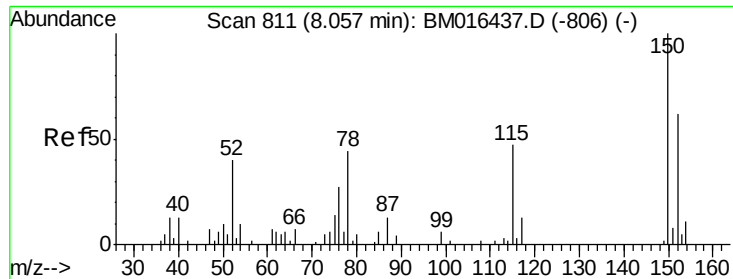

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.06 min Scan# 811

Delta R.T. 0.00 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42

Instrument :

BNA_M

ClientSampleId :

VNJ202RE


Tgt Ion:152 Resp: 13277

Ion Ratio Lower Upper

152 100

150 159.1 119.5 179.3




115 70.8 43.0 64.4#

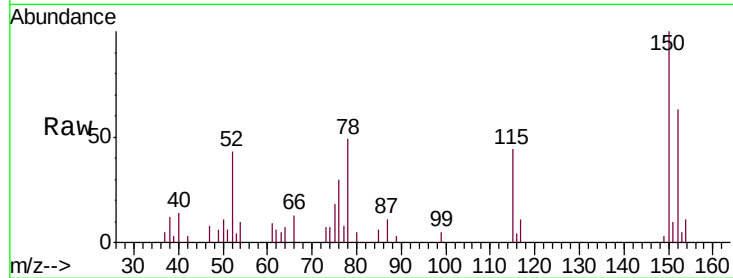

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

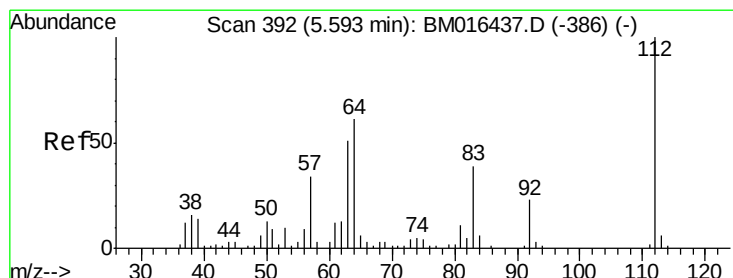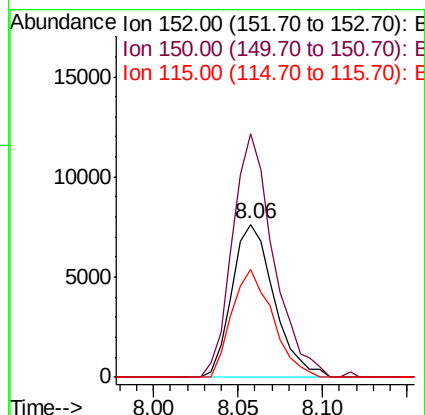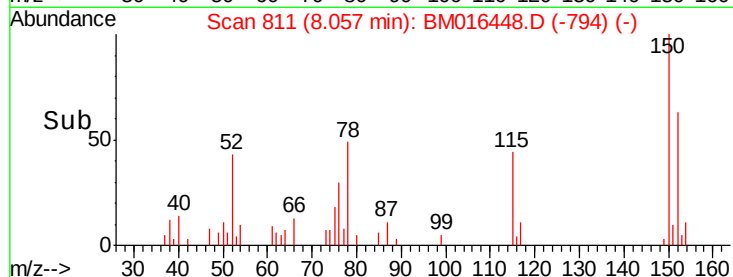

#5

2-Fluorophenol

Concen: N.D. ng

RT: 5.59 min Scan# 392

Delta R.T. 0.00 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42


Tgt Ion:112 Resp: 119941

Ion Ratio Lower Upper

112 100

64 61.4 38.6 57.8#



63 50.1 19.3 28.9#

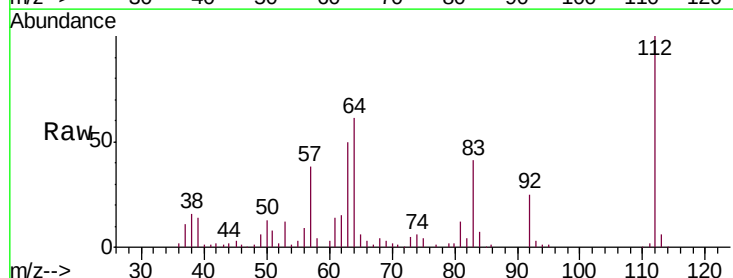


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

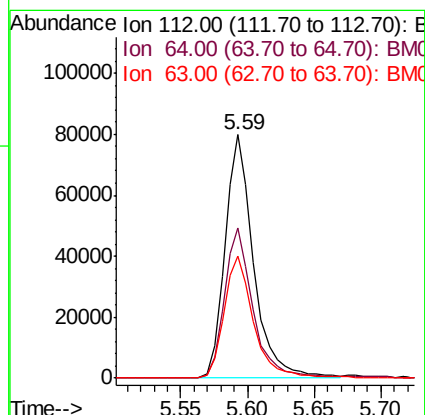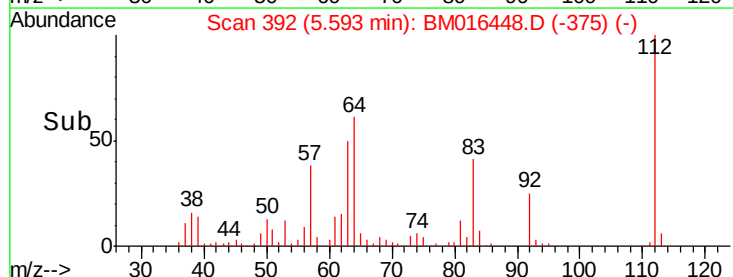

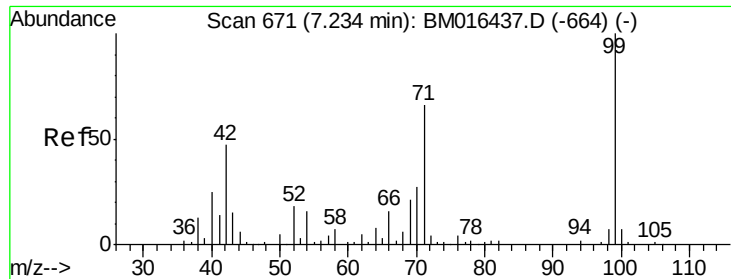

#7

Phenol-d6

Concen: N.D. ng

RT: 7.23 min Scan# 671

Delta R.T. 0.00 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42

Instrument :

BNA_M

ClientSampleId :

VNJ202RE


Tgt Ion: 99 Resp: 131823

Ion Ratio Lower Upper

99 100

42 48.1 11.0 16.4#




71 64.4 23.4 35.2#

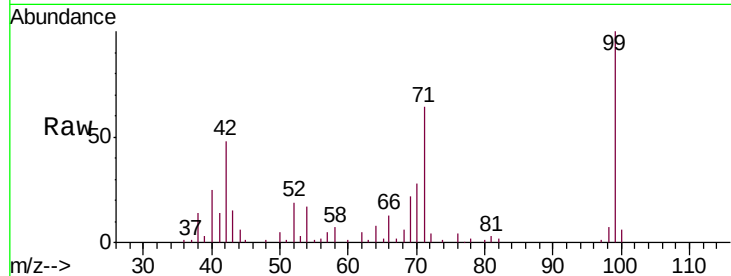

Abundance Ion 99.00 (98.70 to 99.70): BM016437.D (-664) (-)

Ion 42.00 (41.70 to 42.70): BM016437.D (-664) (-)

Ion 71.00 (70.70 to 71.70): BM016437.D (-664) (-)

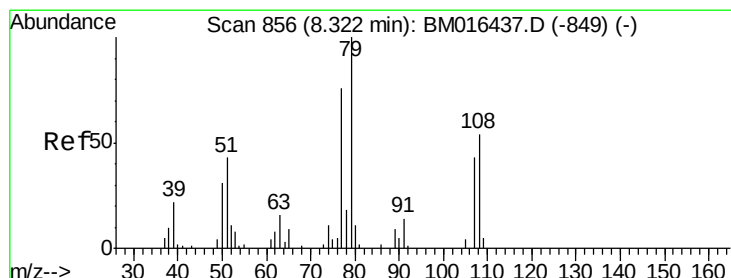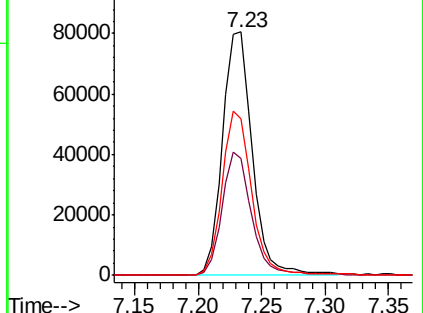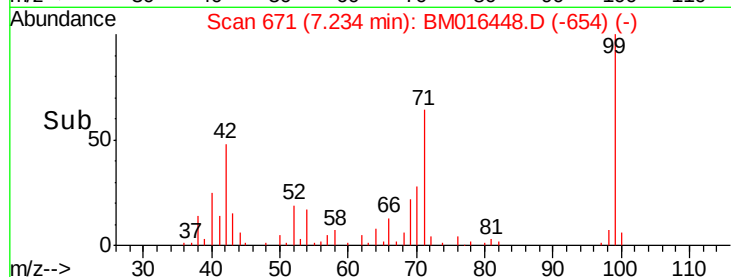

#15

Benzyl Alcohol

Concen: 2.716 ng

RT: 8.37 min Scan# 865

Delta R.T. 0.05 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42


Tgt Ion: 79 Resp: 2618

Ion Ratio Lower Upper

79 100

108 123.1 65.0 97.4#



77 235.5 53.0 79.6#

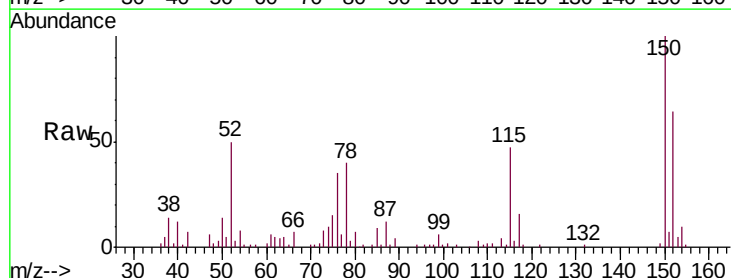


Abundance Ion 79.00 (78.70 to 79.70): BM016437.D (-849) (-)

Ion 108.00 (107.70 to 108.70): BM016437.D (-849) (-)

Ion 77.00 (76.70 to 77.70): BM016437.D (-849) (-)



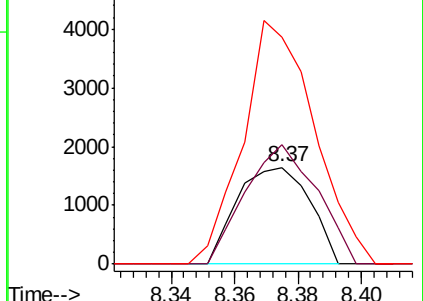
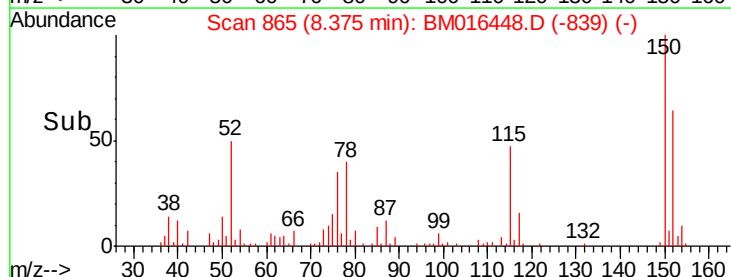


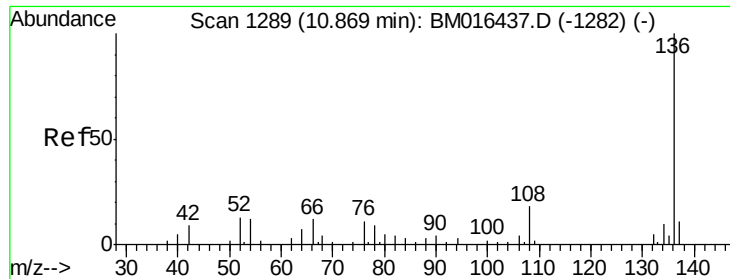

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.87 min Scan# 1289
Delta R.T. 0.00 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42




Instrument :
BNA_M
ClientSampleId :
VNJ202RE


Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.7	13.1
54	11.7	4.6	6.8#
68	3.1	3.7	5.5#

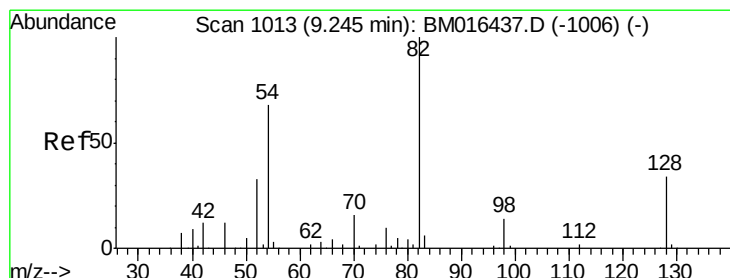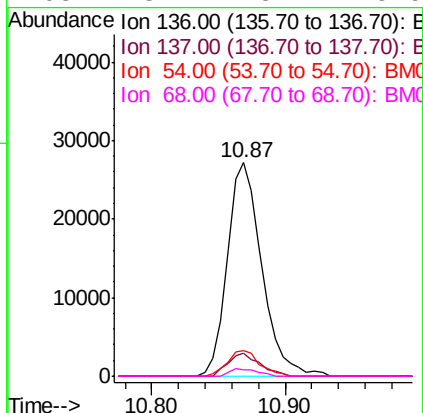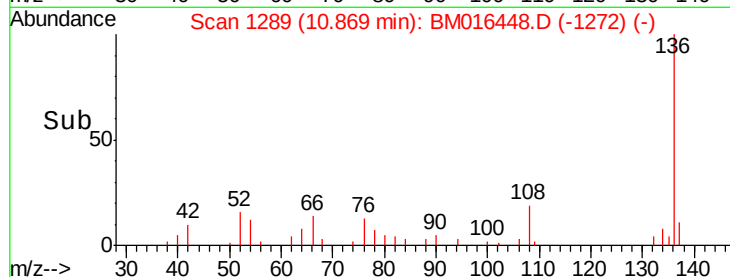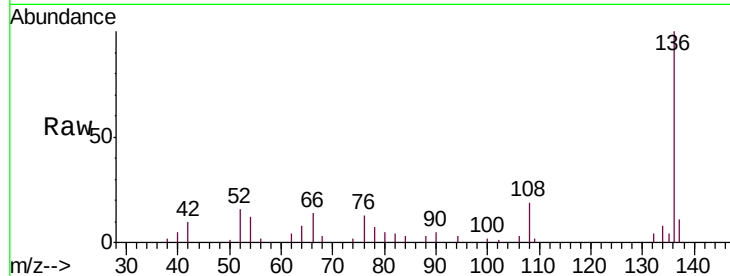

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.25 min Scan# 1013
Delta R.T. 0.00 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42

Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.2	32.8	49.2
54	68.0	40.6	60.8#

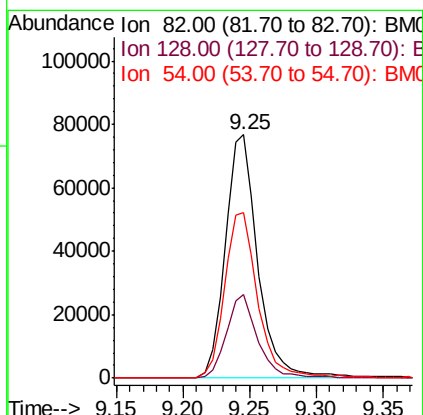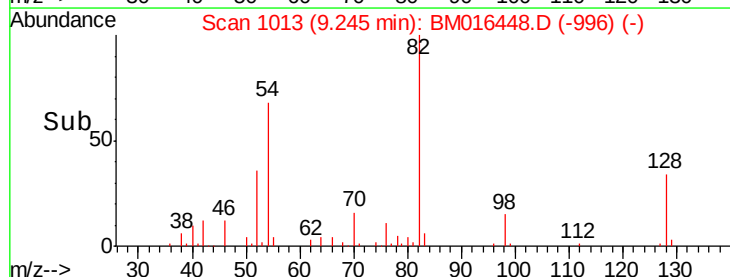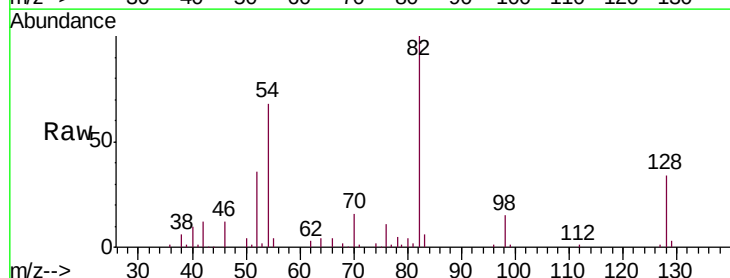

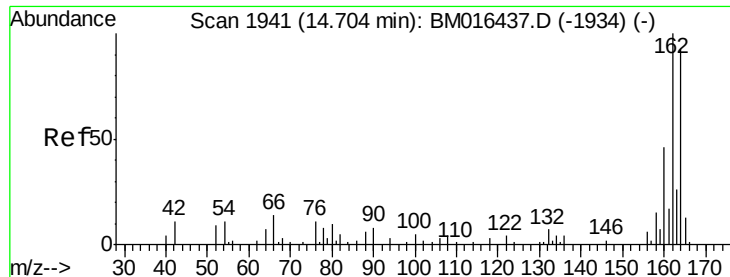

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.70 min Scan# 1940

Delta R.T. -0.01 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42

Instrument :

BNA_M

ClientSampleId :

VNJ202RE


Tgt Ion:164 Resp: 28354

Ion Ratio Lower Upper

164 100

162 112.2 82.4 123.6




160 50.3 35.8 53.6

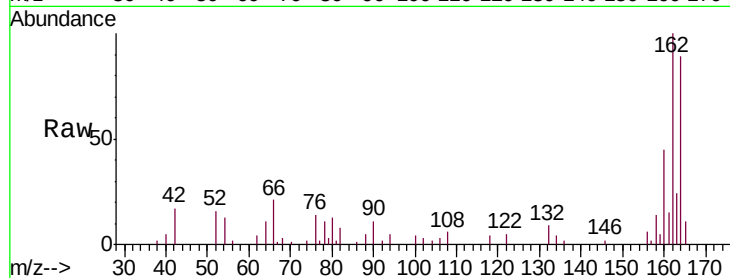

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

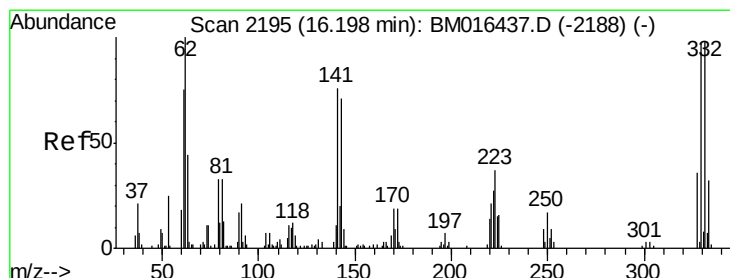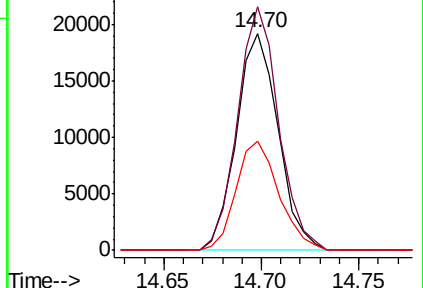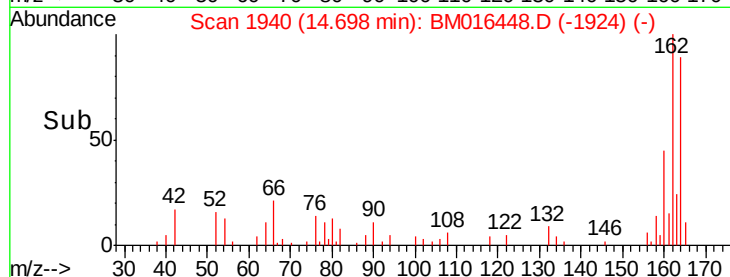

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.19 min Scan# 2194

Delta R.T. -0.01 min

Lab File: BM016448.D

Acq: 17 Aug 2018 21:42


Tgt Ion:330 Resp: 82513

Ion Ratio Lower Upper

330 100

332 97.1 0.0 0.0#



141 94.0 0.0 0.0#

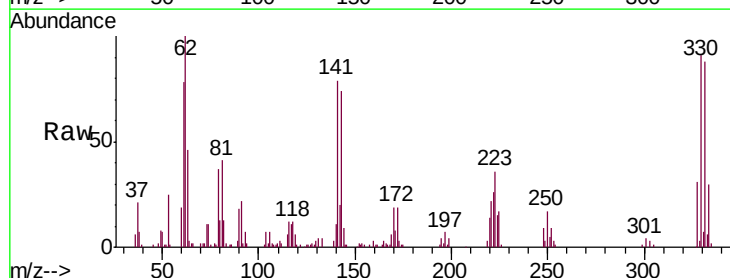


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



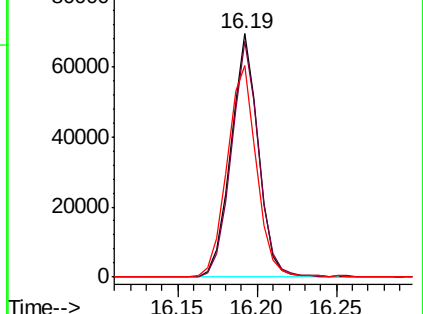
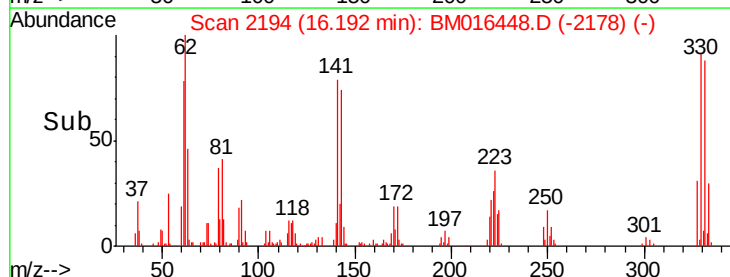


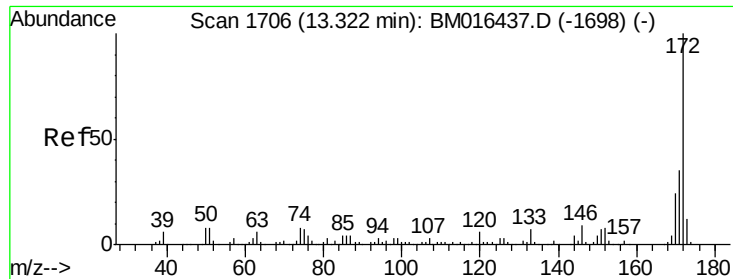

#44
2-Fluorobiphenyl
Concen: N.D. ng
RT: 13.32 min Scan# 1705
Delta R.T. -0.01 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42




Instrument :
BNA_M
ClientSampleId :
VNJ202RE


Tgt Ion:172 Resp: 265282
Ion Ratio Lower Upper
172 100
171 36.6 28.5 42.7
170 25.1 18.8 28.2

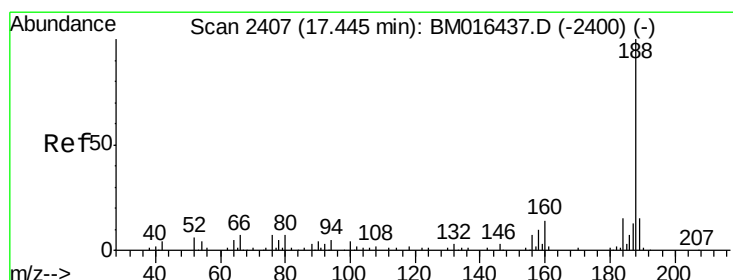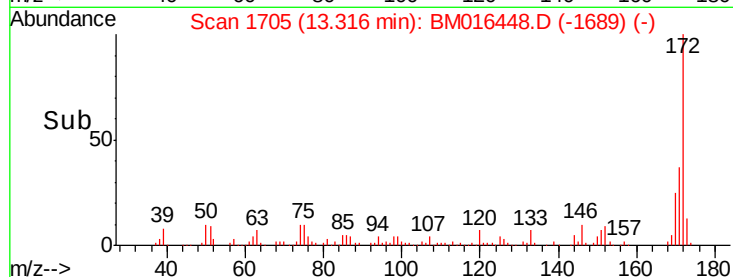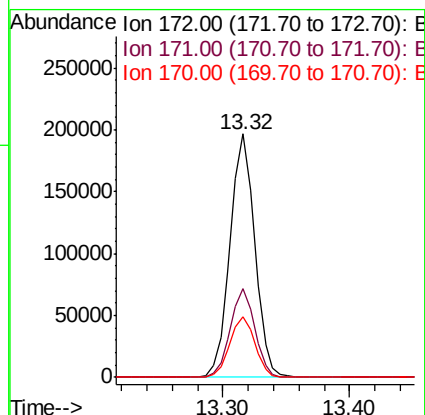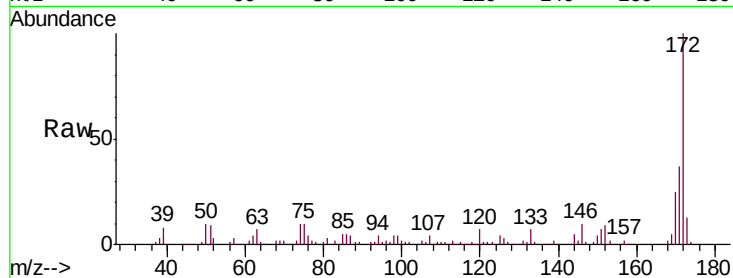

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.44 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42

Tgt Ion:188 Resp: 75196
Ion Ratio Lower Upper
188 100
94 5.9 8.7 13.1#
80 5.7 9.3 13.9#


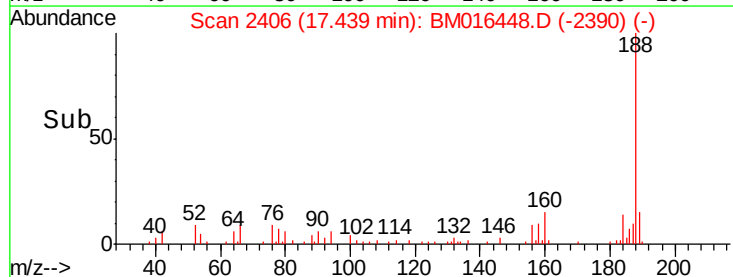
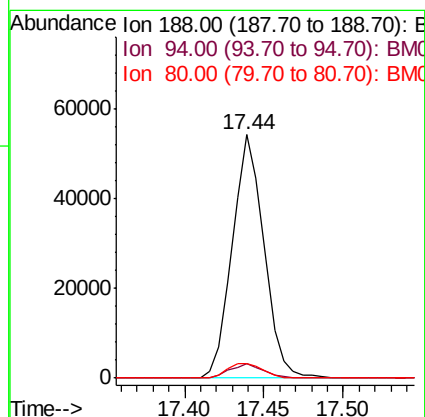
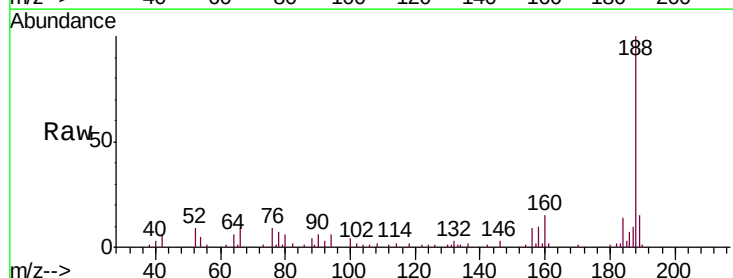


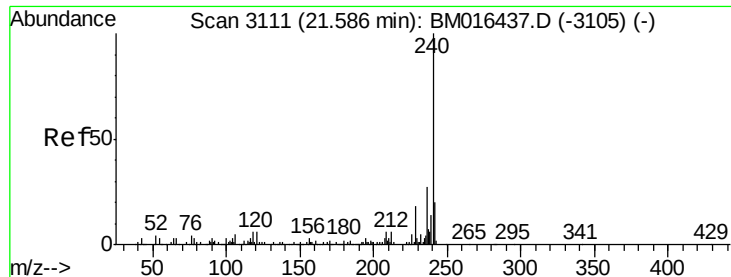

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.58 min Scan# 3110
Delta R.T. -0.01 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42




Instrument :
BNA_M
ClientSampleId :
VNJ202RE


Tgt Ion	Ratio	Lower	Upper
240	100		
120	5.7	8.2	12.2#
236	28.0	20.0	30.0

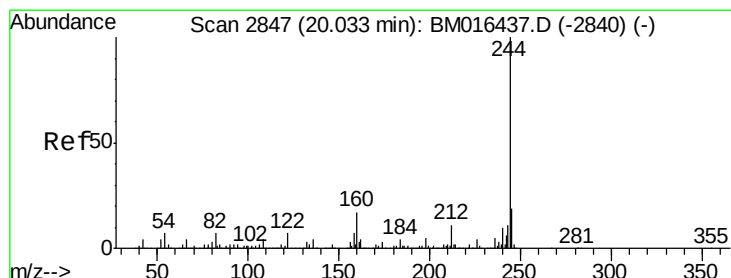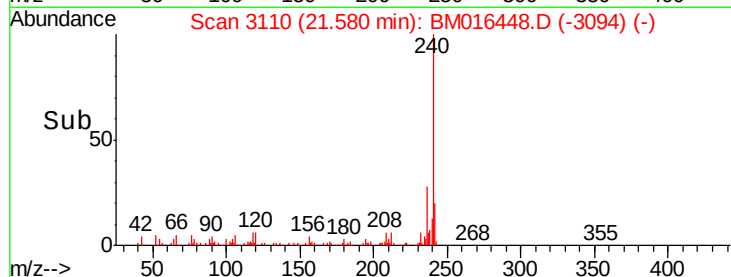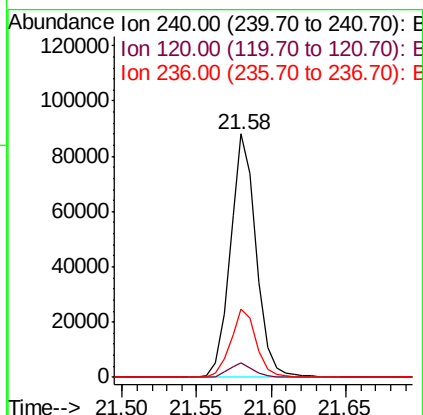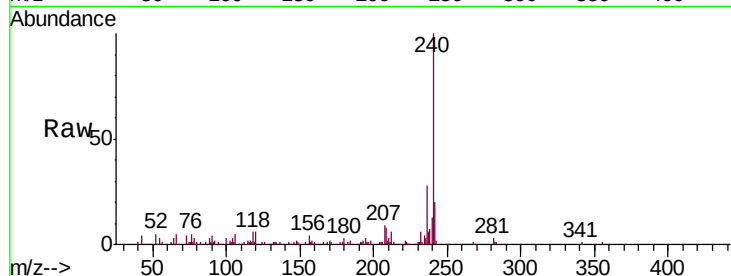

#78
Terphenyl-d14
Concen: N.D. ng
RT: 20.03 min Scan# 2846
Delta R.T. -0.00 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42

Tgt Ion	Ratio	Lower	Upper
244	100		
212	11.1	4.9	7.3#
122	7.6	6.2	9.4

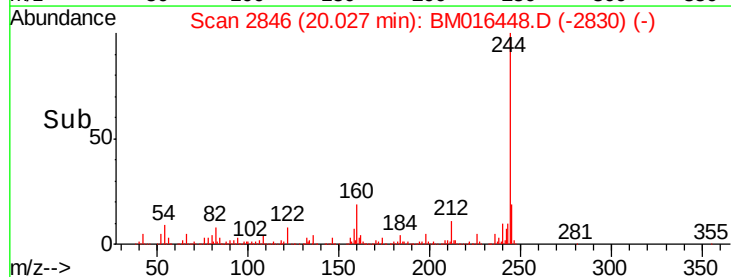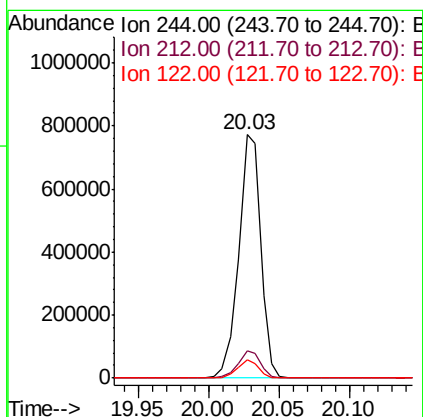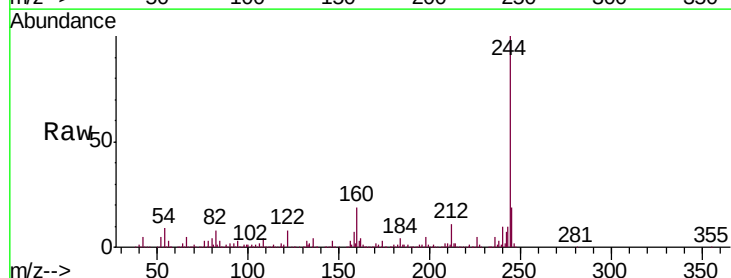

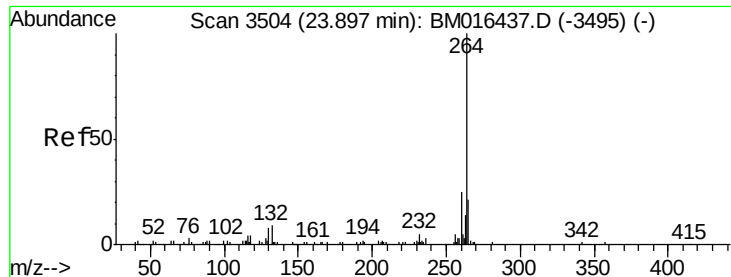

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.89 min Scan# 3503
Delta R.T. -0.01 min
Lab File: BM016448.D
Acq: 17 Aug 2018 21:42

Instrument :
BNA_M
ClientSampleId :
VNJ202RE

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	18.6	27.8
265	21.3	17.3	25.9

