

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
 Data File : BM016472.D
 Acq On : 18 Aug 2018 14:05
 Operator : SJ/JU
 Sample : J4521-24
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 20 01:17:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 16:27:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	7740	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	29333	20.00	ng	0.00
38) Acenaphthene-d10	14.69	164	19460	20.00	ng	-0.01
63) Phenanthrene-d10	17.43	188	56102	20.00	ng	-0.01
75) Chrysene-d12	21.57	240	90118	20.00	ng	-0.01
86) Perylene-d12	23.89	264	105682	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	64296	139.60	ng	0.00
7) Phenol-d6	7.22	99	69655	112.52	ng	-0.01
23) Nitrobenzene-d5	9.24	82	78157	110.97	ng	0.00
41) 2,4,6-Tribromophenol	16.19	330	62124	211.37	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	173657	92.79	ng	-0.01
78) Terphenyl-d14	20.03	244	662720	111.15	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.37	79	1560	2.776	ng	Qvalue # 22
31) Naphthalene	10.92	128	14368	9.658	ng	97
76) Benzidine	19.67	184	50964	25.695	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
Data File : BM016472.D
Acq On : 18 Aug 2018 14:05
Operator : SJ/JU
Sample : J4521-24
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 20 01:17:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 16:27:00 2018
Response via : Initial Calibration

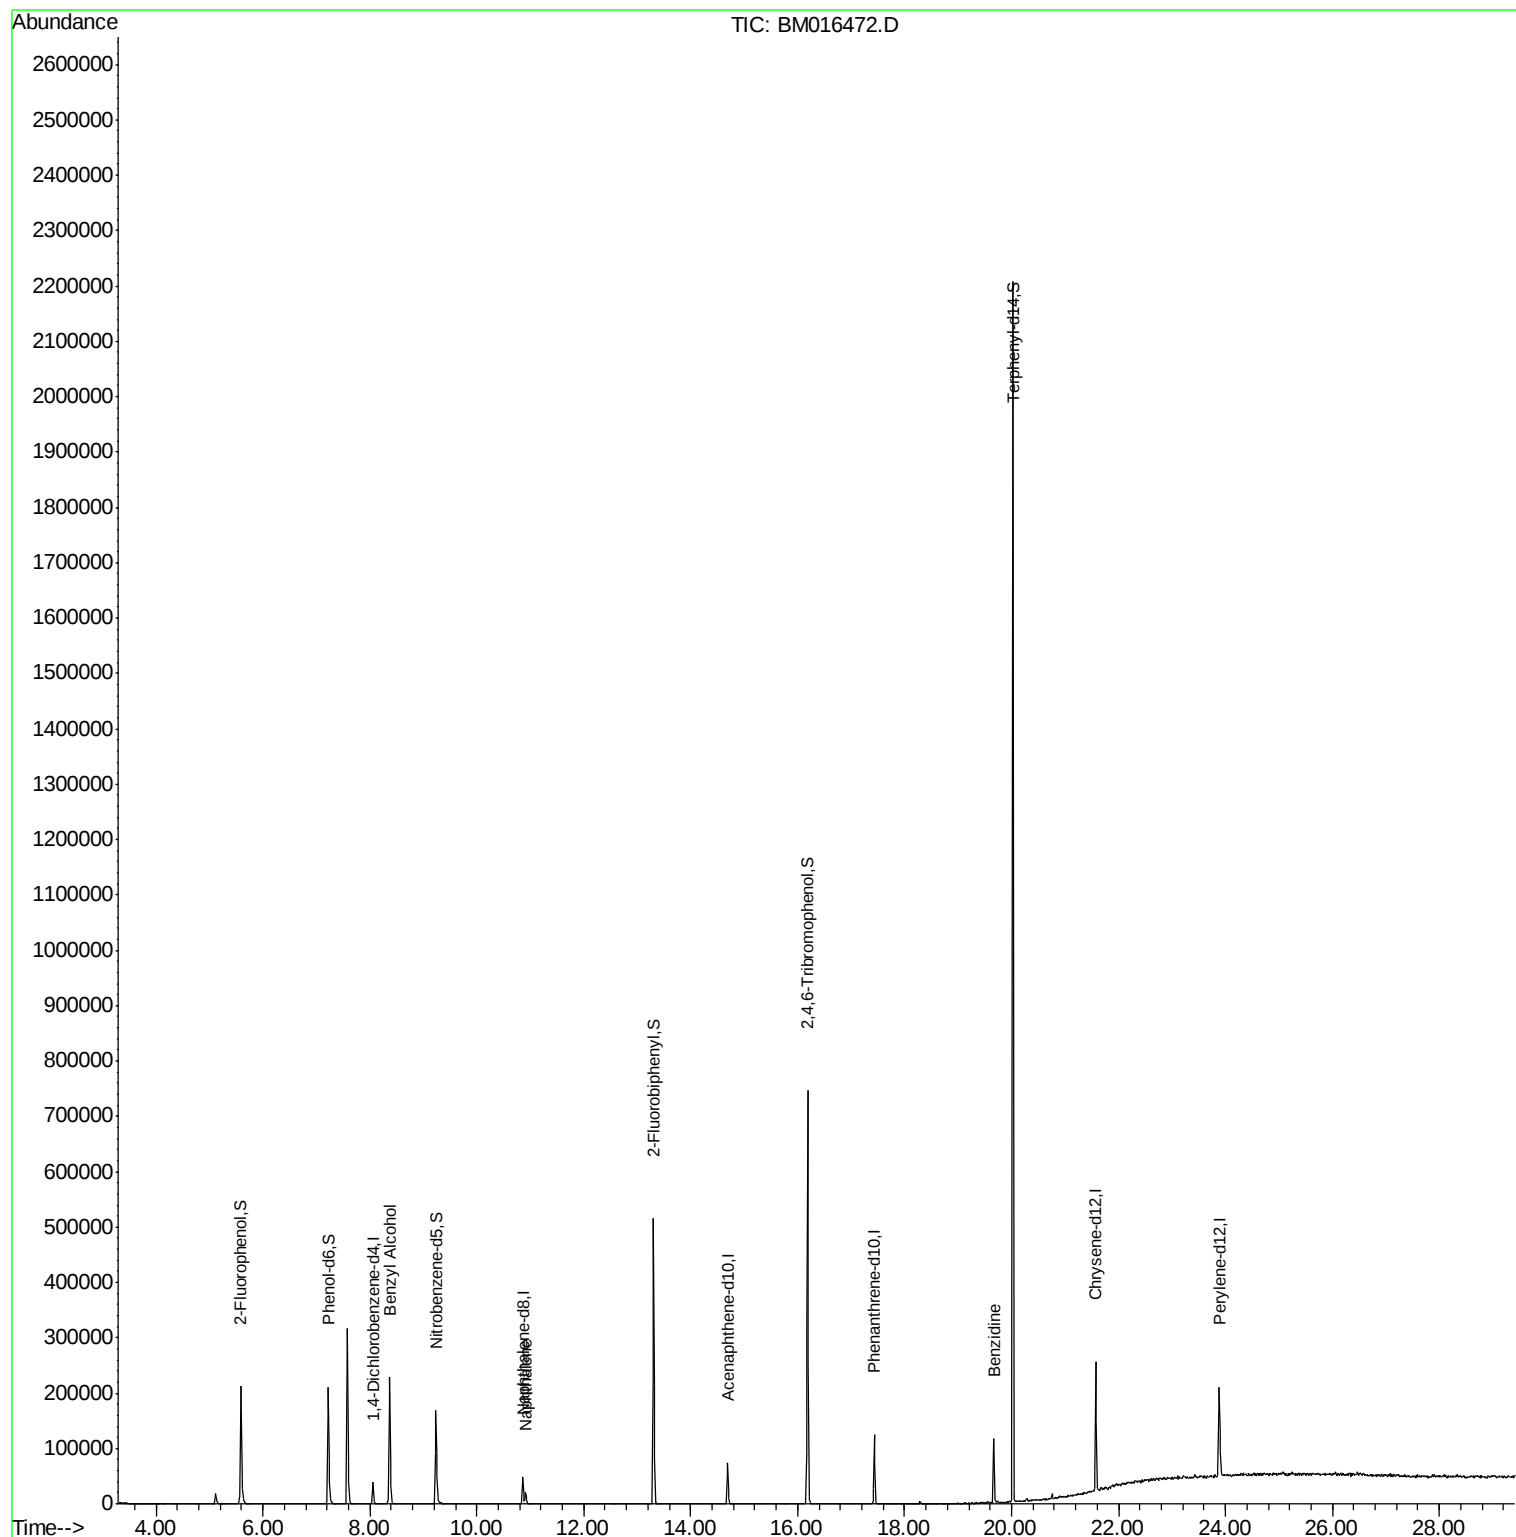

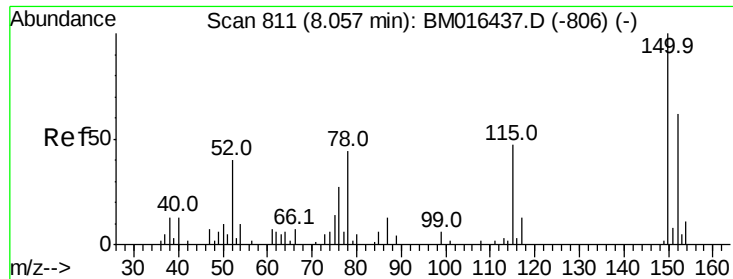


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 811
Delta R.T. -0.00 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Instrument :
BNA_M
ClientSampled :

Tot Ion:152 Resp: 7740
Ion Ratio Lower Upper
152 100
150 148.4 119.5 179.3
115 79.8 43.0 64.4#

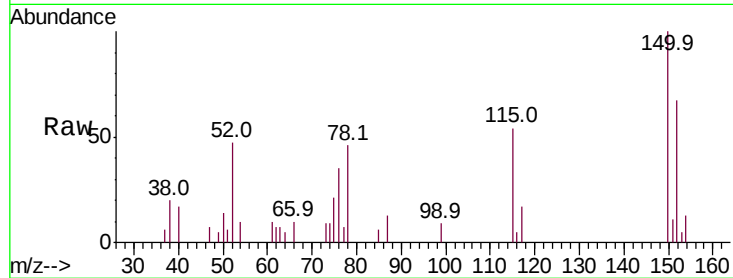


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

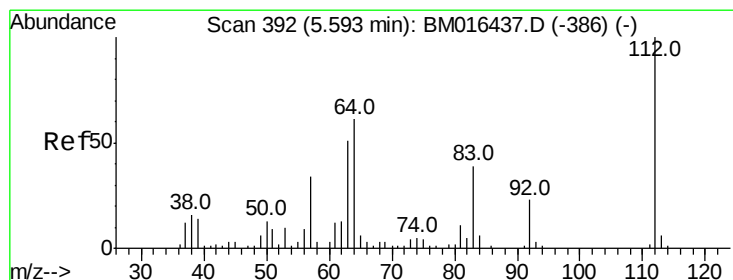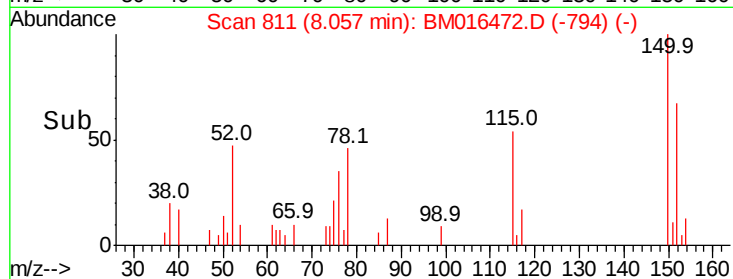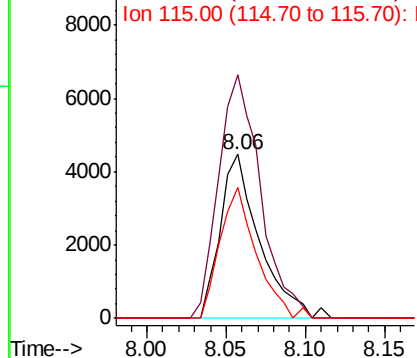



#5


2-Fluorophenol
Concen: N.D. ng
RT: 5.59 min Scan# 391
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Tgt Ion:112 Resp: 64296
Ion Ratio Lower Upper
112 100
64 63.1 38.6 57.8#
63 57.6 19.3 28.9#

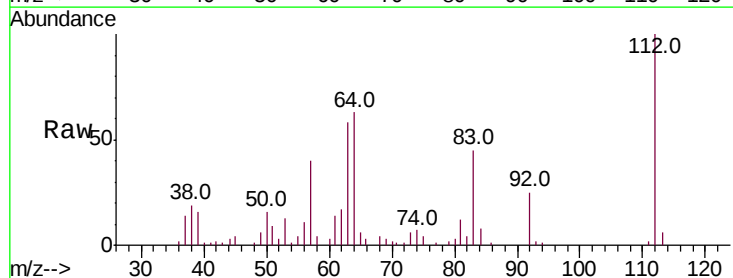

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

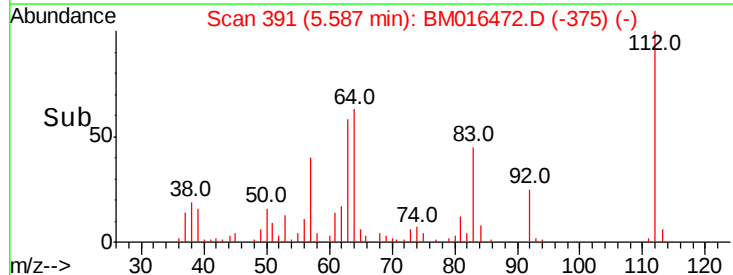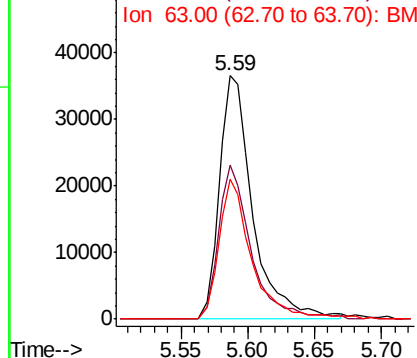

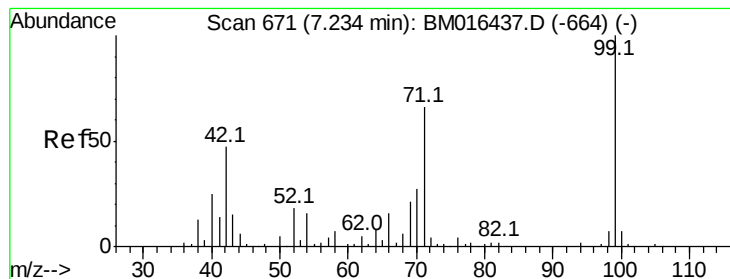

#7

Phenol-d6

Concen: N.D. ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BM016472.D

Acq: 18 Aug 2018 14:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 69655

Ion Ratio Lower Upper

99 100

42 53.2 11.0 16.4#




71 67.0 23.4 35.2#

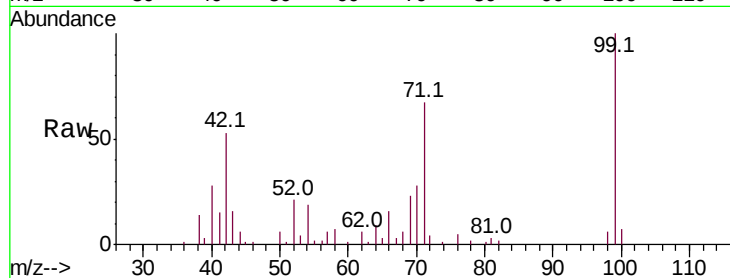

Abundance Ion 99.00 (98.70 to 99.70): BM016472.D (-654) (-)

Ion 42.00 (41.70 to 42.70): BM016472.D (-654) (-)

Ion 71.00 (70.70 to 71.70): BM016472.D (-654) (-)

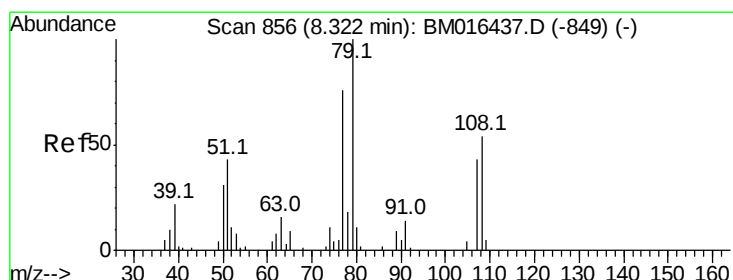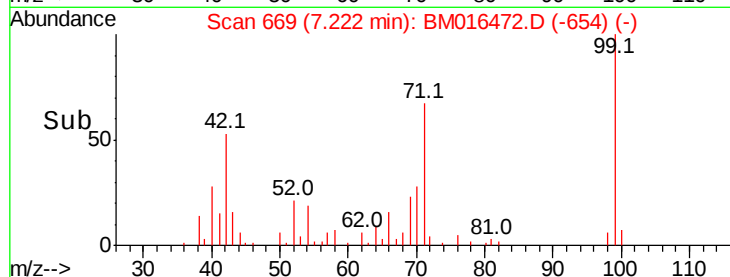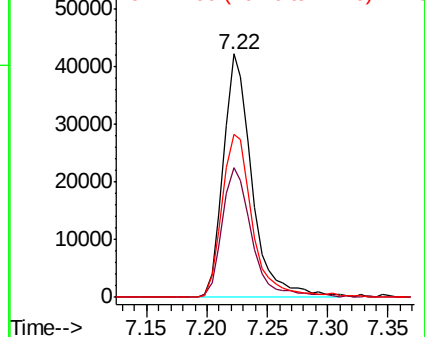

#15

Benzyl Alcohol

Concen: 2.776 ng

RT: 8.37 min Scan# 864

Delta R.T. 0.05 min

Lab File: BM016472.D

Acq: 18 Aug 2018 14:05


Tgt Ion: 79 Resp: 1560

Ion Ratio Lower Upper

79 100

108 77.4 65.0 97.4



77 199.6 53.0 79.6#

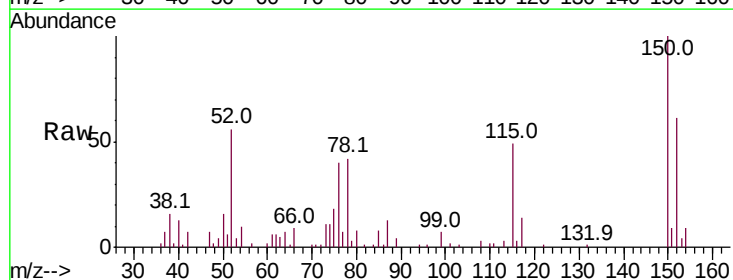


Abundance Ion 79.00 (78.70 to 79.70): BM016472.D (-839) (-)

Ion 108.00 (107.70 to 108.70): BM016472.D (-839) (-)

Ion 77.00 (76.70 to 77.70): BM016472.D (-839) (-)



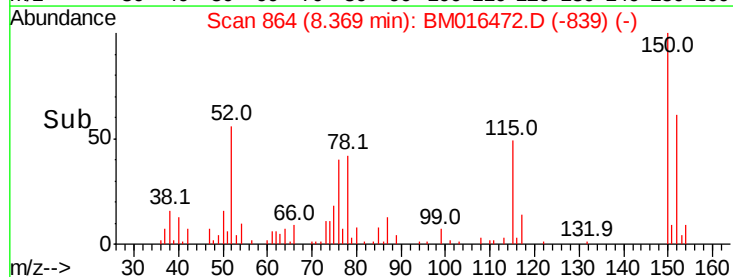
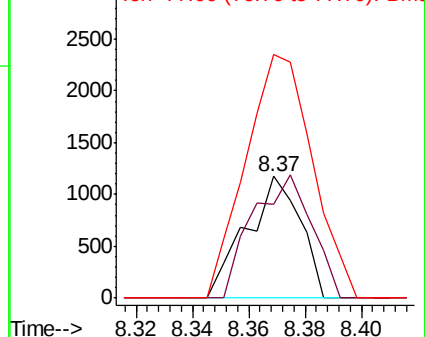


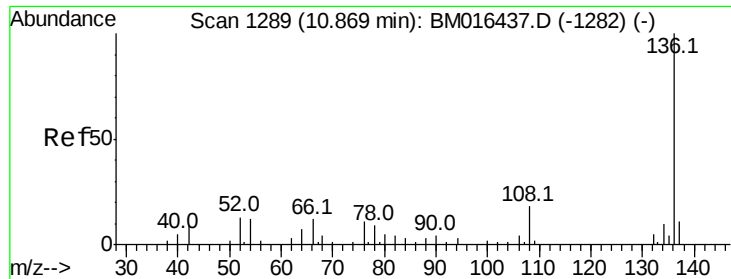

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1288
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05




Instrument :
BNA_M
ClientSampled :


Tot Ion:	136	Resp:	29333
Ion	Ratio	Lower	Upper
136	100		
137	9.9	8.7	13.1
54	11.6	4.6	6.8#
68	3.0	3.7	5.5#

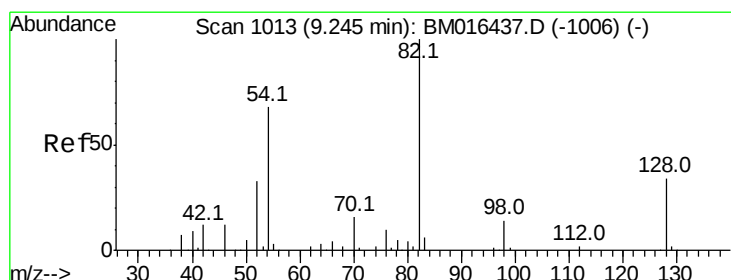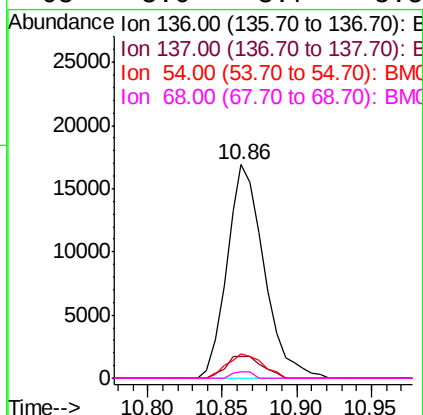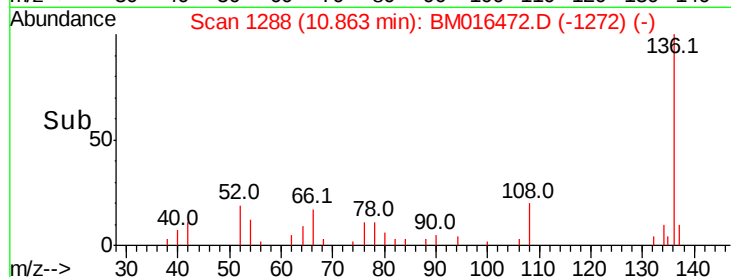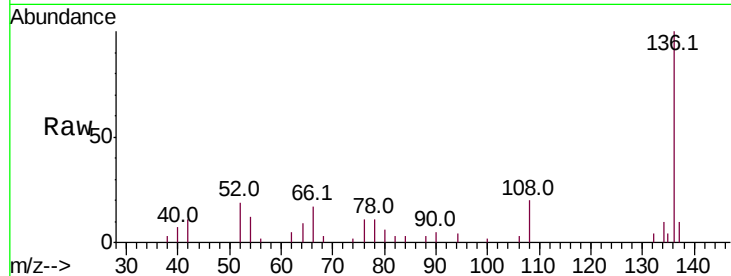

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.24 min Scan# 1012
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Tgt Ion:	82	Resp:	78157
Ion	Ratio	Lower	Upper
82	100		
128	31.8	32.8	49.2#
54	72.3	40.6	60.8#

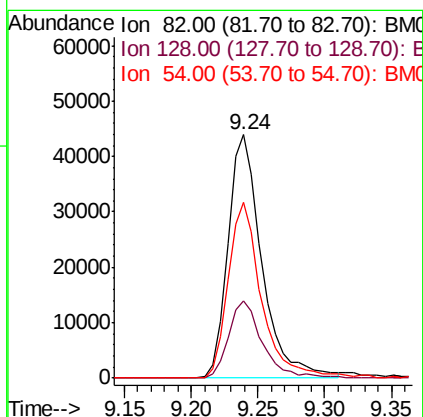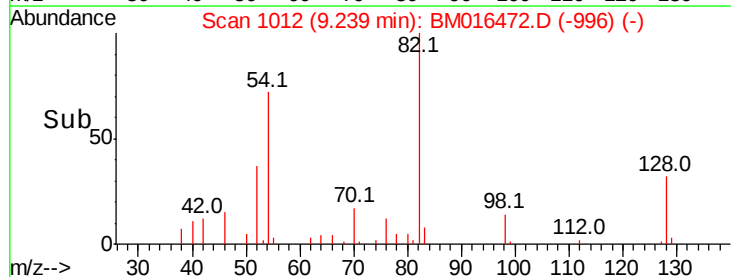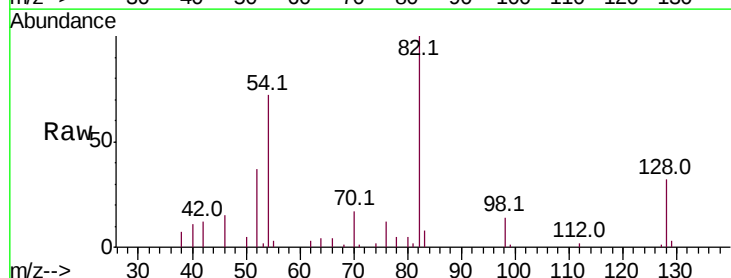


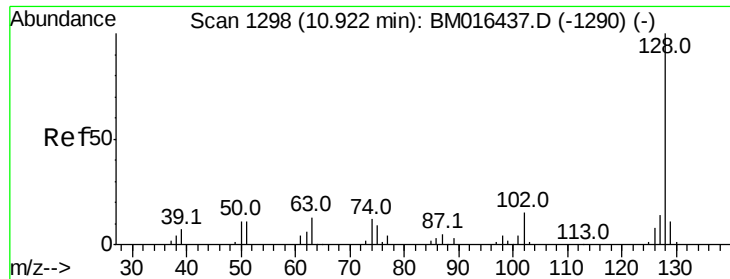




#31
Naphthalene
Concen: 9.658 ng
RT: 10.92 min Scan# 1298
Delta R.T. -0.00 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Instrument :
BNA_M
ClientSampleId :

Tot Ion:128 Resp: 14368
Ion Ratio Lower Upper
128 100
129 9.7 8.9 13.3
127 13.7 10.4 15.6

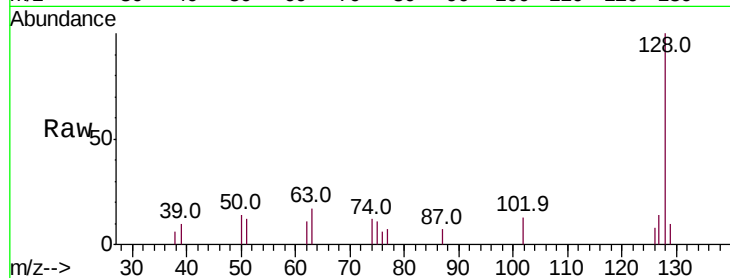


Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

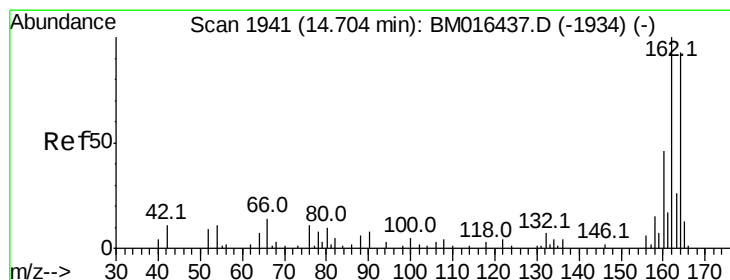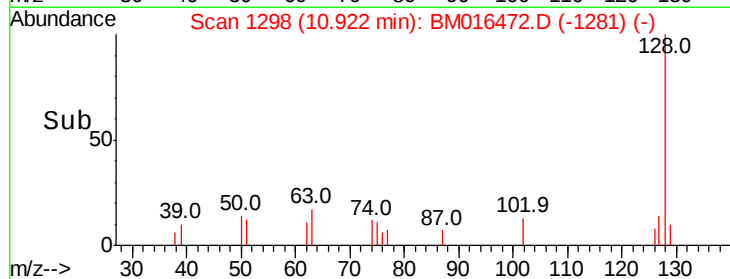
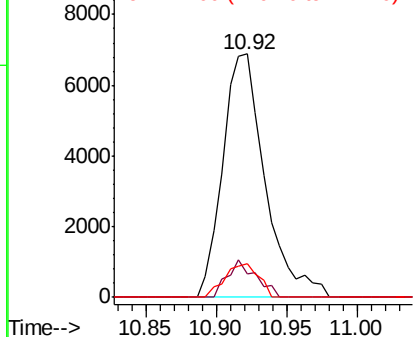



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.69 min Scan# 1939
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Tgt Ion:164 Resp: 19460
Ion Ratio Lower Upper
164 100
162 107.5 82.4 123.6
160 49.8 35.8 53.6

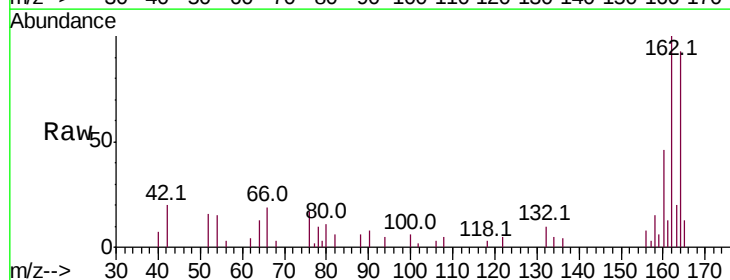

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



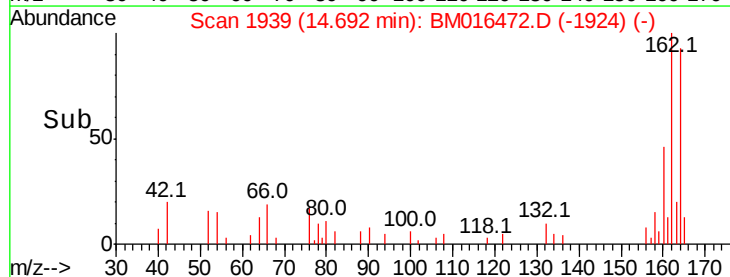
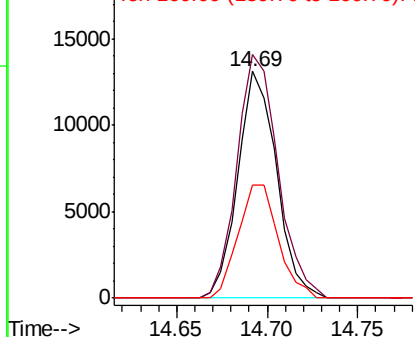


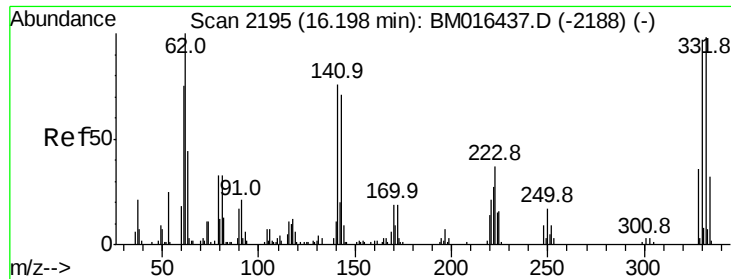

#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.19 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BM016472.D
 Acq: 18 Aug 2018 14:05




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:330 Resp: 62124
 Ion Ratio Lower Upper
 330 100
 332 95.4 0.0 0.0#
 141 87.8 0.0 0.0#

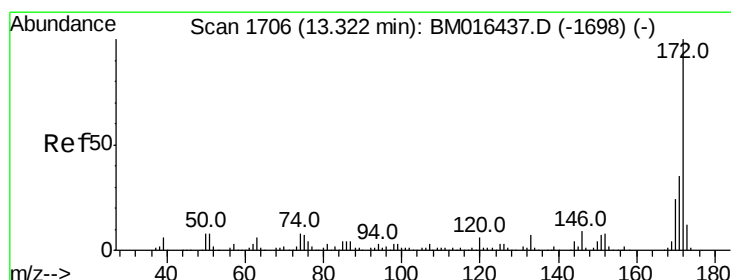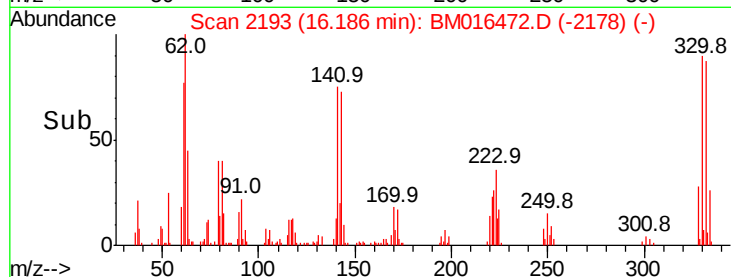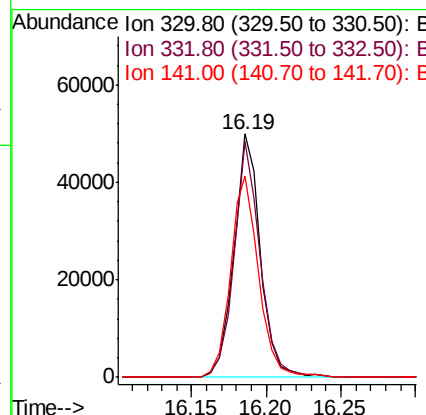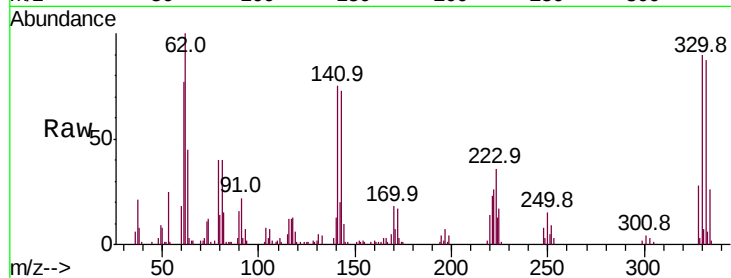

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.31 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BM016472.D
 Acq: 18 Aug 2018 14:05

Tgt Ion:172 Resp: 173657
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.5 42.7
 170 25.1 18.8 28.2

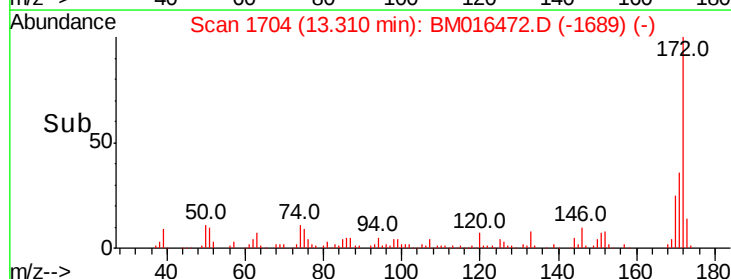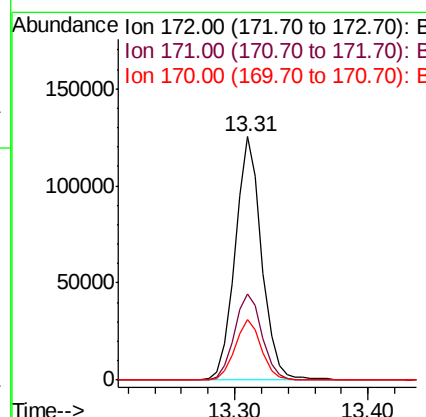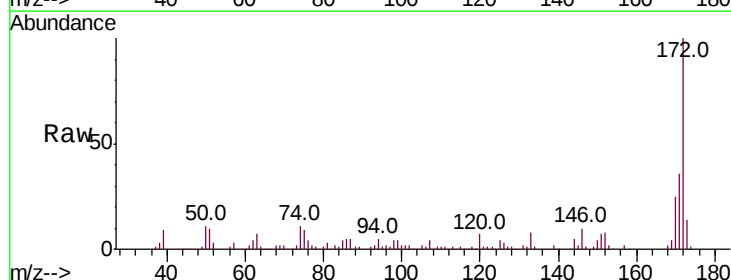


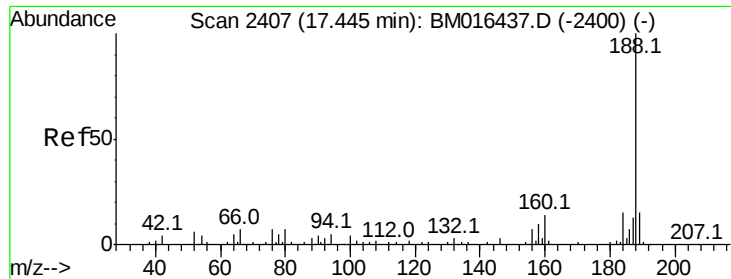




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.43 min Scan# 2405
 Delta R.T. -0.01 min
 Lab File: BM016472.D
 Acq: 18 Aug 2018 14:05

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:188 Resp: 56102
 Ion Ratio Lower Upper
 188 100
 94 5.1 8.7 13.1#
 80 5.5 9.3 13.9#

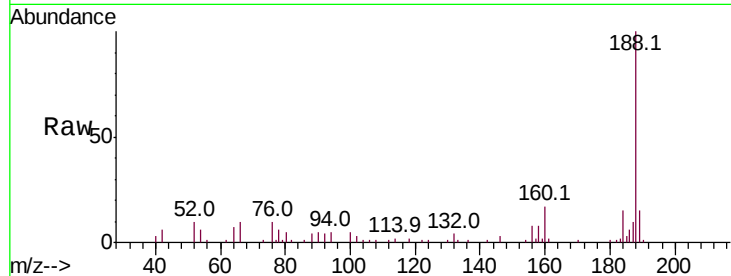


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BM
 Ion 80.00 (79.70 to 80.70): BM

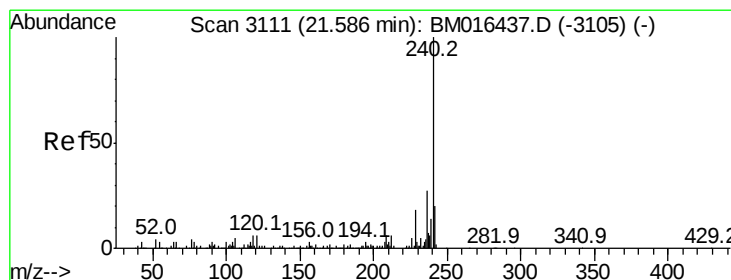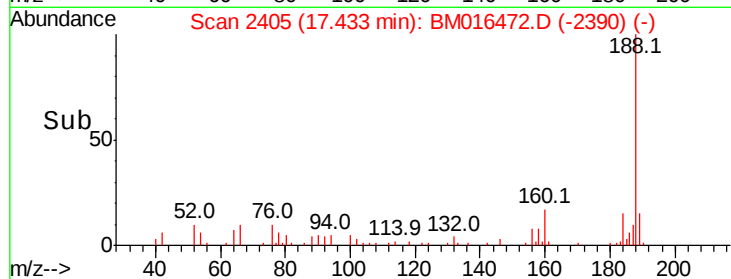
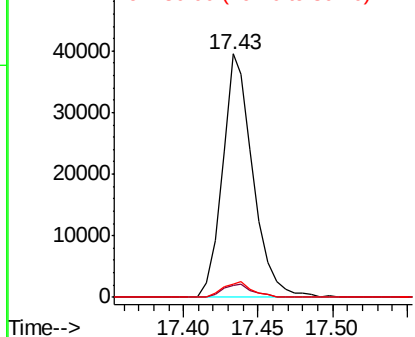



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.57 min Scan# 3109
 Delta R.T. -0.01 min
 Lab File: BM016472.D
 Acq: 18 Aug 2018 14:05

Tgt Ion:240 Resp: 90118
 Ion Ratio Lower Upper
 240 100
 120 4.2 8.2 12.2#
 236 26.7 20.0 30.0

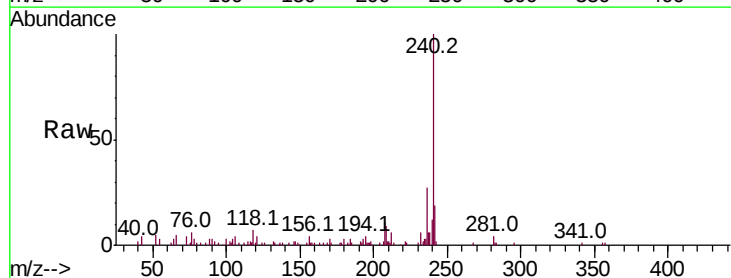

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



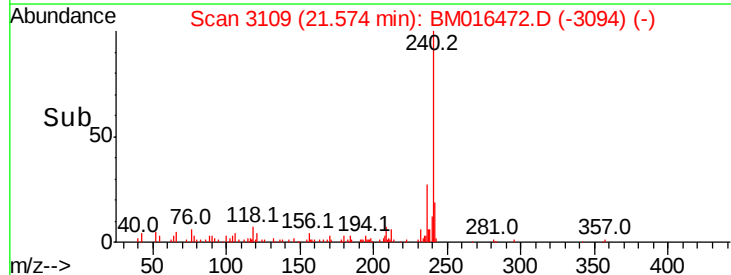
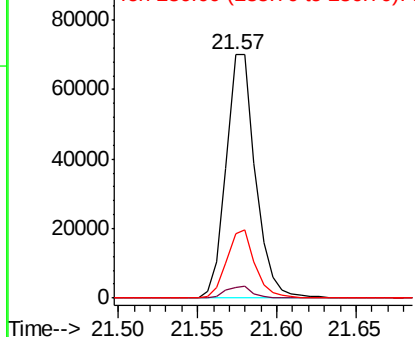


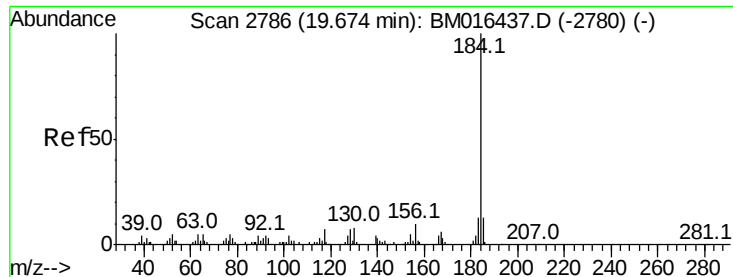

#76
Benzidine
Concen: 25.695 ng
RT: 19.67 min Scan# 2785
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05




Instrument :
BNA_M
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
184	100		
185	14.1	11.3	16.9
183	12.4	8.9	13.3

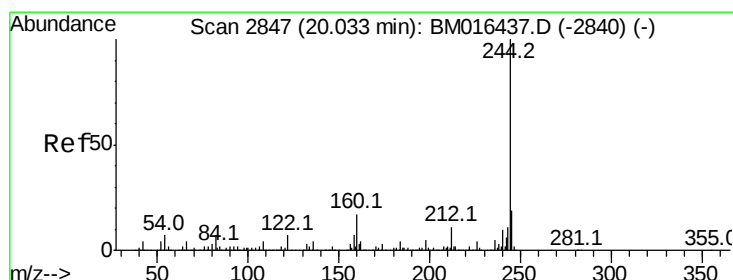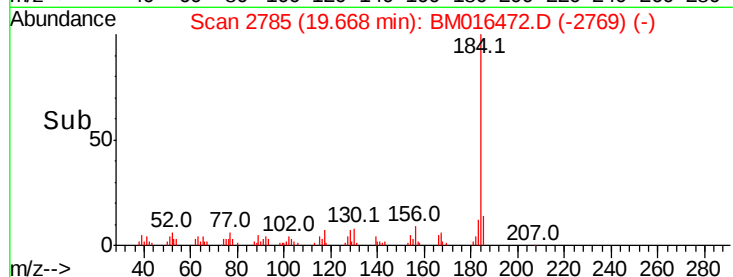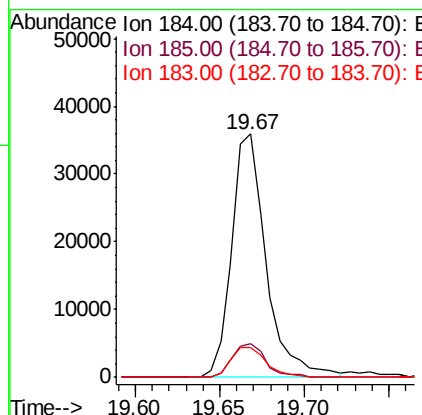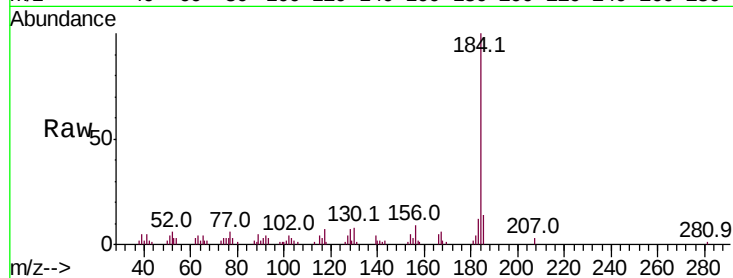

#78
Terphenyl-d14
Concen: N.D. ng
RT: 20.03 min Scan# 2846
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Tgt Ion	Ratio	Lower	Upper
244	100		
212	10.5	4.9	7.3#
122	6.2	6.2	9.4

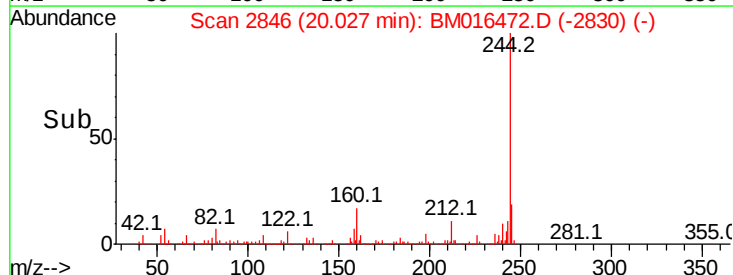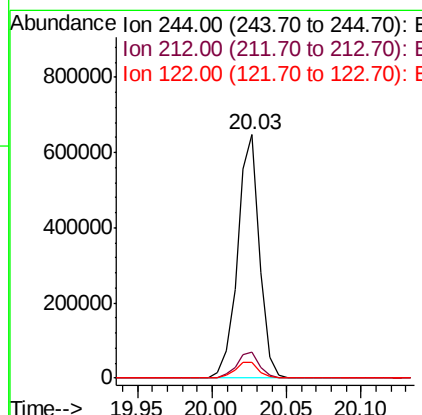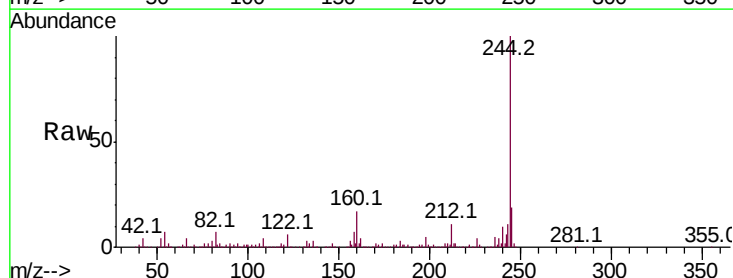

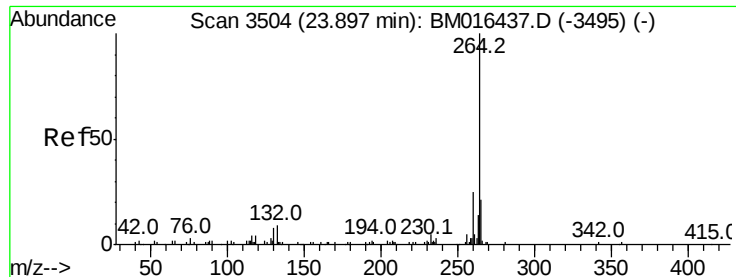

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.89 min Scan# 3502
Delta R.T. -0.01 min
Lab File: BM016472.D
Acq: 18 Aug 2018 14:05

Instrument :
BNA_M
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	18.6	27.8
265	21.4	17.3	25.9

