

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
 Data File : BM016474.D
 Acq On : 18 Aug 2018 15:18
 Operator : SJ/JU
 Sample : J4521-27
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 20 01:17:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 16:27:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	9598	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	36035	20.00	ng	0.00
38) Acenaphthene-d10	14.69	164	22379	20.00	ng	-0.01
63) Phenanthrene-d10	17.43	188	59066	20.00	ng	-0.01
75) Chrysene-d12	21.58	240	85543	20.00	ng	0.00
86) Perylene-d12	23.88	264	99816	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	79648	139.46	ng	0.00
7) Phenol-d6	7.22	99	90269	117.59	ng	-0.01
23) Nitrobenzene-d5	9.24	82	95495	110.37	ng	0.00
41) 2,4,6-Tribromophenol	16.19	330	63022	186.45	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	228545	106.19	ng	-0.01
78) Terphenyl-d14	20.03	244	673006	118.91	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.37	79	1836	2.635	ng	# 1
76) Benzidine	19.67	184	15755	8.368	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
Data File : BM016474.D
Acq On : 18 Aug 2018 15:18
Operator : SJ/JU
Sample : J4521-27
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 20 01:17:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 16:27:00 2018
Response via : Initial Calibration

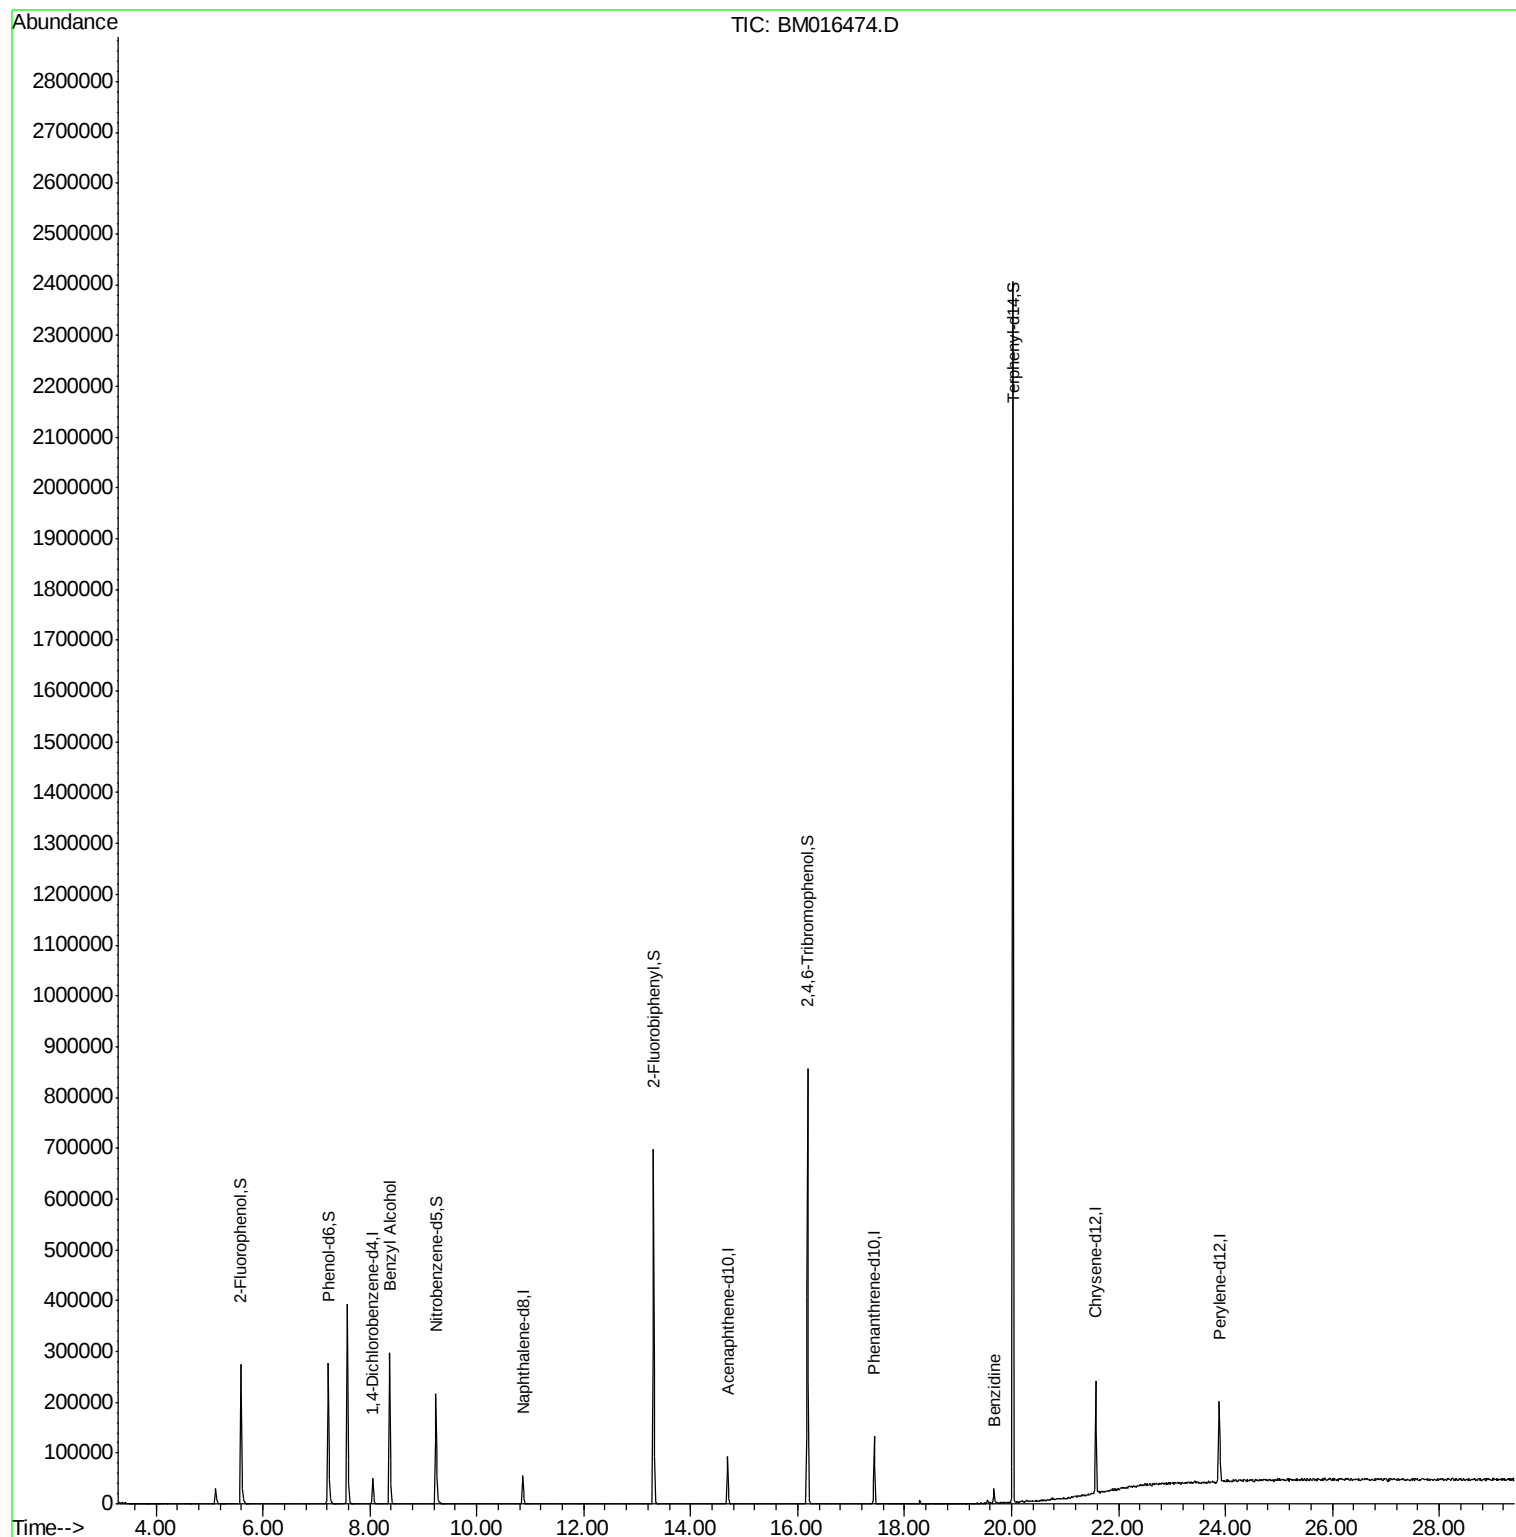

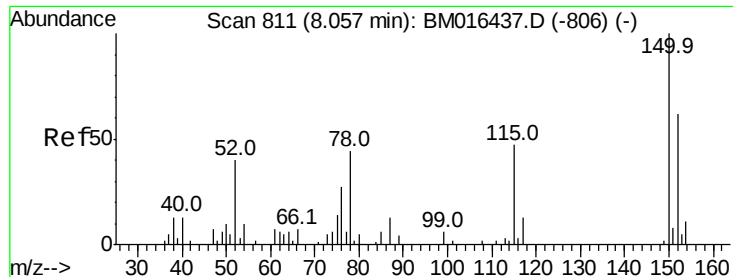


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 810
Delta R.T. -0.01 min
Lab File: BM016474.D
Acq: 18 Aug 2018 15:18

Instrument :
BNA_M
ClientSampleId :

Tot Ion:152 Resp: 9598
Ion Ratio Lower Upper
152 100
150 177.2 119.5 179.3
115 75.8 43.0 64.4#

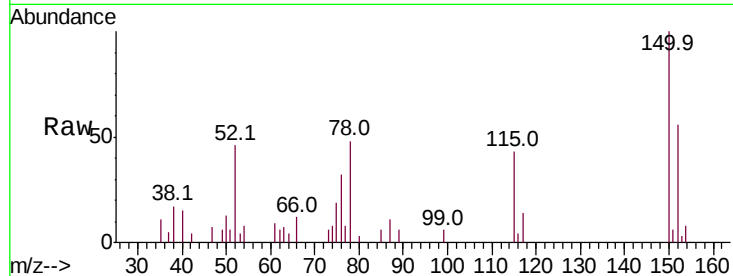


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

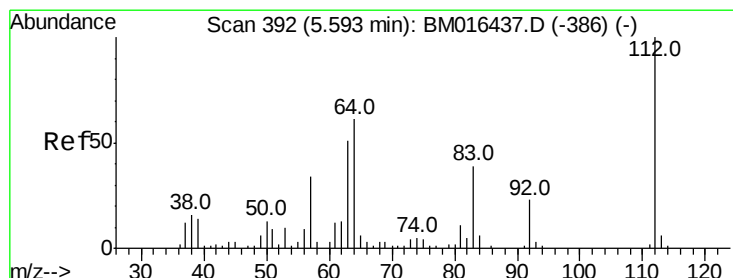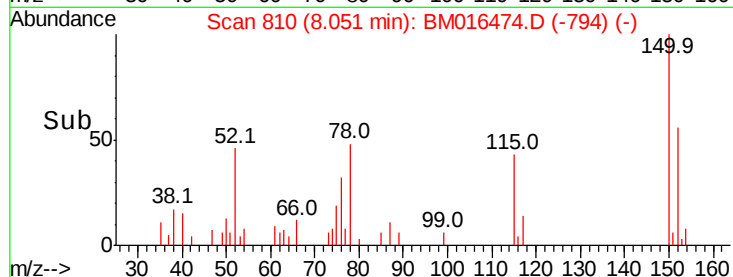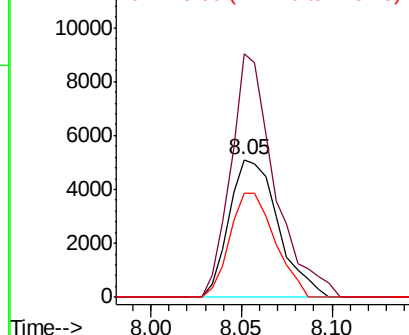



#5


2-Fluorophenol
Concen: N.D. ng
RT: 5.59 min Scan# 391
Delta R.T. -0.01 min
Lab File: BM016474.D
Acq: 18 Aug 2018 15:18

Tgt Ion:112 Resp: 79648
Ion Ratio Lower Upper
112 100
64 64.7 38.6 57.8#
63 56.8 19.3 28.9#

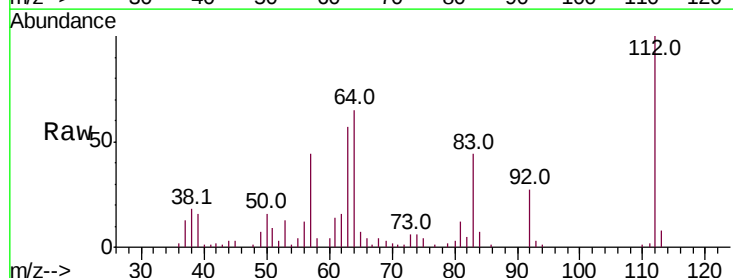

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

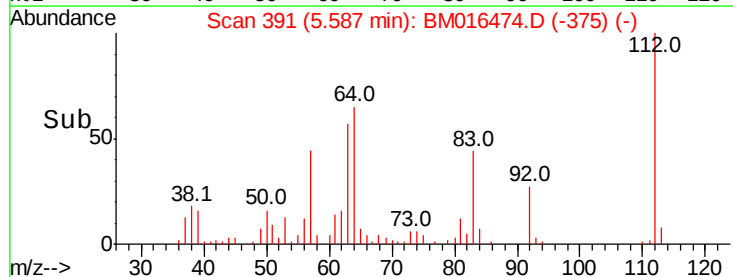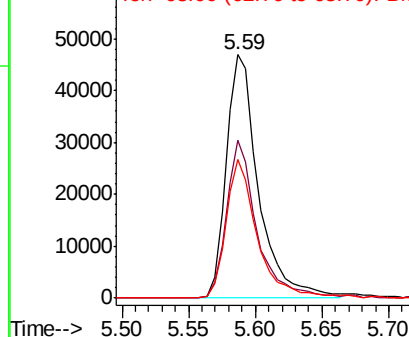

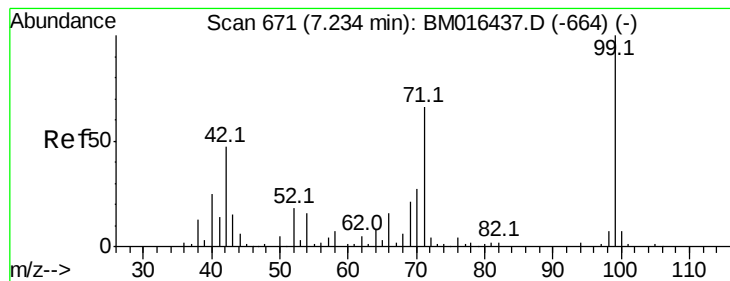

#7

Phenol-d6

Concen: N.D. ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 99 Resp: 90269

Ion Ratio Lower Upper

99 100

42 52.3 11.0 16.4#




71 72.5 23.4 35.2#

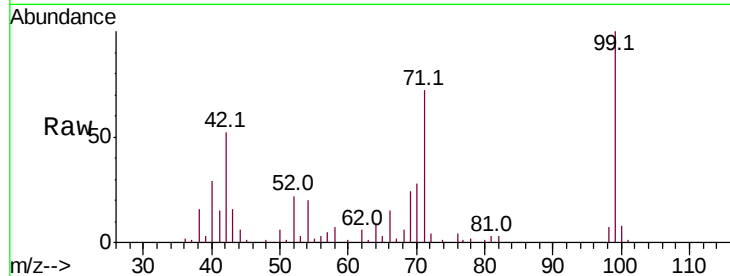

Abundance Ion 99.00 (98.70 to 99.70): BM016437.D (-664) (-)

Ion 42.00 (41.70 to 42.70): BM016437.D (-664) (-)

Ion 71.00 (70.70 to 71.70): BM016437.D (-664) (-)

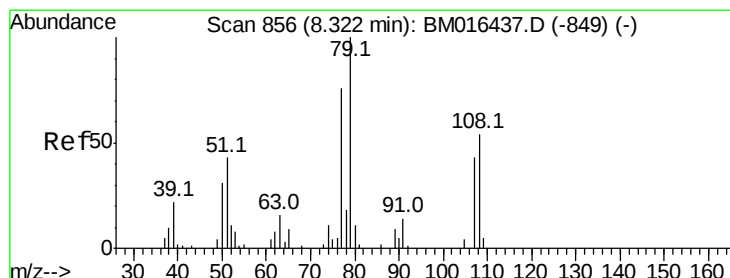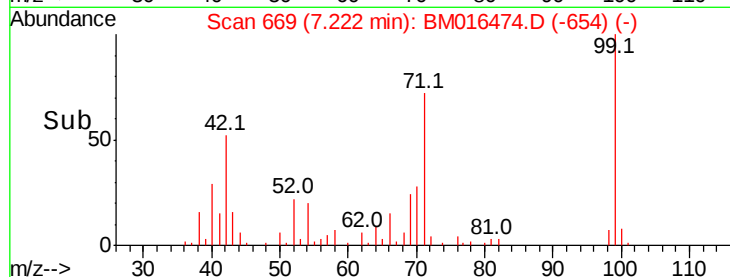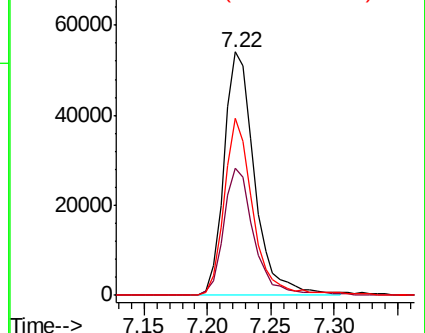

#15

Benzyl Alcohol

Concen: 2.635 ng

RT: 8.37 min Scan# 864

Delta R.T. 0.05 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18


Tgt Ion: 79 Resp: 1836

Ion Ratio Lower Upper

79 100

108 120.0 65.0 97.4#



77 269.1 53.0 79.6#

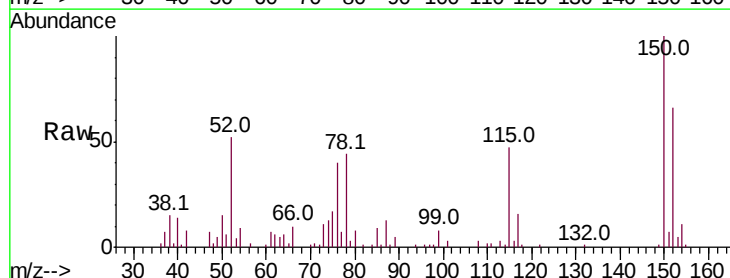


Abundance Ion 79.00 (78.70 to 79.70): BM016437.D (-849) (-)

Ion 108.00 (107.70 to 108.70): BM016437.D (-849) (-)

Ion 77.00 (76.70 to 77.70): BM016437.D (-849) (-)



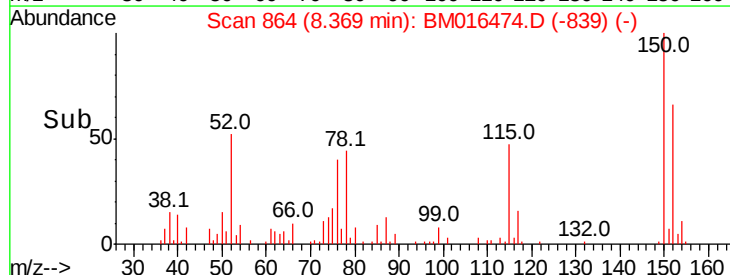
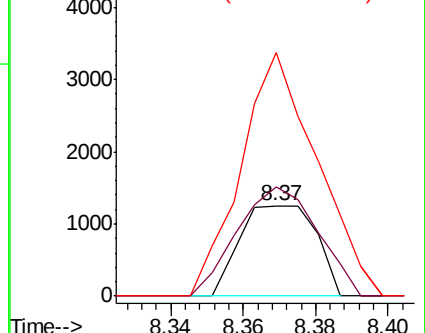


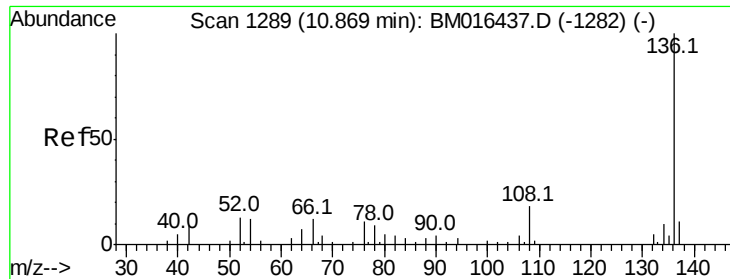

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1288
Delta R.T. -0.01 min
Lab File: BM016474.D
Acq: 18 Aug 2018 15:18




Instrument :
BNA_M
ClientSampleId :


Tot Ion:	136	Resp:	36035
Ion	Ratio	Lower	Upper
136	100		
137	8.9	8.7	13.1
54	11.5	4.6	6.8#
68	1.7	3.7	5.5#

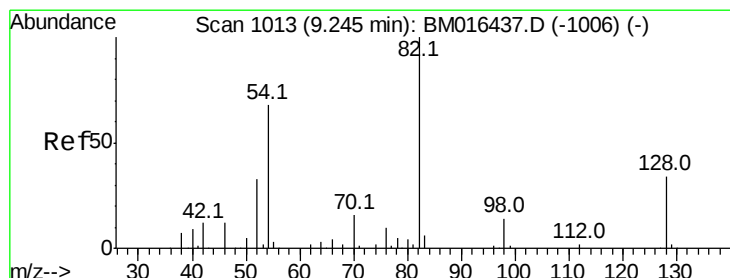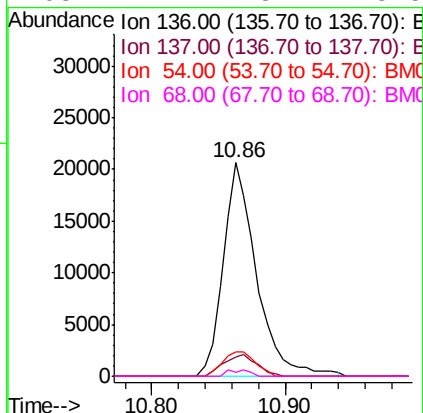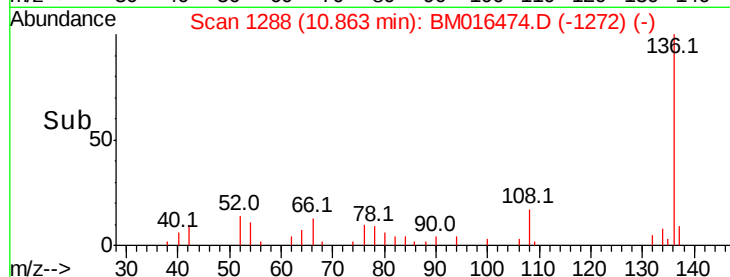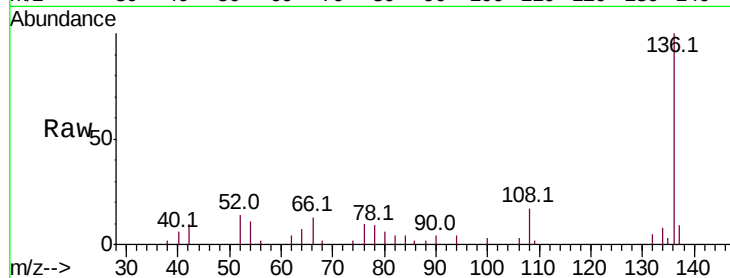

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.24 min Scan# 1012
Delta R.T. -0.01 min
Lab File: BM016474.D
Acq: 18 Aug 2018 15:18

Tgt Ion:	82	Resp:	95495
Ion	Ratio	Lower	Upper
82	100		
128	34.2	32.8	49.2
54	73.9	40.6	60.8#

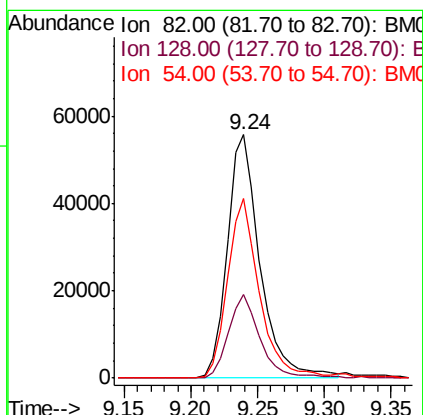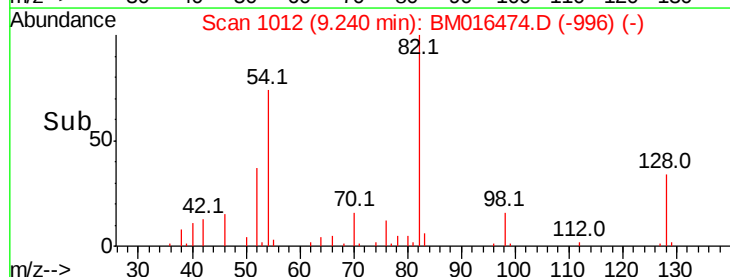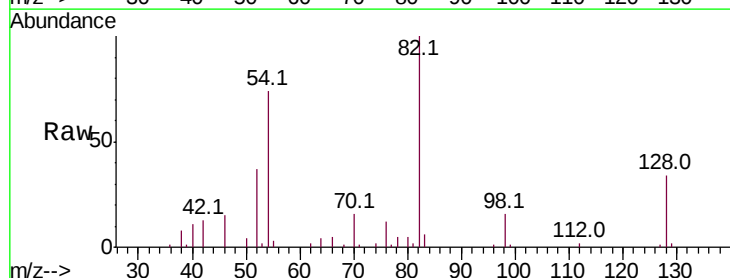

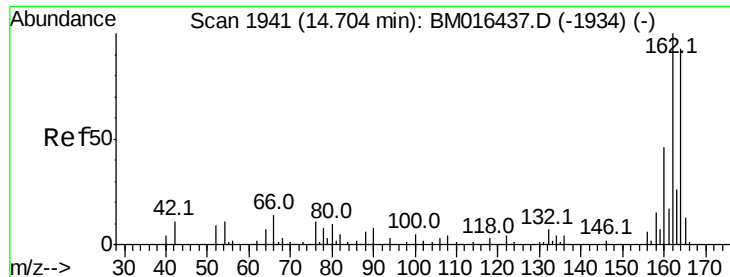

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.69 min Scan# 1939

Delta R.T. -0.01 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18

Instrument :

BNA_M

ClientSampleId :


Tot Ion:164 Resp: 22379

Ion Ratio Lower Upper

164 100

162 117.2 82.4 123.6




160 51.5 35.8 53.6

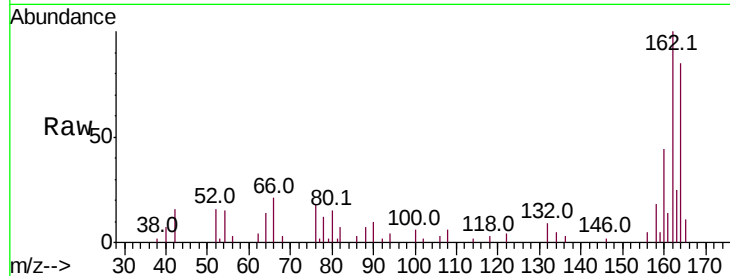

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

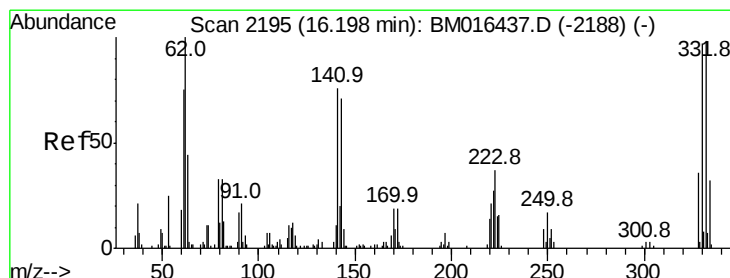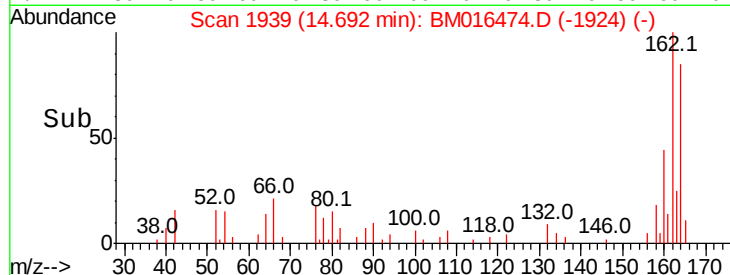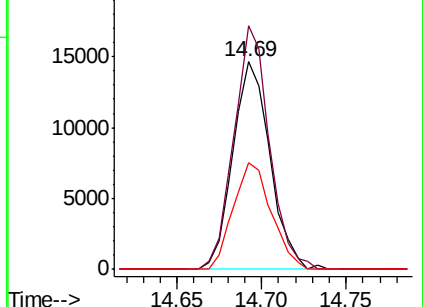

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.19 min Scan# 2193

Delta R.T. -0.01 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18


Tgt Ion:330 Resp: 63022

Ion Ratio Lower Upper

330 100

332 95.7 0.0 0.0#



141 100.5 0.0 0.0#

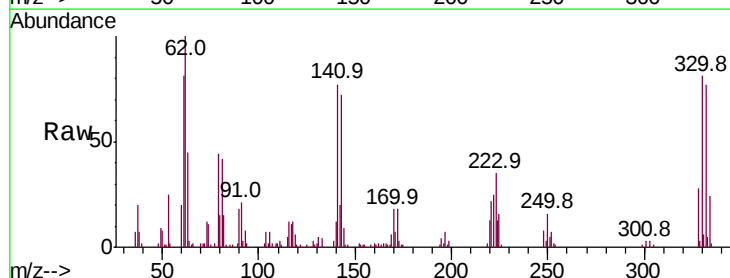


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



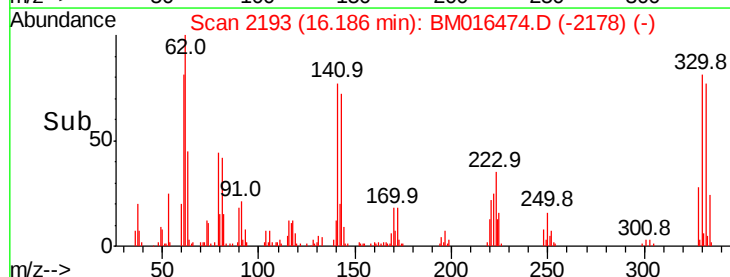
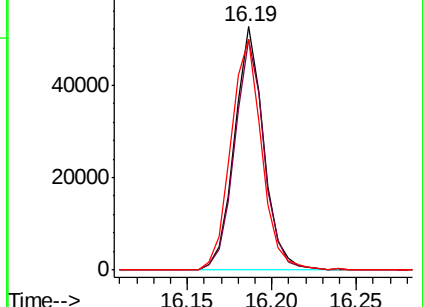


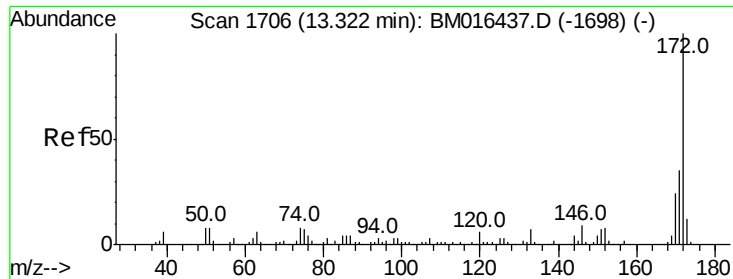

#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.31 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BM016474.D
 Acq: 18 Aug 2018 15:18




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:172 Resp: 228545
 Ion Ratio Lower Upper
 172 100
 171 36.3 28.5 42.7
 170 24.2 18.8 28.2

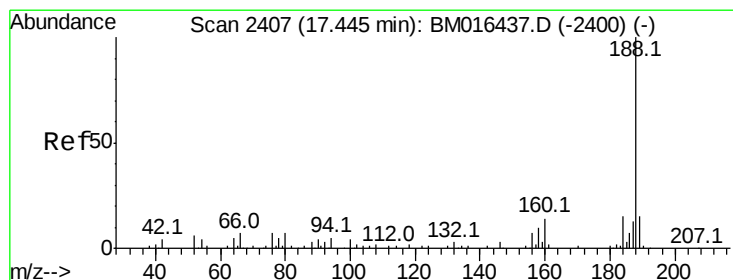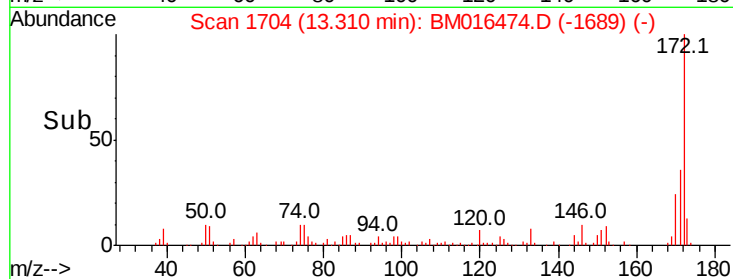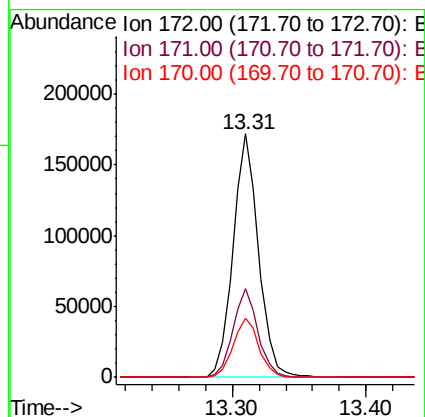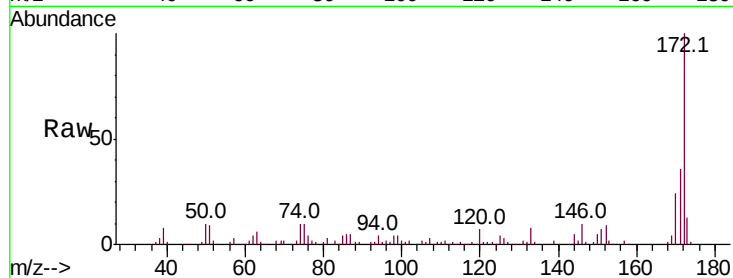

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.43 min Scan# 2405
 Delta R.T. -0.01 min
 Lab File: BM016474.D
 Acq: 18 Aug 2018 15:18

Tgt Ion:188 Resp: 59066
 Ion Ratio Lower Upper
 188 100
 94 6.7 8.7 13.1#
 80 8.0 9.3 13.9#

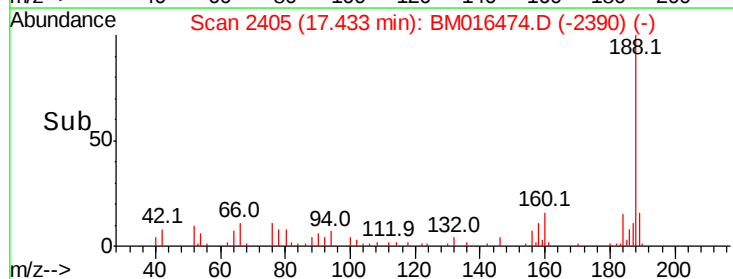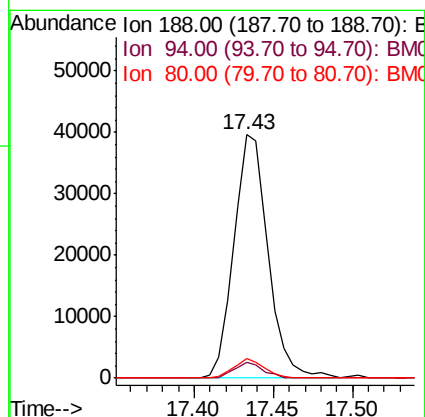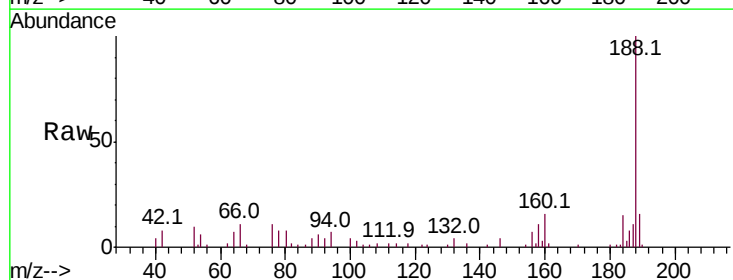

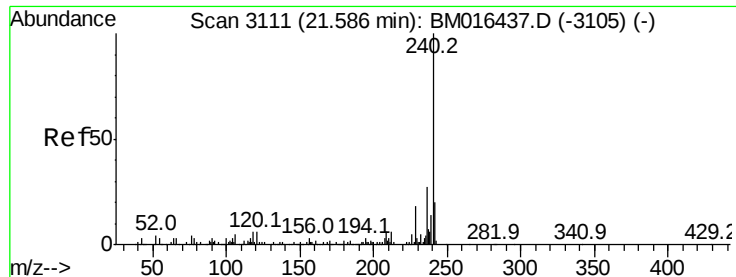

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.58 min Scan# 3110

Delta R.T. -0.01 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18

Instrument :

BNA_M

ClientSampleId :


Tot Ion:240 Resp: 85543

Ion Ratio Lower Upper

240 100

120 5.1 8.2 12.2#




236 26.6 20.0 30.0

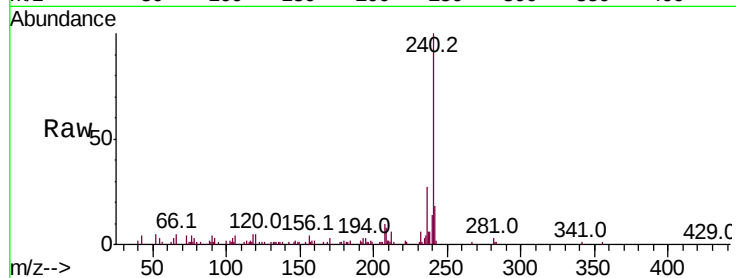

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

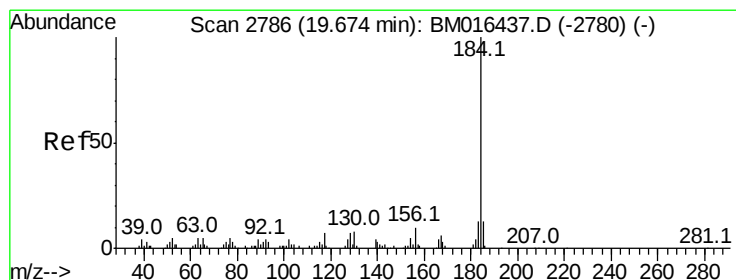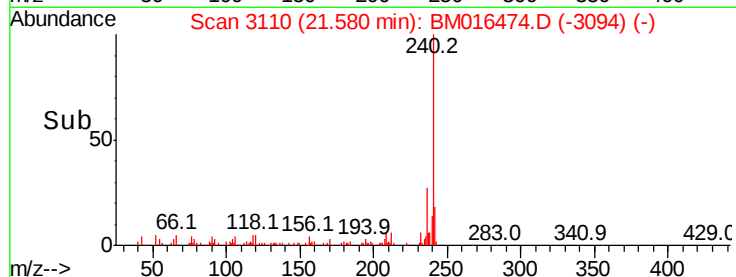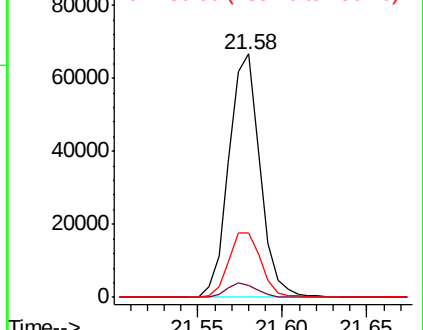

#76

Benzidine

Concen: 8.368 ng

RT: 19.67 min Scan# 2785

Delta R.T. -0.01 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18


Tgt Ion:184 Resp: 15755

Ion Ratio Lower Upper

184 100

185 11.1 11.3 16.9#



183 11.4 8.9 13.3

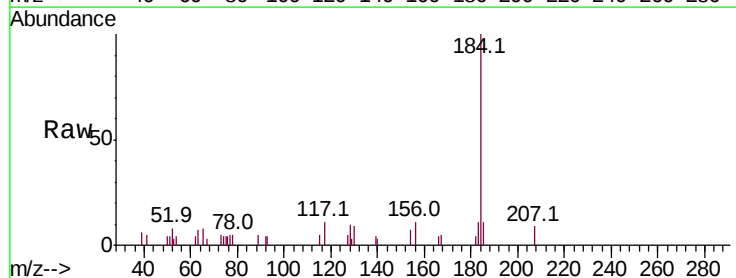


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

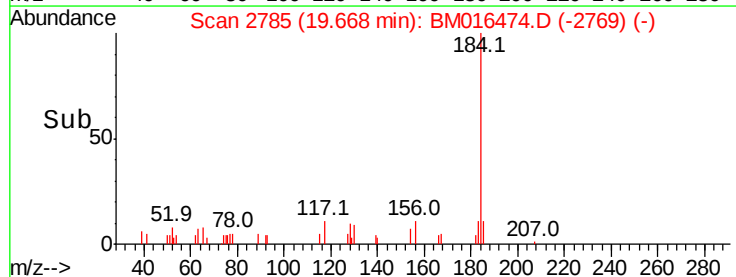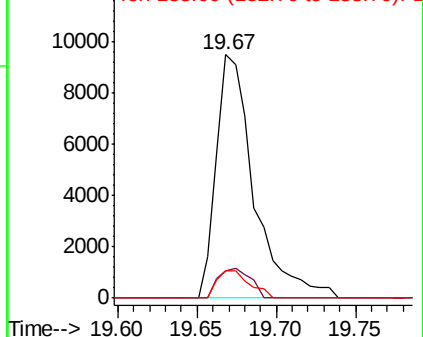

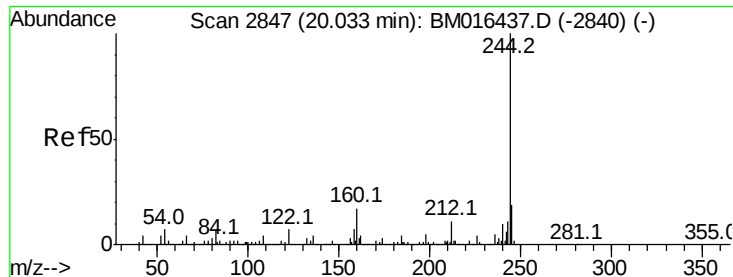

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.03 min Scan# 2846

Delta R.T. -0.00 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 673006

Ion Ratio Lower Upper

244 100

212 10.8 4.9 7.3#




122 6.9 6.2 9.4

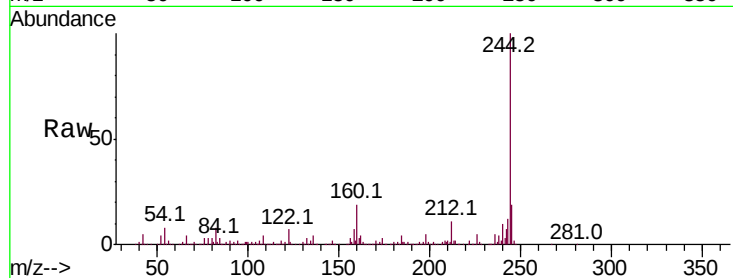

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

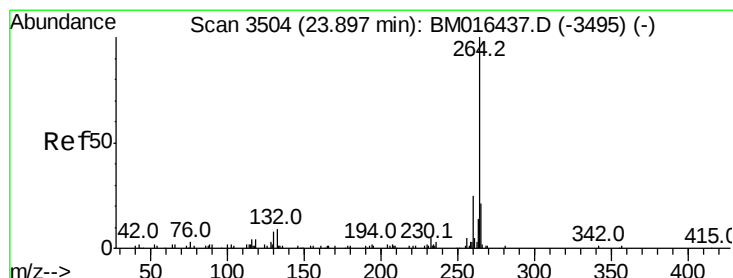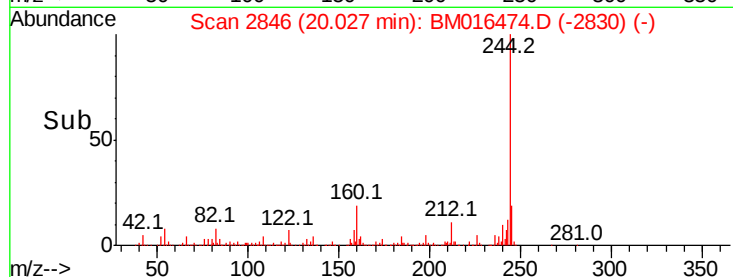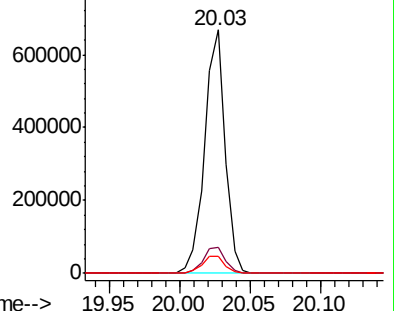

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.88 min Scan# 3501

Delta R.T. -0.02 min

Lab File: BM016474.D

Acq: 18 Aug 2018 15:18


Tgt Ion:264 Resp: 99816

Ion Ratio Lower Upper

264 100

260 24.5 18.6 27.8

265 20.7 17.3 25.9

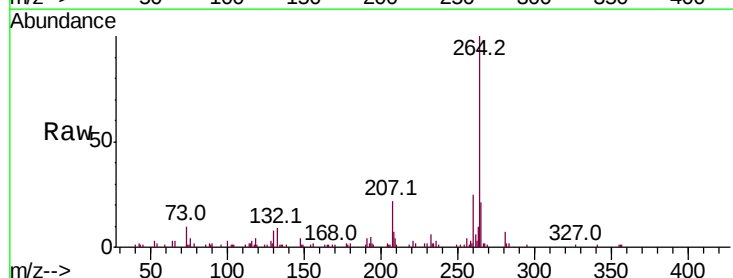

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

