
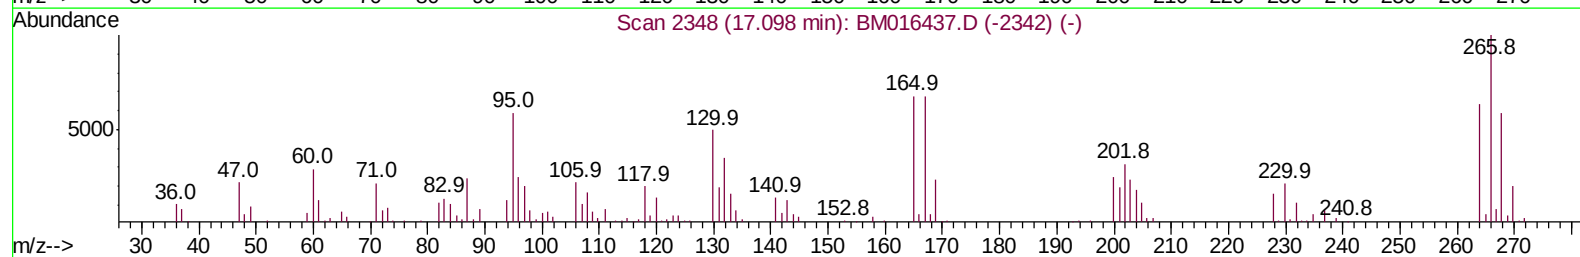
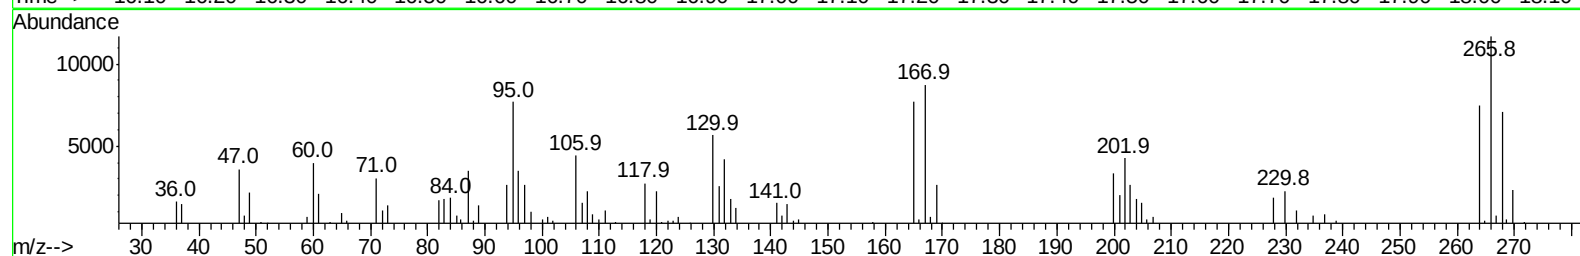


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\  
Data File : BM016433.D  
Acq On : 17 Aug 2018 11:22  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 02:58:12 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 17 16:27:00 2018  
Response via : Initial Calibration

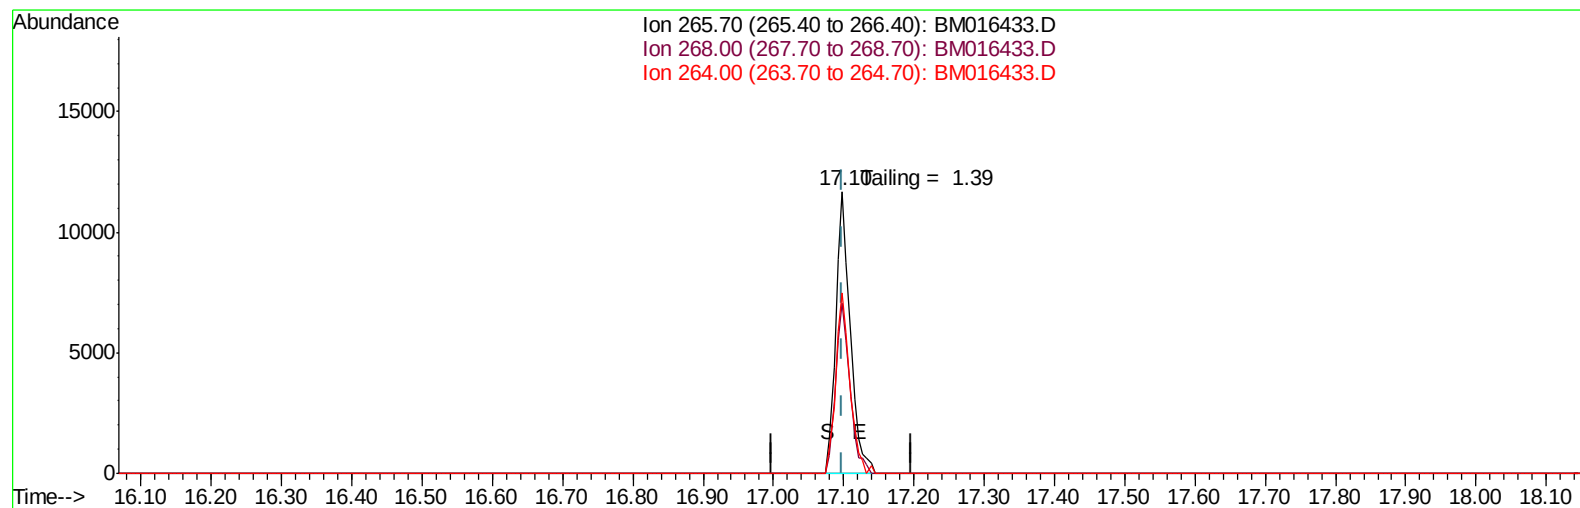

TIC: BM016433.D

(69) Pentachlorophenol (C)




17.098min (-0.000) 0.00ng

response 16622

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 64.82 |
| 264.00 | 61.20 | 64.22 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\  
Data File : BM016433.D  
Acq On : 17 Aug 2018 11:22  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 02:58:12 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 17 16:27:00 2018  
Response via : Initial Calibration

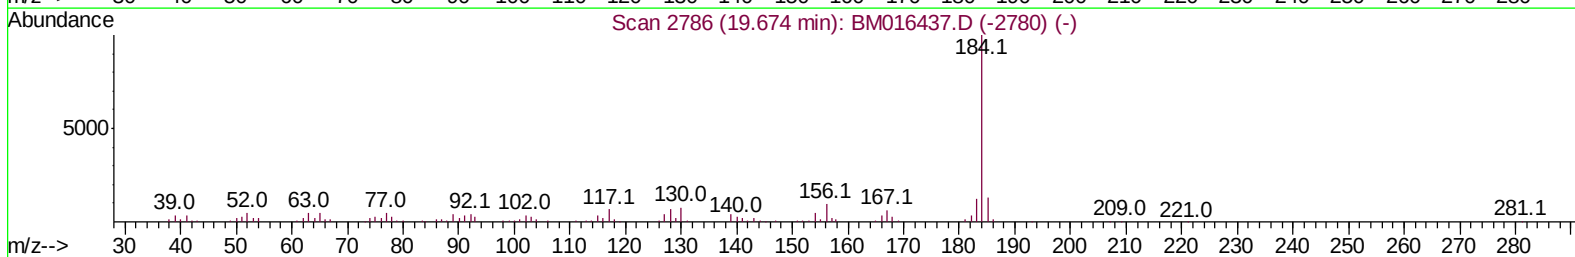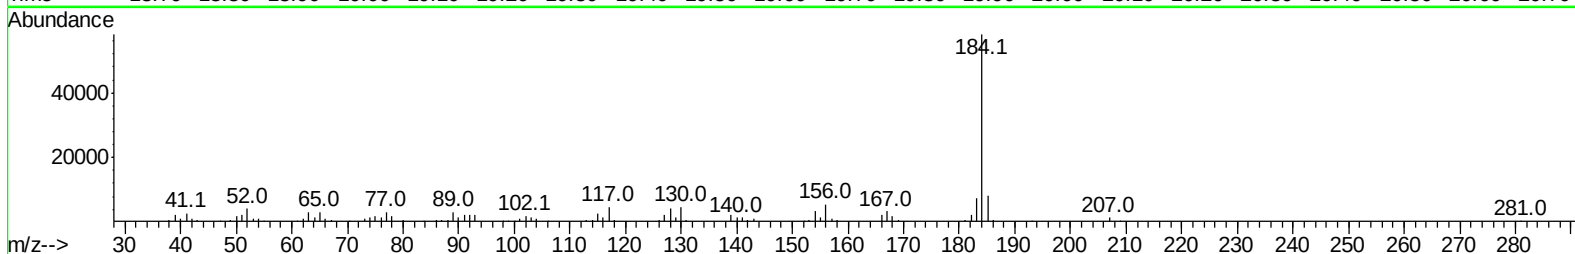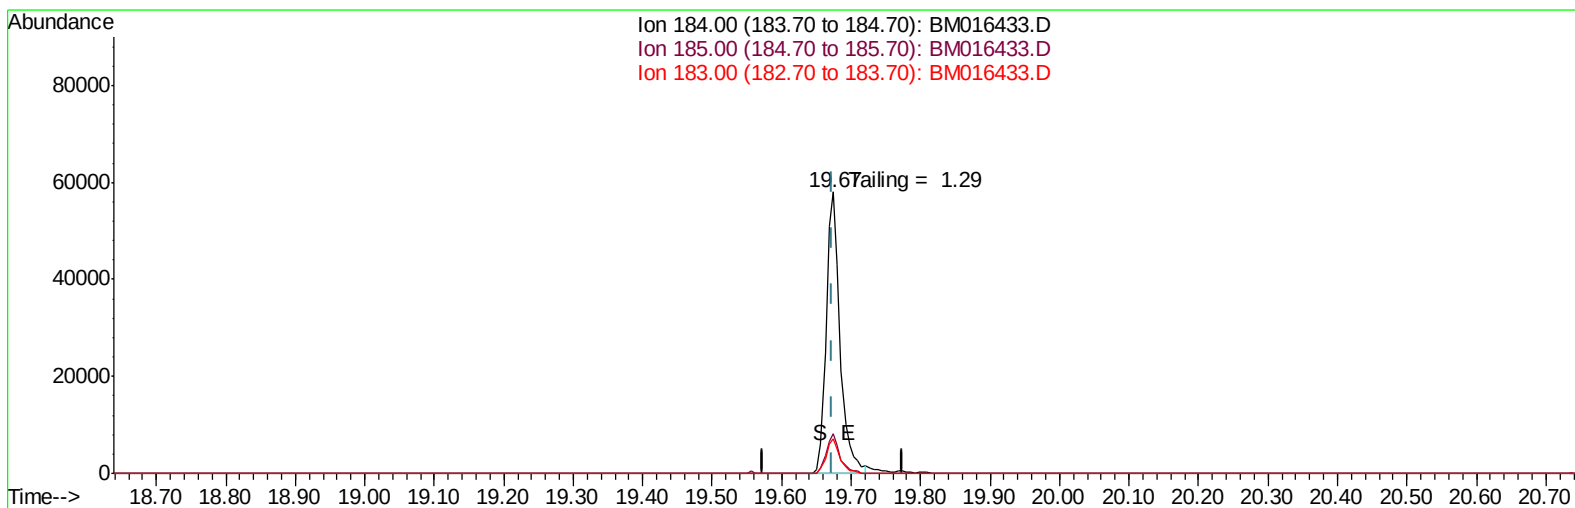

TIC: BM016433.D

(76) Benzidine

19.674min (-0.000) 0.00ng

response 82230

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 14.10 |
| 183.00 | 11.10 | 12.48 |
| 0.00   | 0.00  | 0.00  |