
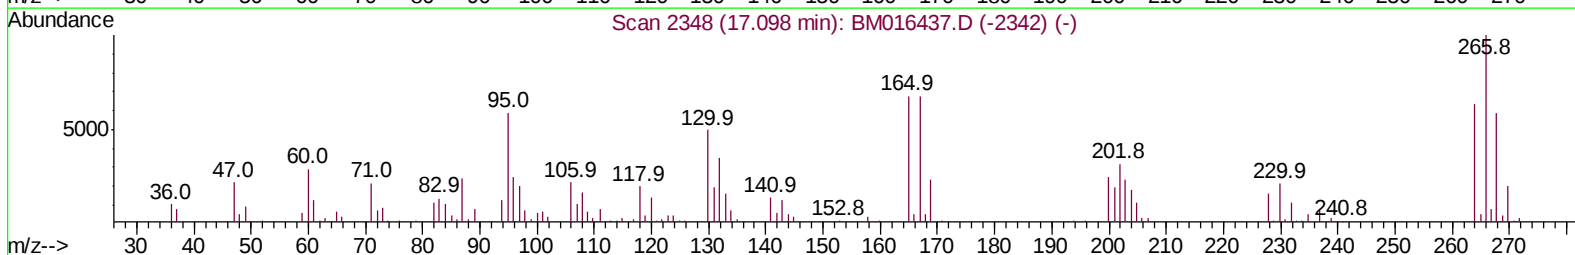
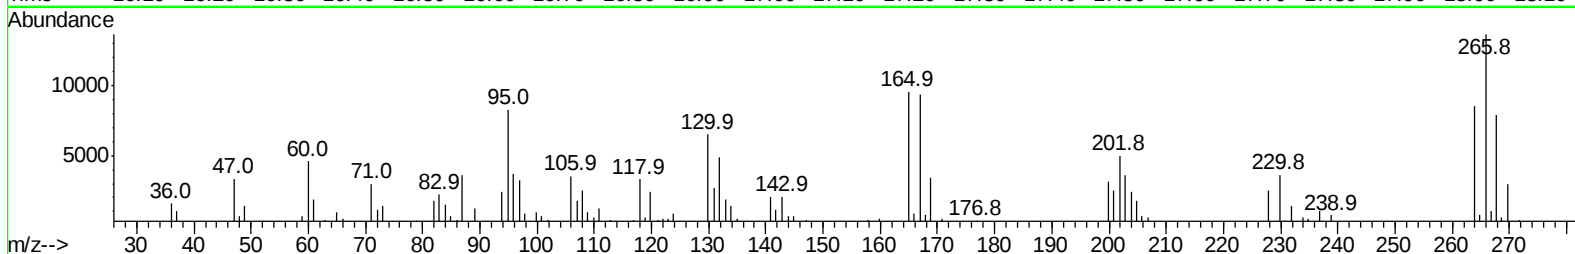


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\
Data File : BM016442.D
Acq On : 17 Aug 2018 18:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 03:03:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 16:27:00 2018
Response via : Initial Calibration

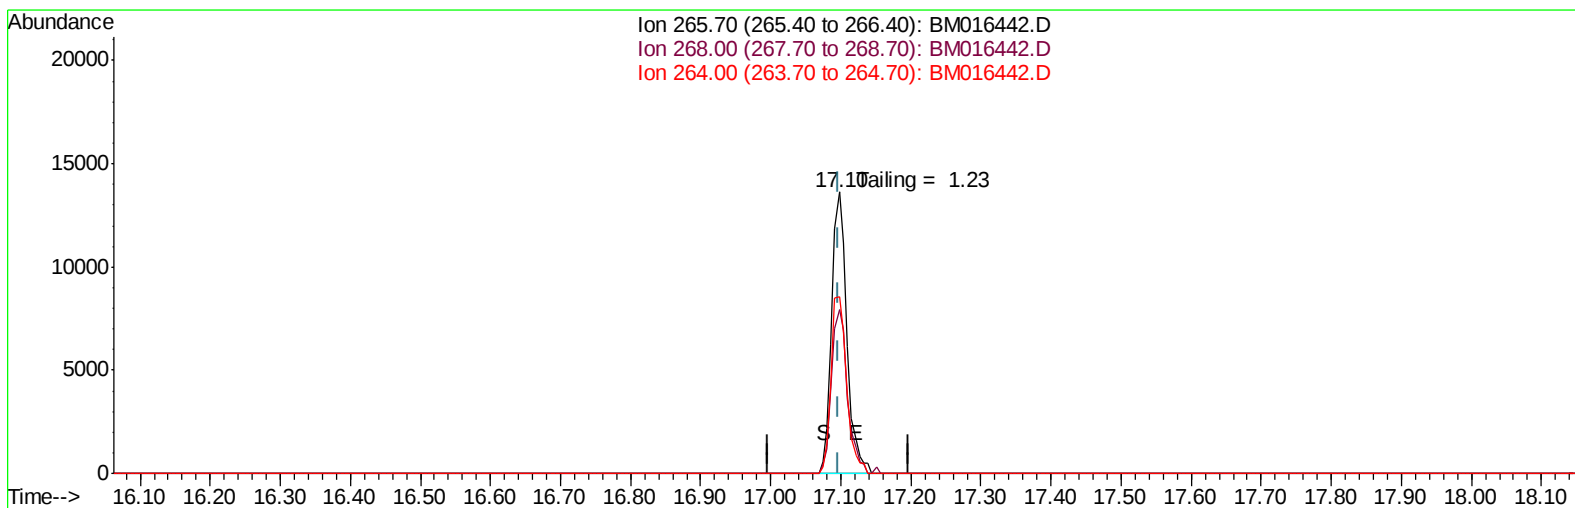

TIC: BM016442.D

(69) Pentachlorophenol (C)




17.098min (-0.000) 0.00ng

response 20460

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.23
264.00	61.20	68.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\
 Data File : BM016442.D
 Acq On : 17 Aug 2018 18:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 20 03:03:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 16:27:00 2018
 Response via : Initial Calibration

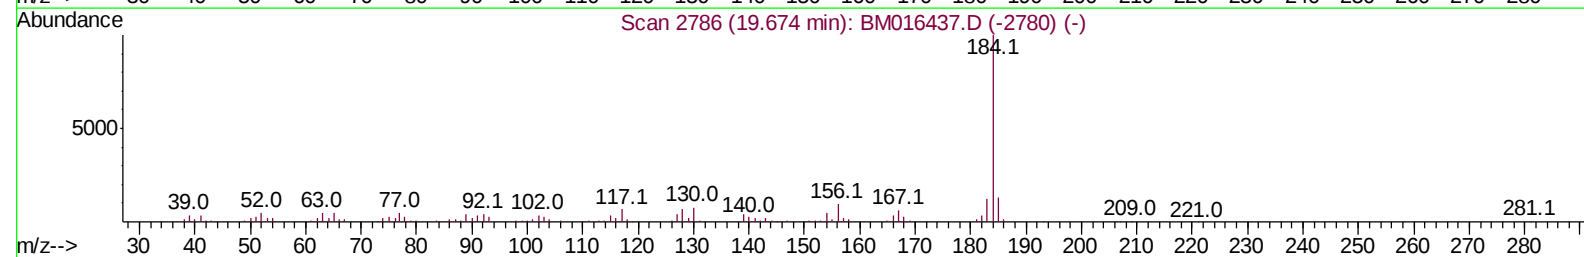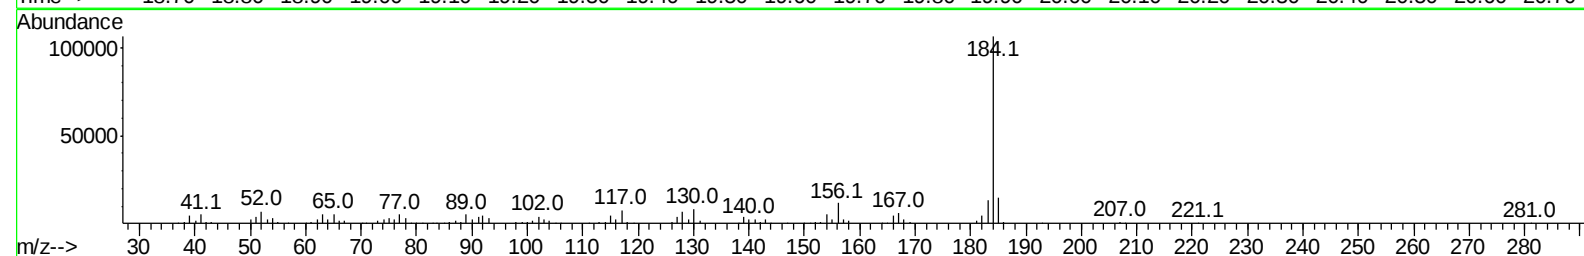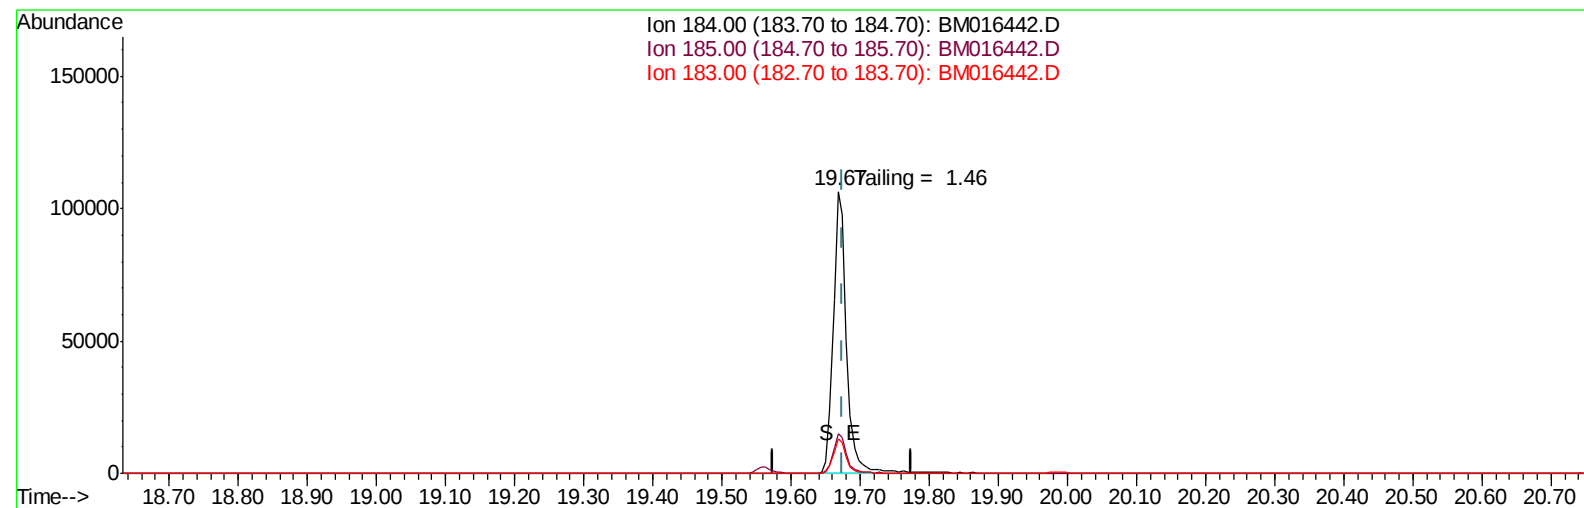

TIC: BM016442.D

(76) Benzidine

19.668min (-0.006) 0.00ng

response 140544

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.97
183.00	11.10	12.49
0.00	0.00	0.00