

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
 Data File : BM016467.D
 Acq On : 18 Aug 2018 11:03
 Operator : SJ/JU
 Sample : J4521-09
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 72-11969

Quant Time: Aug 20 01:49:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 17 16:27:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	8767	20.00	ng	0.00
21) Naphthalene-d8	10.86	136	30721	20.00	ng	0.00
38) Acenaphthene-d10	14.70	164	19946	20.00	ng	0.00
63) Phenanthrene-d10	17.44	188	55758	20.00	ng	0.00
75) Chrysene-d12	21.58	240	88838	20.00	ng	0.00
86) Perylene-d12	23.89	264	121421	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	59118	113.32	ng	0.00
7) Phenol-d6	7.22	99	68414	97.57	ng	-0.01
23) Nitrobenzene-d5	9.24	82	74803	101.41	ng	0.00
41) 2,4,6-Tribromophenol	16.19	330	49757	165.16	ng	-0.01
44) 2-Fluorobiphenyl	13.31	172	164209	85.61	ng	-0.01
78) Terphenyl-d14	20.03	244	570435	97.05	ng	0.00
Target Compounds						
76) Benzidine	19.67	184	20193	10.328	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
Data File : BM016467.D
Acq On : 18 Aug 2018 11:03
Operator : SJ/JU
Sample : J4521-09
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
72-11969

Quant Time: Aug 20 01:49:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 17 16:27:00 2018
Response via : Initial Calibration

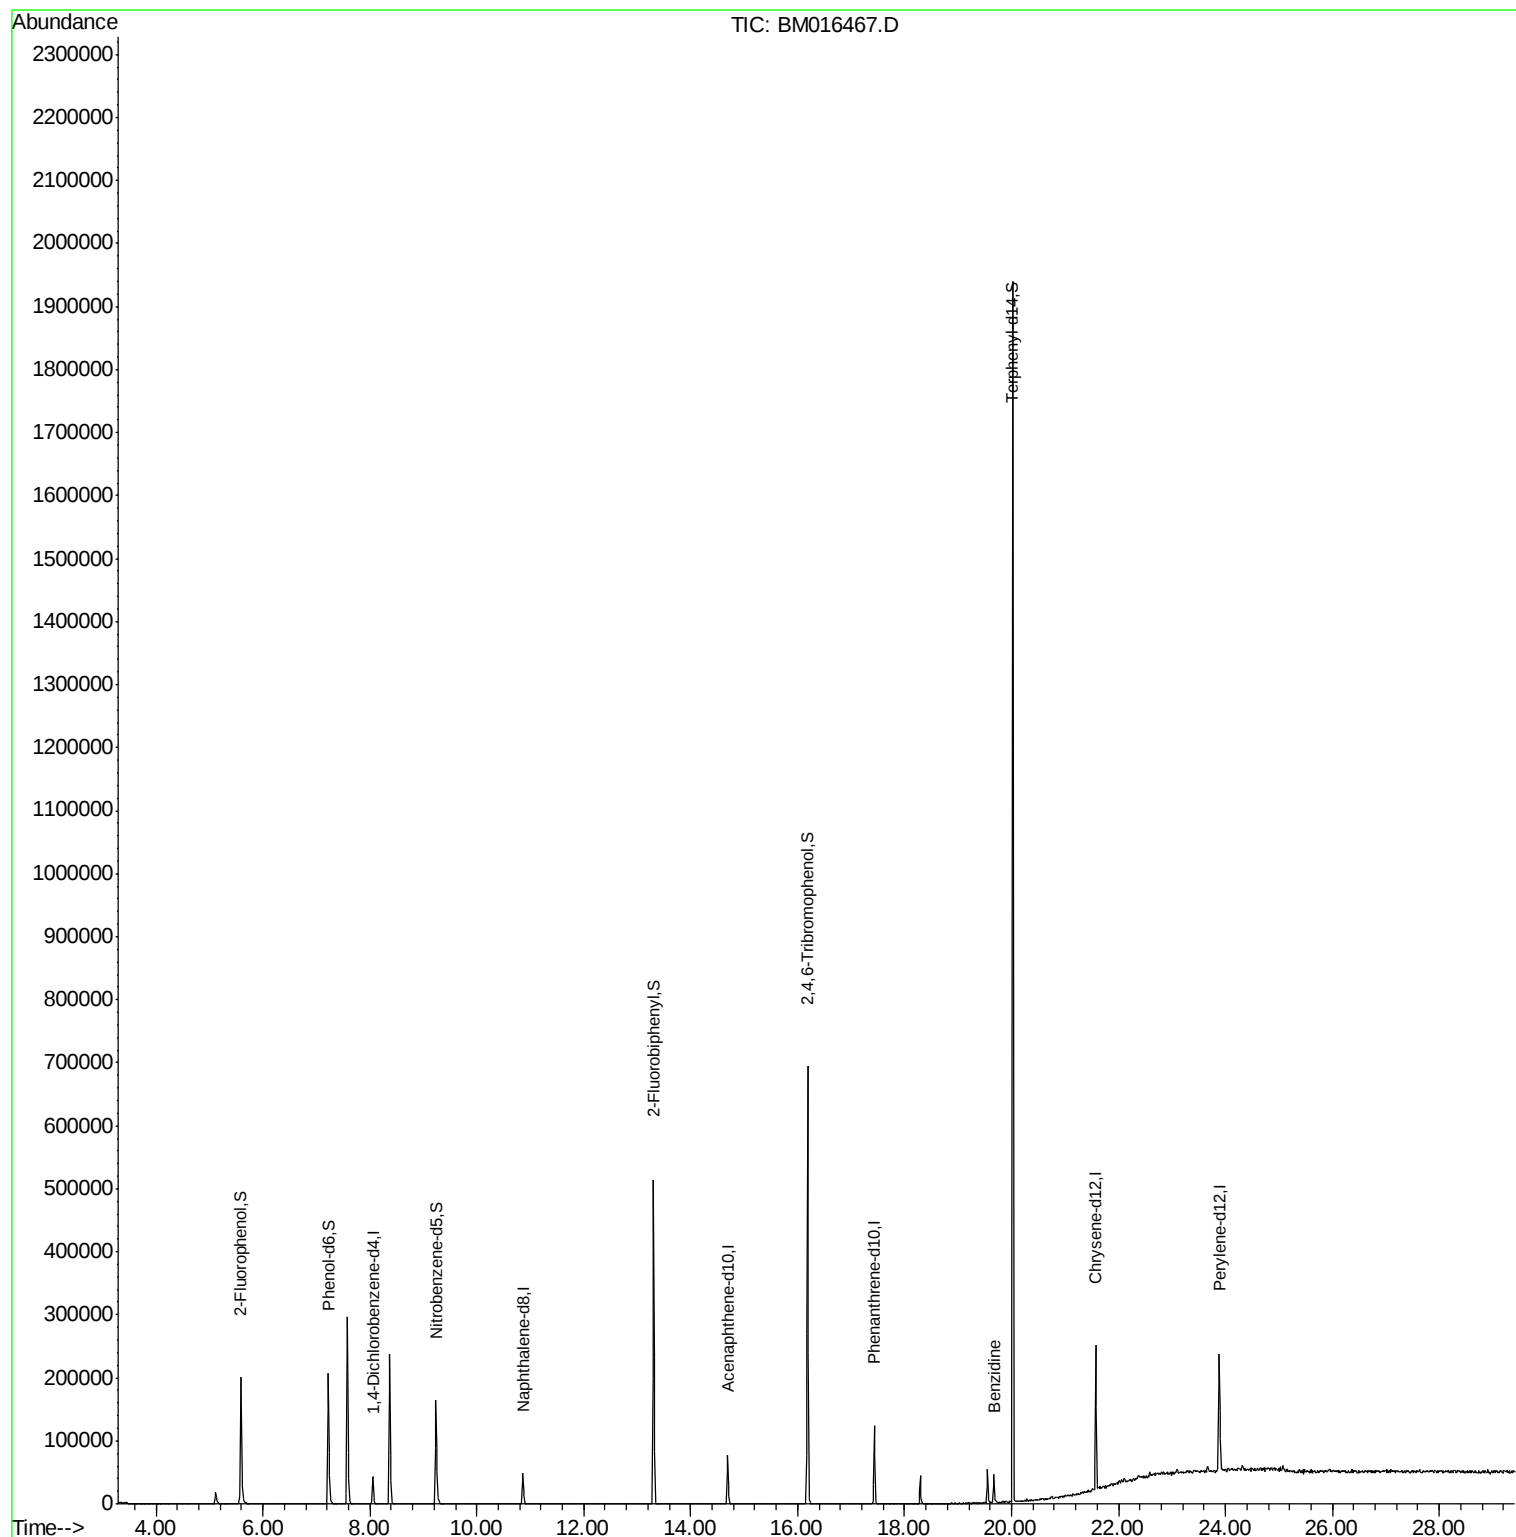




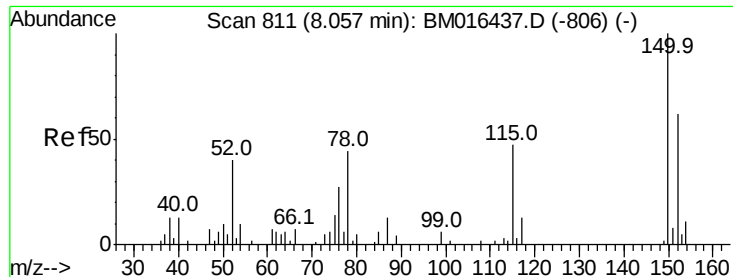


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 811
Delta R.T. -0.00 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Instrument :
BNA_M
ClientSampled :
72-11969




Tot Ion:152 Resp: 8767
Ion Ratio Lower Upper
152 100
150 158.1 119.5 179.3
115 62.1 43.0 64.4

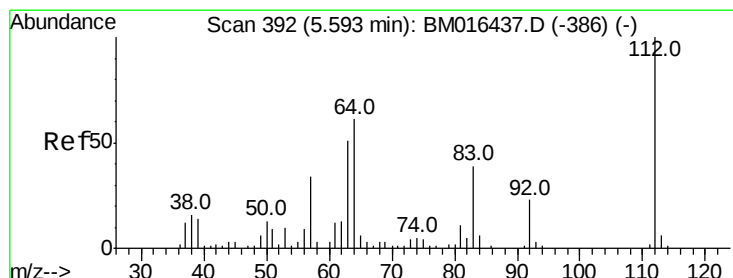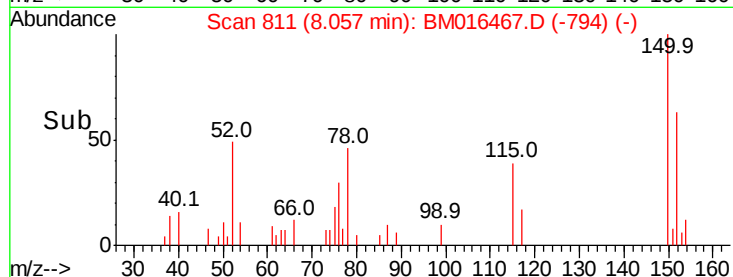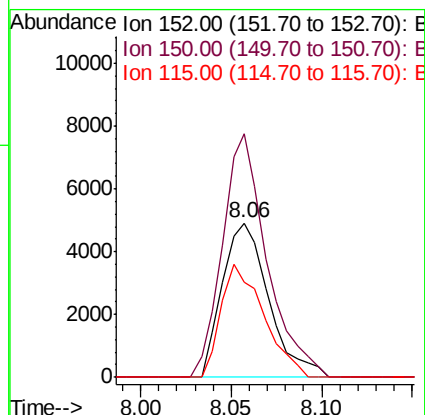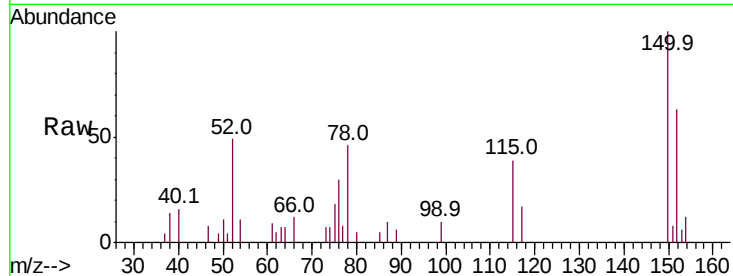


#5

2-Fluorophenol
Concen: N.D. ng
RT: 5.59 min Scan# 391
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Tgt Ion:112 Resp: 59118
Ion Ratio Lower Upper
112 100
64 60.7 38.6 57.8#
63 55.0 19.3 28.9#

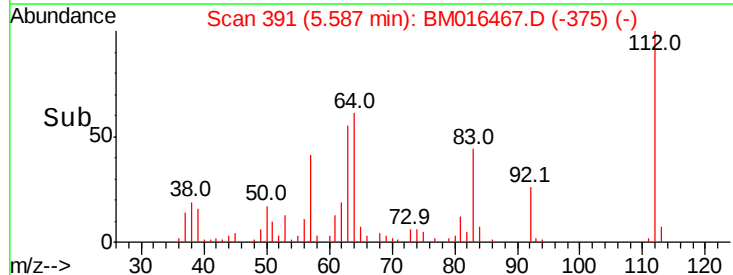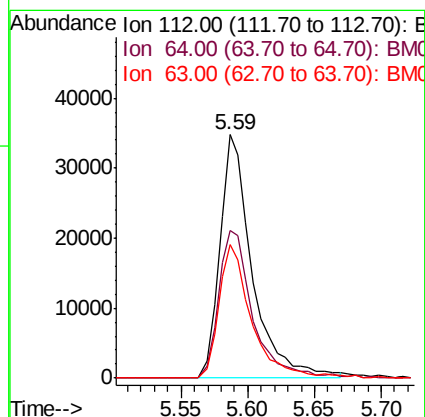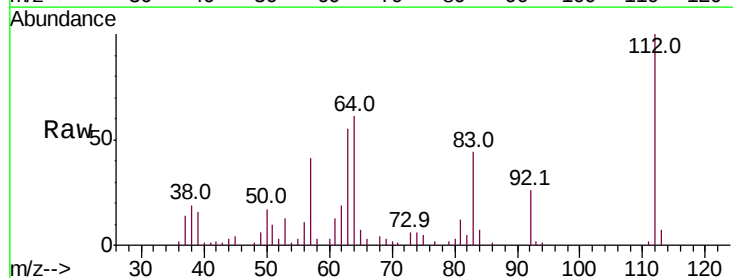

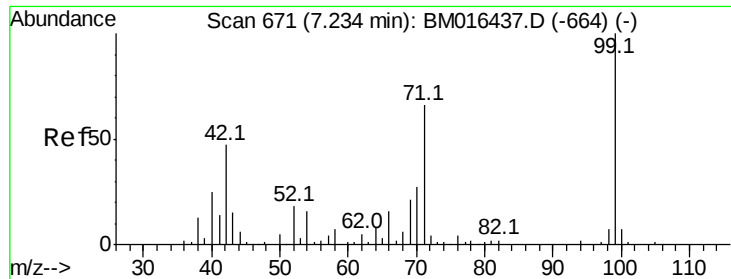

#7

Phenol-d6

Concen: N.D. ng

RT: 7.22 min Scan# 669

Delta R.T. -0.01 min

Lab File: BM016467.D

Acq: 18 Aug 2018 11:03

Instrument :

BNA_M

ClientSampled :

72-11969


Tot Ion: 99 Resp: 68414

Ion Ratio Lower Upper

99 100

42 50.9 11.0 16.4#




71 73.0 23.4 35.2#

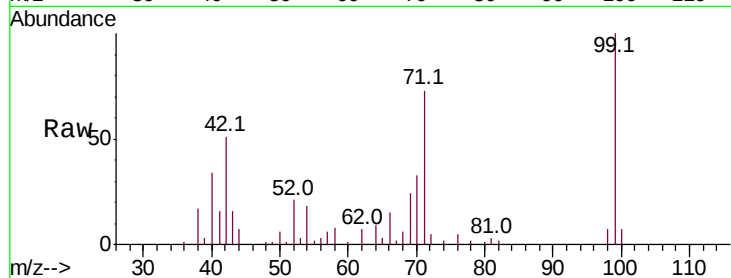

Abundance Ion 99.00 (98.70 to 99.70): BM016467.D (-664) (-)

Ion 42.00 (41.70 to 42.70): BM016467.D (-664) (-)

Ion 71.00 (70.70 to 71.70): BM016467.D (-664) (-)

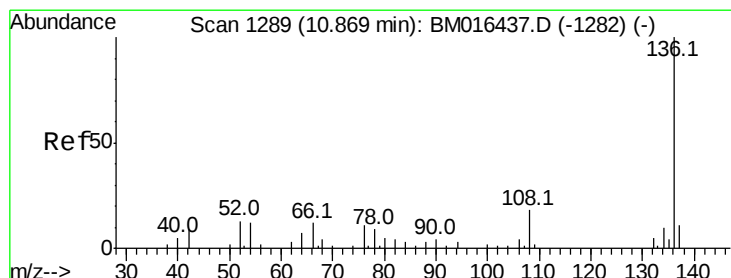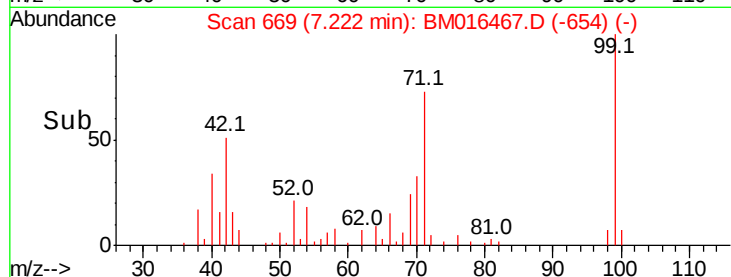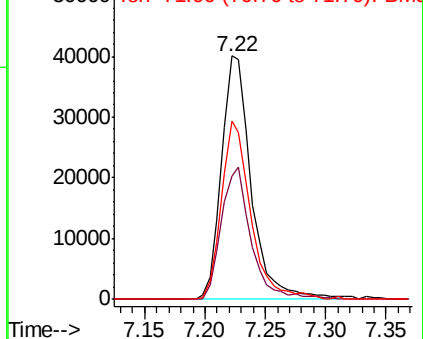

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1288

Delta R.T. -0.01 min

Lab File: BM016467.D

Acq: 18 Aug 2018 11:03

Tgt Ion: 136 Resp: 30721


Ion Ratio Lower Upper

136 100

137 12.1 8.7 13.1

54 15.7 4.6 6.8#

68 3.2 3.7 5.5#


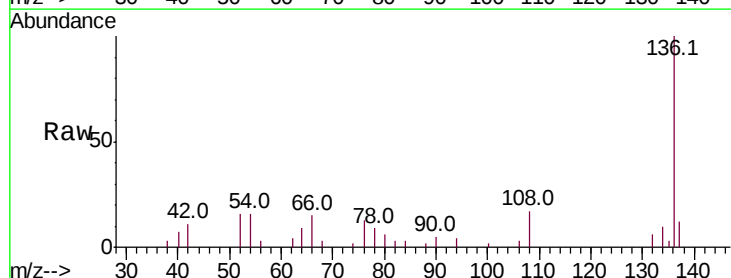



Abundance Ion 136.00 (135.70 to 136.70): BM016467.D (-1272) (-)

Ion 137.00 (136.70 to 137.70): BM016467.D (-1272) (-)

Ion 54.00 (53.70 to 54.70): BM016467.D (-1272) (-)

Ion 68.00 (67.70 to 68.70): BM016467.D (-1272) (-)



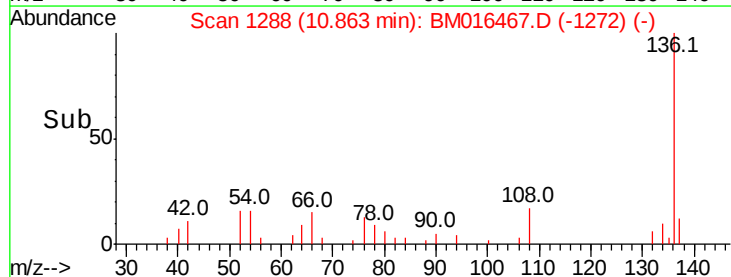
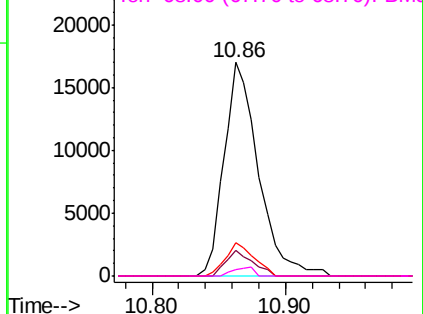


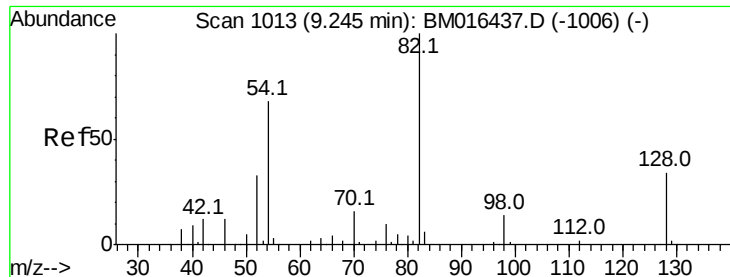

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.24 min Scan# 1012
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03




Instrument :
BNA_M
ClientSampleId :
72-11969


Tot Ion: 82 Resp: 74803
Ion Ratio Lower Upper
82 100
128 31.8 32.8 49.2#
54 70.9 40.6 60.8#

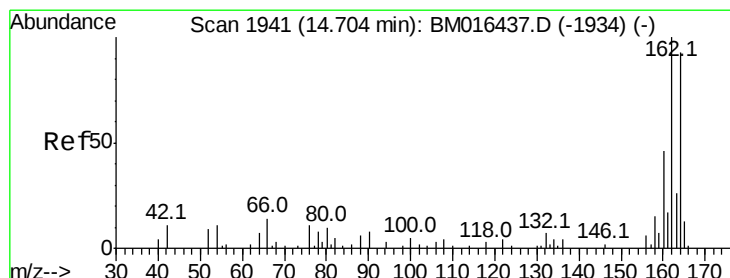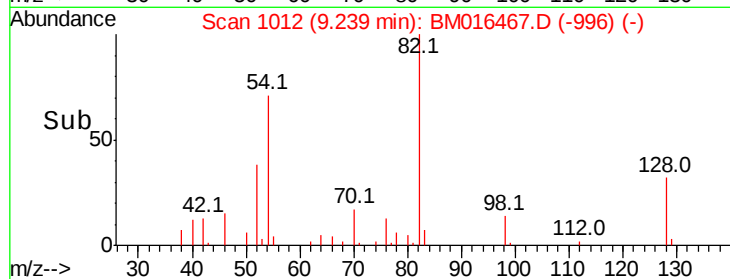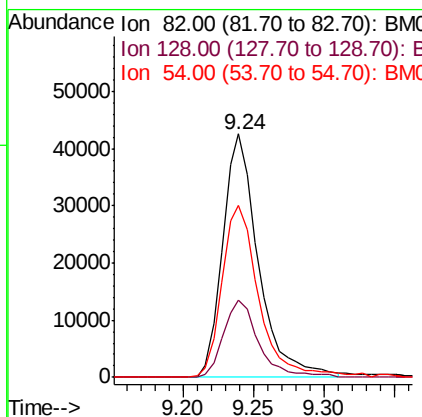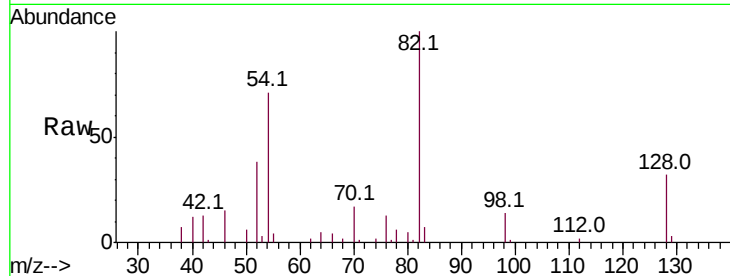

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.70 min Scan# 1940
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Tgt Ion: 164 Resp: 19946
Ion Ratio Lower Upper
164 100
162 107.1 82.4 123.6
160 47.5 35.8 53.6

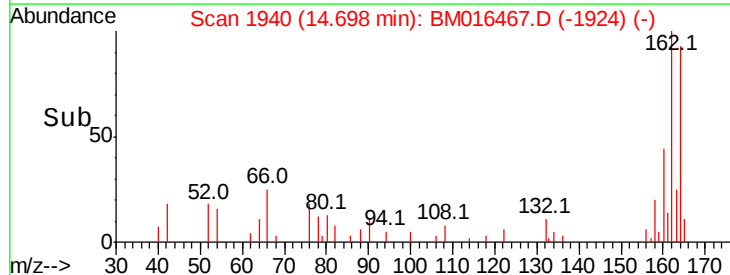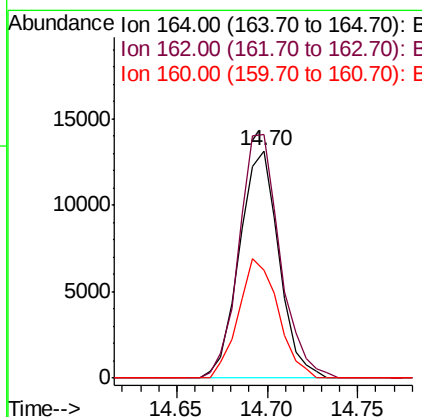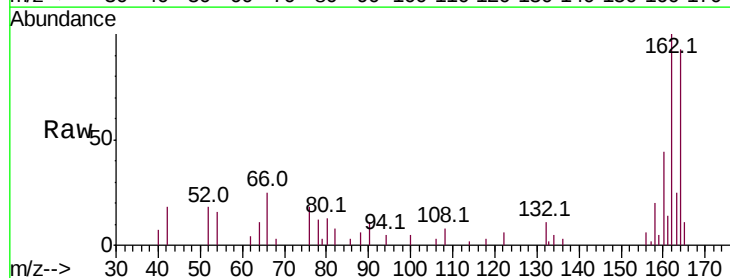


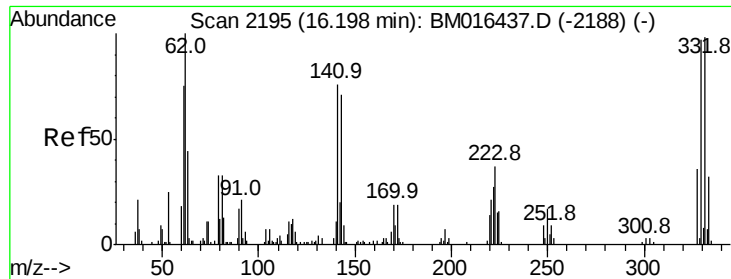




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.19 min Scan# 2193
 Delta R.T. -0.01 min
 Lab File: BM016467.D
 Acq: 18 Aug 2018 11:03

Instrument :
 BNA_M
 ClientSampled :
 72-11969

Tot Ion:330 Resp: 49757
 Ion Ratio Lower Upper
 330 100
 332 95.4 0.0 0.0#
 141 104.7 0.0 0.0#

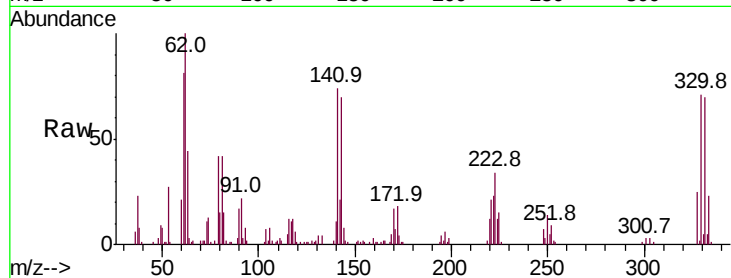


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

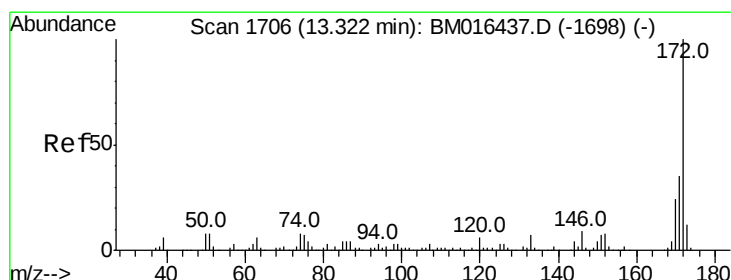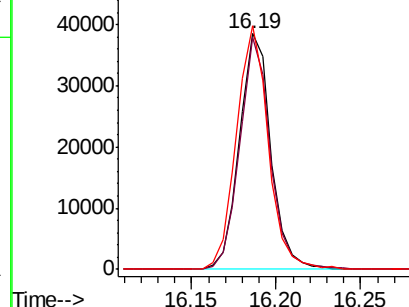
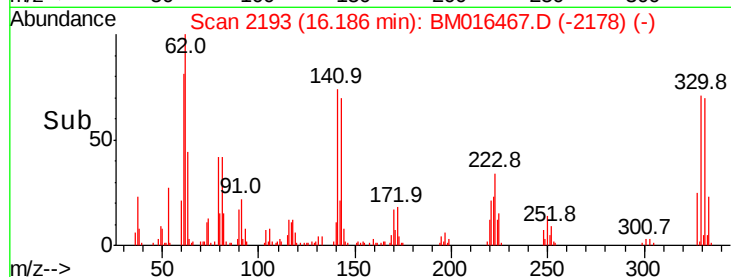



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.31 min Scan# 1704
 Delta R.T. -0.01 min
 Lab File: BM016467.D
 Acq: 18 Aug 2018 11:03

Tgt Ion:172 Resp: 164209
 Ion Ratio Lower Upper
 172 100
 171 37.5 28.5 42.7
 170 24.9 18.8 28.2

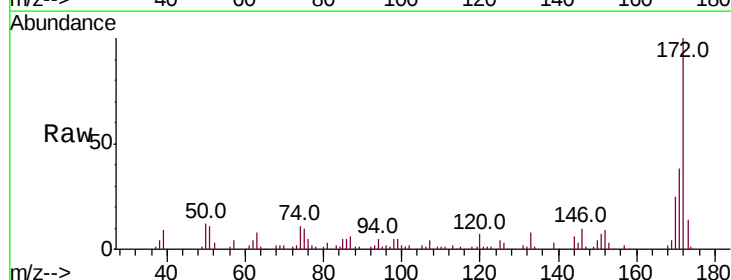

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

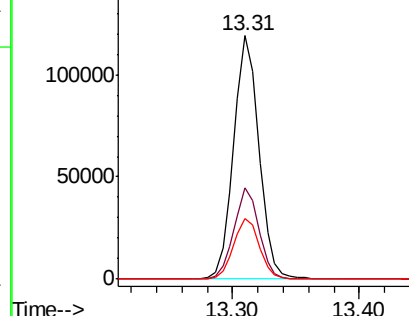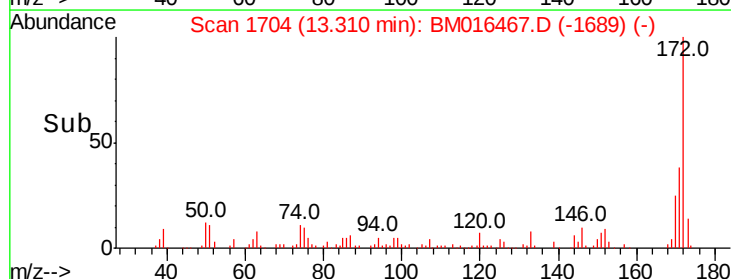


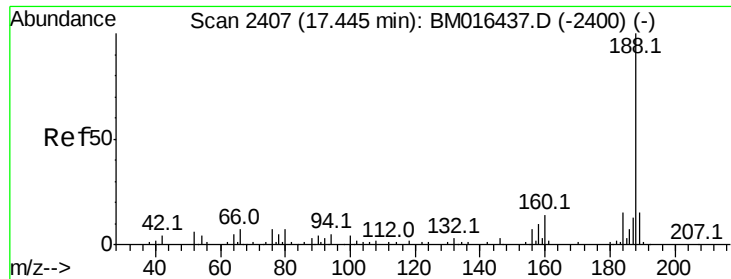




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.44 min Scan# 2406
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Instrument :
BNA_M
ClientSampleId :
72-11969

Tot Ion:188 Resp: 55758
Ion Ratio Lower Upper
188 100
94 5.2 8.7 13.1#
80 7.3 9.3 13.9#

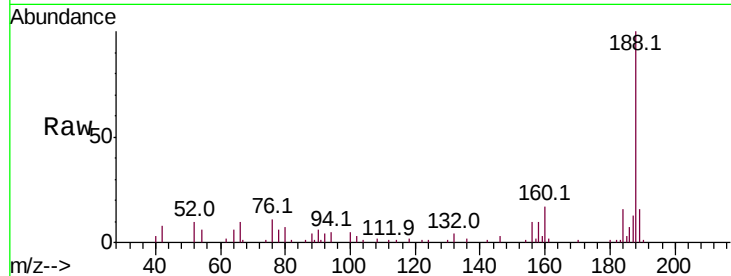


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

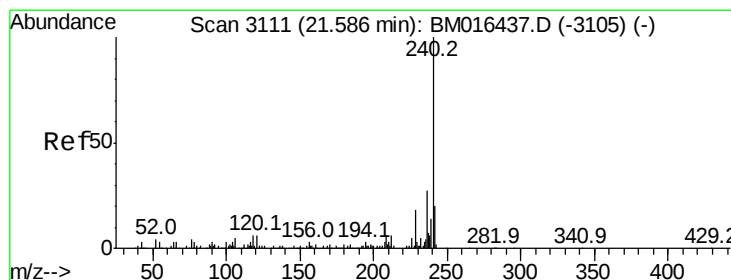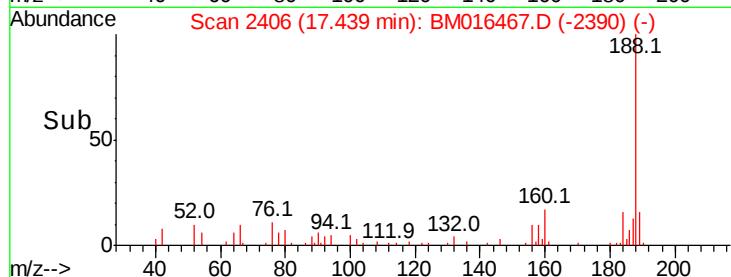
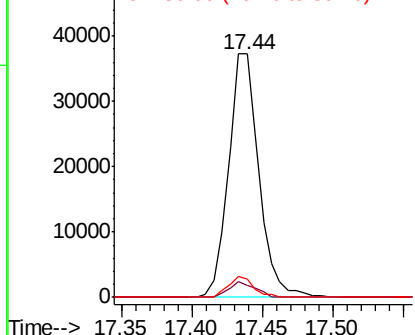



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.58 min Scan# 3110
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Tgt Ion:240 Resp: 88838
Ion Ratio Lower Upper
240 100
120 4.3 8.2 12.2#
236 26.1 20.0 30.0

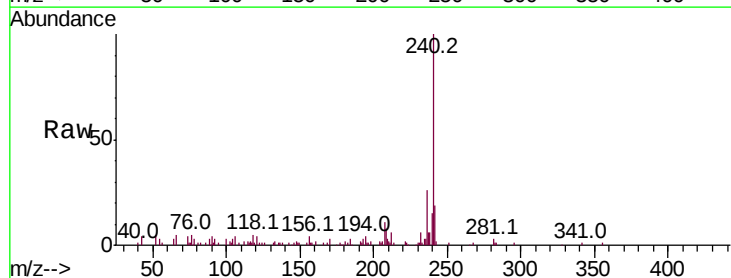

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

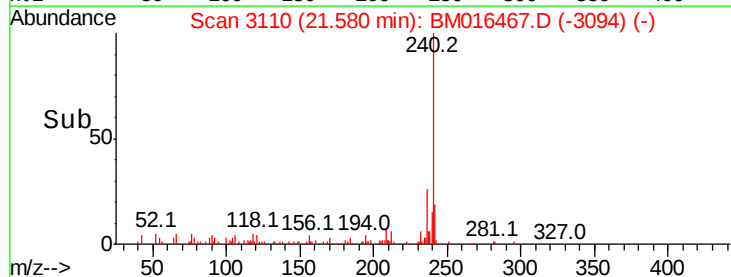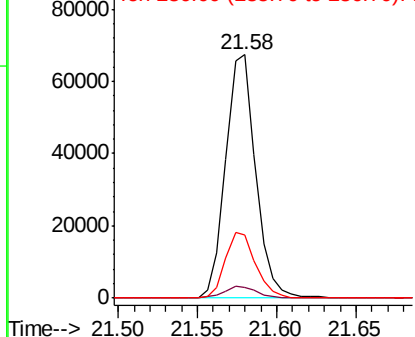

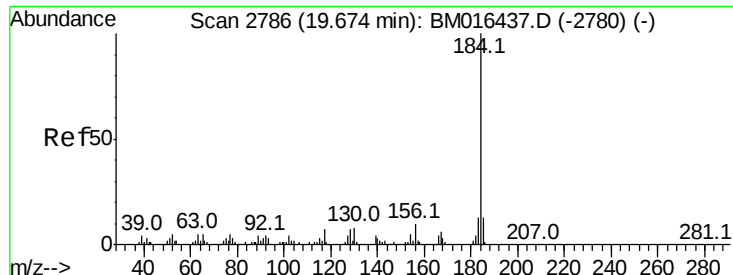

#76

Benzidine

Concen: 10.328 ng

RT: 19.67 min Scan# 2785

Delta R.T. -0.01 min

Lab File: BM016467.D

Acq: 18 Aug 2018 11:03

Instrument :

BNA_M

ClientSampleId :

72-11969


Tot Ion:184 Resp: 20193

Ion Ratio Lower Upper

184 100

185 15.1 11.3 16.9




183 13.0 8.9 13.3

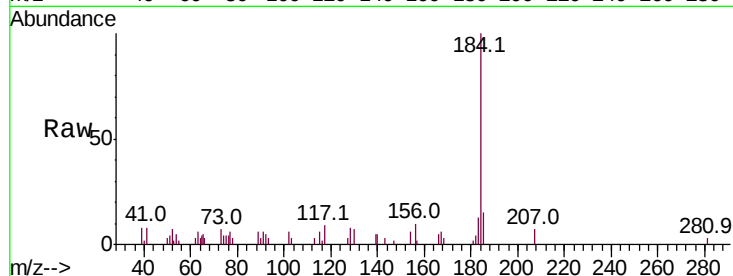

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

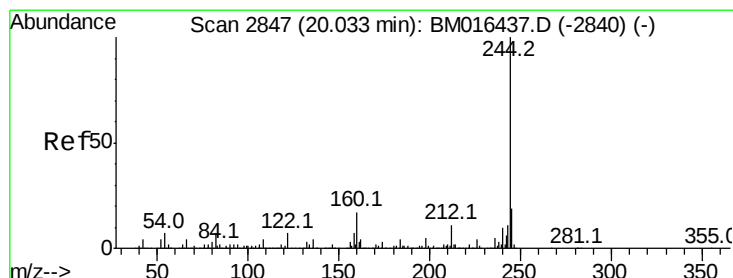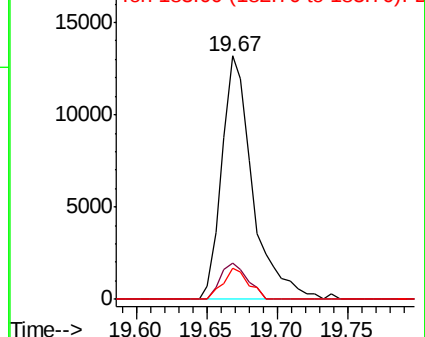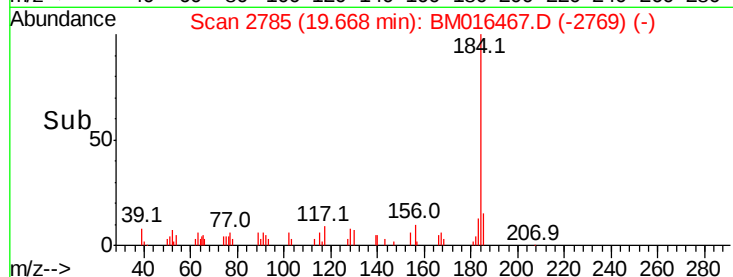

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.03 min Scan# 2846

Delta R.T. -0.01 min

Lab File: BM016467.D

Acq: 18 Aug 2018 11:03


Tgt Ion:244 Resp: 570435

Ion Ratio Lower Upper

244 100

212 11.0 4.9 7.3#



122 6.5 6.2 9.4

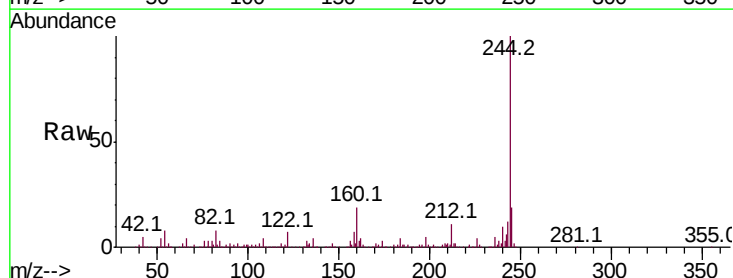


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

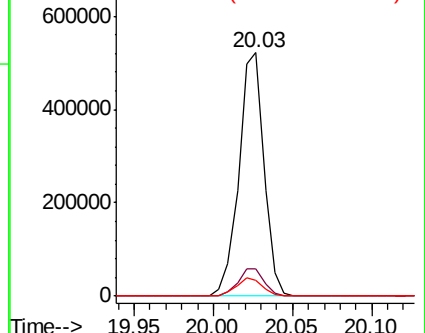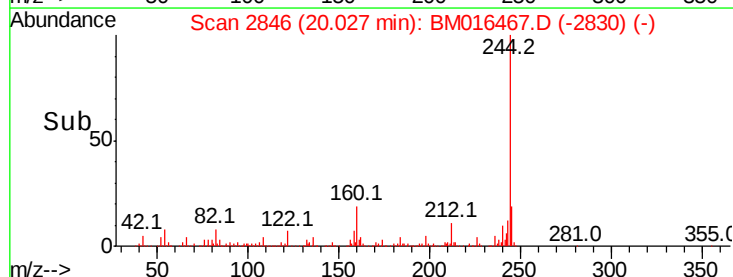


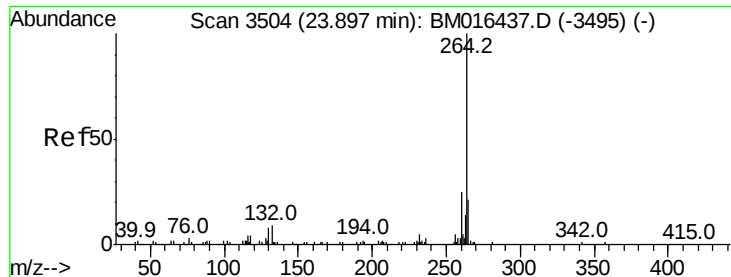

#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.89 min Scan# 3502
Delta R.T. -0.01 min
Lab File: BM016467.D
Acq: 18 Aug 2018 11:03

Instrument :
BNA_M
ClientSampleId :
72-11969

Tot Ion	Ratio	Lower	Upper
264	100		
260	26.1	18.6	27.8
265	22.3	17.3	25.9

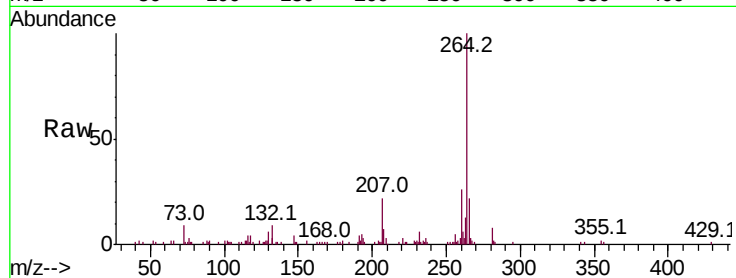

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

