

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
 Data File : BM016460.D
 Acq On : 18 Aug 2018 04:59
 Operator : SJ/JU
 Sample : PB112169BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB112169BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.587	387	391	407	rBV	267571	454000	21.77%	6.198%
2	7.228	664	670	687	rBV	316504	511217	24.52%	6.979%
3	7.581	724	730	743	rBV	353940	561086	26.91%	7.659%
4	8.057	806	811	819	rBV2	53275	86591	4.15%	1.182%
5	8.369	859	864	874	rBV	244940	411897	19.75%	5.623%
6	9.239	1006	1012	1029	rBV	169212	298731	14.33%	4.078%
7	10.869	1283	1289	1304	rBB	61725	106897	5.13%	1.459%
8	13.310	1698	1704	1716	rBV	562956	799043	38.32%	10.908%
9	14.698	1934	1940	1947	rBB2	103492	155734	7.47%	2.126%
10	16.186	2188	2193	2205	rBB	710134	930636	44.63%	12.704%
11	17.439	2401	2406	2415	rBV2	162906	228873	10.98%	3.124%
12	20.027	2840	2846	2851	rBV	1961002	2085029	100.00%	28.463%
13	21.580	3105	3110	3115	rBV	279860	342469	16.43%	4.675%
14	23.886	3496	3502	3512	rVB2	185491	353309	16.95%	4.823%


Sum of corrected areas: 7325512

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
Data File : BM016460.D
Acq On : 18 Aug 2018 04:59
Operator : SJ/JU
Sample : PB112169BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112169BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

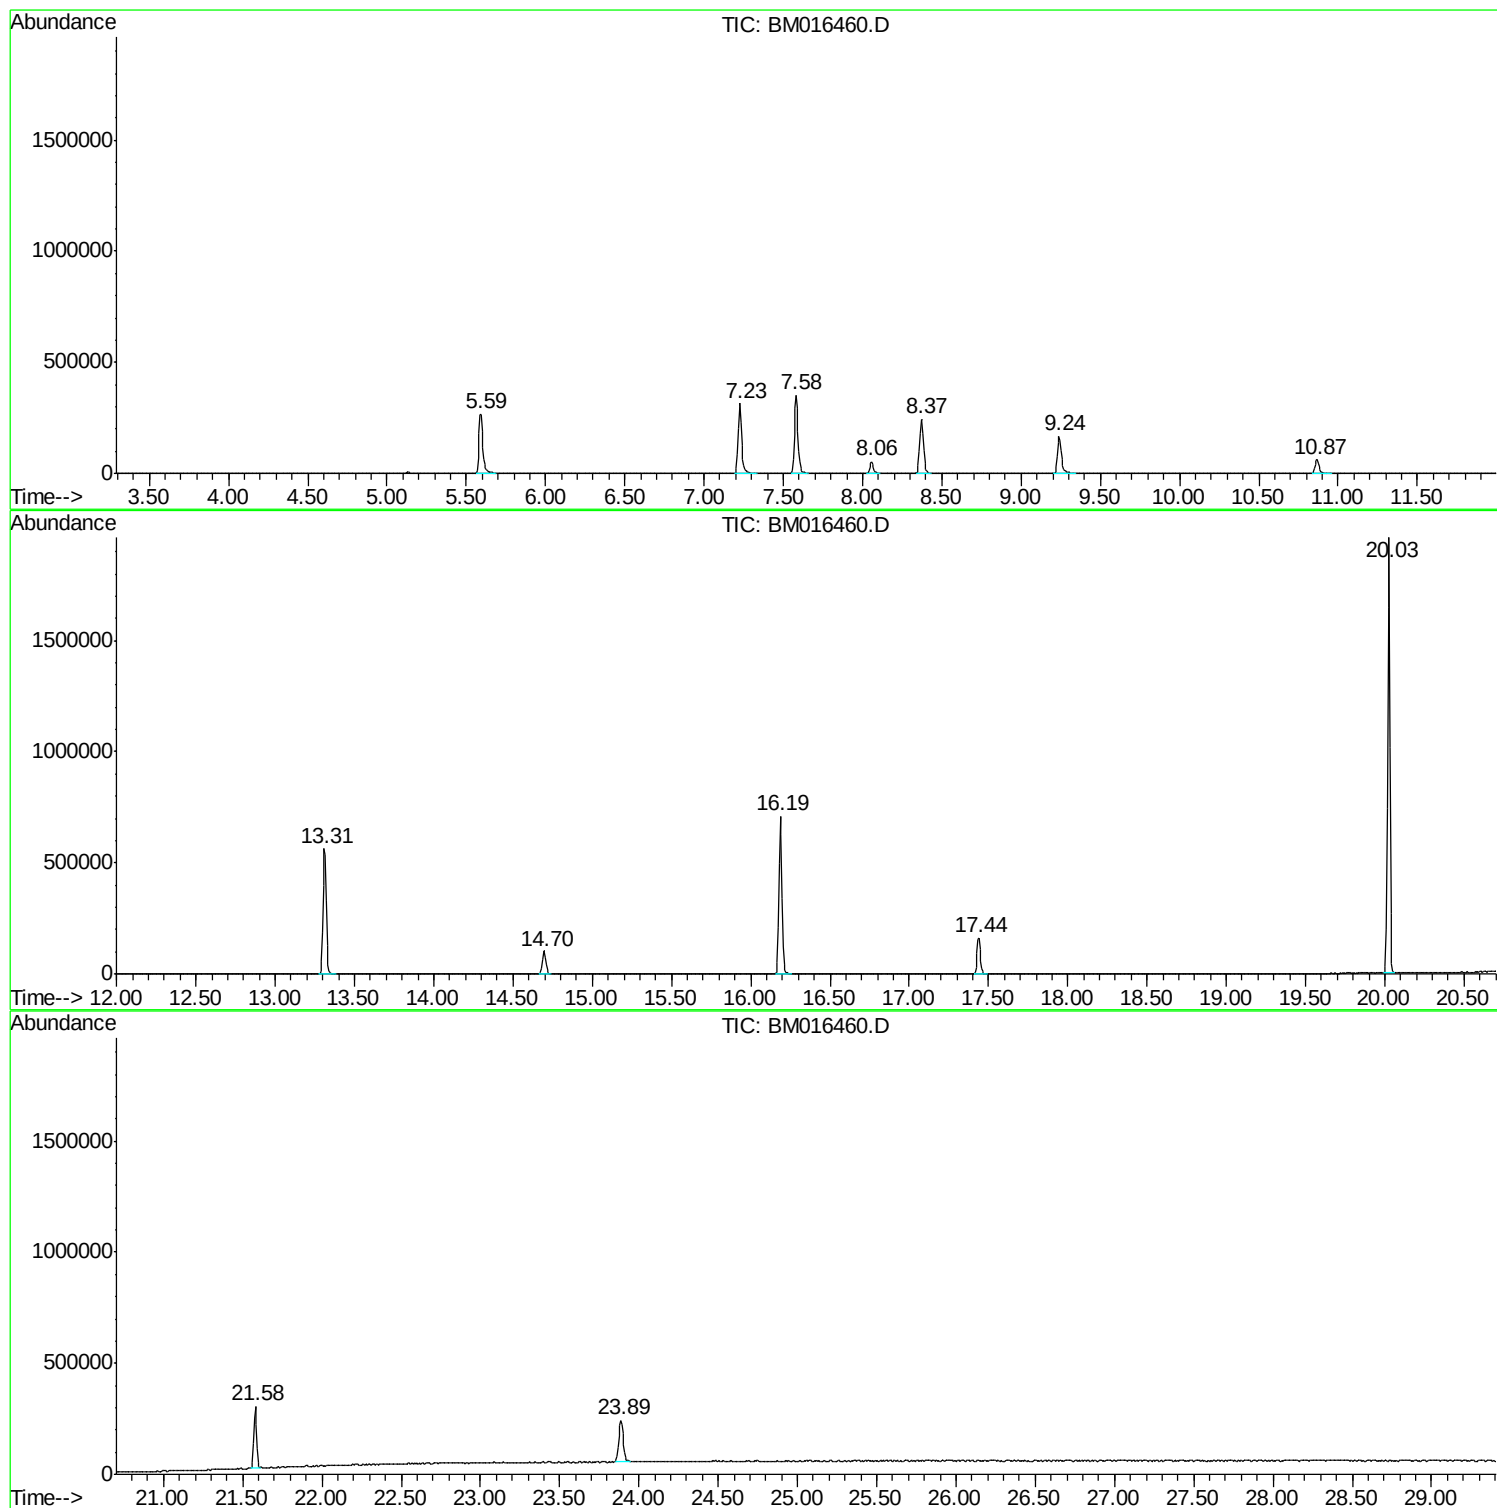

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081718\
Data File : BM016460.D
Acq On : 18 Aug 2018 04:59
Operator : SJ/JU
Sample : PB112169BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112169BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	129.60 ng	561086	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	10
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	10
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	10

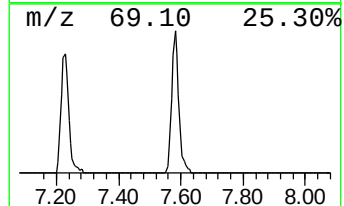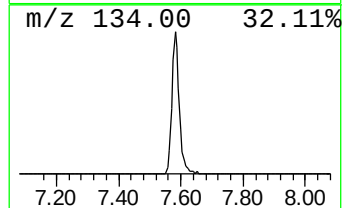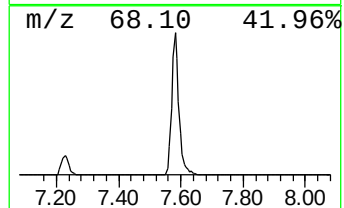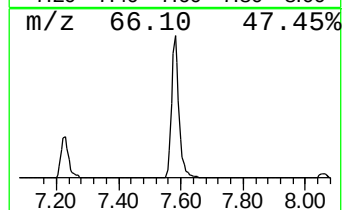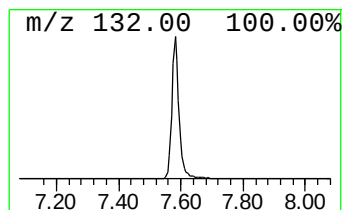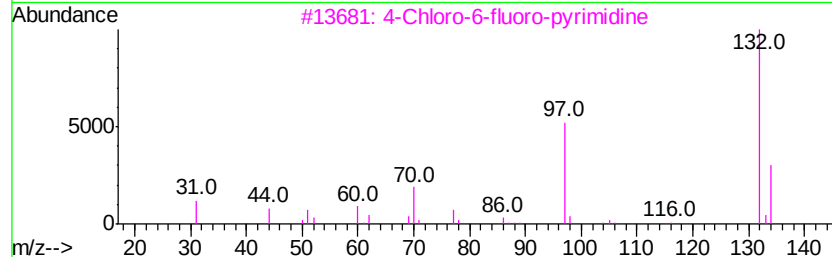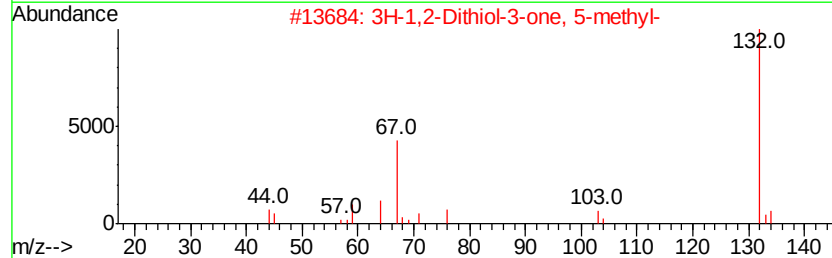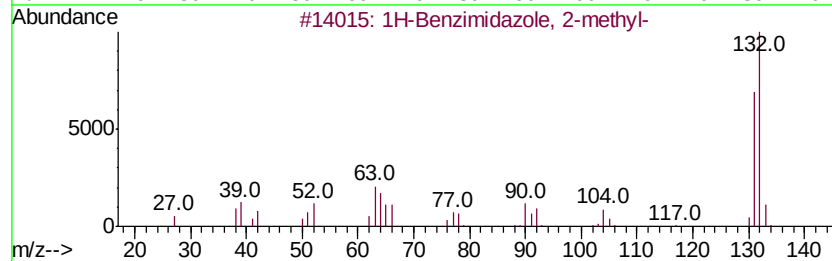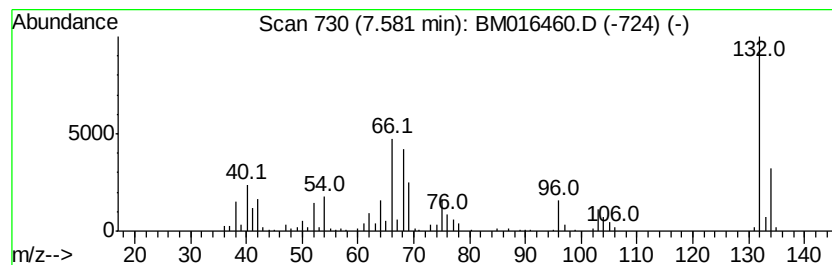

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081718\
Data File : BM016460.D
Acq On : 18 Aug 2018 04:59
Operator : SJ/JU
Sample : PB112169BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB112169BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	129.6	ng	561086	1	8.05	86591	20.0