


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\
 Data File : BM016433.D
 Acq On : 17 Aug 2018 11:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 17 16:27:00 2018

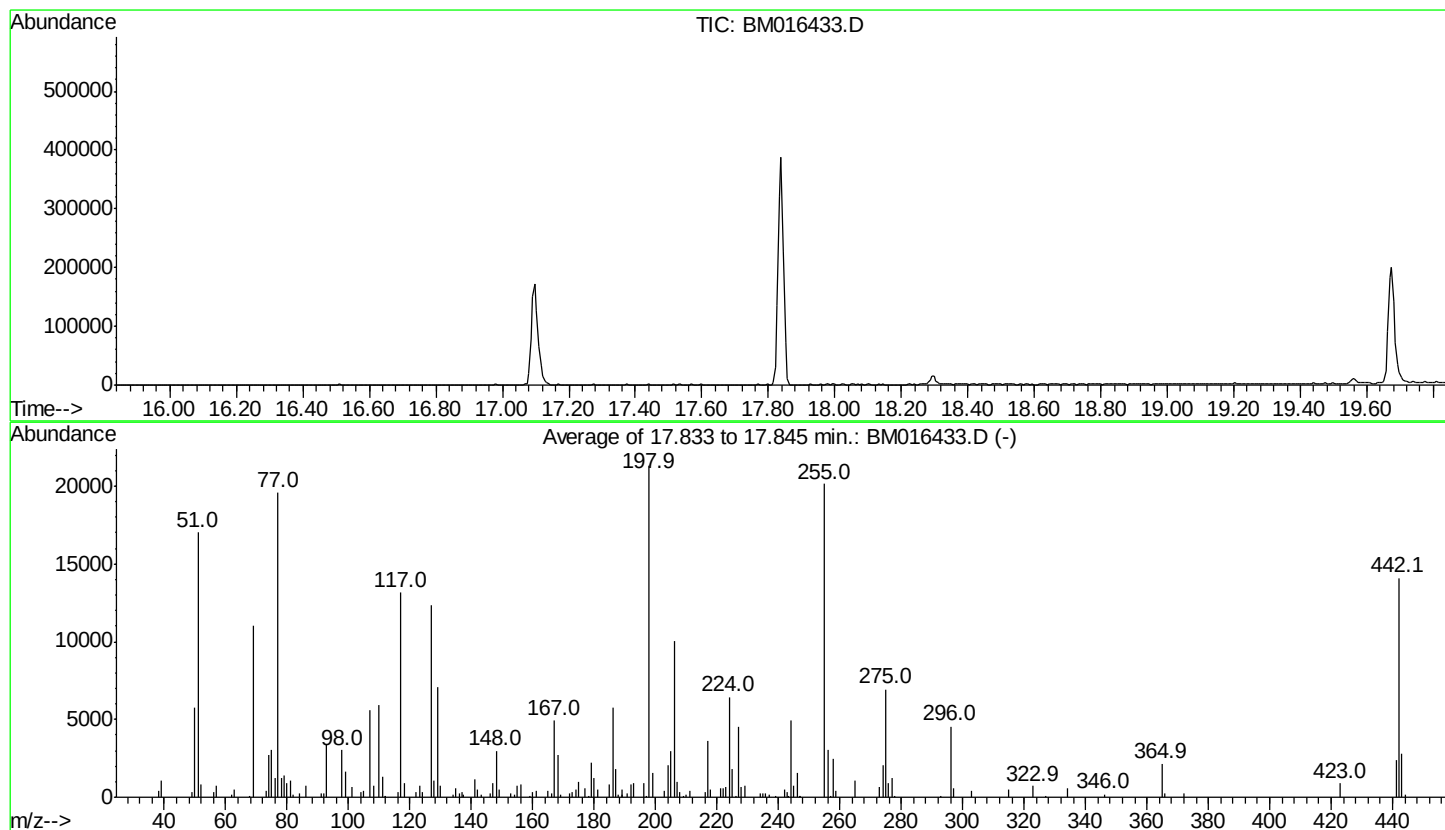

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	79.7	16999	PASS
68	69	0.00	2	0.9	104	PASS
69	198	0.00	100	51.7	11017	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.0	12358	PASS
197	198	0.00	2	0.5	102	PASS
198	198	100	100	100.0	21321	PASS
199	198	5	9	7.4	1578	PASS
275	198	10	60	32.4	6914	PASS
365	198	1	100	10.1	2162	PASS
441	198	0.01	100	11.1	2360	PASS
442	198	50	100	66.2	14105	PASS
443	442	15	24	19.9	2801	PASS