


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\
 Data File : BM016442.D
 Acq On : 17 Aug 2018 18:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 17 16:27:00 2018

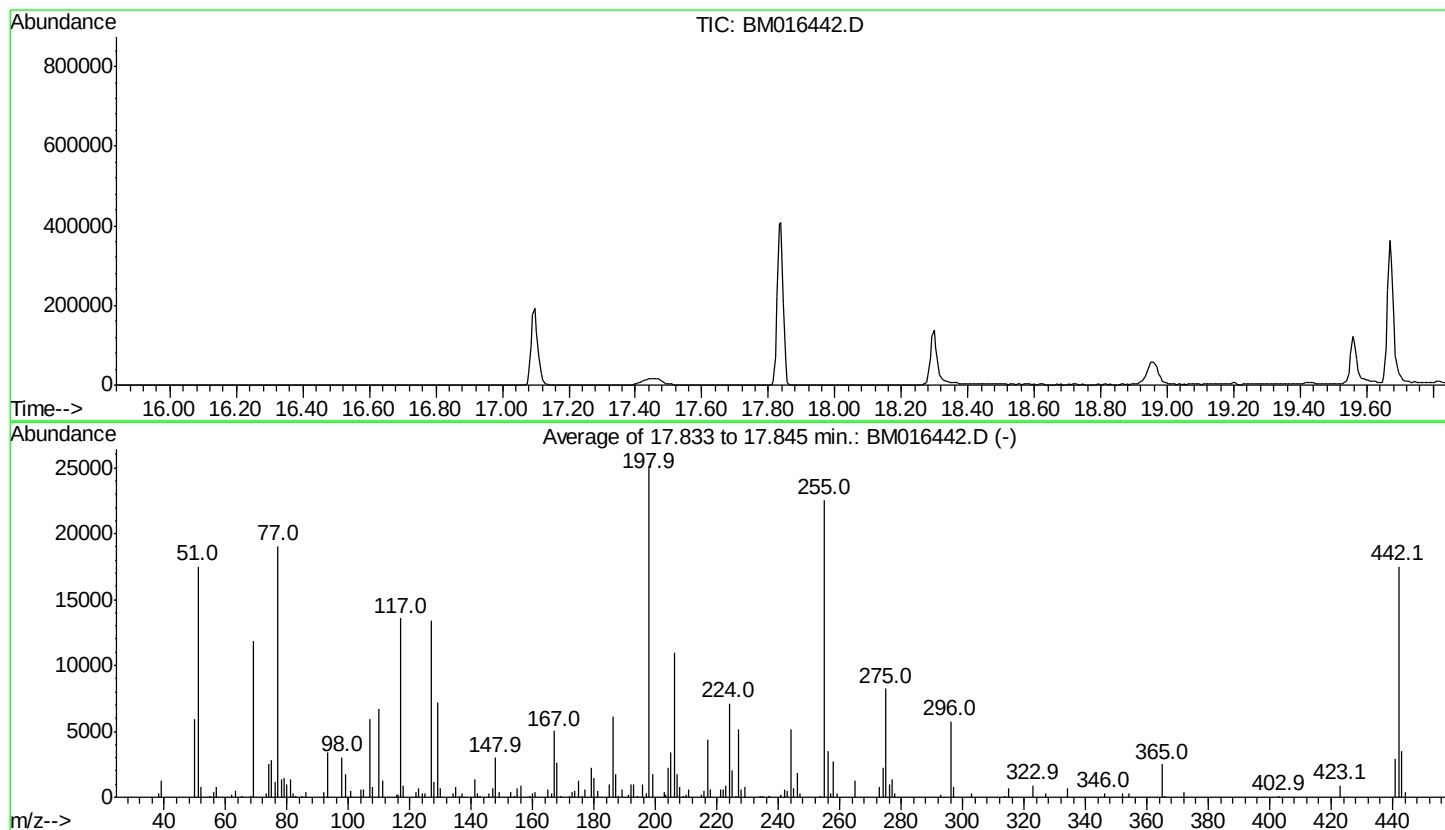

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.5	17488	PASS
68	69	0.00	2	1.1	135	PASS
69	198	0.00	100	46.9	11809	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	13438	PASS
197	198	0.00	2	1.1	283	PASS
198	198	100	100	100.0	25164	PASS
199	198	5	9	7.0	1750	PASS
275	198	10	60	32.8	8248	PASS
365	198	1	100	10.0	2518	PASS
441	198	0.01	100	11.5	2904	PASS
442	198	50	100	69.6	17526	PASS
443	442	15	24	20.2	3546	PASS