


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081718\
 Data File : BM016462.D
 Acq On : 18 Aug 2018 08:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM081718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 17 16:27:00 2018

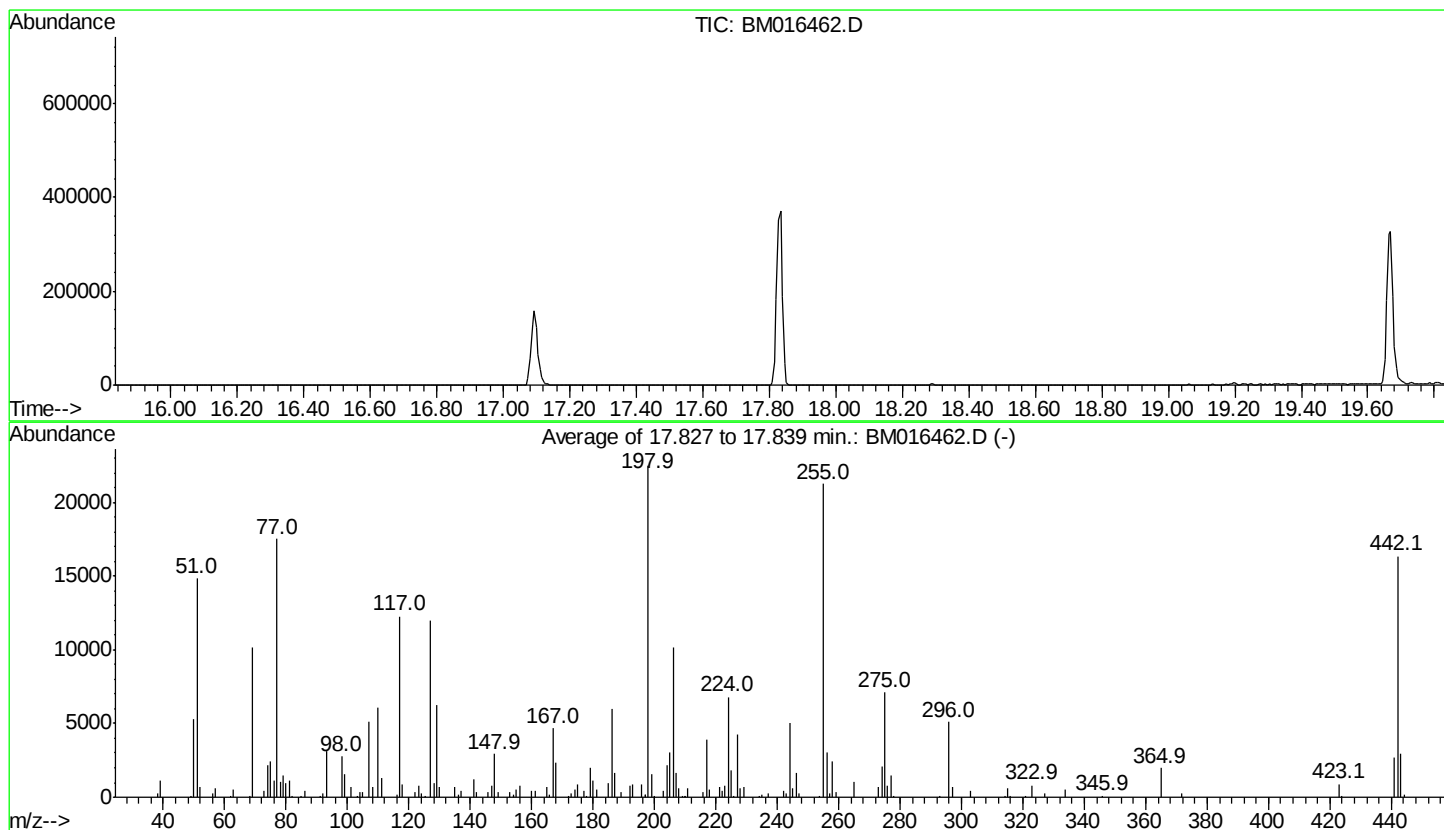

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.9	14819	PASS
68	69	0.00	2	1.2	121	PASS
69	198	0.00	100	45.3	10193	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	11953	PASS
197	198	0.00	2	0.7	148	PASS
198	198	100	100	100.0	22482	PASS
199	198	5	9	7.0	1568	PASS
275	198	10	60	31.6	7108	PASS
365	198	1	100	8.9	1996	PASS
441	198	0.01	100	11.8	2661	PASS
442	198	50	100	72.7	16338	PASS
443	442	15	24	18.3	2984	PASS