




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036322.D
Acq On : 17 Aug 2022 18:37
Operator : CG/JU
Sample : N4176-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P6

Manual IntegrationsAPPROVED

Quant Time: Aug 18 02:19:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 16 15:00:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/19/2022

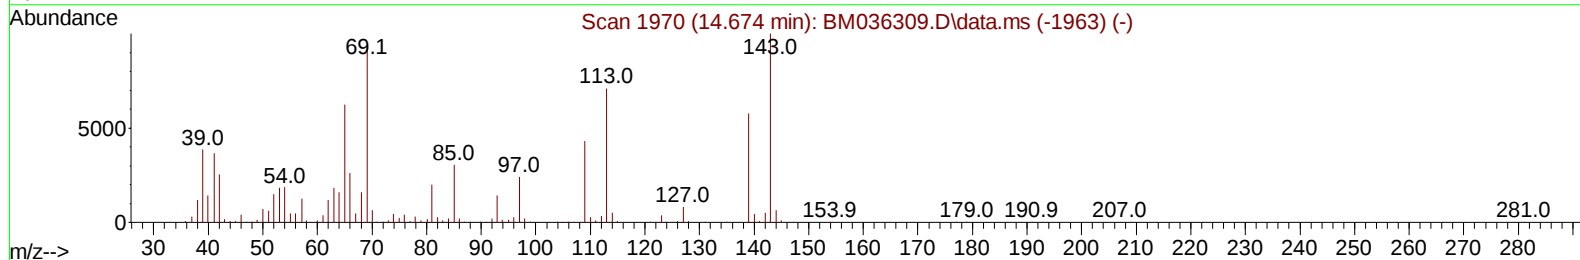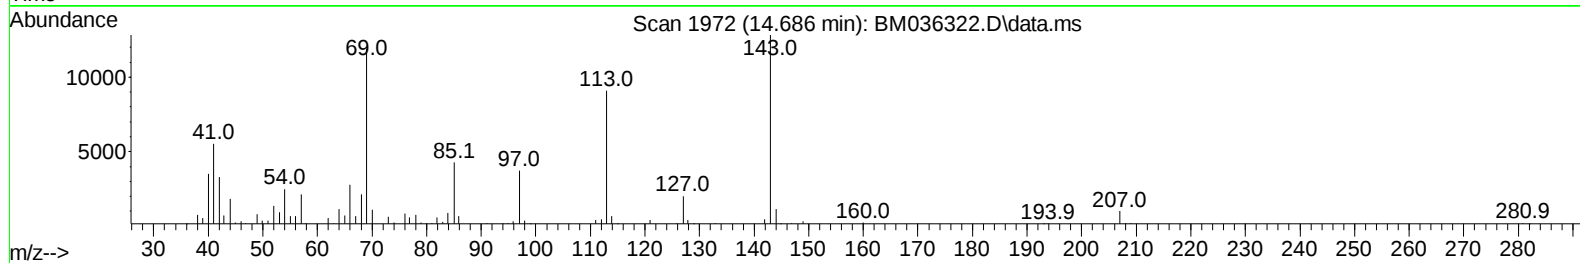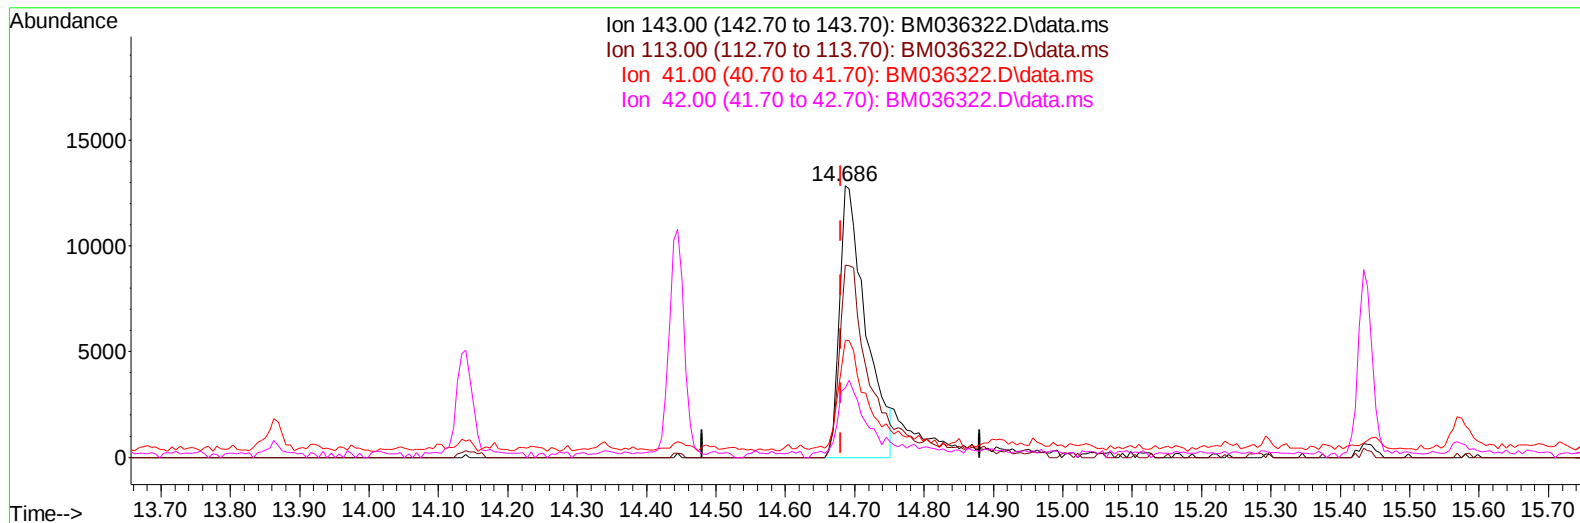

TIC: BM036322.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.006) 4.92 ng/u1

response 33645

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	70.84
41.00	41.00	42.94
42.00	29.30	25.54




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036322.D
Acq On : 17 Aug 2022 18:37
Operator : CG/JU
Sample : N4176-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P6

Manual IntegrationsAPPROVED

Quant Time: Aug 18 02:19:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 16 15:00:33 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/19/2022

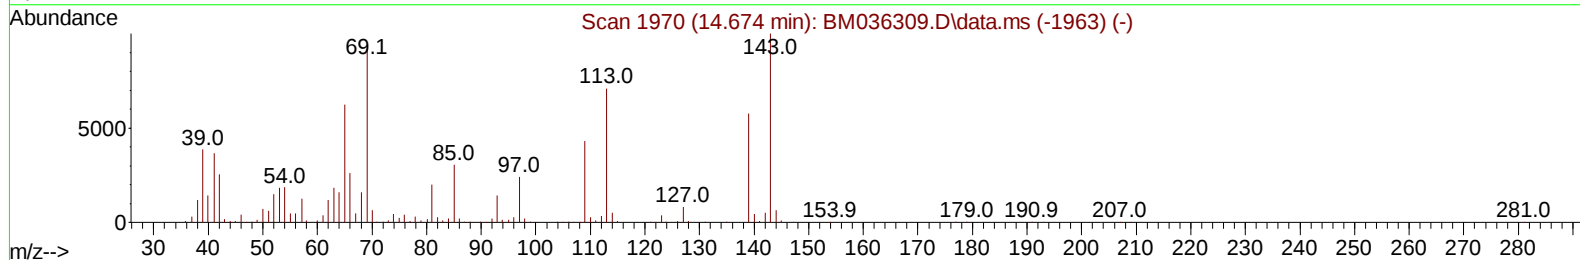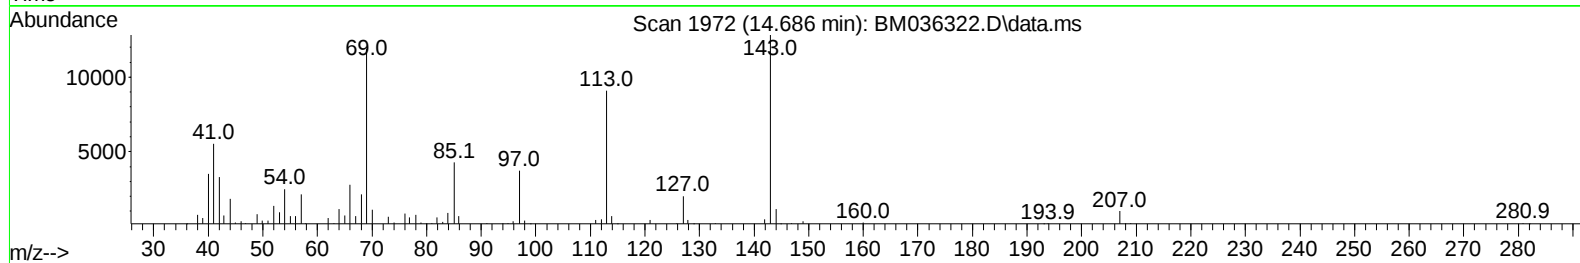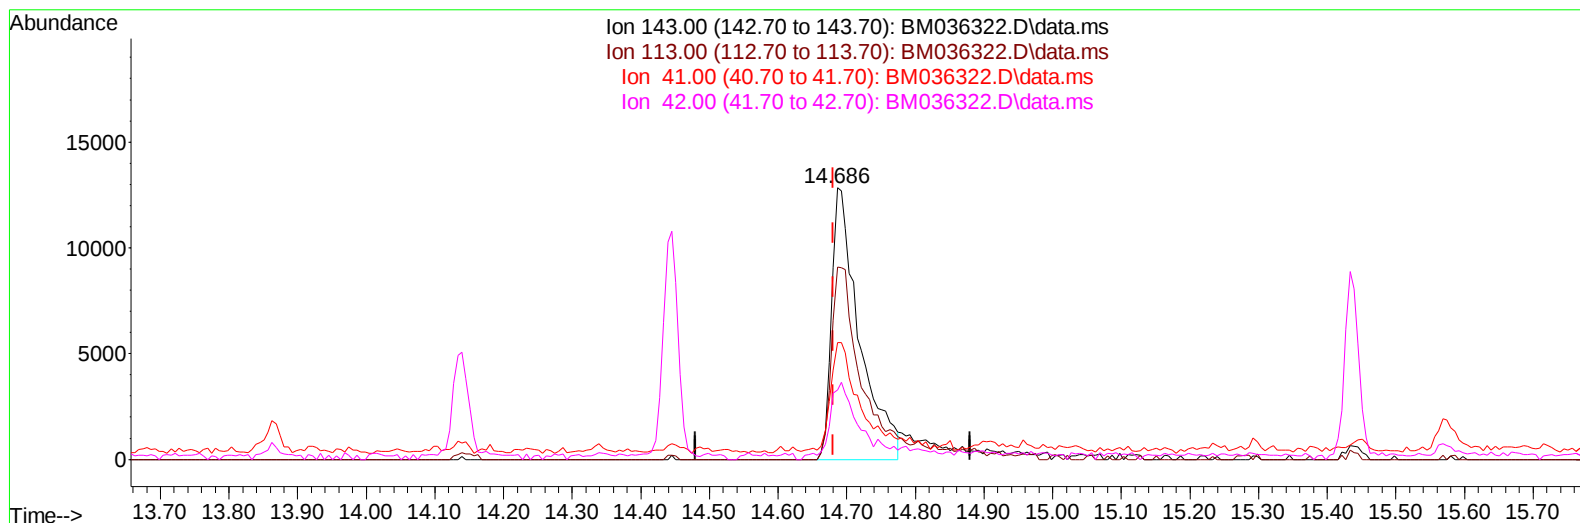

TIC: BM036322.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.686min (+ 0.006) 5.28 ng/ul m

response 36090

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	70.84
41.00	41.00	42.94
42.00	29.30	25.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036322.D
 Acq On : 17 Aug 2022 18:37
 Operator : CG/JU
 Sample : N4176-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7P6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
 Supervised By :Sohil Jodhani 08/19/2022

Quant Time: Aug 18 02:19:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 16 15:00:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.798	152	238417	20.000	ng/ul	0.00
20) Naphthalene-d8	10.598	136	1020588	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	570314	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	1059990	20.000	ng/ul	0.00
79) Chrysene-d12	21.368	240	949456	20.000	ng/ul	0.00
88) Perylene-d12	23.703	264	1003867	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	14569	2.329	ng/uL	0.00
4) Pyridine-d5	3.646	84	99898	5.791	ng/ul	0.00
7) Phenol-d5	6.981	99	270638	13.299	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	182005	14.208	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	232577	14.545	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	216487	14.247	ng/ul	0.00
21) Nitrobenzene-d5	8.969	128	111899	14.461	ng/ul	0.00
24) 2-Nitrophenol-d4	9.692	143	113176	14.419	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	196315	13.998	ng/ul	0.00
31) 4-Chloroaniline-d4	10.751	131	286371	13.172	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	587386	16.280	ng/ul	0.00
49) Acenaphthylene-d8	14.139	160	665954	14.799	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	36090m	5.279	ng/ul	0.00
60) Fluorene-d10	15.439	176	517119	15.861	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.574	200	30718	5.637	ng/ul	0.00
73) Anthracene-d10	17.286	188	827379	17.554	ng/ul	0.00
81) Pyrene-d10	19.580	212	955392	19.398	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.550	264	933299	18.962	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036322.D
Acq On : 17 Aug 2022 18:37
Operator : CG/JU
Sample : N4176-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/18/2022
Supervised By :Sohil Jodhani 08/19/2022

Quant Time: Aug 18 02:19:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 16 15:00:33 2022
Response via : Initial Calibration

