

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036310.D
 Acq On : 17 Aug 2022 11:15
 Operator : CG/JU
 Sample : PB147024BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	28	rVB	67899	88048	1.68%	0.153%
2	3.634	90	93	114	rBV	811953	1196778	22.87%	2.079%
3	3.957	144	148	153	rVB	16876	20904	0.40%	0.036%
4	6.981	655	662	677	rBV	941849	1531467	29.27%	2.660%
5	7.140	682	689	699	rVV	841450	1283489	24.53%	2.230%
6	7.334	715	722	735	rBV	988809	1564356	29.89%	2.718%
7	7.798	793	801	812	rBV	864724	1322151	25.27%	2.297%
8	8.522	917	924	946	rBV	1121958	1928487	36.85%	3.350%
9	8.969	990	1000	1011	rBV	946638	1541234	29.45%	2.677%
10	9.692	1114	1123	1137	rBV	728098	1260115	24.08%	2.189%
11	10.234	1207	1215	1237	rBV	1005773	1886324	36.05%	3.277%
12	10.598	1269	1277	1286	rBV	1217037	2000851	38.24%	3.476%
13	10.751	1295	1303	1322	rBV	1099743	2047943	39.14%	3.558%
14	12.210	1544	1551	1559	rBV2	14007	31069	0.59%	0.054%
15	13.863	1826	1832	1848	rBV	2234397	2982050	56.99%	5.180%
16	14.139	1871	1879	1895	rBV	2478936	3550321	67.85%	6.168%
17	14.445	1924	1931	1941	rBV	1793188	2565874	49.03%	4.457%
18	14.674	1964	1970	1991	rBV	599270	1306501	24.97%	2.270%
19	15.433	2093	2099	2112	rBV	3142950	4432108	84.70%	7.699%
20	15.563	2116	2121	2136	rBV	765704	1213365	23.19%	2.108%
21	15.674	2136	2140	2149	rVB2	34672	62406	1.19%	0.108%
22	16.215	2228	2232	2238	rVB5	8908	14236	0.27%	0.025%
23	16.863	2340	2342	2346	rBV4	5654	6285	0.12%	0.011%
24	16.974	2354	2361	2364	rBV6	5615	10993	0.21%	0.019%
25	17.186	2391	2397	2407	rBV	2036779	2770453	52.94%	4.813%
26	17.286	2407	2414	2432	rVB	3499539	4801605	91.76%	8.341%
27	19.145	2726	2730	2735	rBV	38543	52334	1.00%	0.091%
28	19.215	2738	2742	2749	rBV	35754	60056	1.15%	0.104%
29	19.580	2798	2804	2814	rBV	4038988	5232926	100.00%	9.090%
30	20.580	2971	2974	2979	rBV	70645	79431	1.52%	0.138%
31	21.368	3104	3108	3117	rBV	2074882	2750008	52.55%	4.777%
32	23.550	3473	3479	3492	rVB2	2664506	5220761	99.77%	9.069%
33	23.703	3499	3505	3515	rVB2	1386784	2749907	52.55%	4.777%




Sum of corrected areas: 57564836

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036310.D
Acq On : 17 Aug 2022 11:15
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

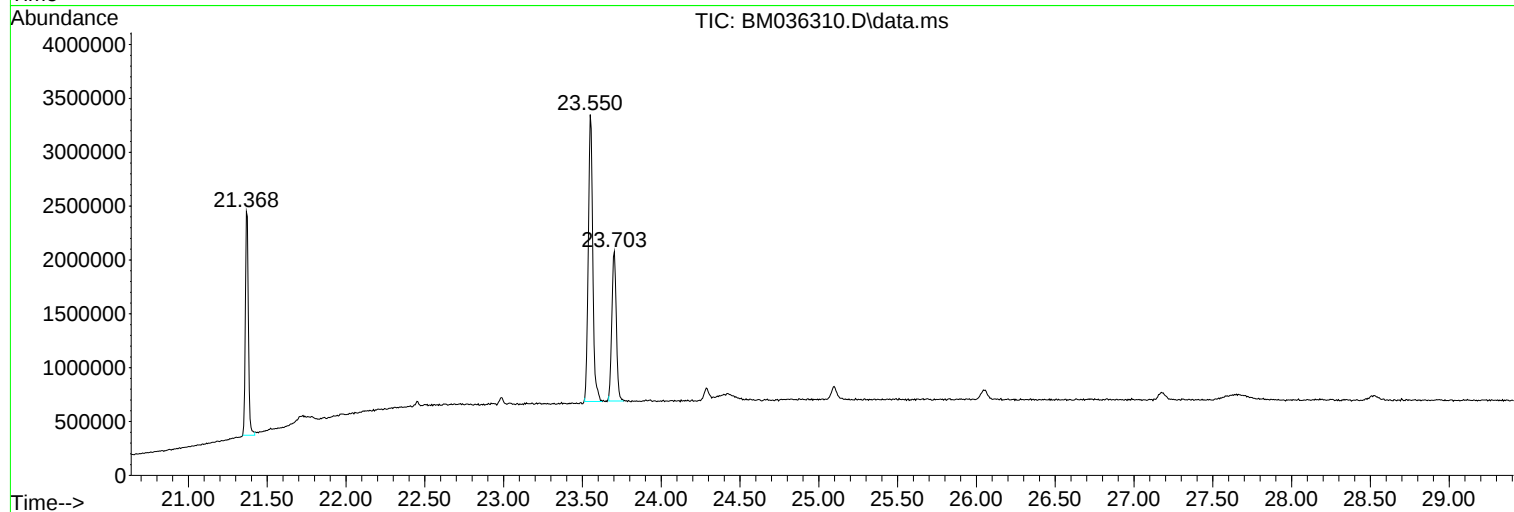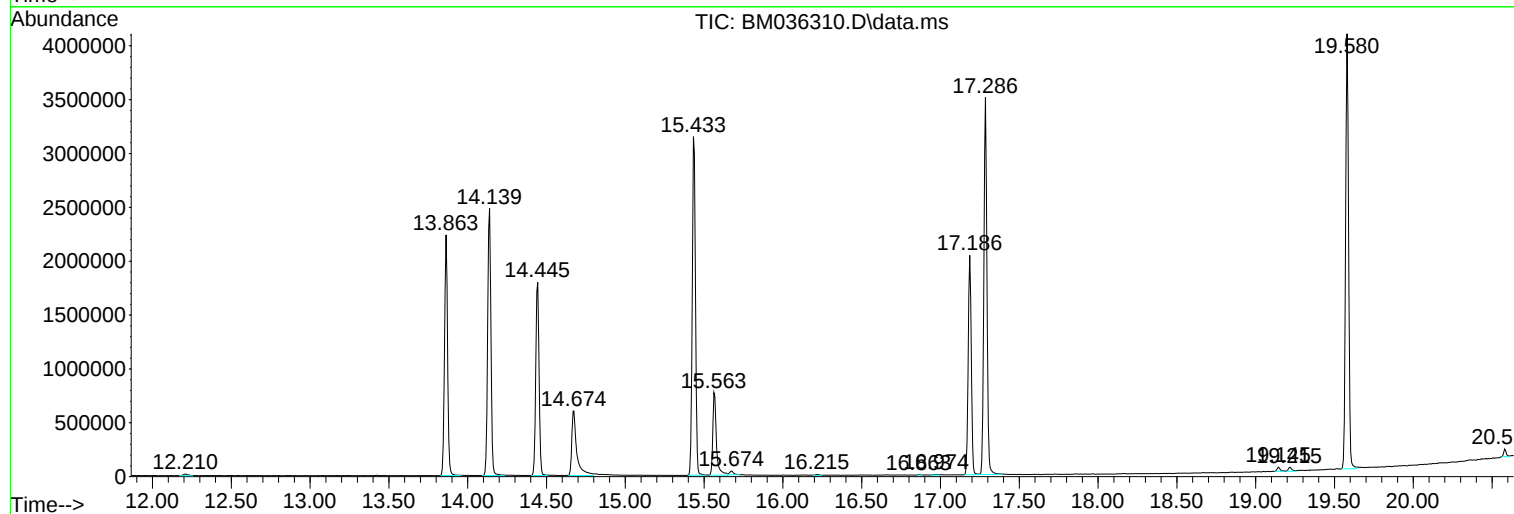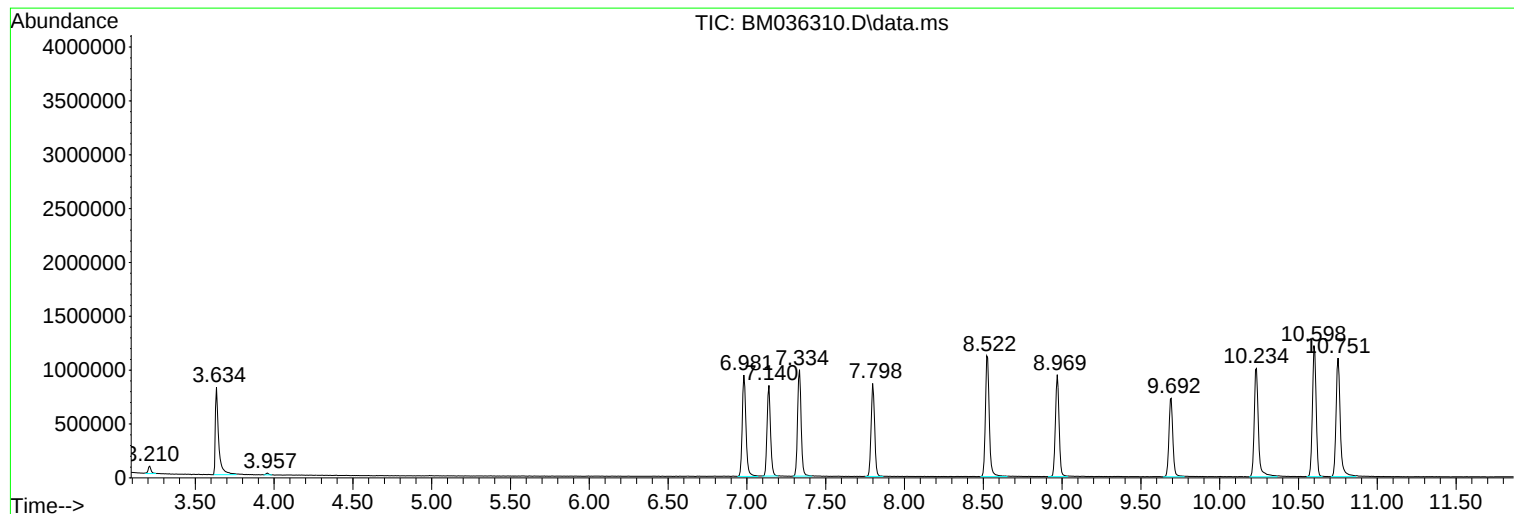

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036310.D
Acq On : 17 Aug 2022 11:15
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036310.D
Acq On : 17 Aug 2022 11:15
Operator : CG/JU
Sample : PB147024BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc