

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036313.D
 Acq On : 17 Aug 2022 13:05
 Operator : CG/JU
 Sample : N4192-01DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.957	144	148	152	rVB	15930	23126	0.53%	0.076%
2	4.193	184	188	197	rVB	70041	93890	2.14%	0.310%
3	4.610	253	259	264	rBV	51216	73527	1.67%	0.243%
4	5.151	345	351	357	rBV3	16533	23637	0.54%	0.078%
5	6.992	658	664	673	rBV2	24937	54292	1.24%	0.179%
6	7.139	682	689	703	rBV	128682	223626	5.09%	0.738%
7	7.334	717	722	733	rBV	108055	194005	4.42%	0.640%
8	7.798	794	801	811	rBV	795102	1273799	29.02%	4.205%
9	8.533	920	926	935	rVV	76788	146538	3.34%	0.484%
10	8.975	994	1001	1009	rBV	138720	249179	5.68%	0.823%
11	9.269	1043	1051	1055	rBV9	9500	21229	0.48%	0.070%
12	9.692	1117	1123	1135	rBV	88816	173971	3.96%	0.574%
13	10.016	1171	1178	1187	rBV	15983	43245	0.99%	0.143%
14	10.098	1187	1192	1196	rBV7	11432	19935	0.45%	0.066%
15	10.239	1210	1216	1231	rVV	113170	255901	5.83%	0.845%
16	10.598	1270	1277	1284	rBV	1108211	1888270	43.01%	6.234%
17	10.780	1297	1308	1316	rVV8	19626	56786	1.29%	0.187%
18	11.198	1373	1379	1388	rVV	50014	93213	2.12%	0.308%
19	11.645	1446	1455	1459	rBV3	20702	42992	0.98%	0.142%
20	11.722	1461	1468	1472	rBV	40443	72798	1.66%	0.240%
21	11.921	1495	1502	1508	rBV9	8327	23199	0.53%	0.077%
22	12.021	1515	1519	1523	rVB	18103	25187	0.57%	0.083%
23	12.157	1533	1542	1548	rBV6	40429	87326	1.99%	0.288%
24	12.327	1566	1571	1576	rBV4	14680	26465	0.60%	0.087%
25	12.439	1585	1590	1597	rBV5	37623	94207	2.15%	0.311%
26	12.621	1612	1621	1625	rBV5	34970	71545	1.63%	0.236%
27	12.657	1625	1627	1630	rVV4	17213	24545	0.56%	0.081%
28	12.698	1630	1634	1641	rVB3	18282	36040	0.82%	0.119%
29	12.792	1647	1650	1654	rBV3	16968	22958	0.52%	0.076%
30	12.874	1659	1664	1671	rVB5	17101	32310	0.74%	0.107%
31	12.968	1675	1680	1684	rVB2	23481	36029	0.82%	0.119%
32	13.251	1721	1728	1729	rBV4	17774	31828	0.73%	0.105%
33	13.498	1765	1770	1779	rVB2	110647	176221	4.01%	0.582%
34	13.592	1781	1786	1788	rBV3	23112	35990	0.82%	0.119%
35	13.633	1789	1793	1800	rVB3	32991	68234	1.55%	0.225%
36	13.780	1812	1818	1819	rBV6	26288	41229	0.94%	0.136%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036313.D
 Acq On : 17 Aug 2022 13:05
 Operator : CG/JU
 Sample : N4192-01DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	13.863	1825	1832	1838	rBV	358018	502560	11.45%	1.659%
38	13.998	1850	1855	1858	rBV2	65718	95235	2.17%	0.314%
39	14.033	1858	1861	1869	rVB	53158	84257	1.92%	0.278%
40	14.139	1873	1879	1882	rBV	385760	600411	13.68%	1.982%
41	14.168	1882	1884	1894	rVB2	132141	195751	4.46%	0.646%
42	14.251	1894	1898	1905	rBV6	25130	45530	1.04%	0.150%
43	14.445	1924	1931	1936	rBV	1640059	2380377	54.22%	7.858%
44	14.510	1936	1942	1949	rVV	3043232	4389915	100.00%	14.493%
45	14.586	1950	1955	1961	rVB4	20742	38915	0.89%	0.128%
46	14.751	1977	1983	1989	rVB	61830	98325	2.24%	0.325%
47	14.839	1995	1998	2006	rVB2	28500	44816	1.02%	0.148%
48	15.062	2030	2036	2042	rBV5	35681	74836	1.70%	0.247%
49	15.315	2075	2079	2087	rVB	40854	66452	1.51%	0.219%
50	15.433	2090	2099	2104	rBV	555825	797961	18.18%	2.634%
51	15.492	2104	2109	2117	rVB	878895	1296421	29.53%	4.280%
52	15.568	2117	2122	2127	rBV2	97770	189714	4.32%	0.626%
53	15.615	2127	2130	2133	rVV2	61095	69793	1.59%	0.230%
54	15.698	2140	2144	2148	rBV3	42838	60018	1.37%	0.198%
55	15.739	2148	2151	2157	rVB3	22650	36528	0.83%	0.121%
56	15.804	2157	2162	2169	rVB5	29304	60209	1.37%	0.199%
57	15.886	2172	2176	2179	rBV5	22267	40414	0.92%	0.133%
58	15.933	2179	2184	2193	rVV2	109410	228782	5.21%	0.755%
59	16.168	2218	2224	2233	rVB2	103087	198485	4.52%	0.655%
60	16.286	2239	2244	2251	rVB	66227	99259	2.26%	0.328%
61	16.362	2252	2257	2263	rBV3	49045	89359	2.04%	0.295%
62	16.451	2268	2272	2273	rVV3	19581	28403	0.65%	0.094%
63	16.492	2277	2279	2284	rVB2	45144	53052	1.21%	0.175%
64	16.539	2284	2287	2292	rBV3	14440	23041	0.52%	0.076%
65	16.639	2301	2304	2309	rVB2	27100	38121	0.87%	0.126%
66	16.845	2331	2339	2347	rVB9	26498	75306	1.72%	0.249%
67	16.921	2347	2352	2354	rBV5	19289	34113	0.78%	0.113%
68	16.974	2357	2361	2363	rBV	33356	46264	1.05%	0.153%
69	17.004	2363	2366	2377	rVB2	91230	151498	3.45%	0.500%
70	17.115	2378	2385	2388	rBV5	25916	52784	1.20%	0.174%
71	17.186	2388	2397	2402	rBV	1840231	2526204	57.55%	8.340%
72	17.227	2402	2404	2408	rVB	50847	57108	1.30%	0.189%
73	17.286	2408	2414	2418	rBV	555670	794934	18.11%	2.624%
74	17.386	2428	2431	2437	rVB4	27122	46357	1.06%	0.153%
75	17.562	2457	2461	2472	rVB2	62325	131412	2.99%	0.434%
76	17.856	2507	2511	2516	rVB2	40561	58792	1.34%	0.194%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036313.D
 Acq On : 17 Aug 2022 13:05
 Operator : CG/JU
 Sample : N4192-01DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

77	17.903	2516	2519	2523	rBV3	19000	24086	0.55%	0.080%
78	17.945	2524	2526	2534	rVV7	18571	32171	0.73%	0.106%
79	18.033	2536	2541	2545	rBV	64413	92849	2.12%	0.307%
80	18.092	2548	2551	2552	rVV3	38935	48032	1.09%	0.159%
81	18.115	2552	2555	2559	rVV2	68649	94216	2.15%	0.311%
82	18.156	2560	2562	2564	rVV2	17188	20627	0.47%	0.068%
83	18.192	2564	2568	2574	rVB2	87404	135235	3.08%	0.446%
84	18.262	2575	2580	2585	rBV	157977	244037	5.56%	0.806%
85	18.350	2591	2595	2601	rBV2	38771	89270	2.03%	0.295%
86	18.456	2610	2613	2618	rVB6	18431	25224	0.57%	0.083%
87	18.509	2618	2622	2628	rBV3	41786	68387	1.56%	0.226%
88	18.568	2629	2632	2636	rVB3	29169	35356	0.81%	0.117%
89	18.609	2636	2639	2644	rBV3	27101	47163	1.07%	0.156%
90	18.956	2695	2698	2700	rBV4	19634	27858	0.63%	0.092%
91	19.039	2708	2712	2715	rVB2	57363	63541	1.45%	0.210%
92	19.168	2732	2734	2737	rBV2	17484	20233	0.46%	0.067%
93	19.245	2743	2747	2756	rVB	362619	496460	11.31%	1.639%
94	19.580	2799	2804	2807	rBV	711658	933496	21.26%	3.082%
95	19.997	2871	2875	2883	rBV	71387	112484	2.56%	0.371%
96	20.580	2971	2974	2978	rBV	88289	99658	2.27%	0.329%
97	20.709	2993	2996	3005	rVB	78139	118948	2.71%	0.393%
98	21.368	3104	3108	3114	rBV	2046507	2525265	57.52%	8.337%
99	23.550	3474	3479	3483	rBV2	380365	687162	15.65%	2.269%
100	23.703	3499	3505	3514	rVB2	1289802	2490033	56.72%	8.220%




Sum of corrected areas: 30290775

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036313.D
Acq On : 17 Aug 2022 13:05
Operator : CG/JU
Sample : N4192-01DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

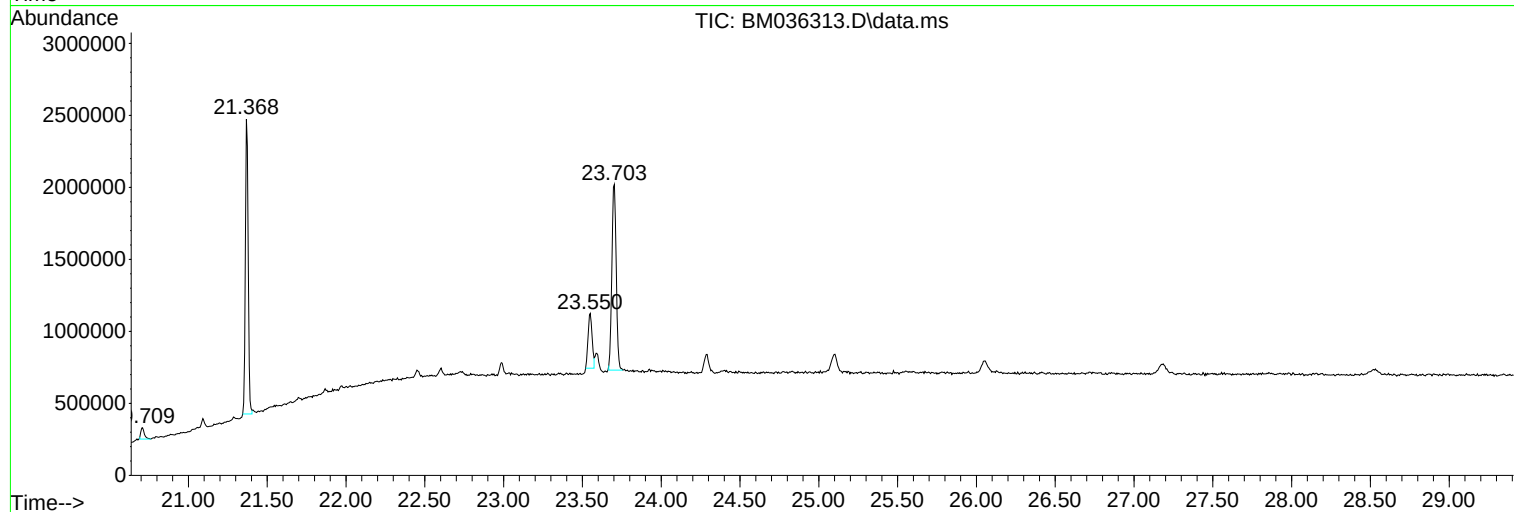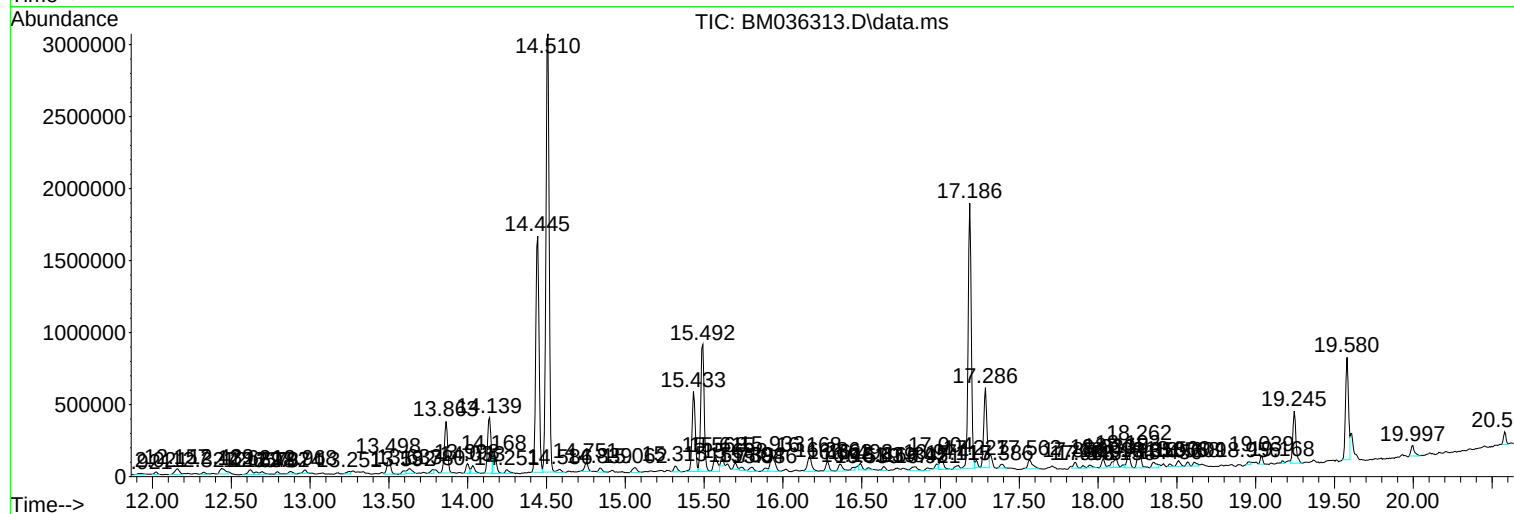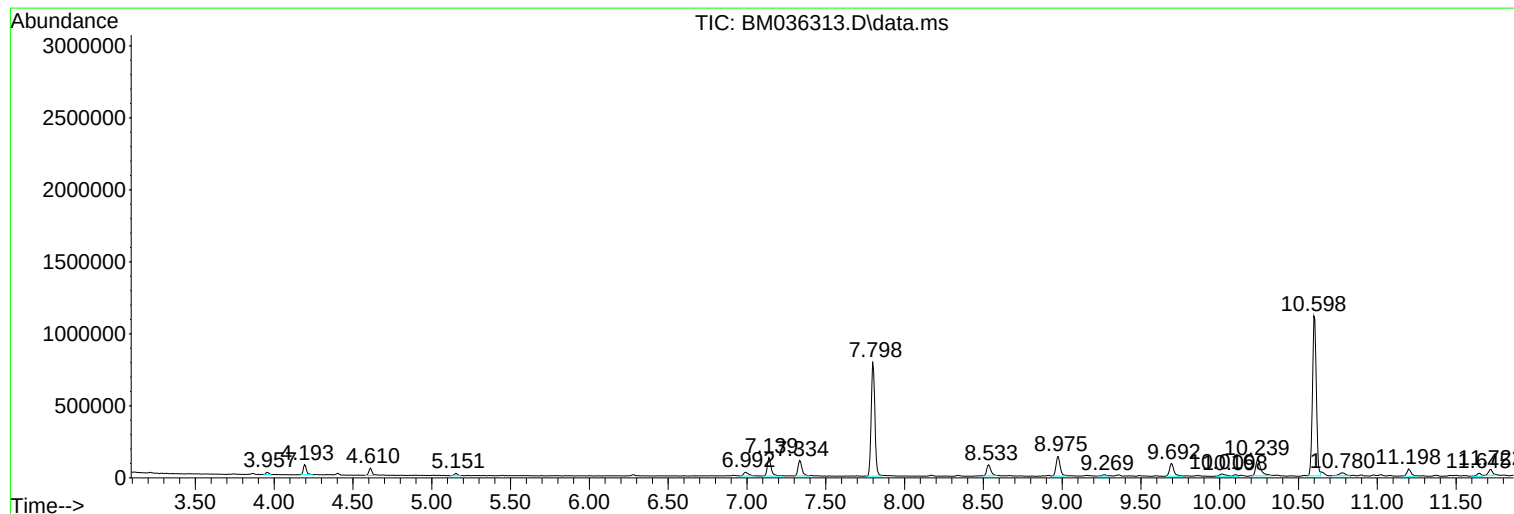

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036313.D
Acq On : 17 Aug 2022 13:05
Operator : CG/JU
Sample : N4192-01DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036313.D
Acq On : 17 Aug 2022 13:05
Operator : CG/JU
Sample : N4192-01DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------