

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036318.D
 Acq On : 17 Aug 2022 16:09
 Operator : CG/JU
 Sample : N4173-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rVB	39733	46071	1.27%	0.117%
2	3.863	126	132	138	rBV	36207	55407	1.53%	0.141%
3	3.957	145	148	157	rVB	19060	28334	0.78%	0.072%
4	4.128	174	177	180	rVB4	4101	5396	0.15%	0.014%
5	4.299	202	206	211	rBV	22079	28306	0.78%	0.072%
6	4.404	220	224	230	rVB	58352	72994	2.01%	0.185%
7	4.663	266	268	272	rBV5	2610	4414	0.12%	0.011%
8	4.757	281	284	288	rBV6	2830	4560	0.13%	0.012%
9	4.887	303	306	308	rBV	18024	24515	0.68%	0.062%
10	5.010	325	327	333	rVB6	6301	7895	0.22%	0.020%
11	5.522	406	414	420	rBV2	10933	20155	0.56%	0.051%
12	6.922	646	652	656	rBV	28711	42099	1.16%	0.107%
13	6.981	656	662	676	rVV	512998	869849	23.99%	2.208%
14	7.140	683	689	701	rBV	507471	786744	21.70%	1.997%
15	7.234	701	705	712	rVV2	7598	12712	0.35%	0.032%
16	7.334	715	722	731	rBV	566121	906696	25.01%	2.302%
17	7.410	733	735	745	rVB6	11243	18680	0.52%	0.047%
18	7.798	794	801	810	rBV	889887	1381158	38.09%	3.507%
19	7.875	811	814	820	rVB3	8349	13568	0.37%	0.034%
20	8.528	918	925	939	rBV	600801	1033988	28.52%	2.625%
21	8.639	939	944	951	rVB3	16576	31721	0.87%	0.081%
22	8.969	993	1000	1013	rBV	559824	937654	25.86%	2.381%
23	9.139	1023	1029	1032	rBV6	4936	8650	0.24%	0.022%
24	9.363	1060	1067	1073	rVB	34506	54553	1.50%	0.139%
25	9.692	1115	1123	1137	rBV	388023	672323	18.54%	1.707%
26	10.234	1208	1215	1238	rBV	518668	1063970	29.35%	2.701%
27	10.598	1270	1277	1291	rBV	1220818	2079672	57.36%	5.280%
28	10.763	1299	1305	1322	rBV	54507	139880	3.86%	0.355%
29	11.857	1485	1491	1497	rVB2	21248	33034	0.91%	0.084%
30	12.204	1543	1550	1556	rBV5	9258	17723	0.49%	0.045%
31	12.804	1647	1652	1657	rBV8	4585	9810	0.27%	0.025%
32	13.057	1690	1695	1702	rVB6	4832	8618	0.24%	0.022%
33	13.269	1727	1731	1736	rBV6	3130	4410	0.12%	0.011%
34	13.345	1738	1744	1749	rBV5	8828	15729	0.43%	0.040%
35	13.422	1752	1757	1760	rBV5	3479	5191	0.14%	0.013%
36	13.863	1824	1832	1845	rBV	1075065	1534708	42.33%	3.897%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036318.D
 Acq On : 17 Aug 2022 16:09
 Operator : CG/JU
 Sample : N4173-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	14.139	1871	1879	1891	rBV	1387032	2026590	55.90%	5.145%
38	14.233	1893	1895	1900	rVB6	3379	5214	0.14%	0.013%
39	14.345	1906	1914	1918	rVB8	3763	8619	0.24%	0.022%
40	14.445	1924	1931	1946	rBV	1825304	2587523	71.37%	6.570%
41	14.616	1957	1960	1965	rBV6	2449	3939	0.11%	0.010%
42	14.680	1965	1971	1992	rBV	221323	568838	15.69%	1.444%
43	14.880	2002	2005	2009	rVB5	5590	6828	0.19%	0.017%
44	15.239	2060	2066	2068	rBV5	6431	9496	0.26%	0.024%
45	15.274	2068	2072	2079	rVB3	7935	16998	0.47%	0.043%
46	15.439	2090	2100	2111	rBV	1753015	2566702	70.79%	6.517%
47	15.568	2116	2122	2136	rVV	312824	538978	14.87%	1.368%
48	15.674	2137	2140	2148	rVV3	15669	31756	0.88%	0.081%
49	16.010	2192	2197	2201	rBV8	3282	5555	0.15%	0.014%
50	16.163	2217	2223	2224	rBV6	5973	9983	0.28%	0.025%
51	16.221	2229	2233	2238	rVB8	2610	4154	0.11%	0.011%
52	16.327	2247	2251	2253	rBV5	4136	4488	0.12%	0.011%
53	16.657	2302	2307	2312	rVB2	14939	23065	0.64%	0.059%
54	16.957	2352	2358	2364	rBV10	11401	29537	0.81%	0.075%
55	17.110	2378	2384	2389	rBV9	6816	12039	0.33%	0.031%
56	17.186	2391	2397	2408	rBV	2055509	2751972	75.90%	6.987%
57	17.286	2408	2414	2428	rVV	2001881	2740183	75.58%	6.957%
58	17.474	2444	2446	2451	rVB5	5637	7593	0.21%	0.019%
59	17.680	2478	2481	2483	rBV4	5981	6106	0.17%	0.016%
60	17.721	2485	2488	2494	rVB3	13578	18621	0.51%	0.047%
61	17.862	2507	2512	2517	rBV3	38602	55562	1.53%	0.141%
62	18.086	2546	2550	2560	rBV3	62347	117315	3.24%	0.298%
63	18.157	2560	2562	2568	rVB	11747	18423	0.51%	0.047%
64	18.374	2597	2599	2603	rBV5	6319	7887	0.22%	0.020%
65	18.668	2647	2649	2653	rVB2	15613	16706	0.46%	0.042%
66	19.145	2727	2730	2737	rBV5	29957	53644	1.48%	0.136%
67	19.221	2739	2743	2745	rBV2	25417	36239	1.00%	0.092%
68	19.374	2766	2769	2776	rBV8	21420	43255	1.19%	0.110%
69	19.580	2798	2804	2811	rBV	2571651	3431336	94.64%	8.712%
70	20.580	2971	2974	2977	rBV	94122	95045	2.62%	0.241%
71	21.086	3057	3060	3069	rVB2	267848	408422	11.26%	1.037%
72	21.368	3104	3108	3118	rBV	2108759	2744482	75.70%	6.968%
73	23.550	3473	3479	3493	rVB2	1754690	3625700	100.00%	9.205%
74	23.703	3499	3505	3516	rVB2	1401860	2766577	76.30%	7.024%

Sum of corrected areas: 39386557

Instrument :

BNA_M

ClientSampleId :




EX7P1

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036318.D
Acq On : 17 Aug 2022 16:09
Operator : CG/JU
Sample : N4173-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

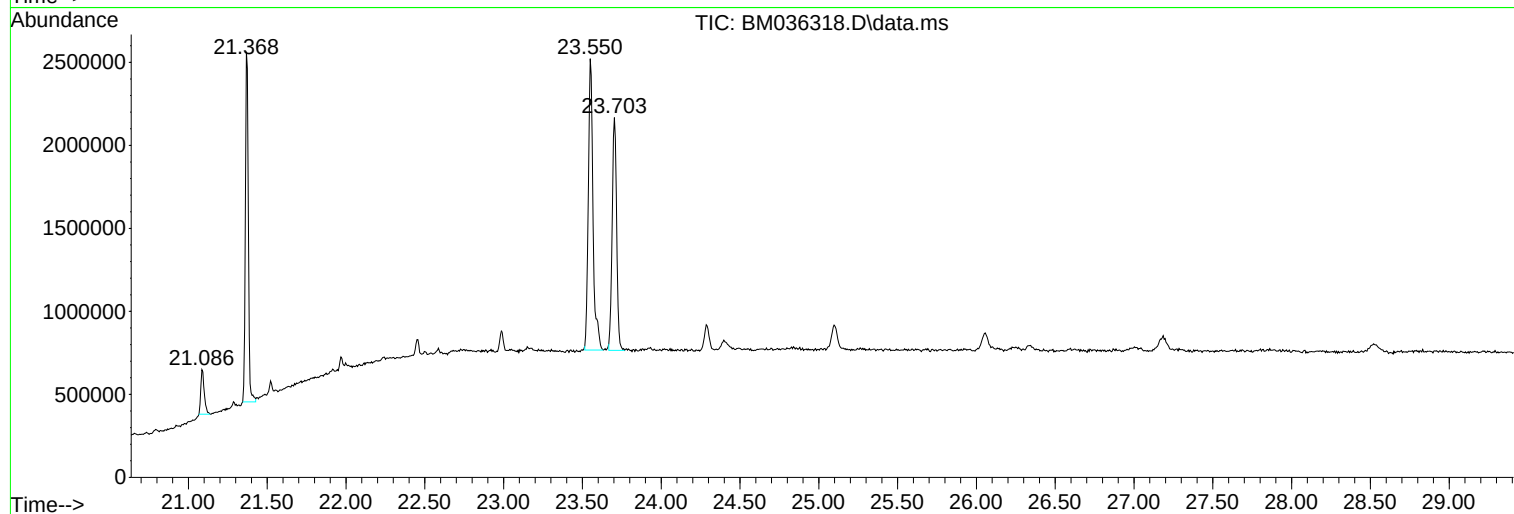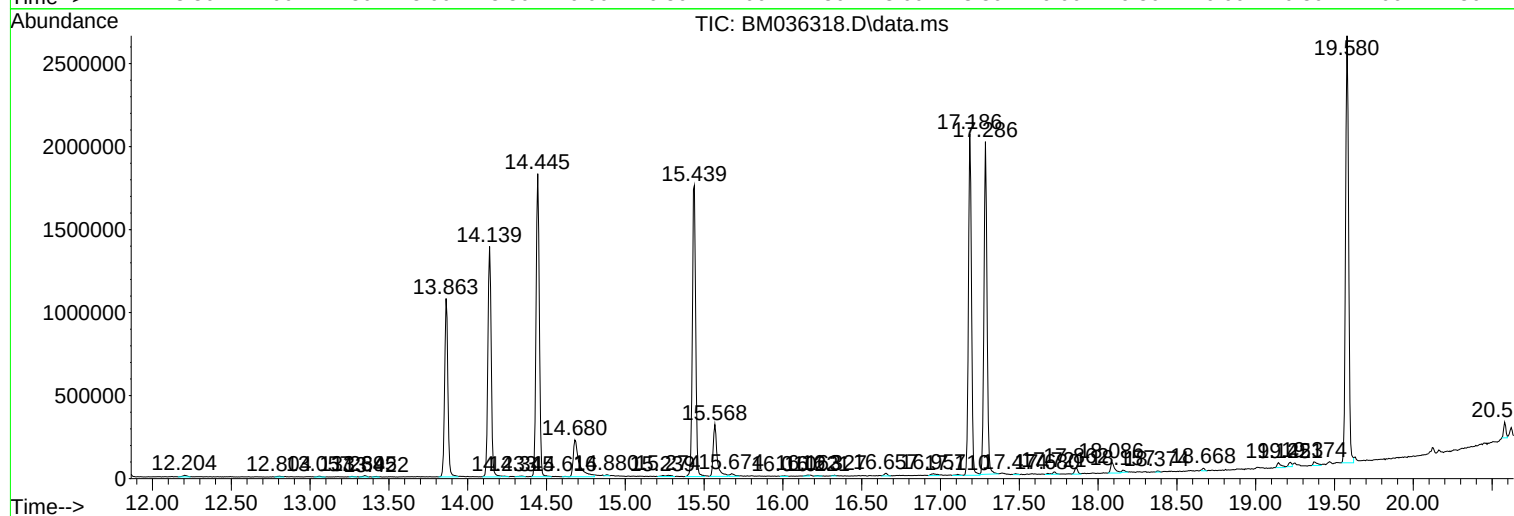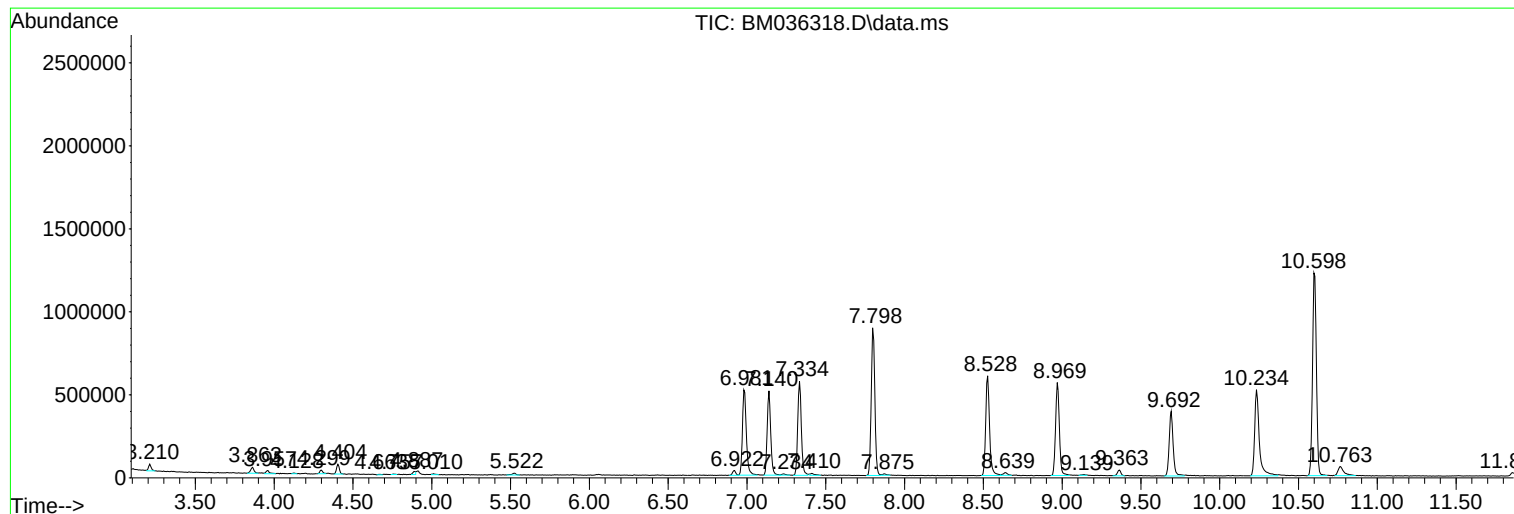

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036318.D
Acq On : 17 Aug 2022 16:09
Operator : CG/JU
Sample : N4173-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.086	2.98 ng/ul	408422	Chrysene-d12	21.368

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	94
2			Tricosyl trifluoroacetate	436	C25H47F3O2	1000351-75-1	91
3			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	91
4			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	91
5			Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	90

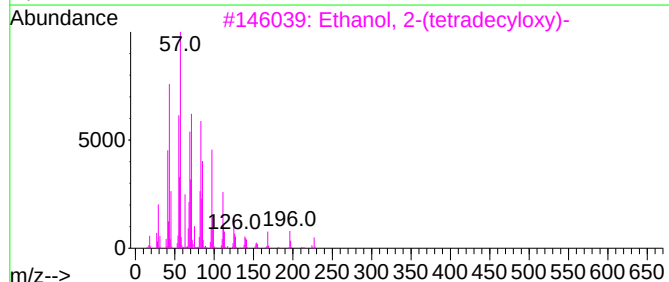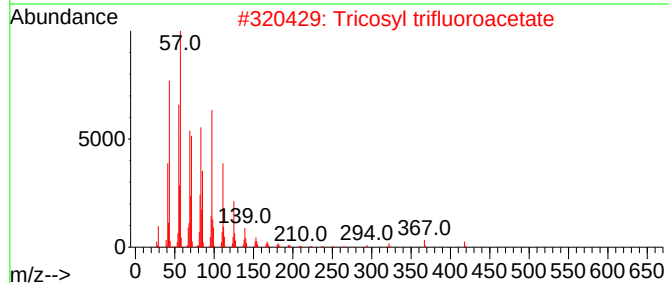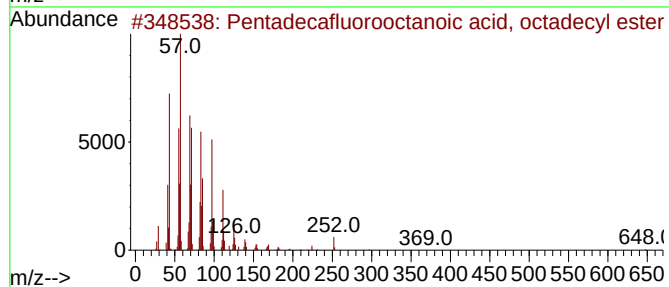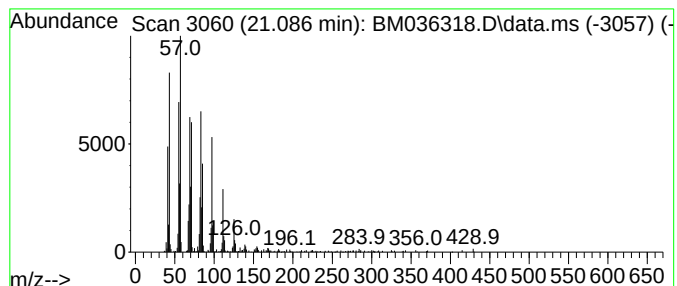

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036318.D
Acq On : 17 Aug 2022 16:09
Operator : CG/JU
Sample : N4173-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7P1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.086	3.0	ng/u1	408422	5	21.368	2744480	20.0