

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036321.D
 Acq On : 17 Aug 2022 18:00
 Operator : CG/JU
 Sample : N4173-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	28	rVB	40303	52340	1.33%	0.124%
2	3.746	109	112	115	rVB3	11706	14333	0.37%	0.034%
3	3.863	128	132	139	rVB	35186	50384	1.28%	0.119%
4	3.957	144	148	155	rVB	18606	24394	0.62%	0.058%
5	4.198	185	189	192	rBV5	8640	11971	0.31%	0.028%
6	4.404	220	224	233	rVB	62048	84092	2.14%	0.199%
7	4.522	242	244	250	rVB7	5298	7435	0.19%	0.018%
8	4.893	302	307	308	rBV	18289	24416	0.62%	0.058%
9	5.010	323	327	331	rVB6	8798	12697	0.32%	0.030%
10	5.222	359	363	366	rBV6	4210	4354	0.11%	0.010%
11	5.292	372	375	380	rVB	8561	10825	0.28%	0.026%
12	5.428	392	398	405	rBV	47200	104350	2.66%	0.247%
13	5.798	456	461	465	rVB3	10729	14710	0.37%	0.035%
14	6.057	498	505	512	rBV9	5215	11355	0.29%	0.027%
15	6.275	539	542	546	rVB5	4403	6595	0.17%	0.016%
16	6.881	641	645	647	rBV5	4340	5668	0.14%	0.013%
17	6.922	647	652	656	rVV	31128	47537	1.21%	0.113%
18	6.981	656	662	675	rVV	588779	980062	24.98%	2.320%
19	7.139	682	689	700	rBV	548701	841455	21.45%	1.992%
20	7.228	700	704	708	rVB	9035	13894	0.35%	0.033%
21	7.334	716	722	732	rBV	637697	1007648	25.68%	2.385%
22	7.416	732	736	738	rVV3	11587	18240	0.46%	0.043%
23	7.439	738	740	747	rVB3	12454	15752	0.40%	0.037%
24	7.798	794	801	810	rBV	900411	1421611	36.23%	3.365%
25	7.869	810	813	818	rVB4	8747	12461	0.32%	0.029%
26	8.281	879	883	887	rVB6	3199	4232	0.11%	0.010%
27	8.433	907	909	916	rVB7	4779	8201	0.21%	0.019%
28	8.528	918	925	938	rBV	695092	1177087	30.00%	2.786%
29	8.639	940	944	951	rVB	23257	40757	1.04%	0.096%
30	8.904	985	989	993	rBV6	3529	6504	0.17%	0.015%
31	8.969	993	1000	1013	rBV	598627	992833	25.30%	2.350%
32	9.145	1022	1030	1035	rVB7	6529	14240	0.36%	0.034%
33	9.363	1061	1067	1073	rVB	36940	54785	1.40%	0.130%
34	9.433	1073	1079	1083	rVB7	3996	6766	0.17%	0.016%
35	9.692	1115	1123	1136	rBV	461440	788172	20.09%	1.866%
36	10.069	1181	1187	1192	rVB8	3872	8627	0.22%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036321.D
 Acq On : 17 Aug 2022 18:00
 Operator : CG/JU
 Sample : N4173-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	10.233	1208	1215	1236	rBV	580144	1176218	29.98%	2.784%
38	10.604	1268	1278	1289	rBV	1260872	2142786	54.61%	5.072%
39	10.769	1301	1306	1319	rVB9	7831	24236	0.62%	0.057%
40	11.857	1486	1491	1499	rVB2	23111	37132	0.95%	0.088%
41	12.027	1515	1520	1526	rBV6	6682	12298	0.31%	0.029%
42	12.204	1546	1550	1556	rBV3	10217	18106	0.46%	0.043%
43	12.798	1645	1651	1655	rBV6	4358	8834	0.23%	0.021%
44	13.057	1691	1695	1700	rVB7	4694	7926	0.20%	0.019%
45	13.268	1725	1731	1737	rBV6	9029	13682	0.35%	0.032%
46	13.427	1753	1758	1759	rBV4	4711	7550	0.19%	0.018%
47	13.680	1796	1801	1806	rBV7	8025	12764	0.33%	0.030%
48	13.774	1810	1817	1821	rVB9	4634	9797	0.25%	0.023%
49	13.863	1821	1832	1847	rBV	1295281	1814596	46.25%	4.295%
50	14.139	1868	1879	1892	rBV	1462113	2149111	54.77%	5.087%
51	14.345	1908	1914	1918	rBV3	10053	15621	0.40%	0.037%
52	14.445	1924	1931	1938	rBV	1804931	2534778	64.60%	6.000%
53	14.680	1963	1971	1994	rBV	306017	731800	18.65%	1.732%
54	14.880	2002	2005	2015	rVB6	15416	30454	0.78%	0.072%
55	15.239	2064	2066	2068	rVB3	5276	5077	0.13%	0.012%
56	15.292	2073	2075	2079	rVB3	10831	12317	0.31%	0.029%
57	15.439	2090	2100	2114	rBV	1909356	2774595	70.71%	6.568%
58	15.568	2116	2122	2135	rVV	387760	623783	15.90%	1.477%
59	15.674	2137	2140	2149	rVB7	14310	36587	0.93%	0.087%
60	16.174	2216	2225	2230	rBV3	22870	54879	1.40%	0.130%
61	16.215	2230	2232	2236	rVB4	7442	7858	0.20%	0.019%
62	16.462	2269	2274	2275	rBV5	3588	5235	0.13%	0.012%
63	16.656	2303	2307	2311	rVB2	18092	24098	0.61%	0.057%
64	16.733	2316	2320	2327	rVB10	10861	22734	0.58%	0.054%
65	16.945	2353	2356	2360	rBV2	16317	24530	0.63%	0.058%
66	17.115	2380	2385	2391	rBV9	6763	13328	0.34%	0.032%
67	17.186	2391	2397	2403	rBV	1868884	2640113	67.29%	6.249%
68	17.286	2408	2414	2425	rVB	2068312	2948145	75.14%	6.979%
69	17.586	2462	2465	2466	rBV3	7733	8286	0.21%	0.020%
70	17.680	2479	2481	2485	rBV3	13176	14334	0.37%	0.034%
71	17.721	2485	2488	2493	rVB2	16416	19517	0.50%	0.046%
72	17.862	2508	2512	2519	rVB	72746	82344	2.10%	0.195%
73	18.092	2546	2551	2559	rBV2	92766	163420	4.16%	0.387%
74	18.380	2597	2600	2602	rBV4	13392	12884	0.33%	0.030%
75	19.145	2727	2730	2733	rBV3	28623	38973	0.99%	0.092%
76	19.215	2740	2742	2744	rBV	22600	23128	0.59%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036321.D
 Acq On : 17 Aug 2022 18:00
 Operator : CG/JU
 Sample : N4173-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7N9

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

77	19.250	2744	2748	2754	rVB	67014	94402	2.41%	0.223%
78	19.580	2799	2804	2817	rBV	2881900	3821319	97.39%	9.045%
79	20.580	2972	2974	2978	rBV	91645	92953	2.37%	0.220%
80	21.086	3057	3060	3071	rVB	512195	790139	20.14%	1.870%
81	21.374	3104	3109	3113	rBV	2017868	2625043	66.90%	6.214%
82	23.550	3473	3479	3493	rVB2	1939261	3923712	100.00%	9.288%
83	23.703	3499	3505	3518	rVB2	1392026	2693642	68.65%	6.376%




Sum of corrected areas: 42245847

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036321.D
Acq On : 17 Aug 2022 18:00
Operator : CG/JU
Sample : N4173-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

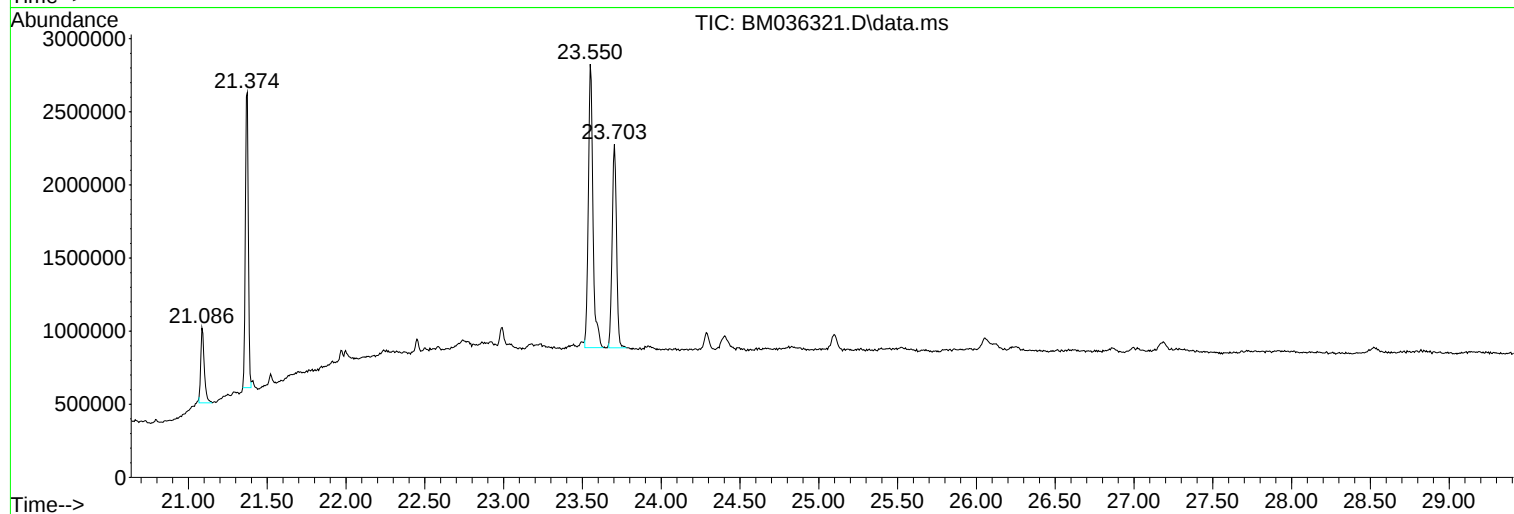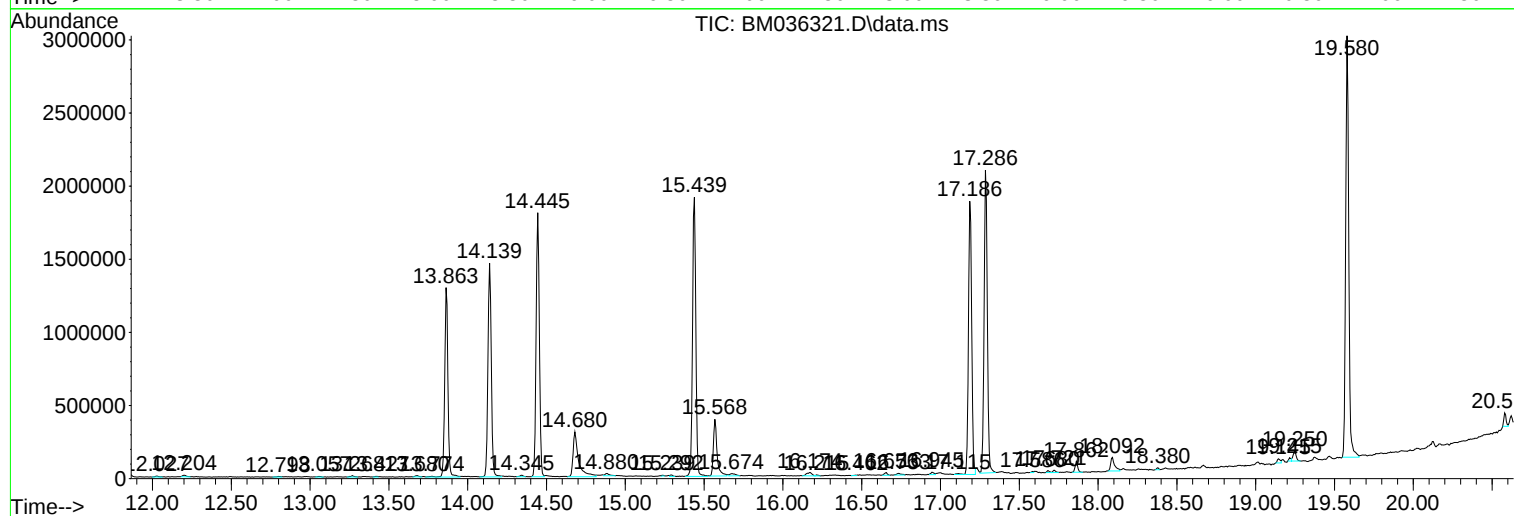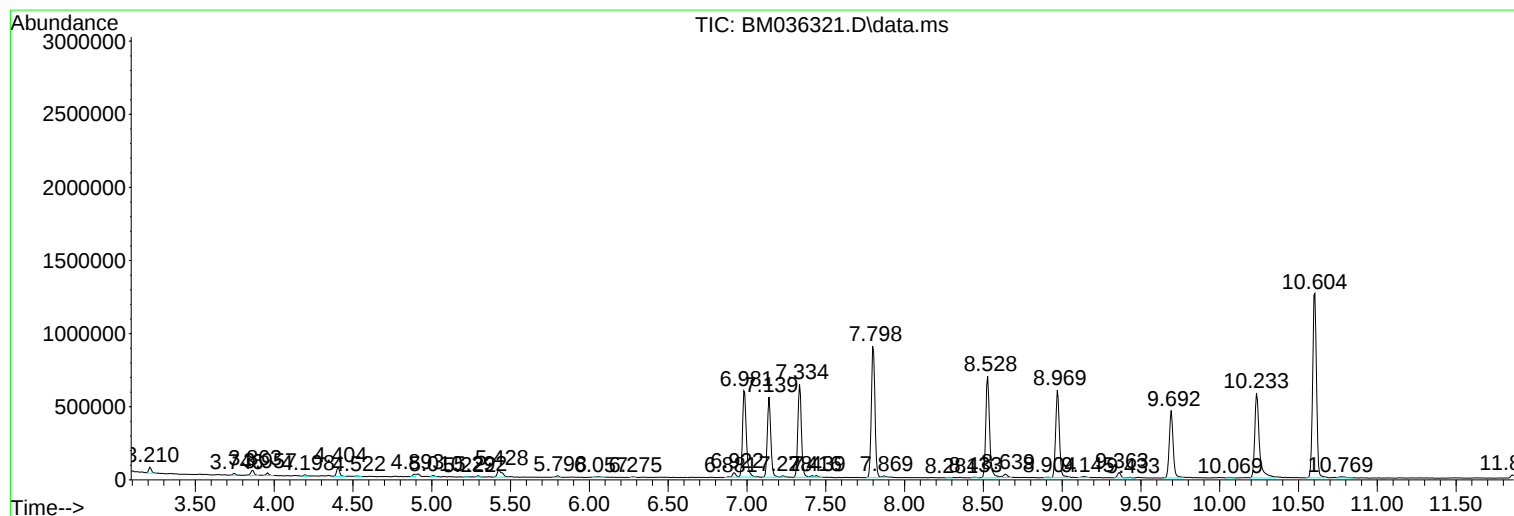

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036321.D
Acq On : 17 Aug 2022 18:00
Operator : CG/JU
Sample : N4173-03
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
EX7N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.086	6.02 ng/ul	790139	Chrysene-d12	21.374	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Tetracosene	336	C24H48	010192-32-2	99
2	2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	94
3	1-Hexacosene	364	C26H52	018835-33-1	94
4	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
5	2- Chloropropionic acid, hexadec...	332	C19H37ClO2	086711-81-1	93

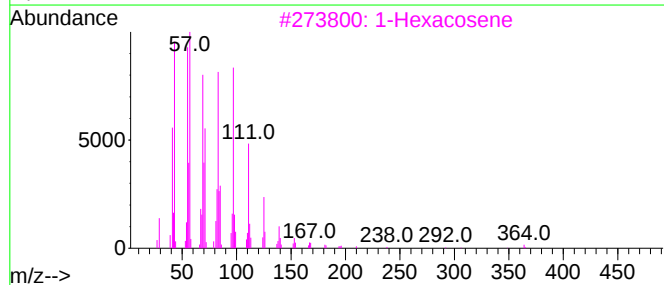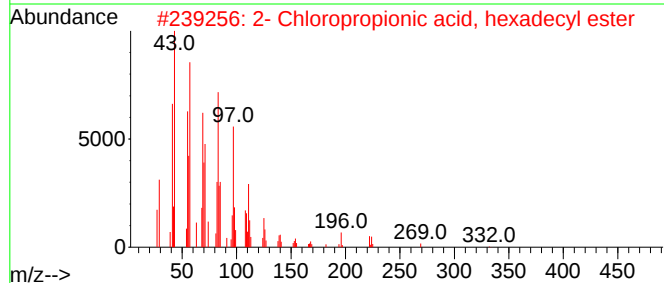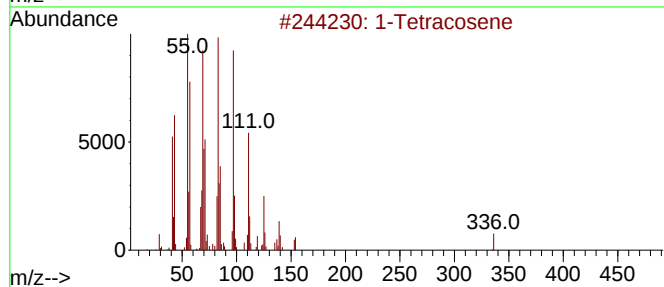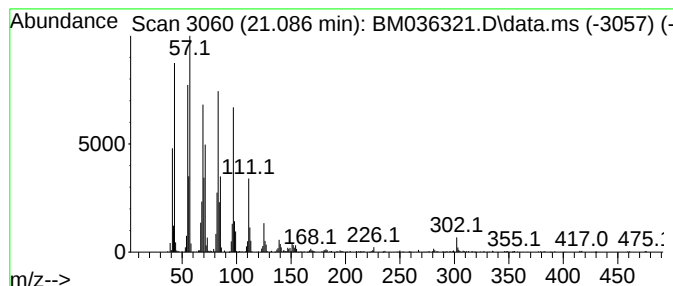

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036321.D
Acq On : 17 Aug 2022 18:00
Operator : CG/JU
Sample : N4173-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.086	6.0	ng/u1	790139	5	21.374	2625040	20.0