

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036324.D
 Acq On : 17 Aug 2022 20:26
 Operator : CG/JU
 Sample : PB147055BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	17	21	37	rVB	81427	122255	2.45%	0.208%
2	3.634	90	93	111	rBV	842193	1272748	25.55%	2.168%
3	3.958	144	148	155	rVB	17424	23614	0.47%	0.040%
4	6.981	655	662	674	rBV	1016248	1626803	32.65%	2.771%
5	7.140	683	689	702	rVB	868877	1335850	26.81%	2.276%
6	7.334	715	722	737	rBV	1031460	1644083	33.00%	2.801%
7	7.798	794	801	814	rBV	977629	1510289	30.32%	2.573%
8	8.522	917	924	938	rBV	1181856	1980714	39.76%	3.374%
9	8.969	992	1000	1014	rBV	980533	1598563	32.09%	2.723%
10	9.687	1115	1122	1138	rBV	757372	1298448	26.06%	2.212%
11	10.228	1207	1214	1231	rBV	1038127	1923848	38.62%	3.277%
12	10.598	1269	1277	1291	rBV	1374867	2240326	44.97%	3.817%
13	10.751	1295	1303	1321	rBV	1123414	2052058	41.19%	3.496%
14	12.204	1543	1550	1555	rBV2	14903	30603	0.61%	0.052%
15	13.422	1753	1757	1759	rBV5	3907	5781	0.12%	0.010%
16	13.863	1826	1832	1847	rBV	1947810	2656796	53.33%	4.526%
17	14.139	1872	1879	1894	rBV	2363811	3439728	69.05%	5.860%
18	14.445	1924	1931	1947	rBV	2032019	2846822	57.14%	4.850%
19	14.674	1964	1970	1991	rBV	584035	1236337	24.82%	2.106%
20	15.433	2093	2099	2111	rBV	2896335	4153521	83.37%	7.076%
21	15.569	2116	2122	2137	rVV	694300	1085960	21.80%	1.850%
22	15.674	2137	2140	2150	rVB5	17607	35250	0.71%	0.060%
23	16.651	2304	2306	2312	rVB7	4209	6233	0.13%	0.011%
24	16.980	2353	2362	2363	rBV7	7190	14640	0.29%	0.025%
25	17.186	2390	2397	2407	rBV	2302053	3167748	63.59%	5.397%
26	17.286	2408	2414	2431	rVB	3212683	4418887	88.70%	7.528%
27	19.145	2726	2730	2735	rBV2	38142	55686	1.12%	0.095%
28	19.215	2739	2742	2746	rVV	36028	46060	0.92%	0.078%
29	19.580	2798	2804	2817	rBV	3741315	4965916	99.68%	8.460%
30	20.580	2971	2974	2979	rBV	88729	96772	1.94%	0.165%
31	21.368	3103	3108	3115	rBV	2639356	3376709	67.78%	5.752%
32	23.550	3472	3479	3490	rBV2	2555429	4981827	100.00%	8.487%
33	23.697	3498	3504	3516	rVB2	1748672	3449016	69.23%	5.876%




Sum of corrected areas: 58699891

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036324.D
Acq On : 17 Aug 2022 20:26
Operator : CG/JU
Sample : PB147055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

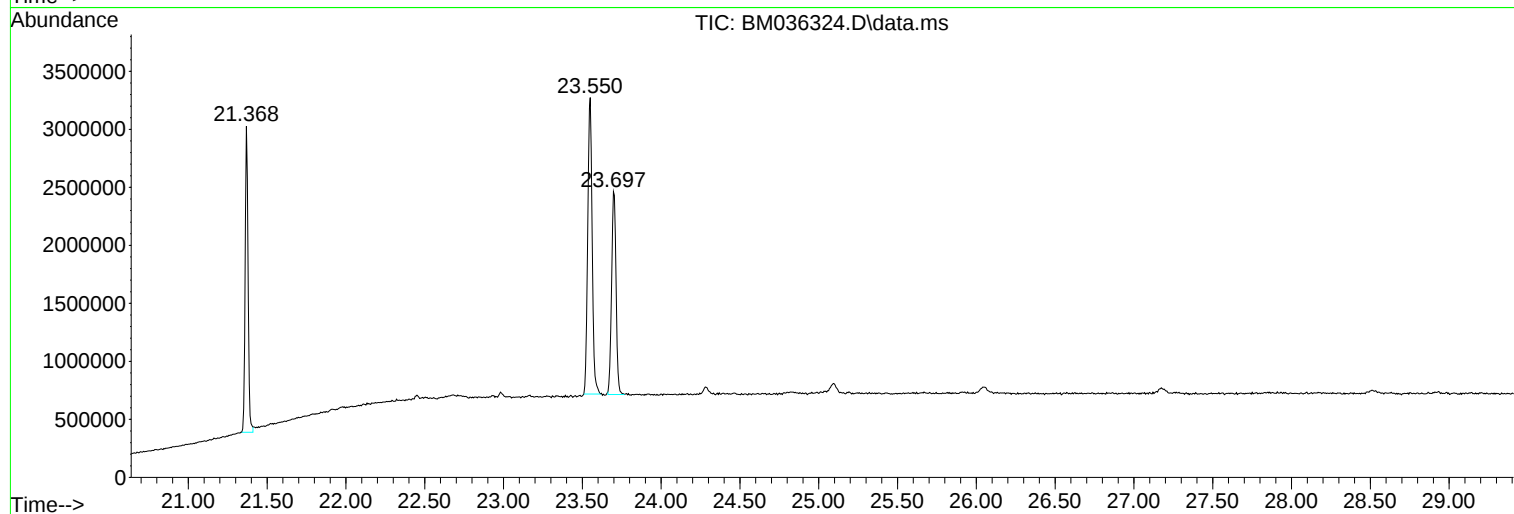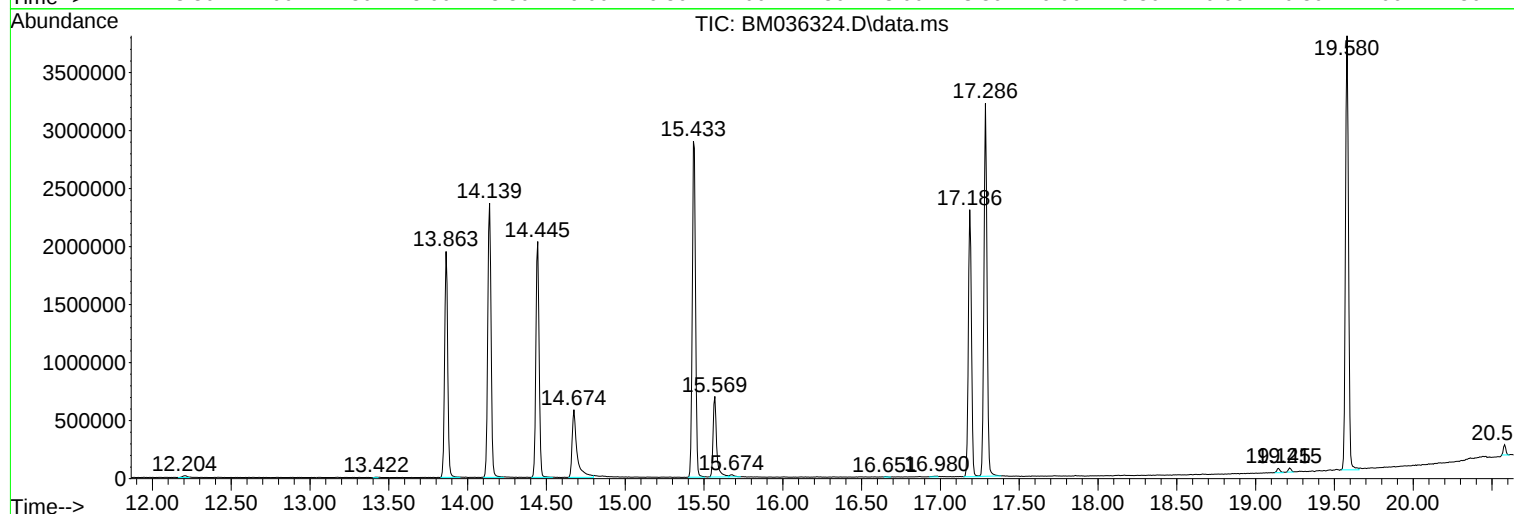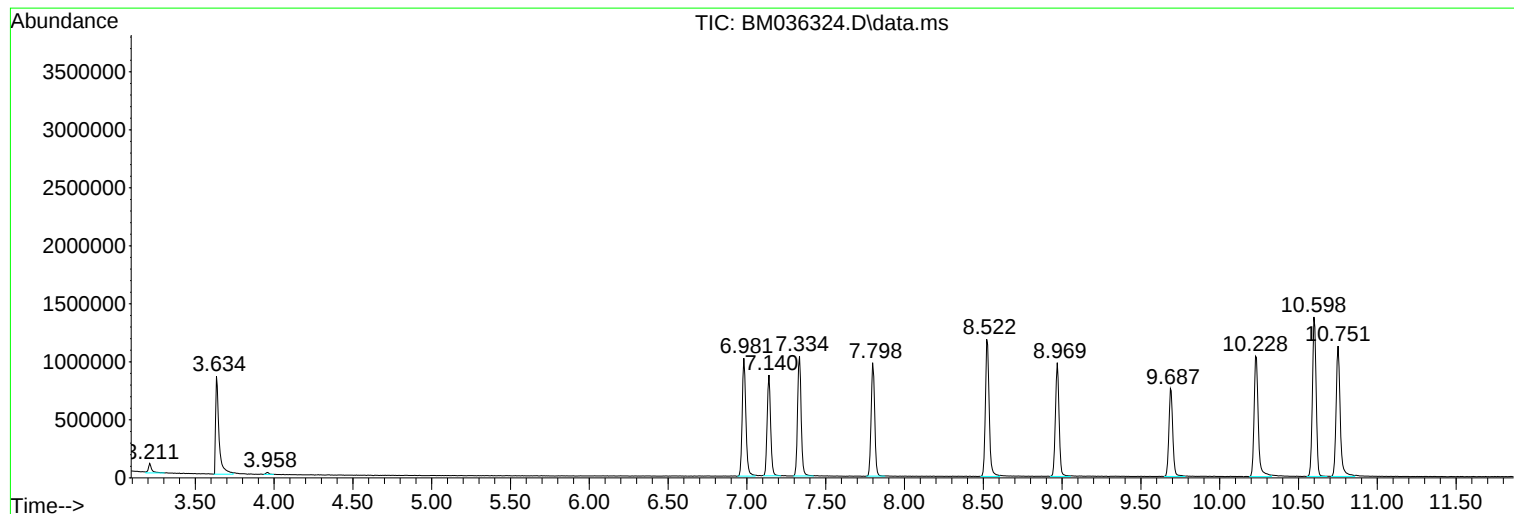

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036324.D
Acq On : 17 Aug 2022 20:26
Operator : CG/JU
Sample : PB147055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036324.D
Acq On : 17 Aug 2022 20:26
Operator : CG/JU
Sample : PB147055BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------