

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036338.D
 Acq On : 18 Aug 2022 04:48
 Operator : CG/JU
 Sample : N4176-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7Q3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	26	rVB	50966	63082	1.48%	0.131%
2	3.516	71	73	81	rVB3	6152	8655	0.20%	0.018%
3	3.640	92	94	110	rBV	199602	329571	7.74%	0.683%
4	3.857	126	131	139	rVB	52866	83330	1.96%	0.173%
5	3.957	144	148	152	rVB	21003	30207	0.71%	0.063%
6	4.340	210	213	216	rVB5	7112	8788	0.21%	0.018%
7	4.404	219	224	230	rVB	55888	73668	1.73%	0.153%
8	4.481	232	237	241	rBV7	3279	6953	0.16%	0.014%
9	4.763	281	285	288	rBV6	2886	4876	0.11%	0.010%
10	4.887	302	306	317	rVB	16873	27821	0.65%	0.058%
11	5.010	325	327	331	rVB5	7356	7092	0.17%	0.015%
12	5.498	406	410	416	rVB7	4169	7180	0.17%	0.015%
13	5.798	456	461	463	rBV6	3860	6422	0.15%	0.013%
14	6.916	646	651	655	rBV	28397	40392	0.95%	0.084%
15	6.981	655	662	676	rVV	742500	1237242	29.06%	2.562%
16	7.134	682	688	699	rBV	653893	1024746	24.07%	2.122%
17	7.222	699	703	713	rVB	15936	31376	0.74%	0.065%
18	7.328	715	721	731	rBV	787723	1260153	29.60%	2.610%
19	7.410	731	735	739	rVB2	10164	14771	0.35%	0.031%
20	7.616	765	770	773	rBV6	5358	7531	0.18%	0.016%
21	7.798	794	801	808	rBV	1017997	1589731	37.34%	3.292%
22	7.869	809	813	820	rVB4	13420	22149	0.52%	0.046%
23	8.004	833	836	842	rVB6	5586	8867	0.21%	0.018%
24	8.522	915	924	938	rBV	931492	1538919	36.15%	3.187%
25	8.969	993	1000	1007	rBV	727418	1216992	28.59%	2.521%
26	9.128	1022	1027	1032	rBV9	7592	13022	0.31%	0.027%
27	9.357	1058	1066	1074	rVB	30859	50470	1.19%	0.105%
28	9.686	1115	1122	1133	rBV	579288	972210	22.84%	2.014%
29	10.228	1207	1214	1234	rBV	788004	1442912	33.89%	2.988%
30	10.386	1236	1241	1244	rVB6	10110	16913	0.40%	0.035%
31	10.598	1269	1277	1289	rBV	1455142	2334205	54.83%	4.834%
32	10.745	1294	1302	1321	rBV	782467	1523031	35.77%	3.154%
33	11.792	1476	1480	1484	rBV6	2805	4887	0.11%	0.010%
34	11.851	1486	1490	1495	rVB2	18874	26031	0.61%	0.054%
35	12.198	1544	1549	1556	rVV2	12240	23692	0.56%	0.049%
36	12.798	1646	1651	1655	rBV6	5042	8531	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036338.D
 Acq On : 18 Aug 2022 04:48
 Operator : CG/JU
 Sample : N4176-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7Q3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	13.051	1688	1694	1699	rBV9	7093	9948	0.23%	0.021%
38	13.257	1726	1729	1734	rBV7	4620	6801	0.16%	0.014%
39	13.333	1741	1742	1748	rVB6	3761	5243	0.12%	0.011%
40	13.416	1752	1756	1760	rVV7	4835	8540	0.20%	0.018%

41	13.774	1813	1817	1825	rBV7	4892	7101	0.17%	0.015%
42	13.863	1825	1832	1845	rBV	1399016	2014340	47.31%	4.172%
43	14.133	1869	1878	1890	rBV	1725393	2510524	58.97%	5.200%
44	14.333	1909	1912	1916	rVB5	4242	5815	0.14%	0.012%
45	14.439	1922	1930	1940	rBV	1917599	2735613	64.26%	5.666%

46	14.674	1963	1970	1987	rBV	312298	715761	16.81%	1.482%
47	14.874	1998	2004	2014	rVB2	29788	54907	1.29%	0.114%
48	15.233	2060	2065	2068	rBV3	5810	9112	0.21%	0.019%
49	15.274	2068	2072	2077	rVB5	5206	9798	0.23%	0.020%
50	15.433	2088	2099	2113	rBV	2192235	3075833	72.25%	6.370%

51	15.568	2116	2122	2136	rBV	290342	511925	12.02%	1.060%
52	15.674	2136	2140	2143	rVB6	11798	17000	0.40%	0.035%
53	15.892	2174	2177	2183	rVB8	3185	6419	0.15%	0.013%
54	16.074	2203	2208	2211	rBV7	5572	9056	0.21%	0.019%
55	16.151	2213	2221	2228	rBV2	32776	63756	1.50%	0.132%

56	16.492	2274	2279	2282	rBV3	8750	13074	0.31%	0.027%
57	16.615	2295	2300	2302	rBV5	11509	17584	0.41%	0.036%
58	16.645	2302	2305	2311	rVV	16198	22769	0.53%	0.047%
59	16.945	2353	2356	2359	rBV4	4856	7478	0.18%	0.015%
60	17.104	2379	2383	2386	rBV5	5163	7078	0.17%	0.015%

61	17.186	2390	2397	2403	rBV	1977895	2817130	66.17%	5.835%
62	17.280	2407	2413	2426	rVV2	2473491	3445432	80.93%	7.136%
63	17.386	2426	2431	2439	rVB2	60383	98218	2.31%	0.203%
64	17.551	2455	2459	2462	rBV5	5295	8252	0.19%	0.017%
65	17.686	2478	2482	2483	rBV3	5267	6090	0.14%	0.013%

66	17.715	2483	2487	2491	rVV6	11169	18159	0.43%	0.038%
67	17.856	2507	2511	2515	rVB	30920	38078	0.89%	0.079%
68	17.968	2525	2530	2538	rBV4	50770	88587	2.08%	0.183%
69	18.086	2545	2550	2559	rBV	130451	217676	5.11%	0.451%
70	18.662	2645	2648	2653	rBV2	11215	12885	0.30%	0.027%

71	18.715	2654	2657	2664	rVB10	21457	25629	0.60%	0.053%
72	19.139	2726	2729	2733	rBV2	29787	37892	0.89%	0.078%
73	19.215	2738	2742	2745	rBV2	39330	63084	1.48%	0.131%
74	19.368	2764	2768	2773	rBV3	39375	63865	1.50%	0.132%
75	19.574	2798	2803	2815	rBV	2930244	3943893	92.64%	8.168%

76	20.580	2971	2974	2977	rVB	66420	71849	1.69%	0.149%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036338.D
Acq On : 18 Aug 2022 04:48
Operator : CG/JU
Sample : N4176-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

77	21.086	3056	3060	3067	rBV3	135931	240025	5.64%	0.497%
78	21.368	3103	3108	3117	rBV	2349967	2921057	68.61%	6.050%
79	23.544	3472	3478	3491	rVB2	2135883	4257418	100.00%	8.818%
80	23.697	3498	3504	3515	rVB2	1548777	2996569	70.38%	6.206%




Sum of corrected areas: 48283681

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036338.D
Acq On : 18 Aug 2022 04:48
Operator : CG/JU
Sample : N4176-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

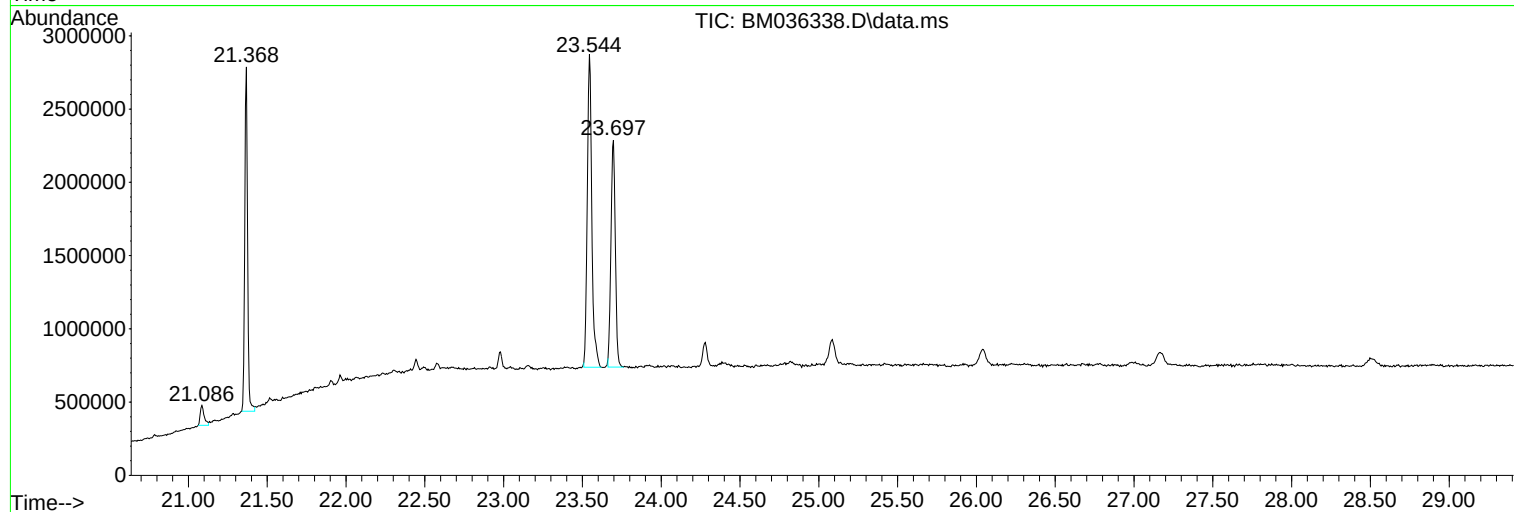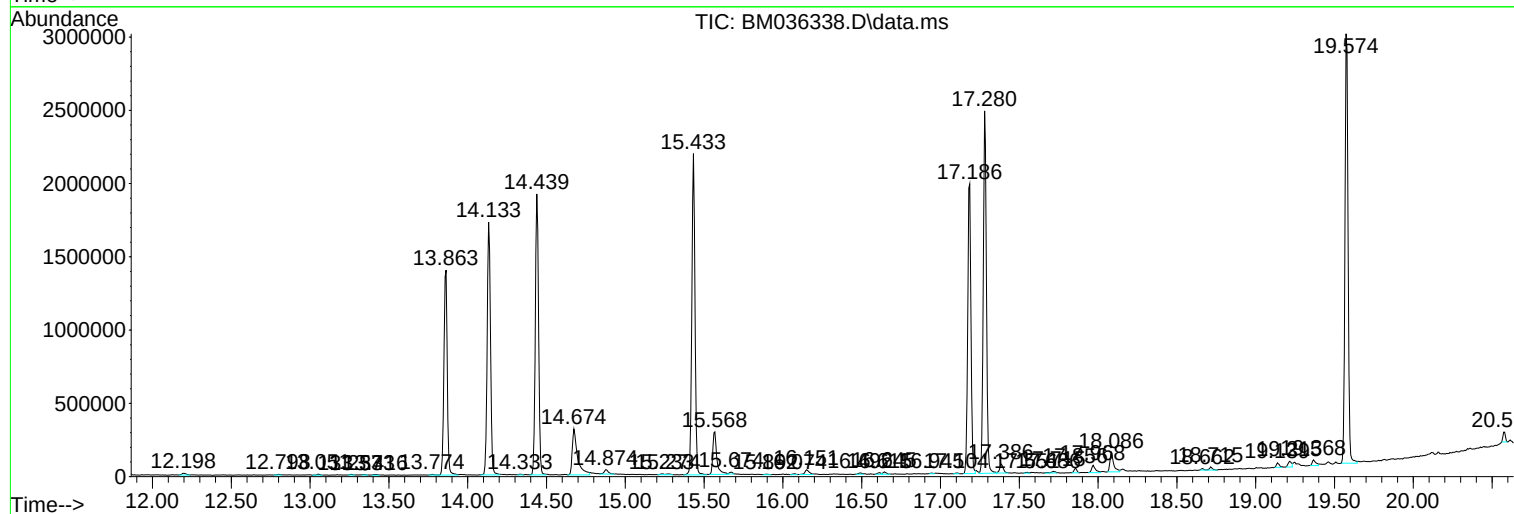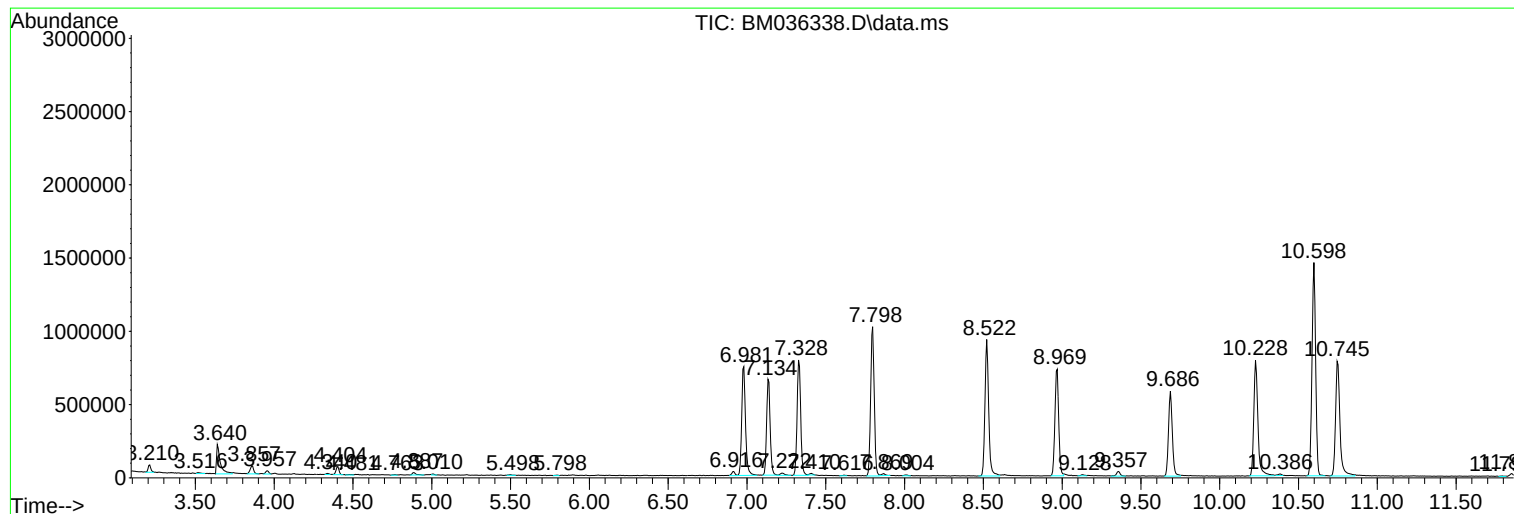

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036338.D
Acq On : 18 Aug 2022 04:48
Operator : CG/JU
Sample : N4176-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036338.D
Acq On : 18 Aug 2022 04:48
Operator : CG/JU
Sample : N4176-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------