

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036339.D
 Acq On : 18 Aug 2022 05:23
 Operator : CG/JU
 Sample : N4176-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	25	rBV	35294	43699	1.42%	0.117%
2	3.646	93	95	109	rBV	124834	205383	6.67%	0.550%
3	3.740	109	111	118	rVB6	9887	16369	0.53%	0.044%
4	3.857	126	131	137	rVB	40774	62979	2.05%	0.169%
5	3.957	144	148	153	rVB	20262	27249	0.89%	0.073%
6	4.340	209	213	217	rBV7	7598	11871	0.39%	0.032%
7	4.398	219	223	231	rVB	42140	60043	1.95%	0.161%
8	4.593	252	256	259	rBV4	2485	3087	0.10%	0.008%
9	4.757	282	284	288	rVB5	4303	5603	0.18%	0.015%
10	4.887	301	306	316	rBV2	17552	30312	0.98%	0.081%
11	5.004	323	326	331	rVB6	6007	8595	0.28%	0.023%
12	5.493	405	409	412	rVB4	3995	5215	0.17%	0.014%
13	5.798	457	461	465	rVB7	2485	3890	0.13%	0.010%
14	5.898	476	478	483	rVB5	2943	4027	0.13%	0.011%
15	6.063	502	506	509	rVB6	3343	5666	0.18%	0.015%
16	6.910	646	650	655	rBV	21125	29123	0.95%	0.078%
17	6.975	655	661	677	rVV	475963	823028	26.73%	2.205%
18	7.134	682	688	700	rVV	431572	681400	22.13%	1.826%
19	7.228	700	704	710	rVB	8946	17738	0.58%	0.048%
20	7.328	715	721	730	rVV	518675	823426	26.75%	2.206%
21	7.410	732	735	740	rVB5	10040	15372	0.50%	0.041%
22	7.798	794	801	809	rBV	995584	1563012	50.77%	4.187%
23	7.863	809	812	819	rVB4	7716	13637	0.44%	0.037%
24	8.010	833	837	842	rVB7	5940	9842	0.32%	0.026%
25	8.522	915	924	939	rBV	576748	1000131	32.48%	2.679%
26	8.628	941	942	948	rVB5	5410	7495	0.24%	0.020%
27	8.963	991	999	1012	rBV	457268	802173	26.05%	2.149%
28	9.133	1023	1028	1030	rBV6	5351	8573	0.28%	0.023%
29	9.357	1059	1066	1070	rBV	21855	34539	1.12%	0.093%
30	9.686	1115	1122	1135	rBV	356240	606445	19.70%	1.625%
31	10.228	1207	1214	1235	rBV	478899	924744	30.04%	2.477%
32	10.598	1269	1277	1287	rBV	1385570	2277934	73.99%	6.103%
33	10.751	1295	1303	1319	rBV	474308	962248	31.25%	2.578%
34	11.851	1485	1490	1495	rVB2	12334	20313	0.66%	0.054%
35	12.204	1542	1550	1554	rBV5	7232	14376	0.47%	0.039%
36	12.804	1646	1652	1653	rBV5	2870	4172	0.14%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036339.D
 Acq On : 18 Aug 2022 05:23
 Operator : CG/JU
 Sample : N4176-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

37	13.051	1690	1694	1698	rBV5	4119	5481	0.18%	0.015%
38	13.174	1711	1715	1717	rBV5	3220	4200	0.14%	0.011%
39	13.257	1727	1729	1734	rVB6	3775	4948	0.16%	0.013%
40	13.421	1752	1757	1762	rBV9	2828	4936	0.16%	0.013%
41	13.774	1815	1817	1822	rVB6	3106	5157	0.17%	0.014%
42	13.857	1822	1831	1845	rBV	858231	1279889	41.57%	3.429%
43	14.133	1871	1878	1892	rBV	1095152	1600481	51.98%	4.288%
44	14.333	1908	1912	1916	rBV5	4194	6151	0.20%	0.016%
45	14.439	1924	1930	1943	rVB	1856849	2687455	87.29%	7.200%
46	14.621	1956	1961	1964	rBV7	4298	7424	0.24%	0.020%
47	14.680	1964	1971	1995	rBV	128458	384218	12.48%	1.029%
48	14.880	2000	2005	2012	rVB5	14547	25679	0.83%	0.069%
49	15.233	2060	2065	2068	rBV5	6389	9363	0.30%	0.025%
50	15.274	2068	2072	2073	rBV4	2721	3765	0.12%	0.010%
51	15.433	2090	2099	2112	rBV	1364701	1953144	63.44%	5.233%
52	15.568	2117	2122	2132	rBV	112389	211266	6.86%	0.566%
53	15.668	2137	2139	2144	rVB6	7192	9513	0.31%	0.025%
54	16.068	2203	2207	2214	rBV7	5043	10485	0.34%	0.028%
55	16.151	2214	2221	2231	rVV4	21295	47564	1.54%	0.127%
56	16.315	2246	2249	2257	rVB8	3392	9126	0.30%	0.024%
57	16.604	2294	2298	2302	rBV4	9996	16713	0.54%	0.045%
58	16.645	2302	2305	2310	rVB3	9906	14006	0.45%	0.038%
59	16.821	2332	2335	2339	rBV6	3476	4962	0.16%	0.013%
60	16.951	2353	2357	2359	rBV4	6505	10018	0.33%	0.027%
61	17.104	2380	2383	2387	rVV6	5411	9230	0.30%	0.025%
62	17.186	2390	2397	2407	rBV	1970593	2820622	91.61%	7.557%
63	17.280	2407	2413	2426	rVV	1512697	2173751	70.60%	5.824%
64	17.386	2426	2431	2440	rVV6	36784	69342	2.25%	0.186%
65	17.474	2444	2446	2450	rVB5	4412	4891	0.16%	0.013%
66	17.545	2455	2458	2459	rBV2	6160	6007	0.20%	0.016%
67	17.680	2477	2481	2482	rBV3	3709	5010	0.16%	0.013%
68	17.715	2483	2487	2491	rVB6	9044	12396	0.40%	0.033%
69	17.856	2507	2511	2515	rBV2	22280	25847	0.84%	0.069%
70	17.968	2526	2530	2538	rBV2	66073	109059	3.54%	0.292%
71	18.086	2545	2550	2556	rBV	109771	172925	5.62%	0.463%
72	18.151	2559	2561	2569	rVB	13079	22315	0.72%	0.060%
73	18.398	2601	2603	2606	rBV4	4437	4190	0.14%	0.011%
74	18.662	2646	2648	2652	rVB5	10070	9638	0.31%	0.026%
75	19.145	2727	2730	2733	rVB2	16081	17884	0.58%	0.048%
76	19.221	2738	2743	2747	rBV2	32943	66360	2.16%	0.178%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
 Data File : BM036339.D
 Acq On : 18 Aug 2022 05:23
 Operator : CG/JU
 Sample : N4176-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EX7Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

77	19.368	2765	2768	2773	rBV6	17992	30476	0.99%	0.082%
78	19.574	2798	2803	2815	rBV	2015328	2804186	91.08%	7.513%
79	20.580	2971	2974	2977	rVB	65689	66676	2.17%	0.179%
80	21.086	3056	3060	3066	rBV4	153198	256563	8.33%	0.687%
81	21.368	3103	3108	3119	rBV	2369928	3034582	98.56%	8.130%
82	23.544	3472	3478	3490	rVB2	1566894	3075984	99.91%	8.241%
83	23.697	3498	3504	3516	rVB2	1548100	3078794	100.00%	8.248%




Sum of corrected areas: 37326381

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036339.D
Acq On : 18 Aug 2022 05:23
Operator : CG/JU
Sample : N4176-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

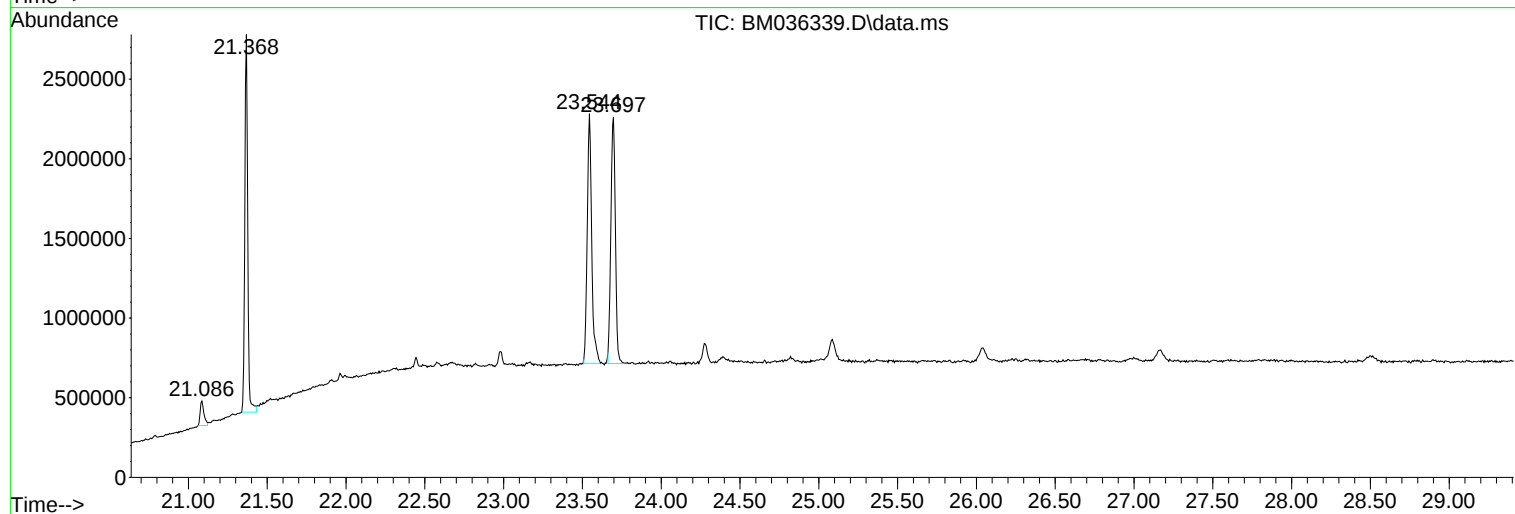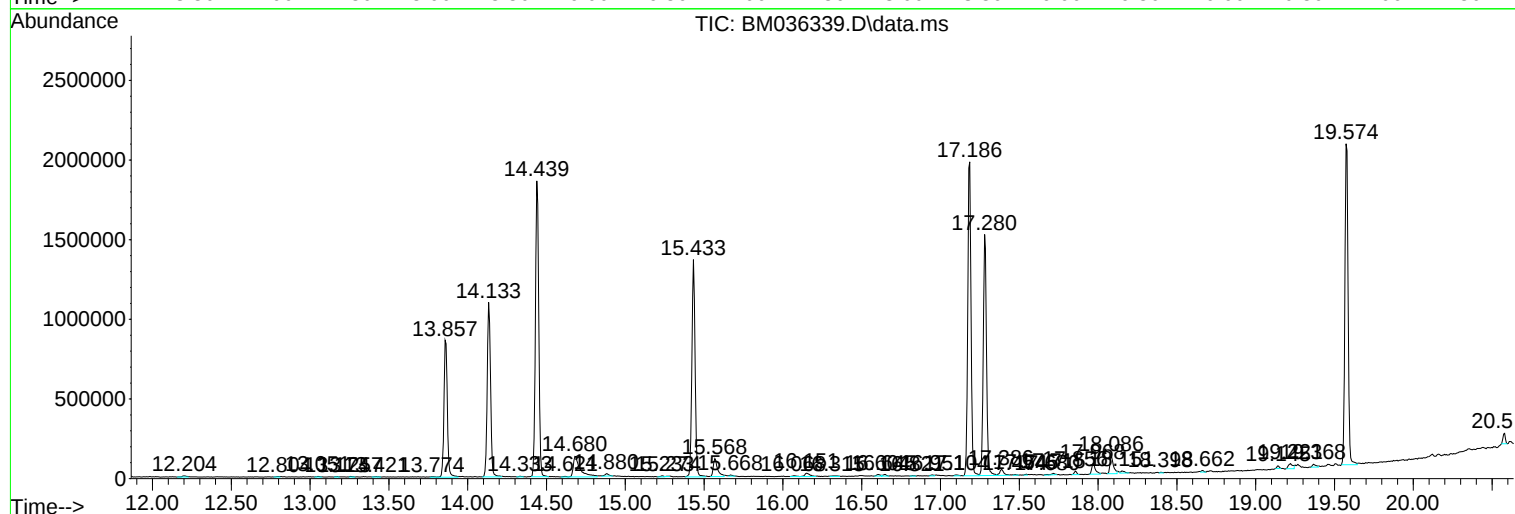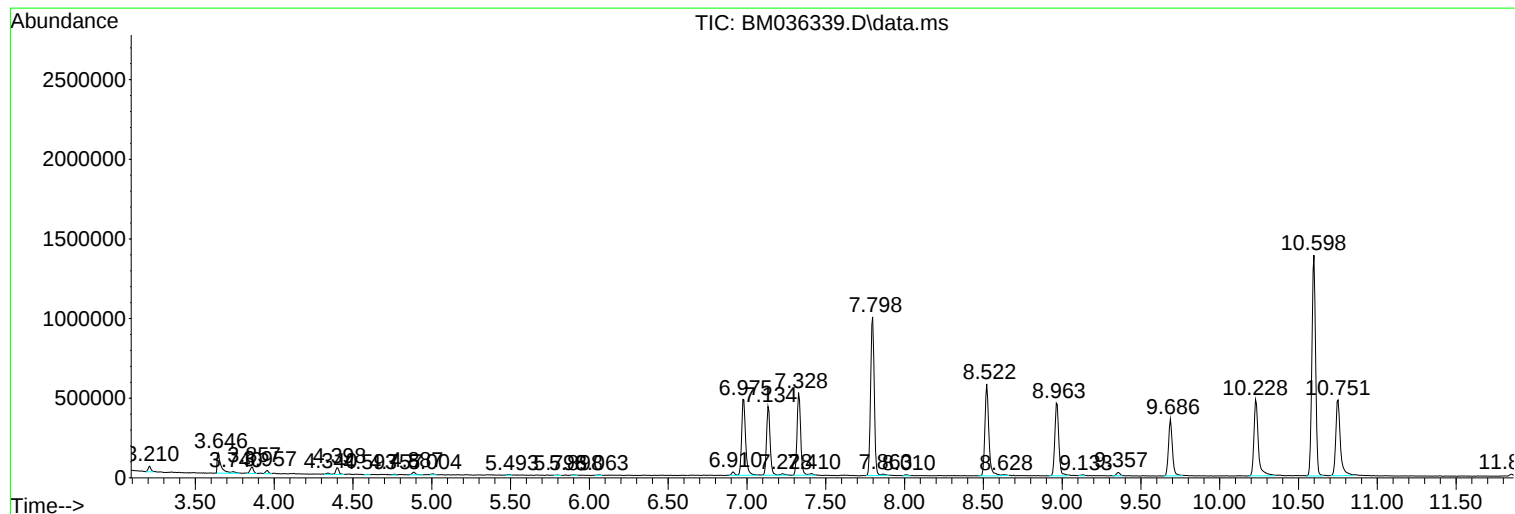

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036339.D
Acq On : 18 Aug 2022 05:23
Operator : CG/JU
Sample : N4176-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081722\
Data File : BM036339.D
Acq On : 18 Aug 2022 05:23
Operator : CG/JU
Sample : N4176-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EX7Q5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------