


Data Path : Z:\HPCHEM1\BNA_M\Data\BM081815\
Data File : BM002476.D
Acq On : 18 Aug 2015 08:18
Operator : UM/IZ
Sample : DFTPP02
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP02

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Title : SVOA CALIBRATION
Last Update : Tue Aug 18 18:25:22 2015

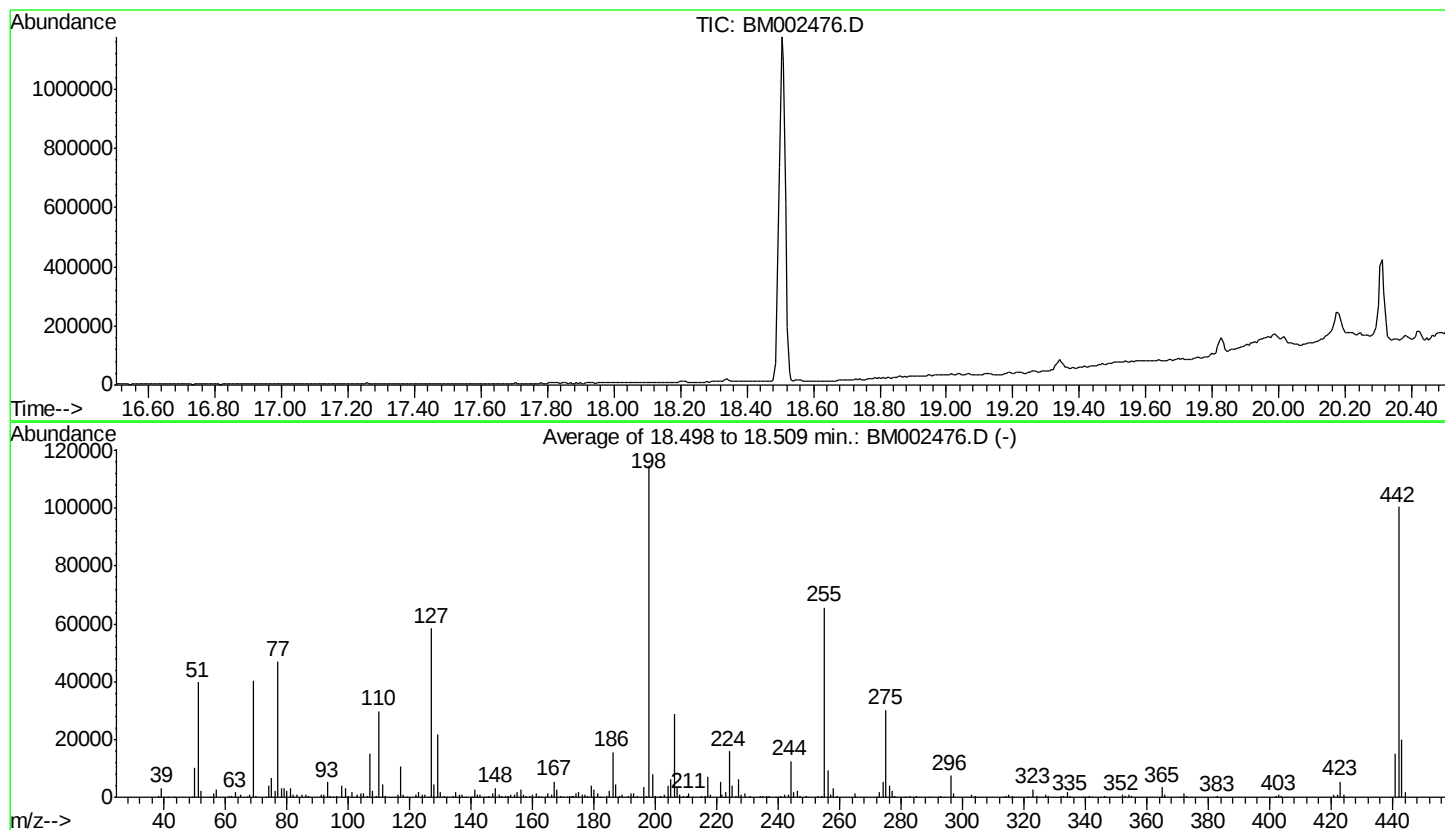

AutoFind: Scans 2620, 2621, 2622; Background Corrected with Scan 2615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	39821	PASS
68	69	0.00	2	1.9	760	PASS
69	198	0.00	100	35.1	40255	PASS
70	69	0.00	2	0.8	342	PASS
127	198	10	80	50.8	58314	PASS
197	198	0.00	2	0.5	537	PASS
198	198	100	100	100.0	114776	PASS
199	198	5	9	7.0	8044	PASS
275	198	10	60	26.5	30360	PASS
365	198	1	100	3.1	3507	PASS
441	443	0.01	100	75.9	15117	PASS
442	198	50	100	87.5	100429	PASS
443	442	15	24	19.8	19915	PASS

m/z	Abundance
38.00	445.0
39.10	2830.0
40.00	534.0
41.00	533.0
43.10	495.0
44.00	2297.0
49.00	310.0
50.00	8326.0
51.00	33736.0
52.00	1519.0
55.00	772.0
56.00	1148.0
57.00	2826.0
60.90	358.0
62.10	465.0
63.00	1439.0
65.00	784.0
68.00	690.0
69.00	34560.0
70.00	323.0
73.00	776.0
74.00	3230.0
75.00	5468.0
76.00	1918.0
77.10	39008.0
78.10	2777.0
79.00	2635.0
80.00	1788.0
81.00	3119.0
82.00	814.0
83.00	946.0
84.90	704.0
86.00	796.0
87.00	402.0
91.00	960.0
92.00	727.0
93.00	4420.0
94.00	458.0
95.10	500.0
96.00	409.0
97.00	358.0
98.00	3181.0
99.00	2419.0
100.00	330.0
101.00	1705.0
103.00	783.0
104.00	940.0
105.00	1050.0
105.90	375.0
107.00	12211.0
108.00	1928.0
109.10	543.0
110.00	24104.0
111.00	3674.0
112.00	443.0
115.90	774.0
117.00	8803.0
118.00	794.0
121.90	902.0
123.00	1288.0
123.90	689.0
124.90	576.0
127.00	46816.0
128.00	3859.0
129.00	17192.0
129.90	1560.0
131.00	368.0
134.00	525.0
135.00	1606.0
135.90	598.0
137.00	740.0
141.00	2238.0
142.00	736.0
142.90	540.0
145.80	510.0
147.00	1173.0
147.90	2412.0
149.00	646.0
149.90	416.0
151.10	384.0
153.00	876.0
154.00	710.0
155.00	1297.0
156.00	1940.0
157.00	596.0
157.90	523.0
159.00	428.0
160.00	757.0
160.90	1158.0
161.90	559.0
162.90	567.0

Instrument :

BNA_M

ClientSampleId :

DFTPP02

164.90	872.0
166.00	733.0
167.00	4004.0
168.00	2078.0
169.00	629.0
169.90	426.0
170.90	393.0
172.00	383.0
173.10	495.0
174.00	1137.0
175.00	1734.0
176.00	863.0
176.90	857.0
178.00	460.0
179.00	3248.0
180.00	2170.0
181.00	1299.0
185.00	1543.0
186.00	11081.0
187.00	3376.0
188.10	402.0
189.00	997.0
191.00	467.0
192.00	911.0
193.00	1231.0
193.90	396.0
196.00	2462.0
196.90	633.0
197.90	83856.0
198.90	6140.0
199.90	538.0
201.40	415.0
203.00	667.0
204.00	3055.0
205.00	4720.0
206.00	20872.0
207.10	3671.0
207.90	744.0
209.00	358.0
210.00	421.0
211.00	844.0
214.90	357.0
216.00	449.0
216.90	5004.0
218.00	694.0
221.00	3908.0
221.80	704.0
223.00	1257.0
224.00	11099.0
225.00	2698.0
226.10	435.0
227.00	4462.0
228.00	695.0
229.00	1002.0
230.90	442.0
233.90	310.0
235.00	391.0
237.00	364.0
240.90	323.0
242.00	592.0
243.00	676.0
244.00	8566.0
245.00	1102.0
246.00	1724.0
246.90	418.0
249.00	390.0
254.00	393.0
255.00	45248.0
256.00	6250.0
256.90	399.0
258.00	2489.0
258.90	377.0
265.00	959.0
273.00	1241.0
274.00	3851.0
275.00	20416.0
276.00	2930.0
277.00	1673.0
281.00	332.0
292.90	407.0
296.00	4981.0
297.00	868.0
303.00	783.0
314.00	360.0
315.00	609.0
316.10	499.0
323.00	1899.0
324.00	385.0
326.10	459.0
327.00	553.0
328.00	303.0
334.00	1182.0
335.10	390.0
340.10	485.0
341.00	612.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

342.00	548.0
346.00	455.0
352.00	977.0
353.00	572.0
354.00	774.0
355.00	376.0
365.00	2399.0
365.90	554.0
372.00	990.0
373.00	305.0
402.00	372.0
403.00	387.0
421.00	512.0
421.90	376.0
423.00	3254.0
424.00	584.0
441.00	8145.0
442.00	55576.0
443.00	11185.0
444.00	1209.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
38.00	632.0
39.10	3761.0
40.00	586.0
41.00	683.0
43.10	585.0
44.00	2361.0
49.00	357.0
50.00	12095.0
51.10	48008.0
52.00	2567.0
55.00	797.0
56.00	1609.0
57.00	3538.0
61.00	613.0
62.00	660.0
63.00	1912.0
63.90	323.0
65.10	1021.0
68.00	938.0
69.00	48560.0
70.00	399.0
73.10	735.0
74.00	4836.0
75.00	7565.0
76.00	2661.0
77.00	56048.0
78.10	3594.0
79.00	3919.0
80.00	2894.0
81.00	4163.0
82.00	1105.0
83.00	1197.0
85.00	732.0
86.00	1155.0
87.00	573.0
91.00	1209.0
91.90	1033.0
93.00	5951.0
94.00	540.0
95.00	447.0
96.10	422.0
97.10	341.0
98.00	4439.0
99.00	3656.0
99.90	409.0
101.00	2175.0
103.00	810.0
104.00	1529.0
105.00	1528.0
106.00	566.0
107.00	18424.0
108.00	2887.0
109.10	790.0
110.00	35960.0
111.00	5070.0
111.90	695.0
116.00	1142.0
117.00	12451.0
118.00	951.0
118.90	313.0
121.90	1226.0
123.00	1922.0
124.00	918.0
125.00	883.0
126.20	384.0
127.00	68880.0
128.00	5168.0
129.00	26136.0
130.00	2303.0
131.00	599.0
132.00	313.0
133.90	895.0
135.00	2146.0
136.00	971.0
137.00	1350.0
138.10	305.0
139.90	374.0
141.00	3326.0
142.00	1197.0
142.90	883.0
144.00	319.0
145.90	619.0
147.00	1668.0
148.00	3653.0
149.00	804.0
150.00	374.0
151.10	563.0
151.90	414.0
153.00	1244.0
153.90	867.0
155.00	2078.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

156.00	3085.0
156.90	854.0
157.80	776.0
158.90	577.0
160.00	1075.0
161.00	1726.0
161.90	740.0
163.10	513.0
163.90	429.0
165.00	1408.0
165.90	992.0
167.00	6637.0
168.00	2906.0
168.90	683.0
170.10	383.0
171.00	614.0
172.00	481.0
173.00	793.0
174.00	1549.0
175.10	2854.0
176.00	1002.0
176.90	1281.0
177.90	646.0
179.00	4901.0
180.00	3326.0
181.00	1574.0
181.80	359.0
184.00	488.0
185.00	2611.0
186.00	18696.0
187.00	5205.0
187.90	612.0
188.90	1077.0
191.10	782.0
192.00	1671.0
193.00	1734.0
194.00	450.0
196.00	4169.0
197.10	825.0
197.90	135296.0
198.90	9489.0
200.00	767.0
201.40	801.0
203.00	909.0
204.00	4800.0
205.00	7544.0
206.00	34840.0
207.00	4952.0
208.00	1304.0
209.00	540.0
210.20	576.0
210.90	1389.0
214.90	358.0
216.00	750.0
217.00	8576.0
218.00	1214.0
221.00	6400.0
221.70	1432.0
223.00	2011.0
224.00	18696.0
225.00	4954.0
226.00	510.0
227.00	6741.0
228.00	990.0
229.00	1589.0
231.00	752.0
233.90	484.0
235.00	586.0
236.00	472.0
237.00	668.0
239.00	357.0
240.00	301.0
241.00	472.0
242.00	968.0
243.10	1090.0
244.00	14905.0
245.00	2105.0
246.00	2572.0
247.00	707.0
249.00	544.0
253.00	380.0
254.00	577.0
255.00	77160.0
256.00	11042.0
256.90	956.0
258.00	3797.0
259.00	667.0
264.90	1497.0
273.00	2226.0
274.00	6167.0
275.00	35672.0
276.00	4634.0
277.00	2709.0
277.90	388.0
283.00	436.0

Instrument :

BNA_M

ClientSampleId :

DFTPP02

285.00	485.0
289.00	317.0
292.90	700.0
296.00	8491.0
296.90	1193.0
303.00	1122.0
304.00	352.0
314.00	688.0
315.00	1143.0
316.00	707.0
323.00	3119.0
324.00	592.0
326.10	435.0
327.00	789.0
328.10	514.0
332.00	410.0
333.00	406.0
334.00	1923.0
334.90	547.0
339.20	308.0
340.10	735.0
341.00	675.0
342.10	522.0
346.00	824.0
352.00	1259.0
353.00	889.0
354.00	1329.0
355.00	459.0
365.00	3921.0
366.00	884.0
371.00	349.0
372.00	1556.0
373.00	369.0
383.00	554.0
402.00	729.0
403.00	1032.0
403.90	403.0
421.00	734.0
422.00	822.0
423.00	6240.0
424.00	1345.0
441.00	16960.0
442.00	111760.0
443.00	22784.0
444.00	1971.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
38.00	433.0
39.10	3051.0
40.00	643.0
41.00	556.0
43.00	602.0
44.00	1948.0
50.00	9564.0
51.00	37720.0
52.00	2002.0
55.00	859.0
56.00	1362.0
57.00	3238.0
61.00	393.0
62.00	482.0
63.00	1614.0
65.00	975.0
67.10	332.0
67.90	654.0
69.00	38968.0
70.10	304.0
73.00	758.0
74.10	3924.0
75.00	6628.0
76.10	2060.0
77.10	45776.0
78.00	3144.0
79.00	3006.0
80.00	2524.0
81.00	3477.0
82.00	868.0
83.00	984.0
85.00	827.0
86.00	897.0
87.00	470.0
91.00	1017.0
92.00	859.0
93.00	5165.0
93.90	419.0
95.00	463.0
95.90	468.0
97.00	314.0
98.00	3765.0
99.00	3102.0
100.00	320.0
101.00	1942.0
103.00	728.0
104.00	1231.0
105.00	1320.0
106.00	445.0
107.00	15241.0
108.00	2524.0
109.10	632.0
110.00	29056.0
111.00	4720.0
112.00	522.0
116.00	845.0
117.00	11049.0
118.00	926.0
118.90	355.0
122.00	1037.0
123.00	1843.0
124.00	751.0
125.00	751.0
127.00	59248.0
128.00	4436.0
129.00	22224.0
130.00	1886.0
130.90	486.0
134.00	593.0
135.00	2033.0
136.00	800.0
137.00	1189.0
138.00	321.0
140.10	363.0
141.00	3000.0
142.00	1079.0
143.00	762.0
145.00	349.0
146.00	481.0
147.00	1703.0
148.00	3490.0
149.00	837.0
150.00	350.0
151.00	666.0
151.90	379.0
152.90	973.0
154.00	865.0
155.00	1740.0
156.00	2441.0
157.00	766.0
158.00	605.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

158.80	516.0
160.00	1082.0
161.00	1425.0
162.00	676.0
163.00	414.0
164.90	1447.0
166.00	912.0
167.00	5476.0
168.00	2597.0
169.00	725.0
169.80	373.0
170.90	438.0
172.00	528.0
172.80	771.0
173.90	1269.0
175.00	2415.0
176.00	767.0
177.00	973.0
177.90	553.0
179.00	4467.0
180.00	3019.0
181.00	1333.0
184.00	627.0
185.00	2278.0
186.00	17016.0
187.00	4782.0
188.10	511.0
189.00	1111.0
190.90	598.0
191.90	1382.0
193.00	1641.0
194.00	517.0
196.00	3499.0
197.10	786.0
197.90	125176.0
198.90	8505.0
199.90	731.0
201.60	598.0
202.90	906.0
204.00	4270.0
205.00	7001.0
206.00	31152.0
207.00	5037.0
208.00	1184.0
209.00	457.0
210.20	694.0
210.90	1144.0
212.00	308.0
214.80	353.0
216.00	667.0
217.00	7609.0
218.00	1019.0
221.00	5583.0
221.80	1087.0
223.00	1826.0
224.00	17592.0
225.00	4507.0
226.00	429.0
227.00	7030.0
228.00	989.0
229.00	1461.0
231.00	601.0
233.90	477.0
235.00	698.0
236.00	360.0
236.90	658.0
240.90	427.0
242.00	1164.0
243.00	1022.0
244.00	13845.0
245.00	1839.0
246.00	2547.0
247.00	409.0
249.00	734.0
252.90	330.0
255.00	74656.0
256.00	10494.0
257.00	746.0
258.00	3644.0
258.90	571.0
265.00	1627.0
272.00	327.0
273.00	2222.0
274.00	5862.0
275.00	34992.0
276.00	4544.0
277.00	2667.0
277.90	395.0
281.00	374.0
283.00	450.0
285.00	782.0
292.00	301.0
293.00	607.0
296.00	8943.0
297.00	1369.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

302.90	1084.0
304.00	505.0
313.10	313.0
314.10	592.0
315.00	1018.0
316.00	574.0
321.00	349.0
323.00	3170.0
324.00	674.0
326.00	501.0
327.00	840.0
328.00	560.0
332.00	412.0
333.00	312.0
334.00	2055.0
335.10	529.0
339.10	363.0
340.10	532.0
341.00	695.0
342.10	596.0
346.00	745.0
352.00	1150.0
353.00	832.0
354.00	1196.0
355.00	472.0
365.00	4203.0
366.00	695.0
371.00	340.0
372.00	1812.0
373.00	541.0
383.00	461.0
402.00	678.0
403.00	1094.0
403.90	462.0
421.00	912.0
422.00	940.0
423.00	6953.0
424.00	1367.0
441.00	20248.0
442.00	133952.0
443.00	25776.0
444.00	2123.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
40.00	498.0
41.00	528.0
43.10	474.0
44.00	2454.0
55.00	587.0
57.10	435.0
69.10	441.0
73.00	574.0
81.10	448.0
83.10	325.0
95.10	378.0
97.10	345.0
156.70	338.0
163.00	412.0
168.70	459.0
169.90	356.0
171.10	305.0
175.00	359.0
207.10	915.0
326.10	542.0
340.10	579.0
342.10	467.0
352.10	321.0
353.00	303.0
354.10	396.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02