
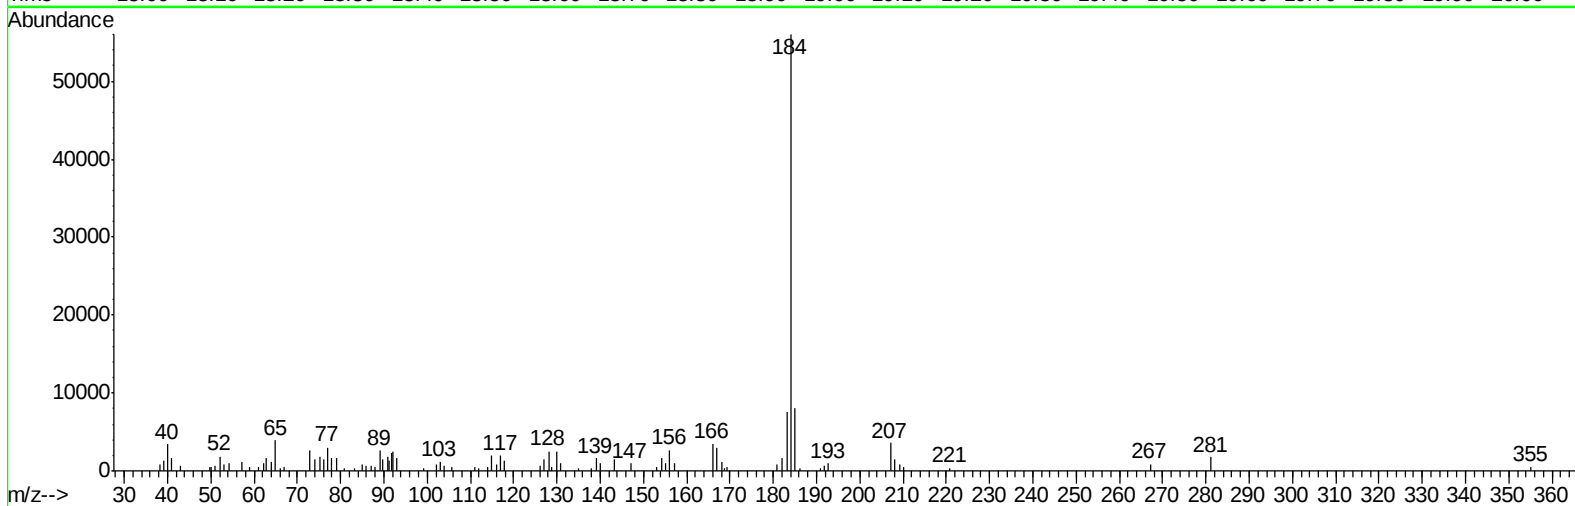


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081817\
Data File : BM011292.D
Acq On : 18 Aug 2017 16:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 04:22:33 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

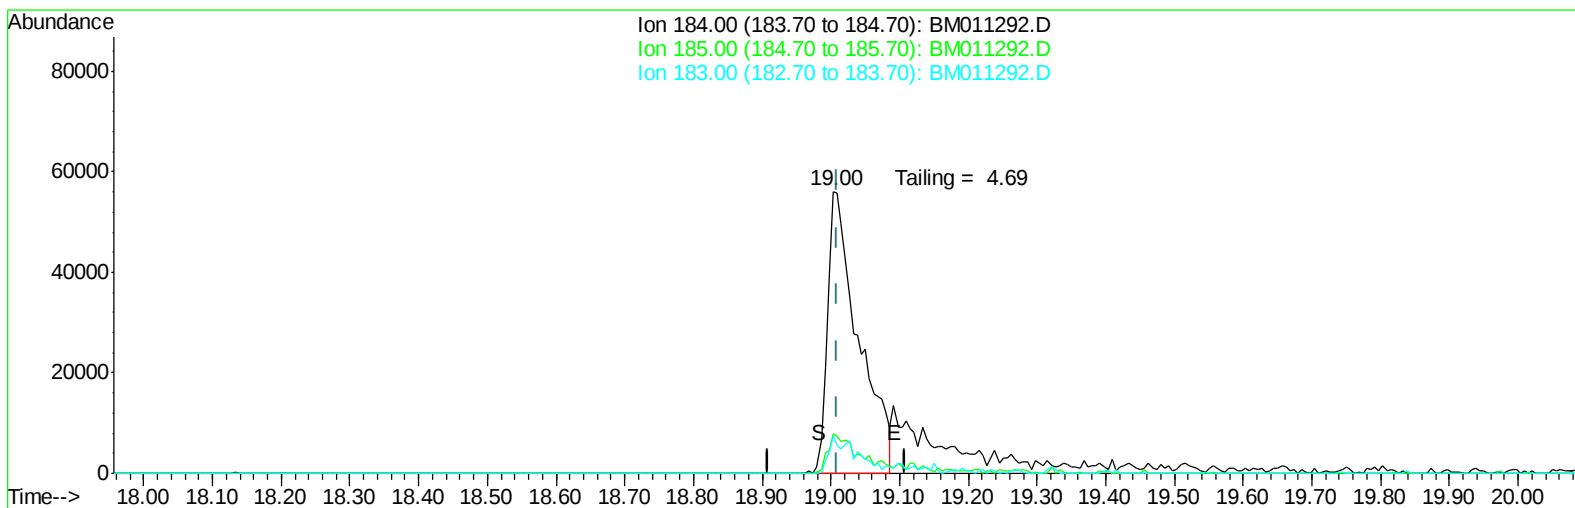

TIC: BM011292.D

(76) Benzidine



19.003min (-0.006) 58197.19ng

response 175422

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.31
183.00	11.10	13.38#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081817\
Data File : BM011292.D
Acq On : 18 Aug 2017 16:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 19 04:22:33 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

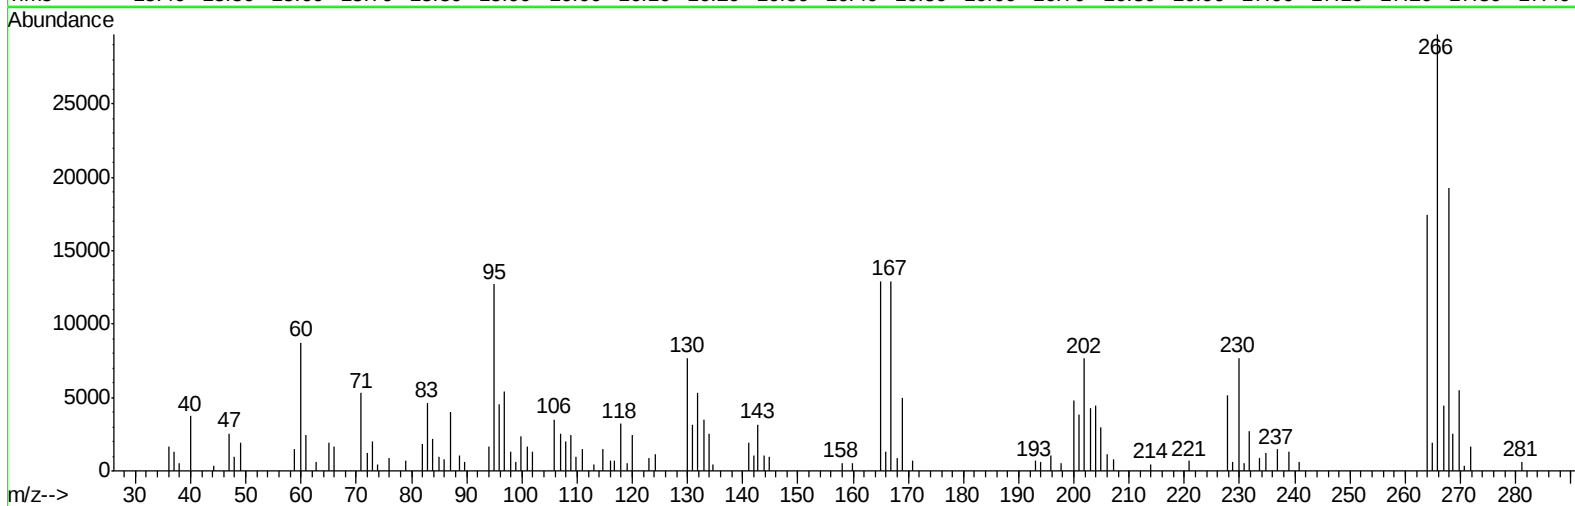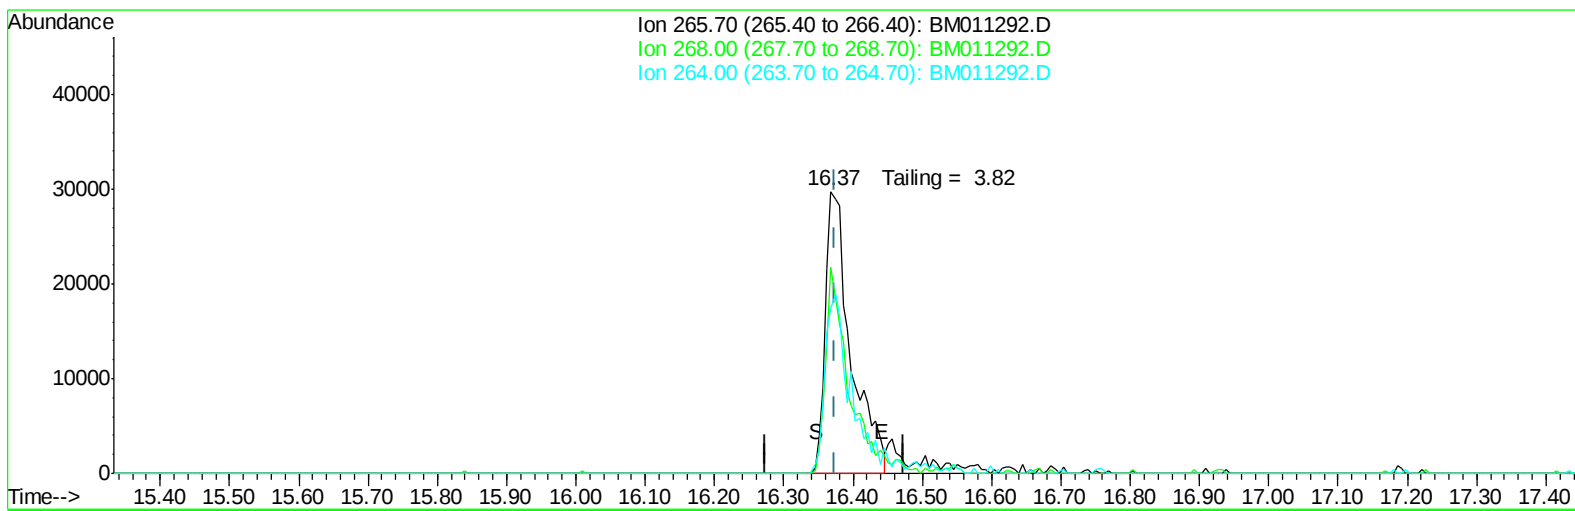

TIC: BM011292.D

(69) Pentachlorophenol (C)

16.368min (-0.006) 0.00ng

response 75972

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	73.27
264.00	61.20	58.60
0.00	0.00	0.00