


Data Path : Z:\HPCHEM1\BNA M\Data\BM081817\
 Data File : BM011292.D
 Acq On : 18 Aug 2017 16:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

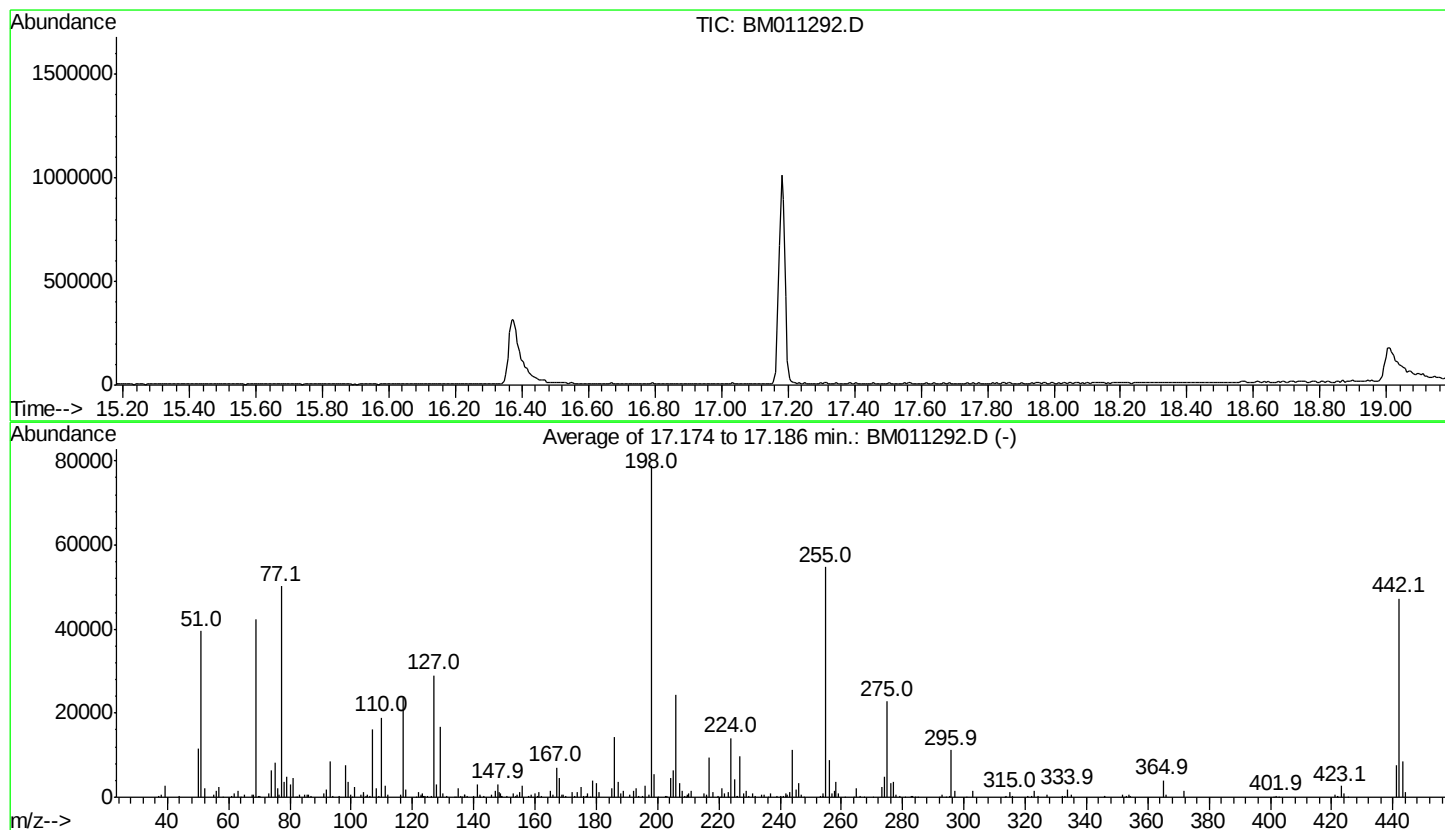

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	39485	PASS
68	69	0.00	2	1.3	561	PASS
69	198	0.00	100	53.8	42426	PASS
70	69	0.00	2	0.8	345	PASS
127	198	10	80	36.7	28933	PASS
197	198	0.00	2	0.8	633	PASS
198	198	100	100	100.0	78880	PASS
199	198	5	9	6.9	5418	PASS
275	198	10	60	28.9	22824	PASS
365	198	1	100	5.1	3993	PASS
441	442	0.01	24	16.0	7548	PASS
442	198	50	100	59.9	47221	PASS
443	442	15	24	18.3	8639	PASS