

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081822\
 Data File : BM036346.D
 Acq On : 18 Aug 2022 15:15
 Operator : CG/JU
 Sample : PB146658BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	29	rVB	69467	89501	1.93%	0.175%
2	3.628	89	92	115	rBV	595646	952570	20.56%	1.867%
3	3.952	143	147	153	rVB	16359	22775	0.49%	0.045%
4	6.969	654	660	675	rBV	835604	1411207	30.46%	2.766%
5	7.128	681	687	702	rVB	725719	1146115	24.74%	2.246%
6	7.322	713	720	742	rVB	894977	1434723	30.97%	2.812%
7	7.792	794	800	816	rVB	879060	1376017	29.70%	2.697%
8	8.516	916	923	941	rBV	1022756	1704398	36.79%	3.341%
9	8.963	989	999	1012	rBV	833579	1382061	29.84%	2.709%
10	9.681	1114	1121	1135	rBV	647861	1088530	23.50%	2.134%
11	10.222	1206	1213	1230	rBV	906369	1653139	35.69%	3.240%
12	10.592	1269	1276	1290	rVV	1235334	2003098	43.24%	3.926%
13	10.745	1294	1302	1324	rBV	849946	1630698	35.20%	3.196%
14	12.198	1543	1549	1559	rBV2	13040	31808	0.69%	0.062%
15	13.857	1824	1831	1842	rBV	1634296	2278974	49.20%	4.467%
16	14.133	1870	1878	1891	rBV	2059689	2918150	63.00%	5.720%
17	14.439	1923	1930	1943	rBV	1802415	2487853	53.71%	4.876%
18	14.669	1963	1969	1990	rBV	433142	1045002	22.56%	2.048%
19	15.433	2090	2099	2115	rBV	2514908	3567816	77.02%	6.993%
20	15.563	2115	2121	2135	rVV	599743	924443	19.96%	1.812%
21	15.668	2135	2139	2149	rVB	25012	46814	1.01%	0.092%
22	16.215	2227	2232	2236	rVB6	5755	7997	0.17%	0.016%
23	16.315	2245	2249	2257	rBV10	4003	8052	0.17%	0.016%
24	16.645	2302	2305	2314	rVV4	6611	14424	0.31%	0.028%
25	16.968	2353	2360	2364	rBV8	4834	11685	0.25%	0.023%
26	17.180	2390	2396	2406	rBV	1939281	2711813	58.54%	5.315%
27	17.280	2407	2413	2435	rVB	2732677	3815815	82.37%	7.479%
28	17.715	2484	2487	2490	rBV3	5207	5911	0.13%	0.012%
29	18.098	2547	2552	2555	rBV6	9723	18349	0.40%	0.036%
30	18.162	2559	2563	2567	rBV6	5518	10197	0.22%	0.020%
31	19.139	2725	2729	2734	rBV2	28380	43201	0.93%	0.085%
32	19.215	2738	2742	2746	rBV2	26231	37756	0.82%	0.074%
33	19.580	2798	2804	2819	rBV	3226720	4333038	93.54%	8.493%
34	20.580	2971	2974	2978	rVB	153624	158308	3.42%	0.310%
35	21.368	3104	3108	3117	rBV	2206185	2914939	62.93%	5.713%
36	23.550	3473	3479	3494	rVB2	2328772	4632296	100.00%	9.079%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081822\
Data File : BM036346.D
Acq On : 18 Aug 2022 15:15
Operator : CG/JU
Sample : PB146658BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK658

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Title : SVOA CALIBRATION

37 23.697 3498 3504 3518 rVB2 1564289 3100236 66.93% 6.077%




Sum of corrected areas: 51019709

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081822\
Data File : BM036346.D
Acq On : 18 Aug 2022 15:15
Operator : CG/JU
Sample : PB146658BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

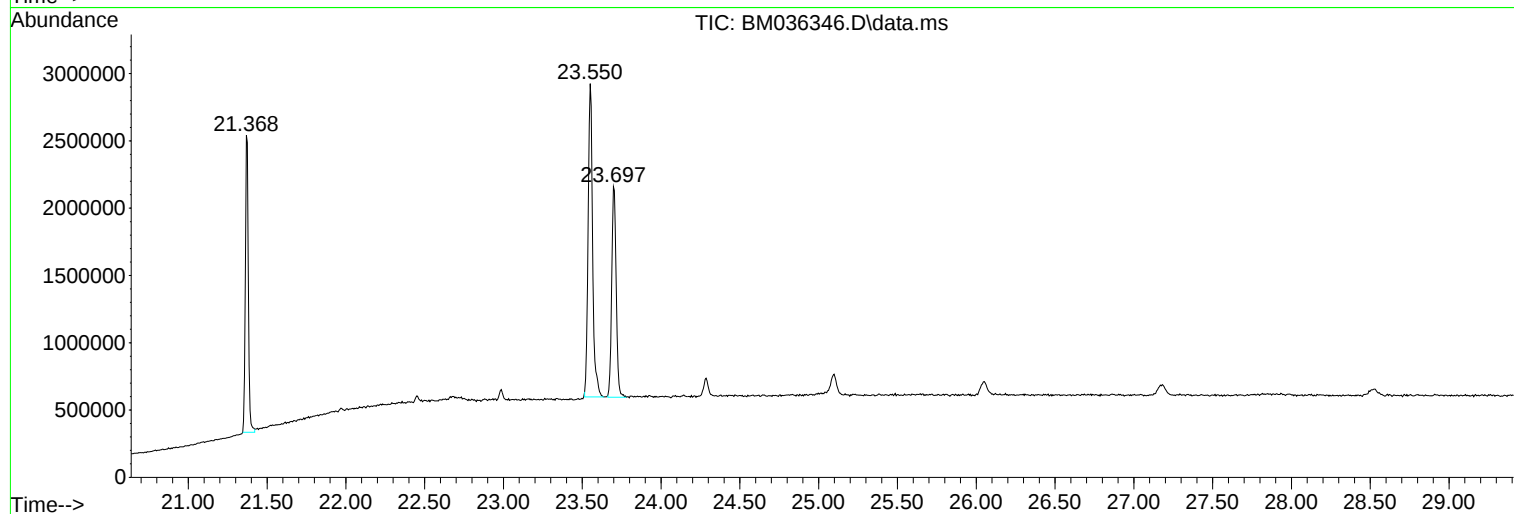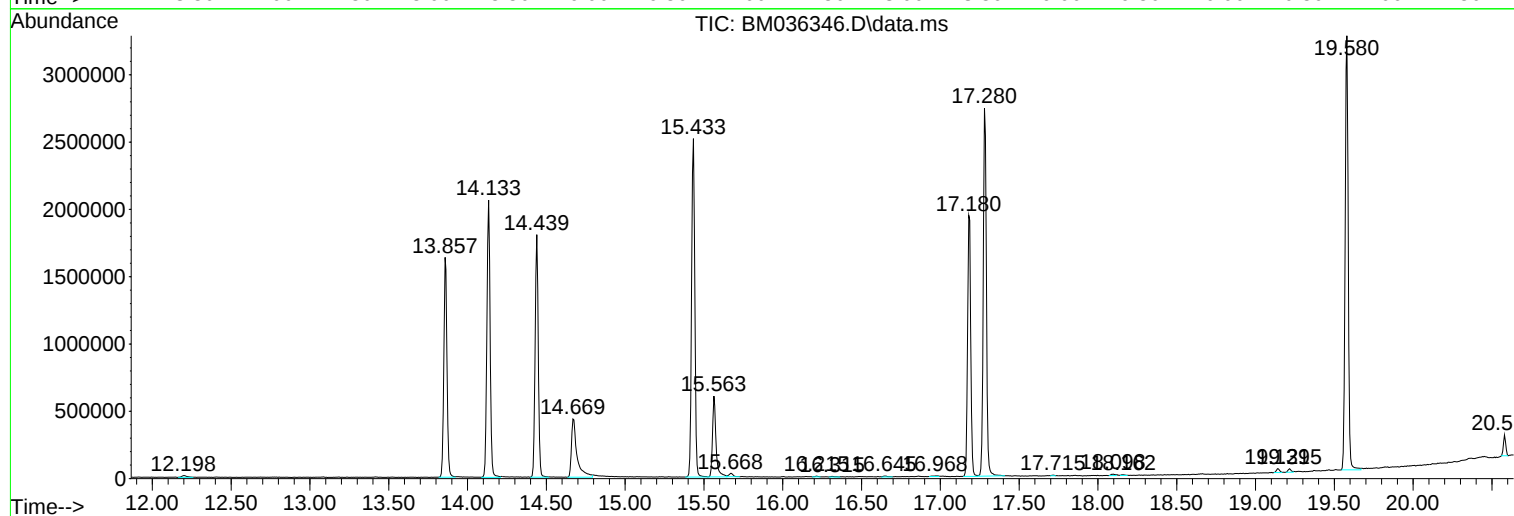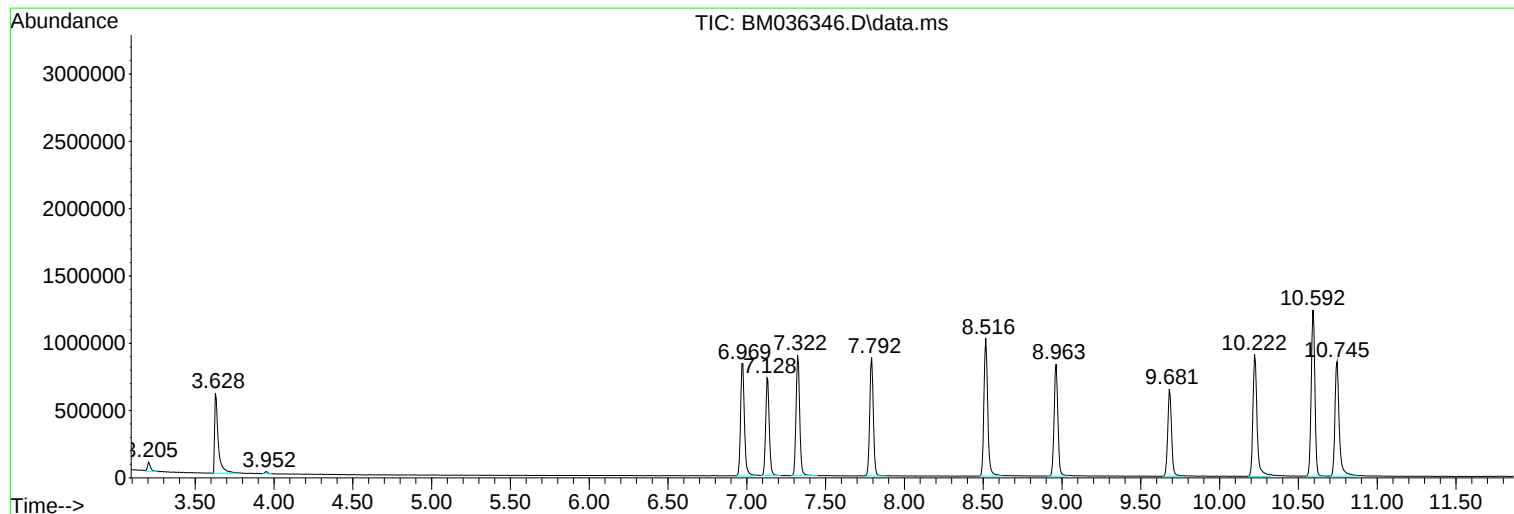

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081822\
Data File : BM036346.D
Acq On : 18 Aug 2022 15:15
Operator : CG/JU
Sample : PB146658BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081822\
Data File : BM036346.D
Acq On : 18 Aug 2022 15:15
Operator : CG/JU
Sample : PB146658BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK658

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM081622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc