


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081915\
Data File : BM002487.D
Acq On : 19 Aug 2015 11:40
Operator : UM/IZ
Sample : DFTPP03
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP03

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715.M
Title : SVOA CALIBRATION
Last Update : Thu Aug 20 05:32:43 2015

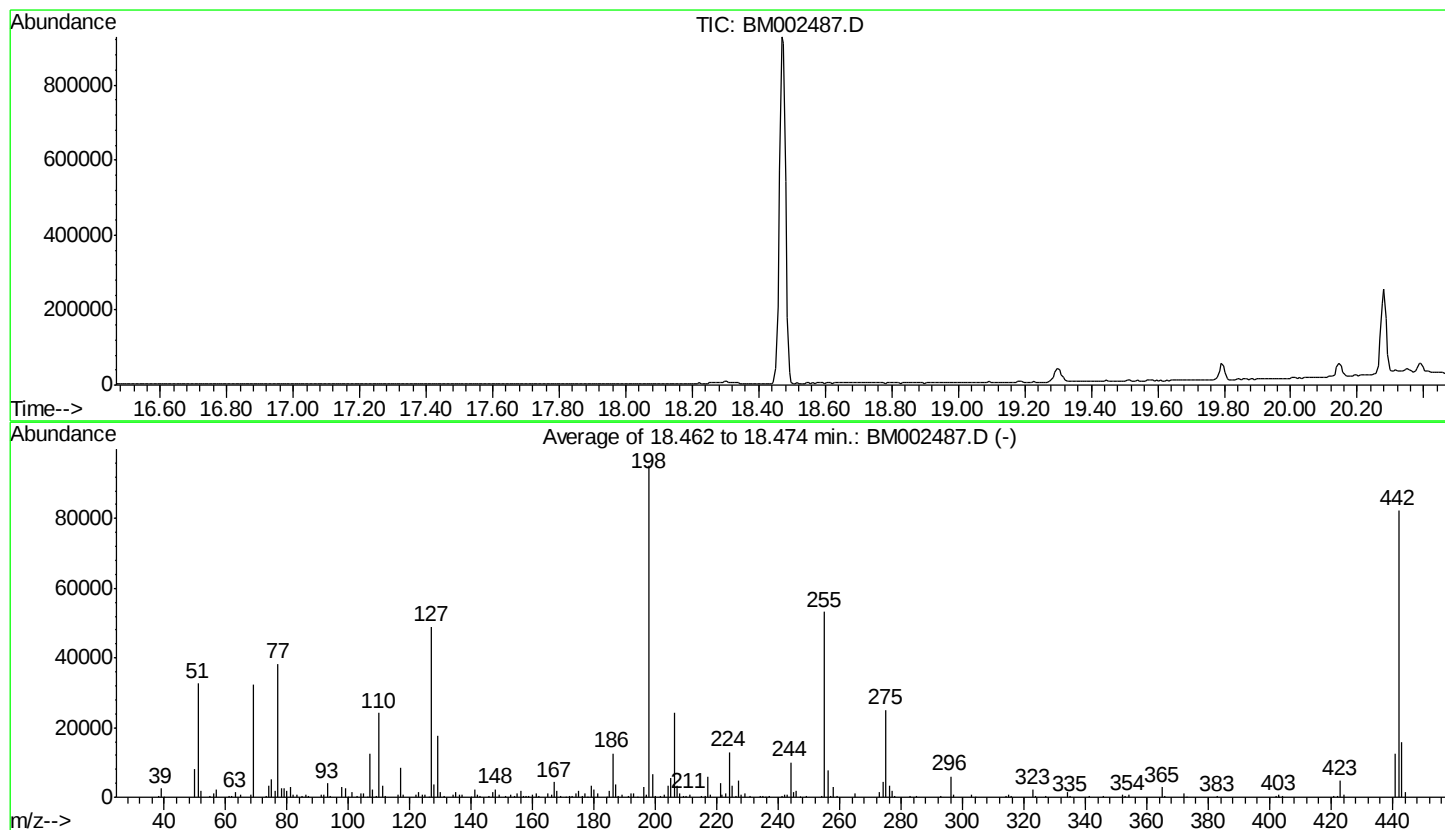

AutoFind: Scans 2614, 2615, 2616; Background Corrected with Scan 2609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	32592	PASS
68	69	0.00	2	1.9	627	PASS
69	198	0.00	100	34.1	32509	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	49026	PASS
197	198	0.00	2	0.6	606	PASS
198	198	100	100	100.0	95218	PASS
199	198	5	9	6.9	6611	PASS
275	198	10	60	26.3	25008	PASS
365	198	1	100	3.0	2868	PASS
441	443	0.01	100	78.3	12529	PASS
442	198	50	100	86.4	82245	PASS
443	442	15	24	19.4	15992	PASS

m/z	Abundance
39.00	2166.0
39.90	415.0
43.10	310.0
44.00	2535.0
50.00	6827.0
51.00	26888.0
52.00	1484.0
55.10	342.0
56.00	912.0
57.00	2092.0
62.00	399.0
63.00	1176.0
65.00	525.0
68.20	481.0
69.00	26896.0
73.00	708.0
74.00	2664.0
75.00	4284.0
76.10	1565.0
77.00	31200.0
78.00	2305.0
79.00	1966.0
80.00	1447.0
81.00	2345.0
82.00	598.0
83.00	531.0
85.00	482.0
85.90	666.0
87.00	339.0
91.00	558.0
92.00	504.0
93.00	3185.0
93.90	318.0
98.00	2607.0
99.00	2076.0
101.00	1265.0
102.90	437.0
104.00	861.0
105.00	867.0
107.00	9905.0
108.00	1708.0
109.10	402.0
110.00	19504.0
111.00	2766.0
111.90	397.0
116.00	607.0
117.00	6835.0
117.90	489.0
121.90	692.0
122.90	1026.0
123.90	531.0
124.90	530.0
127.00	37664.0
128.00	3092.0
129.00	13627.0
129.90	1169.0
133.90	479.0
135.00	1142.0
135.90	494.0
137.00	604.0
141.00	1633.0
141.90	627.0
142.90	365.0
145.90	361.0
147.00	1153.0
148.00	1788.0
148.90	529.0
153.00	537.0
153.90	496.0
155.00	963.0
156.00	1393.0
157.90	363.0
160.10	540.0
160.90	800.0
164.90	658.0
165.90	584.0
167.00	3357.0
168.00	1587.0
168.90	430.0
172.00	339.0
173.00	339.0
174.00	801.0
175.00	1385.0
176.00	369.0
176.90	731.0
178.90	2434.0
180.00	1834.0
181.00	790.0
184.90	1246.0
186.00	8909.0
186.90	2668.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

187.90	339.0
188.90	568.0
191.00	372.0
192.00	824.0
193.00	940.0
195.90	1976.0
196.80	376.0
197.10	450.0
197.90	67520.0
199.00	5018.0
199.90	464.0
201.30	355.0
202.90	550.0
204.00	2354.0
205.00	3988.0
206.00	17296.0
207.00	3302.0
207.90	771.0
211.00	758.0
216.00	386.0
217.00	4229.0
217.90	510.0
221.10	2734.0
221.70	645.0
223.00	974.0
224.00	8887.0
225.00	2321.0
227.00	3144.0
227.90	543.0
228.90	760.0
230.90	327.0
237.00	341.0
242.00	424.0
243.00	501.0
244.00	6991.0
245.00	1037.0
245.90	1311.0
249.00	304.0
255.00	35992.0
256.00	5639.0
256.80	416.0
258.00	1884.0
264.90	773.0
273.00	993.0
274.00	3061.0
275.00	16600.0
276.00	2267.0
276.90	1279.0
282.90	309.0
293.00	412.0
296.00	4014.0
296.90	555.0
303.00	458.0
314.90	455.0
323.00	1231.0
334.00	832.0
346.00	336.0
351.90	495.0
353.90	395.0
365.00	1861.0
365.90	302.0
372.00	645.0
402.00	316.0
402.90	421.0
423.00	2491.0
423.90	460.0
441.00	7085.0
442.00	45376.0
443.00	9241.0
444.00	861.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	435.0
39.00	2995.0
40.00	479.0
41.00	348.0
43.00	401.0
44.00	2557.0
50.00	9383.0
51.00	38192.0
52.00	1912.0
55.00	391.0
56.00	1267.0
57.00	2539.0
61.00	390.0
62.00	494.0
63.00	1430.0
65.00	857.0
68.00	720.0
69.00	38128.0
73.00	505.0
74.00	3879.0
75.00	5773.0
76.00	2202.0
77.00	44568.0
78.00	3132.0
79.00	2764.0
80.00	2282.0
81.00	3315.0
82.00	870.0
83.00	843.0
85.00	650.0
85.90	923.0
86.90	434.0
91.00	887.0
92.00	684.0
93.00	4599.0
94.00	314.0
98.00	3640.0
99.00	3158.0
100.00	311.0
101.00	1825.0
103.00	642.0
104.00	1200.0
105.00	1125.0
106.10	338.0
107.00	14203.0
108.00	2304.0
109.00	466.0
110.00	28048.0
111.00	4055.0
112.00	492.0
116.00	777.0
117.00	9938.0
117.90	806.0
122.00	1144.0
123.00	1659.0
123.90	689.0
124.90	715.0
126.20	327.0
127.00	57480.0
128.00	4115.0
129.00	20696.0
130.00	1839.0
131.00	377.0
133.90	604.0
135.00	1665.0
136.00	680.0
137.00	867.0
141.00	2521.0
142.00	794.0
142.80	597.0
145.90	391.0
147.00	1662.0
148.00	2685.0
149.00	733.0
151.10	402.0
153.00	847.0
153.90	543.0
155.00	1383.0
156.00	2390.0
157.00	512.0
157.90	499.0
158.80	361.0
159.90	689.0
160.90	1168.0
162.00	336.0
164.90	1085.0
166.00	776.0
167.00	5010.0
168.00	2210.0
169.00	439.0
170.90	341.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

172.00	421.0
172.90	589.0
174.00	1115.0
175.00	2268.0
176.00	616.0
177.00	964.0
178.90	4052.0
179.90	2580.0
181.00	1195.0
184.00	302.0
185.00	1854.0
186.00	14772.0
187.00	3988.0
188.00	561.0
189.00	967.0
191.00	581.0
191.90	1044.0
192.90	1424.0
196.00	3285.0
196.80	682.0
197.00	684.0
197.90	110576.0
199.00	7615.0
199.90	636.0
201.40	537.0
203.00	844.0
204.00	3909.0
205.00	6281.0
206.00	28112.0
207.00	4263.0
208.00	1109.0
209.00	420.0
210.00	390.0
211.10	1007.0
214.90	328.0
216.00	596.0
217.00	6677.0
218.00	935.0
221.00	4666.0
221.70	1063.0
223.00	1592.0
224.00	15128.0
225.00	3697.0
226.00	385.0
227.00	5671.0
227.90	785.0
229.00	1297.0
231.00	462.0
233.90	375.0
235.00	415.0
236.90	516.0
241.00	360.0
242.00	890.0
243.00	744.0
244.00	11639.0
245.00	1704.0
246.00	2526.0
246.80	364.0
248.90	481.0
254.10	474.0
255.00	61408.0
256.00	9081.0
256.90	568.0
258.00	3364.0
259.00	562.0
265.00	1353.0
273.00	1874.0
274.00	5080.0
275.00	29160.0
276.00	3629.0
277.00	2233.0
278.00	318.0
283.00	347.0
284.90	474.0
293.00	519.0
296.00	6662.0
296.90	991.0
303.00	912.0
304.00	306.0
313.90	372.0
314.90	629.0
316.00	485.0
323.00	2472.0
323.90	434.0
326.90	505.0
334.00	1463.0
335.00	443.0
341.00	323.0
346.00	506.0
352.00	652.0
353.00	482.0
354.00	747.0
365.00	3317.0
365.90	468.0
372.00	1417.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

382.90	463.0
402.00	602.0
403.10	907.0
404.00	315.0
421.00	742.0
422.00	708.0
423.00	5180.0
424.00	984.0
441.00	13680.0
442.00	91824.0
443.00	17992.0
444.00	1791.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	418.0
39.00	2480.0
39.90	469.0
41.00	352.0
43.00	330.0
44.00	2514.0
50.00	7995.0
51.00	32696.0
52.00	1653.0
55.00	394.0
56.00	1077.0
57.00	2534.0
61.00	382.0
62.00	436.0
63.00	1338.0
65.00	753.0
68.10	682.0
69.00	32504.0
73.00	536.0
74.00	3558.0
75.00	5691.0
76.00	1806.0
77.10	39136.0
78.10	2769.0
79.00	2576.0
80.00	1709.0
81.00	2832.0
82.00	733.0
83.00	879.0
85.00	533.0
86.00	758.0
87.00	417.0
91.00	767.0
91.90	708.0
93.00	4212.0
93.90	323.0
98.00	3090.0
99.00	2583.0
101.00	1825.0
102.90	602.0
104.00	1073.0
104.90	865.0
107.00	13038.0
108.00	2276.0
109.00	418.0
110.00	24832.0
111.00	3477.0
112.00	421.0
116.00	768.0
117.00	9048.0
118.00	699.0
122.00	916.0
123.00	1558.0
124.00	717.0
125.00	506.0
127.00	51936.0
128.00	3897.0
129.00	19136.0
129.90	1668.0
130.90	315.0
134.00	698.0
135.00	1619.0
136.00	612.0
137.00	889.0
139.90	314.0
141.00	2439.0
142.00	833.0
142.90	622.0
145.90	521.0
147.00	1351.0
148.00	2480.0
148.90	702.0
151.00	395.0
153.00	775.0
153.90	652.0
155.00	1471.0
156.00	1929.0
157.00	487.0
157.90	470.0
158.90	309.0
160.00	736.0
161.00	1239.0
161.90	319.0
165.00	1096.0
166.00	667.0
167.00	4633.0
168.00	2179.0
169.00	404.0
172.00	536.0
173.00	655.0
173.90	1003.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

175.00	1971.0
175.90	552.0
176.90	1177.0
177.90	360.0
179.00	3622.0
179.90	2428.0
181.00	1294.0
185.00	2003.0
186.00	14333.0
187.00	3980.0
187.90	411.0
189.00	1031.0
191.00	442.0
192.00	1171.0
193.00	1459.0
194.00	332.0
196.00	3249.0
197.00	686.0
197.90	107560.0
199.00	7201.0
199.90	563.0
201.50	582.0
202.90	729.0
204.00	3566.0
205.00	6526.0
206.00	27296.0
207.00	4619.0
208.00	1123.0
208.90	475.0
210.10	530.0
211.00	1025.0
215.00	314.0
216.10	494.0
217.00	6841.0
218.00	856.0
221.00	4328.0
222.90	1287.0
224.00	14808.0
225.00	3580.0
226.00	436.0
227.00	6103.0
227.90	880.0
229.00	1580.0
230.90	490.0
233.90	428.0
235.00	469.0
235.90	335.0
237.00	548.0
241.00	378.0
242.00	851.0
243.00	834.0
244.00	11430.0
245.00	1388.0
246.00	2064.0
247.00	370.0
249.00	489.0
254.10	496.0
255.00	62392.0
256.00	8988.0
257.00	626.0
258.00	3440.0
259.00	507.0
265.00	1307.0
273.00	1983.0
274.00	4663.0
275.00	29264.0
276.00	4154.0
277.00	2478.0
277.90	336.0
285.00	481.0
292.90	446.0
296.00	7128.0
297.00	1078.0
303.00	899.0
314.00	414.0
315.00	865.0
315.90	520.0
323.00	2509.0
323.90	468.0
326.90	531.0
334.00	1752.0
335.00	393.0
341.00	355.0
345.90	587.0
352.00	777.0
353.00	696.0
354.00	1013.0
365.00	3426.0
366.00	545.0
372.00	1804.0
373.00	443.0
383.00	489.0
401.90	714.0
403.00	1014.0
404.00	364.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

421.00	877.0
422.00	811.0
423.00	6213.0
424.00	1242.0
441.00	16824.0
442.00	109536.0
443.00	20744.0
444.00	1964.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

Scan 2609 (18.433 min): BM002487.D
DFTPP03

m/z	Abundance
40.00	411.0
41.00	330.0
43.00	382.0
44.00	2553.0
73.00	351.0
207.00	744.0
281.00	312.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03