

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007219.D
 Acq On : 18 Aug 2016 23:03
 Operator : UM/SJ
 Sample : H4445-16
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK19

Quant Time: Aug 19 04:49:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 04:48:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	293887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1186556	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	692029	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1623087	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	2092454	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2155488	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	17699	2.63	ng/uL	0.00
5) Phenol-d5	6.97	99	321291	13.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	209077	15.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	274826	14.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	224083	11.44	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	132411	15.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	143376	15.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	276667	14.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	307729	13.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	886109	15.50	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	1076039	15.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	100725	9.83	ng/ul	0.00
57) Fluorene-d10	15.43	176	793190	15.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	80874	9.02	ng/ul	0.00
70) Anthracene-d10	17.27	188	1260003	16.76	ng/ul	0.00
76) Pyrene-d10	19.56	212	1594961	18.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.48	264	1811809	18.38	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.89	163	286224	5.01 ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007219.D
Acq On : 18 Aug 2016 23:03
Operator : UM/SJ
Sample : H4445-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK19

Quant Time: Aug 19 04:49:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 04:48:28 2016
Response via : Initial Calibration

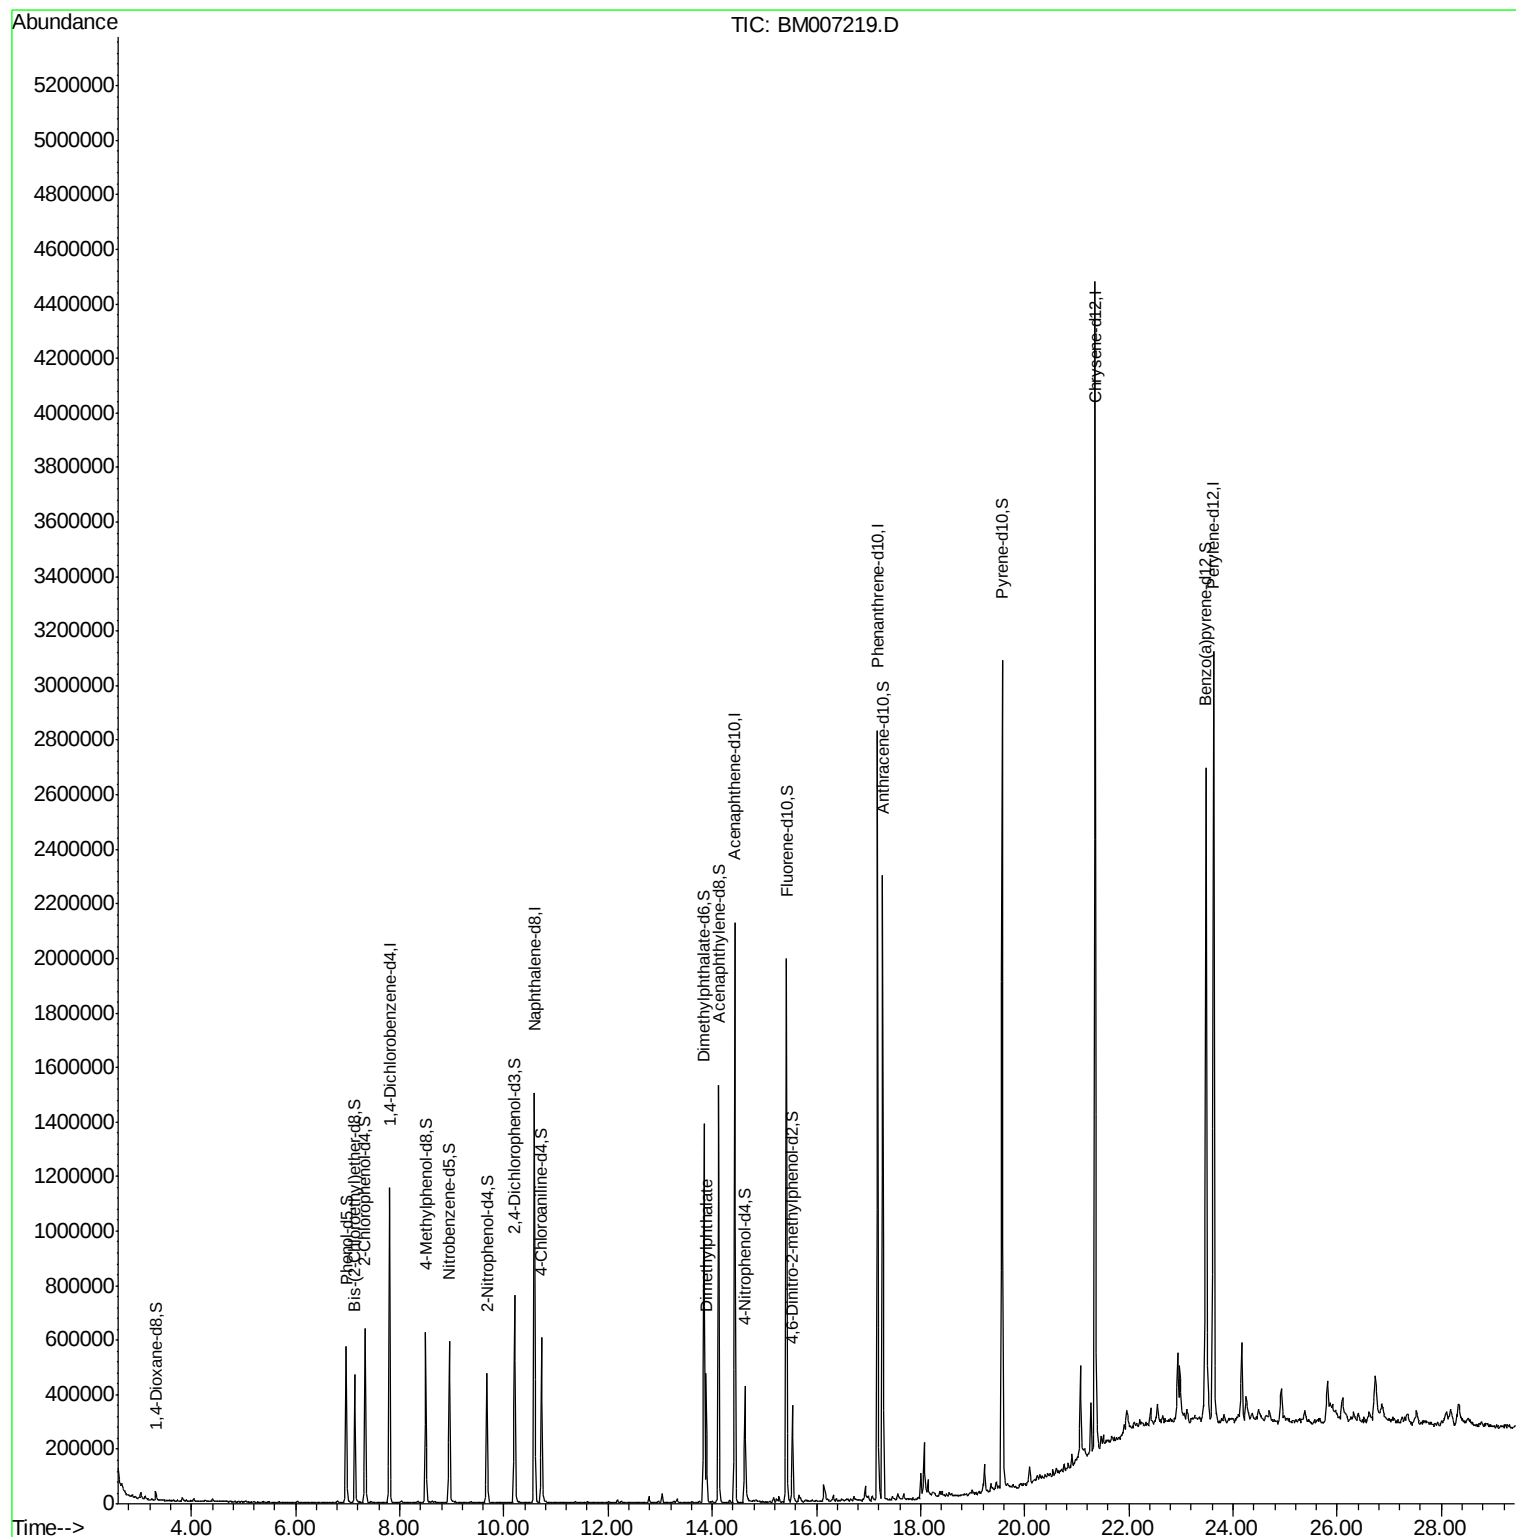

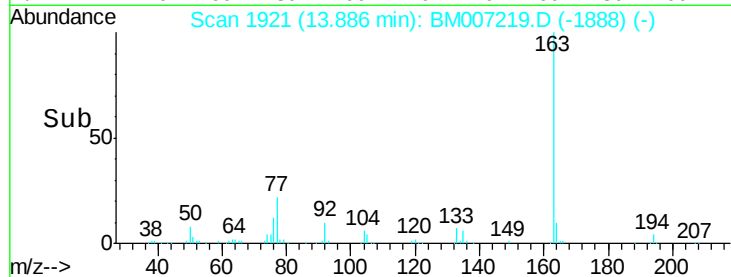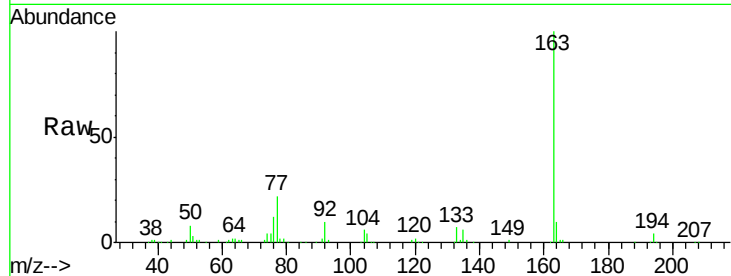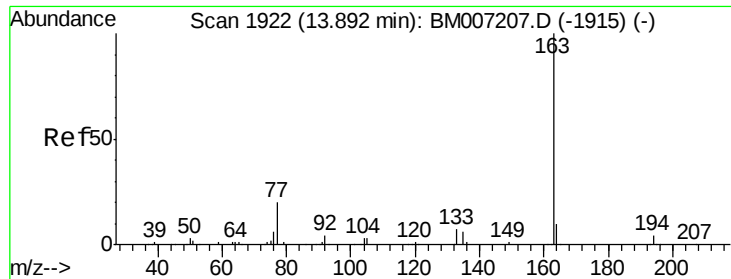

#44

Dimethylphthalate

Concen: 5.01 ng/ul

RT: 13.89 min Scan# 1921

Delta R.T. -0.01 min

Lab File: BM007219.D

Acq: 18 Aug 2016 23:03

Instrument :

BNA_M

ClientSampleId :

SBLK19

Tgt Ion:163 Resp: 286224

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.9 7.8 11.8

