

Data Path : Z:\HPCHEM1\BNA_M\Data\BM081916\
 Data File : BM007237.D
 Acq On : 19 Aug 2016 15:05
 Operator : UM/SJ
 Sample : H4436-16
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA215

Quant Time: Aug 19 15:43:42 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 09:10:25 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	235477	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	954289	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	551840	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1302994	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1557152	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1641818	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	17447	3.24	ng/uL	0.00
5) Phenol-d5	6.97	99	376965	19.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	206510	18.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	301141	19.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	298682	19.03	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	142914	20.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	153935	20.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	309336	19.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	319039	17.29	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	933957	20.48	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1155940	21.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	140559	17.20	ng/ul	0.00
57) Fluorene-d10	15.43	176	838251	21.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	71716	9.96	ng/ul	0.00
70) Anthracene-d10	17.27	188	1330101	22.03	ng/ul	0.00
76) Pyrene-d10	19.57	212	1595665	24.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	1662896	22.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.89	163	728594	15.99	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM081916\
Data File : BM007237.D
Acq On : 19 Aug 2016 15:05
Operator : UM/SJ
Sample : H4436-16
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA215

Quant Time: Aug 19 15:43:42 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 09:10:25 2016
Response via : Initial Calibration

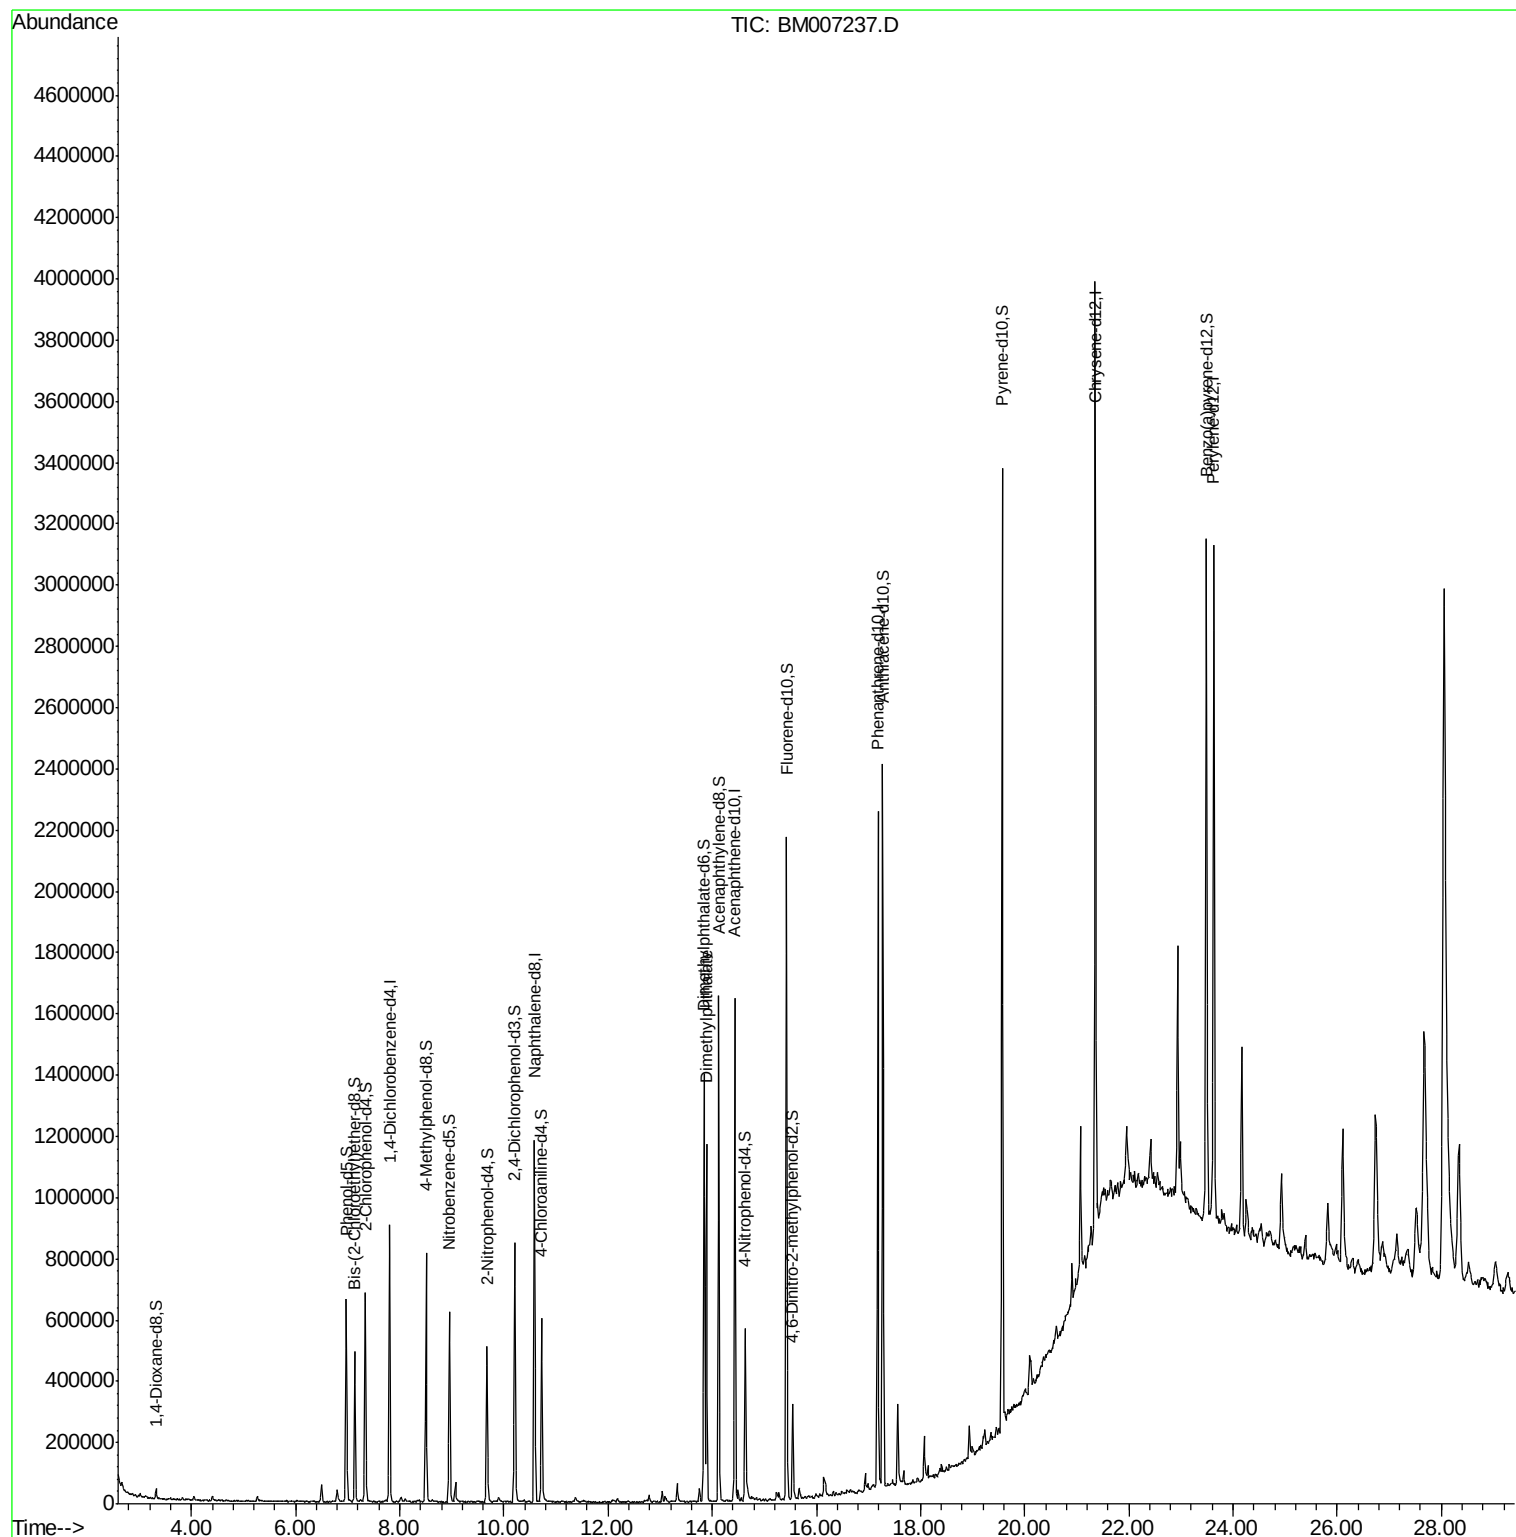

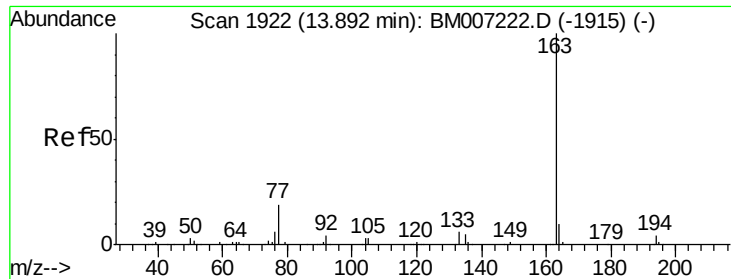

#44

Dimethylphthalate

Concen: 15.99 ng/ul

RT: 13.89 min Scan# 1922

Delta R.T. 0.00 min

Lab File: BM007237.D

Acq: 19 Aug 2016 15:05

Instrument :

BNA_M

ClientSampleId :

DA215


Tgt Ion:163 Resp: 728594

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 10.3 7.8 11.8

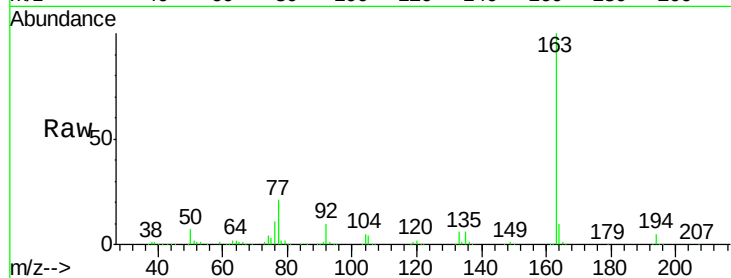

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

