

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007209.D
 Acq On : 18 Aug 2016 18:15
 Operator : UM/SJ
 Sample : H4445-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N21

Quant Time: Aug 19 04:48:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 04:48:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	246502	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	992580	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	583742	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1374831	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1787122	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1851381	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	27557	4.88	ng/uL	0.00
5) Phenol-d5	6.97	99	524087	26.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	315878	27.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	434039	27.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	420617	25.60	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	203617	28.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	227589	29.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	432237	26.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	534205	27.83	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1312486	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1620266	27.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	169388	19.59	ng/ul	0.00
57) Fluorene-d10	15.43	176	1154255	27.38	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	139084	18.31	ng/ul	0.00
70) Anthracene-d10	17.27	188	1837353	28.85	ng/ul	0.00
76) Pyrene-d10	19.57	212	2241564	29.72	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2514843	29.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.89	163	495140	10.27	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007209.D
Acq On : 18 Aug 2016 18:15
Operator : UM/SJ
Sample : H4445-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N21

Quant Time: Aug 19 04:48:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 04:48:28 2016
Response via : Initial Calibration

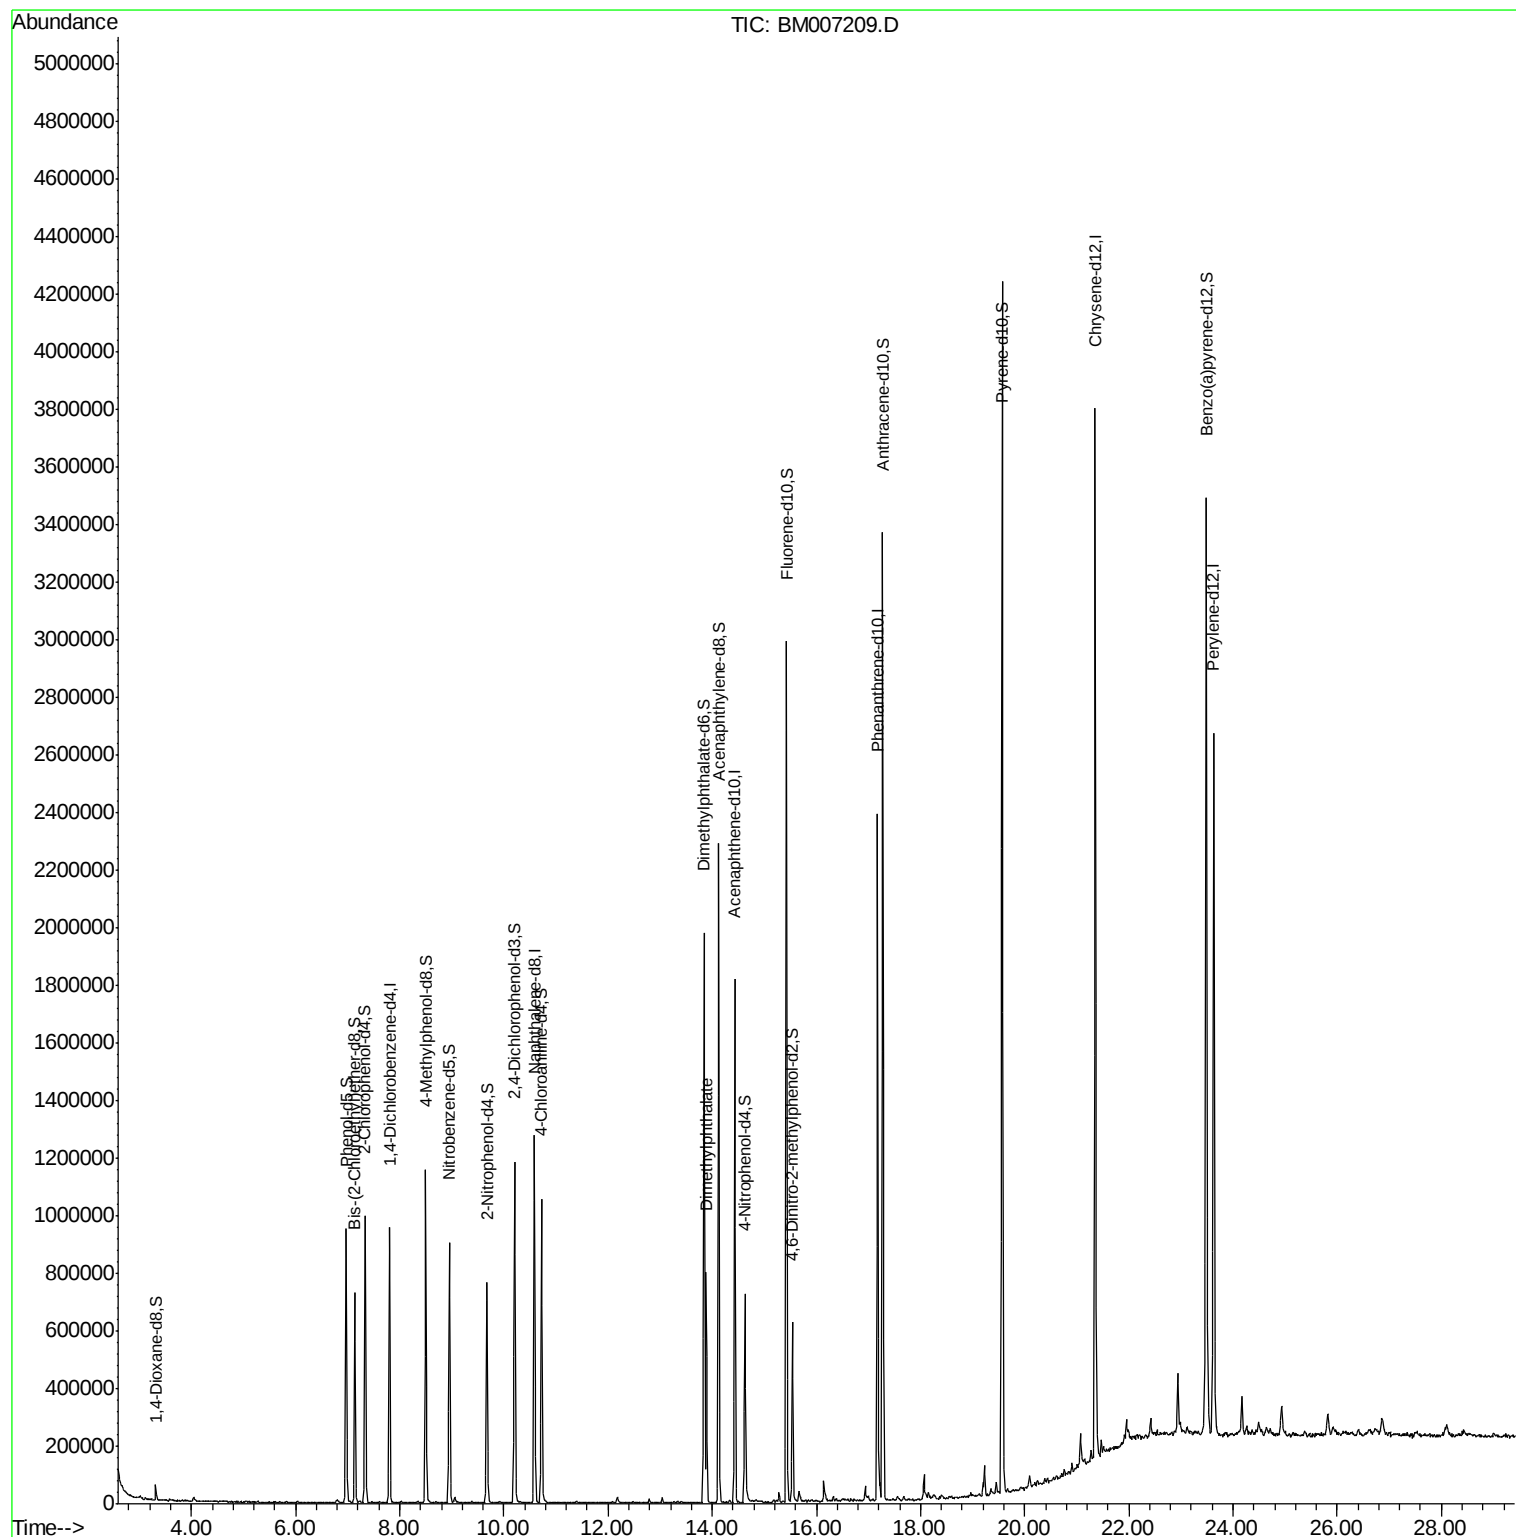

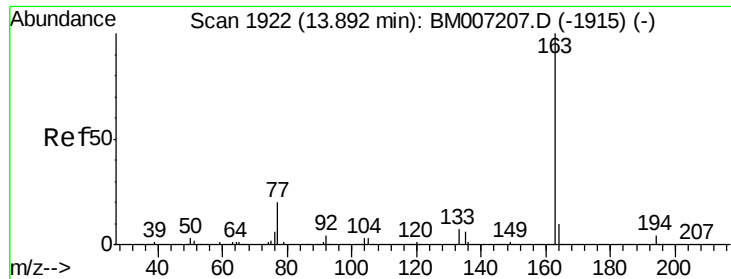

#44
 Dimethylphthalate
 Concen: 10.27 ng/ul
 RT: 13.89 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BM007209.D
 Acq: 18 Aug 2016 18:15

Instrument :
 BNA_M
 ClientSampleId :
 E5N21

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	10.4	7.8	11.8

