

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007232.D
 Acq On : 19 Aug 2016 12:05
 Operator : UM/SJ
 Sample : H4436-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA216

Quant Time: Aug 19 13:18:14 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 09:10:25 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	253497	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1015255	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	579283	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1367484	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1613634	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	1657424	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	13131	2.26	ng/uL	0.00
5) Phenol-d5	6.97	99	270493	13.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	158034	13.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	219699	13.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	221235	13.09	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	96252	13.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	101201	12.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	219387	13.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	198733	10.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	661632	13.82	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	827919	14.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	86477	10.08	ng/ul	0.00
57) Fluorene-d10	15.43	176	605071	14.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	45084	5.97	ng/ul	0.00
70) Anthracene-d10	17.27	188	960938	15.17	ng/ul	0.00
76) Pyrene-d10	19.57	212	1136195	16.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	1158780	15.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.89	163	260465	5.44	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007232.D
Acq On : 19 Aug 2016 12:05
Operator : UM/SJ
Sample : H4436-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA216

Quant Time: Aug 19 13:18:14 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 09:10:25 2016
Response via : Initial Calibration

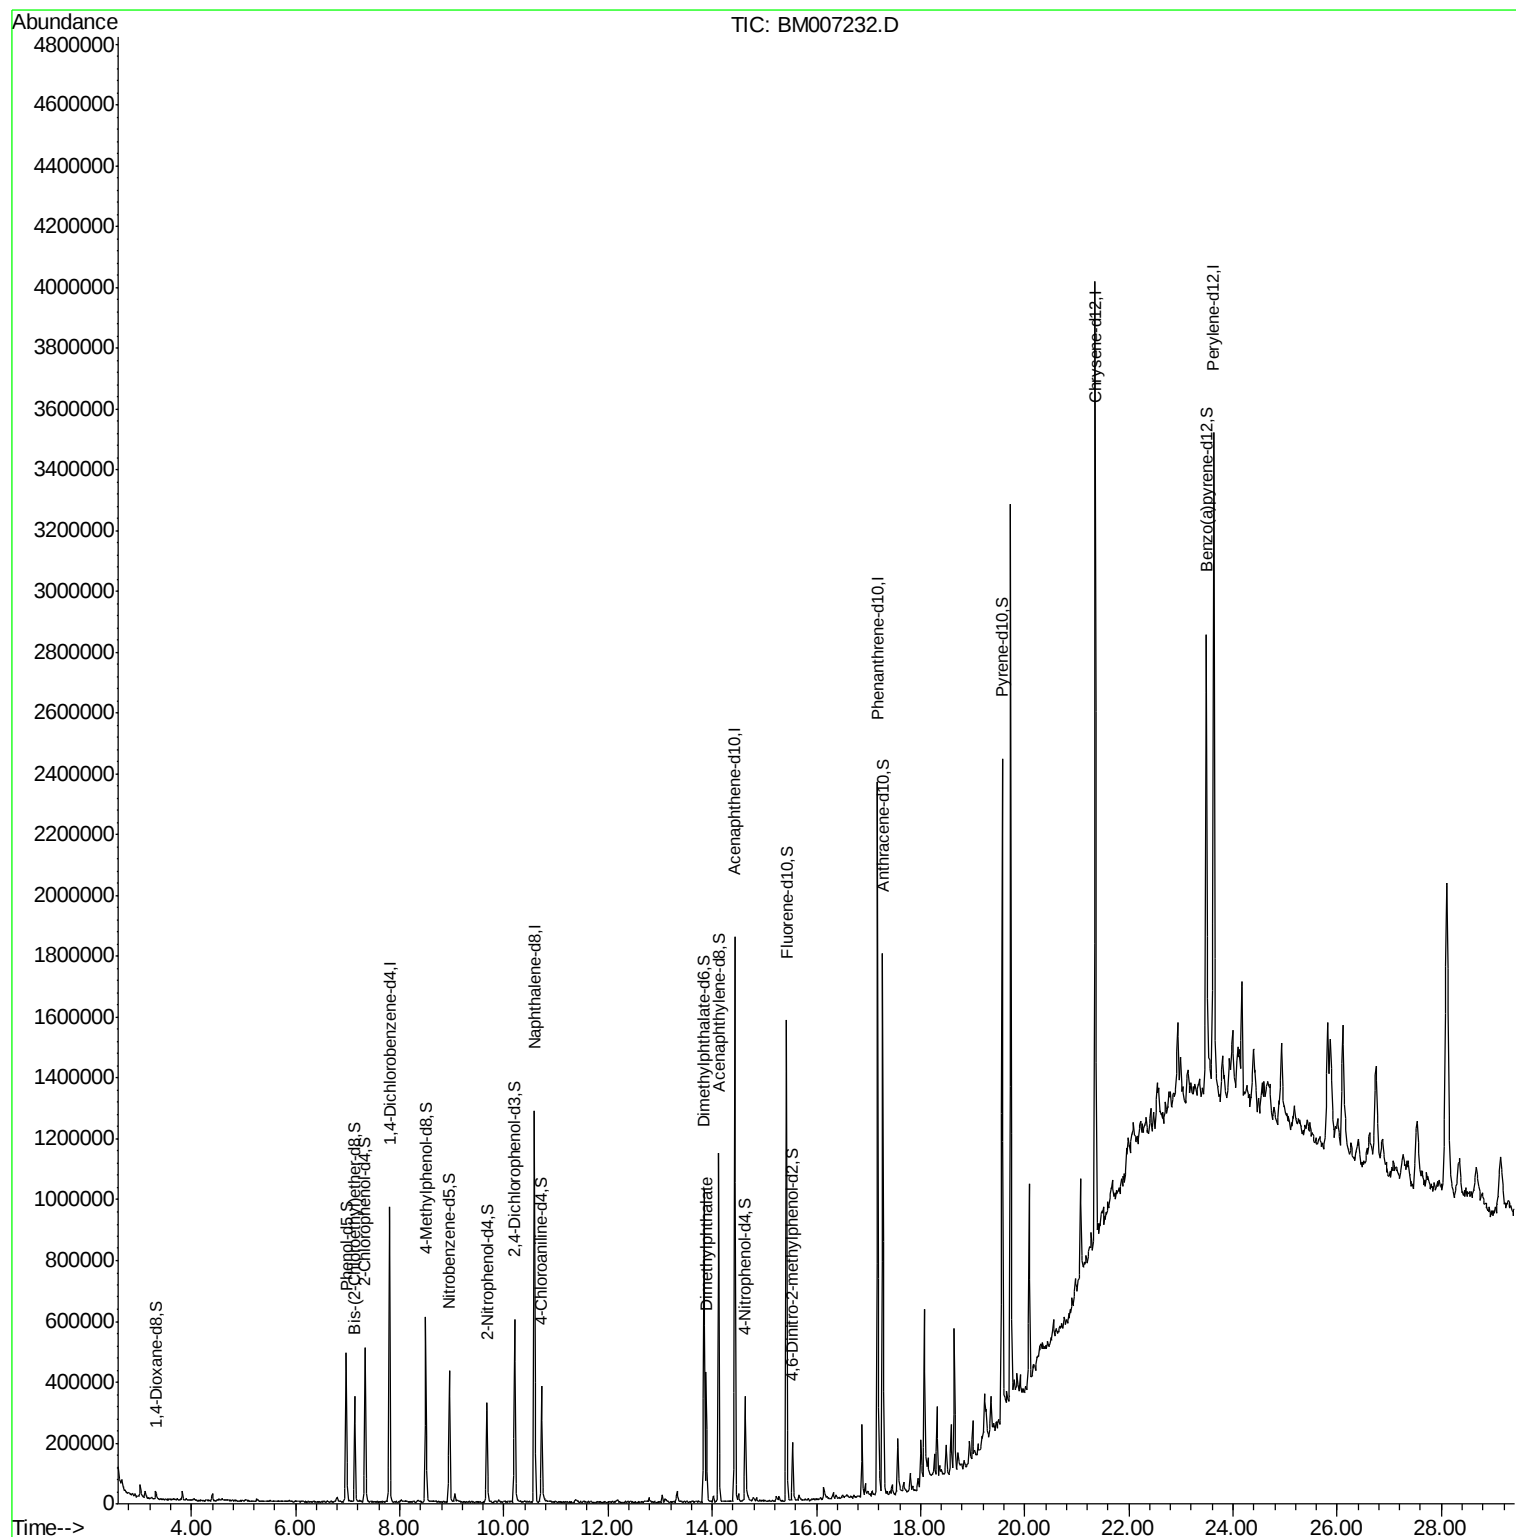


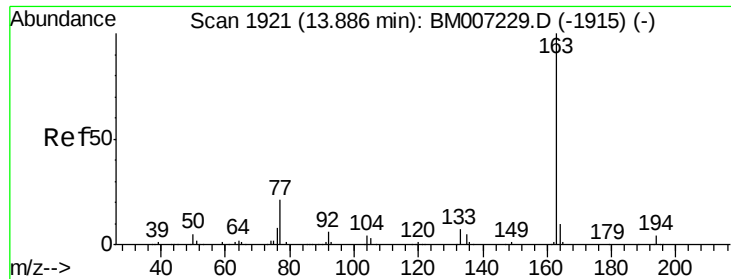

#44
 Dimethylphthalate
 Concen: 5.44 ng/ul
 RT: 13.89 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BM007232.D
 Acq: 19 Aug 2016 12:05

Instrument :
 BNA_M
 ClientSampleId :
 DA216

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.3	7.8	11.8

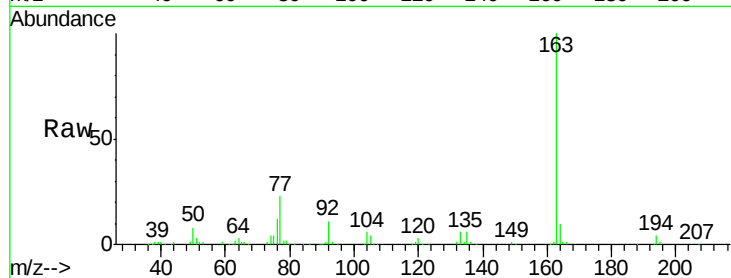

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

