

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007236.D
 Acq On : 19 Aug 2016 14:29
 Operator : UM/SJ
 Sample : H4436-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA210

Quant Time: Aug 19 15:06:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 19 09:10:25 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	216664	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	887205	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	513354	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1112332	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1302857	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1347899	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	8988	1.81	ng/uL	0.00
5) Phenol-d5	6.97	99	217882	12.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	122555	12.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	176776	12.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	172508	11.94	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	81966	12.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	86706	12.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	180110	12.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	178942	10.43	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	565609	13.33	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	700472	13.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	71455	9.40	ng/ul	0.00
57) Fluorene-d10	15.43	176	512122	13.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	19895	3.24	ng/ul	0.00
70) Anthracene-d10	17.27	188	741207	14.38	ng/ul	0.00
76) Pyrene-d10	19.57	212	936469	17.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	976923	15.85	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.89	163	197266	4.65	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007236.D
Acq On : 19 Aug 2016 14:29
Operator : UM/SJ
Sample : H4436-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA210

Quant Time: Aug 19 15:06:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 19 09:10:25 2016
Response via : Initial Calibration

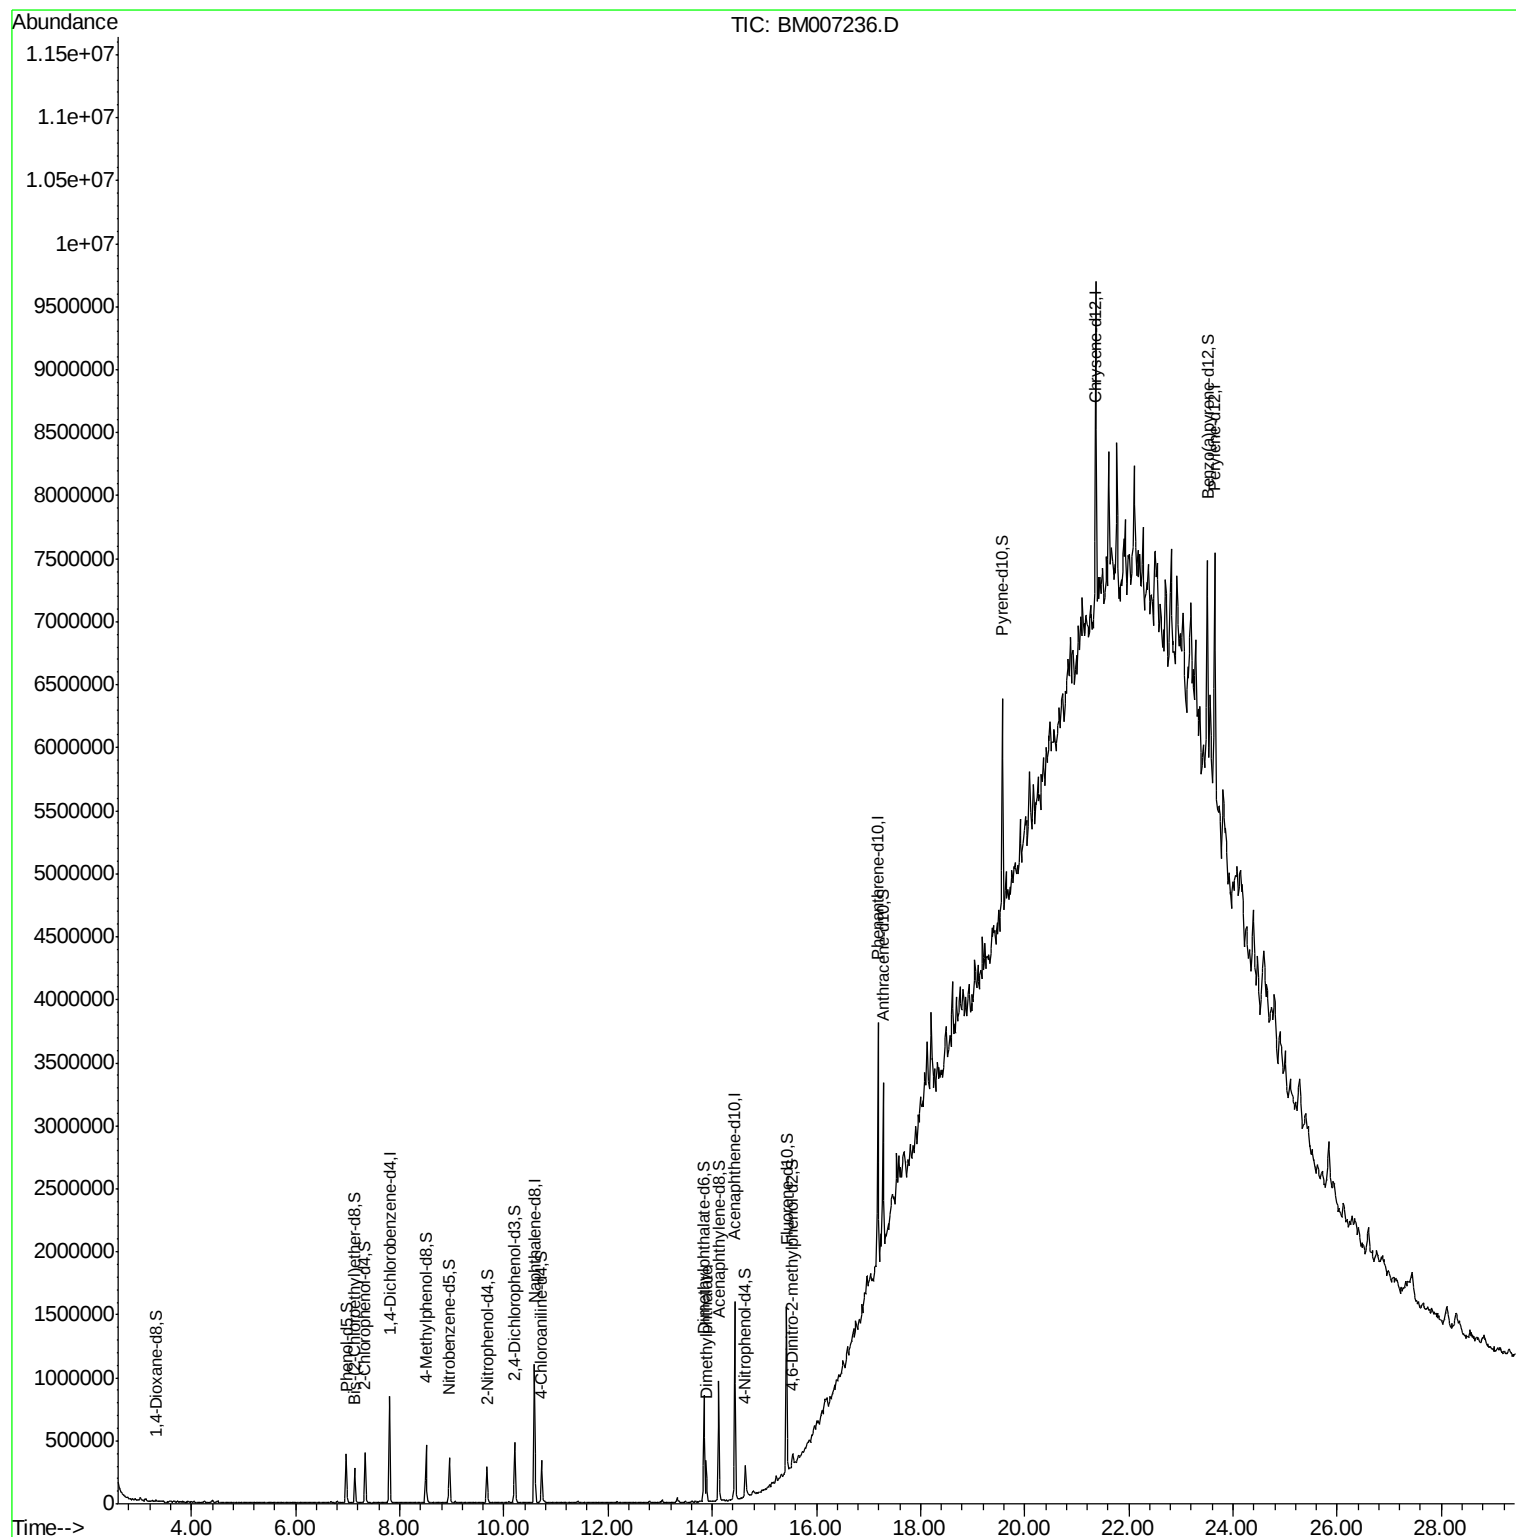


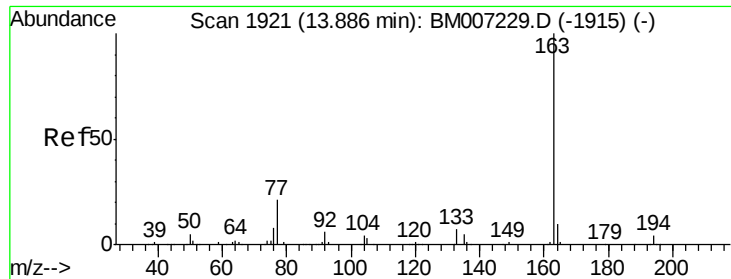

#44
 Dimethylphthalate
 Concen: 4.65 ng/ul
 RT: 13.89 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BM007236.D
 Acq: 19 Aug 2016 14:29

Instrument :
 BNA_M
 ClientSampleId :
 DA210

Tgt Ion:163 Resp: 197266
 Ion Ratio Lower Upper
 163 100
 194 4.6 3.4 5.2
 164 10.1 7.8 11.8

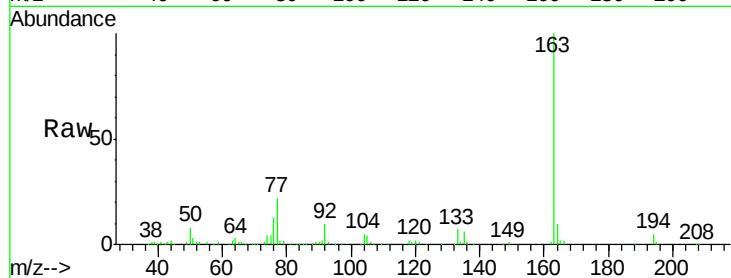

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

