

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007210.D
 Acq On : 18 Aug 2016 18:51
 Operator : UM/SJ
 Sample : H4445-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	121	124	131	rBV	39326	55681	1.00%	0.092%
2	6.969	738	745	753	rBV	672377	1084341	19.49%	1.799%
3	7.140	768	774	780	rBV	565843	885309	15.91%	1.469%
4	7.334	800	807	818	rVB	752735	1233528	22.17%	2.046%
5	7.451	818	827	834	rVB3	39727	81803	1.47%	0.136%
6	7.804	878	887	896	rBV	1002457	1620511	29.12%	2.688%
7	8.498	999	1005	1014	rVB	639148	1029001	18.49%	1.707%
8	8.957	1076	1083	1090	rBV	700983	1156304	20.78%	1.918%
9	9.675	1198	1205	1218	rBV	590193	997084	17.92%	1.654%
10	10.204	1287	1295	1306	rBV	903223	1552680	27.90%	2.576%
11	10.586	1351	1360	1366	rBV	1284145	2233077	40.13%	3.704%
12	10.639	1366	1369	1376	rVB	97870	148717	2.67%	0.247%
13	10.722	1376	1383	1396	rBV	759678	1346235	24.19%	2.233%
14	12.251	1637	1643	1652	rVB	161184	263618	4.74%	0.437%
15	12.469	1674	1680	1688	rVB	90247	140194	2.52%	0.233%
16	13.263	1807	1815	1822	rBV2	77632	121968	2.19%	0.202%
17	13.751	1893	1898	1903	rBV2	51216	90282	1.62%	0.150%
18	13.839	1908	1913	1918	rVV	1615334	2349536	42.22%	3.897%
19	13.886	1918	1921	1931	rVB	599488	863124	15.51%	1.432%
20	14.127	1951	1962	1975	rBV	1833147	2806178	50.43%	4.655%
21	14.333	1993	1997	2002	rVB	57813	75383	1.35%	0.125%
22	14.433	2005	2014	2022	rBV2	1818064	2877961	51.72%	4.774%
23	14.627	2040	2047	2058	rBV	489756	822522	14.78%	1.364%
24	14.833	2077	2082	2089	rVB	98212	149861	2.69%	0.249%
25	15.286	2155	2159	2164	rVB	99057	122780	2.21%	0.204%
26	15.427	2176	2183	2188	rBV	2372423	3497180	62.85%	5.801%
27	15.468	2188	2190	2196	rVB2	43392	60849	1.09%	0.101%
28	15.545	2196	2203	2211	rBV	421029	649376	11.67%	1.077%
29	15.668	2217	2224	2226	rBV2	37652	65175	1.17%	0.108%
30	15.692	2226	2228	2234	rVV3	48862	66561	1.20%	0.110%
31	15.780	2238	2243	2248	rVB4	37331	65554	1.18%	0.109%
32	15.915	2260	2266	2275	rVB5	33717	77658	1.40%	0.129%
33	16.151	2300	2306	2308	rBV	185540	282752	5.08%	0.469%
34	16.721	2397	2403	2406	rBV4	48276	87022	1.56%	0.144%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007210.D
Acq On : 18 Aug 2016 18:51
Operator : UM/SJ
Sample : H4445-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N22

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Title : SVOA CALIBRATION

35	16.833	2418	2422	2429	rVB2	61841	95983	1.72%	0.159%
36	16.939	2429	2440	2446	rBV4	133054	228766	4.11%	0.379%
37	16.992	2446	2449	2453	rVB2	47748	63066	1.13%	0.105%
38	17.174	2474	2480	2485	rBV2	2491810	3600067	64.70%	5.972%
39	17.215	2485	2487	2491	rVV	129171	168753	3.03%	0.280%
40	17.274	2491	2497	2507	rVB	2765532	3919908	70.44%	6.502%
41	17.674	2561	2565	2571	rVB	104920	124006	2.23%	0.206%
42	18.068	2625	2632	2635	rBV3	88945	167174	3.00%	0.277%
43	18.368	2679	2683	2686	rBV	75471	97505	1.75%	0.162%
44	18.974	2782	2786	2788	rBV3	59237	90021	1.62%	0.149%
45	18.998	2788	2790	2797	rVB	76597	96893	1.74%	0.161%
46	19.227	2827	2829	2835	rVB	68674	89663	1.61%	0.149%
47	19.568	2881	2887	2896	rBV	3627339	5306102	95.36%	8.802%
48	19.668	2902	2904	2914	rVB7	70737	136395	2.45%	0.226%
49	20.009	2959	2962	2967	rBV2	61699	74564	1.34%	0.124%
50	20.109	2973	2979	2984	rBV3	87705	160782	2.89%	0.267%
51	20.609	3061	3064	3067	rBV	83606	88079	1.58%	0.146%
52	20.827	3098	3101	3106	rVB	244166	307271	5.52%	0.510%
53	21.074	3139	3143	3149	rBV	158294	226049	4.06%	0.375%
54	21.356	3185	3191	3200	rBV	3855100	5090959	91.49%	8.445%
55	21.509	3214	3217	3221	rVB3	79735	87058	1.56%	0.144%
56	21.950	3289	3292	3295	rBV	85805	89969	1.62%	0.149%
57	22.421	3369	3372	3378	rVB	96749	125955	2.26%	0.209%
58	22.933	3456	3459	3465	rVB2	142198	202042	3.63%	0.335%
59	23.486	3545	3553	3564	rVB2	2815253	5564550	100.00%	9.230%
60	23.627	3570	3577	3585	rVB2	2437040	4840388	86.99%	8.029%
61	24.168	3665	3669	3678	rVB2	141890	284339	5.11%	0.472%


Sum of corrected areas: 60286112

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007210.D
Acq On : 18 Aug 2016 18:51
Operator : UM/SJ
Sample : H4445-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

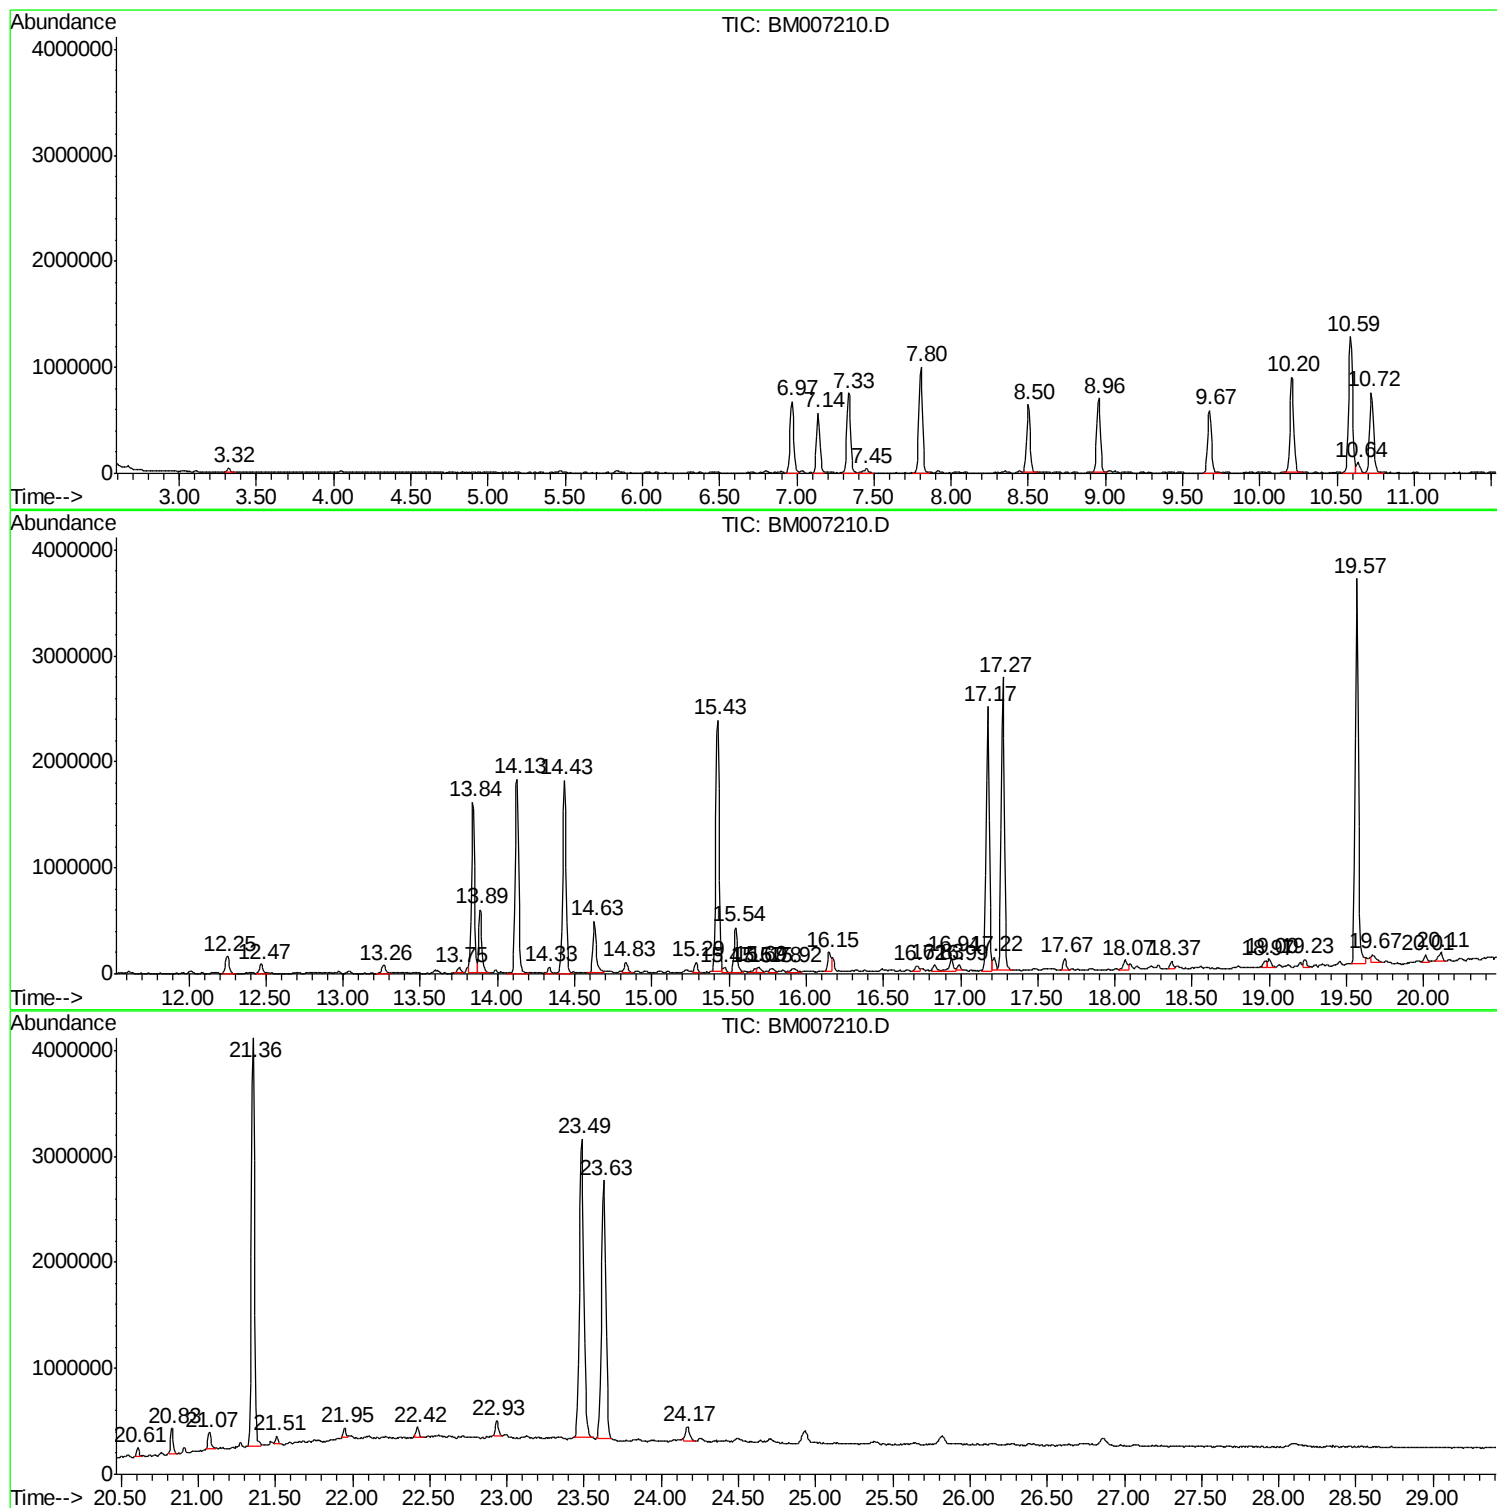

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007210.D
Acq On : 18 Aug 2016 18:51
Operator : UM/SJ
Sample : H4445-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007210.D
Acq On : 18 Aug 2016 18:51
Operator : UM/SJ
Sample : H4445-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N22

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc