

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007211.D
 Acq On : 18 Aug 2016 19:27
 Operator : UM/SJ
 Sample : H4445-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N23

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.663	11	13	23	rVB4	33663	58943	1.09%	0.116%
2	5.810	540	548	560	rVB4	73922	144720	2.69%	0.284%
3	6.969	737	745	753	rBV	500474	827940	15.37%	1.626%
4	7.140	767	774	780	rBV	400048	630686	11.71%	1.239%
5	7.334	800	807	818	rBV	540538	873723	16.22%	1.716%
6	7.451	818	827	834	rVB2	47265	87502	1.62%	0.172%
7	7.804	879	887	898	rVB	1002669	1621489	30.10%	3.184%
8	8.498	999	1005	1014	rVB	474707	782789	14.53%	1.537%
9	8.957	1076	1083	1091	rBV	480750	812797	15.09%	1.596%
10	9.675	1198	1205	1217	rVB	407831	693509	12.87%	1.362%
11	10.204	1288	1295	1304	rBV	626588	1071306	19.89%	2.104%
12	10.586	1351	1360	1366	rBV	1292539	2220342	41.21%	4.360%
13	10.639	1366	1369	1375	rVB	65517	96397	1.79%	0.189%
14	10.722	1376	1383	1400	rBV	515989	929881	17.26%	1.826%
15	12.251	1635	1643	1650	rVB	61901	98622	1.83%	0.194%
16	12.469	1674	1680	1688	rVB	44673	69360	1.29%	0.136%
17	13.839	1908	1913	1918	rVV	1097455	1634995	30.35%	3.211%
18	13.886	1918	1921	1931	rVB	404917	595251	11.05%	1.169%
19	14.127	1952	1962	1972	rBV	1230847	1932469	35.87%	3.795%
20	14.433	2006	2014	2022	rBV2	1867694	2889469	53.63%	5.674%
21	14.627	2041	2047	2058	rBV	345851	609992	11.32%	1.198%
22	14.833	2077	2082	2089	rVB2	41042	69260	1.29%	0.136%
23	15.286	2156	2159	2164	rVB	56620	70262	1.30%	0.138%
24	15.427	2172	2183	2189	rBV	1651599	2471795	45.88%	4.854%
25	15.545	2196	2203	2211	rBV	279359	431591	8.01%	0.848%
26	15.921	2260	2267	2274	rBV7	24350	58861	1.09%	0.116%
27	16.151	2300	2306	2308	rBV2	105352	163459	3.03%	0.321%
28	16.721	2396	2403	2407	rBV5	33211	71216	1.32%	0.140%
29	16.939	2436	2440	2445	rBV2	72335	96682	1.79%	0.190%
30	17.174	2474	2480	2485	rBV2	2395351	3626335	67.31%	7.121%
31	17.215	2485	2487	2491	rVV	166221	215332	4.00%	0.423%
32	17.274	2491	2497	2507	rVB	1926912	2763800	51.30%	5.427%
33	17.674	2562	2565	2576	rVB2	57630	85673	1.59%	0.168%
34	18.068	2625	2632	2635	rBV3	101673	187113	3.47%	0.367%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007211.D
Acq On : 18 Aug 2016 19:27
Operator : UM/SJ
Sample : H4445-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N23

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Title : SVOA CALIBRATION

35	18.098	2635	2637	2642	rVB	54089	65349	1.21%	0.128%
36	18.368	2679	2683	2686	rVB	70850	89772	1.67%	0.176%
37	18.968	2779	2785	2788	rBV5	30266	55624	1.03%	0.109%
38	19.109	2805	2809	2816	rVB6	41272	73083	1.36%	0.144%
39	19.233	2822	2830	2837	rVB	309728	464521	8.62%	0.912%
40	19.568	2880	2887	2898	rBV2	2496844	3955627	73.42%	7.768%
41	20.092	2972	2976	2978	rBV3	53287	75575	1.40%	0.148%
42	21.068	3139	3142	3150	rVB4	210434	311468	5.78%	0.612%
43	21.356	3184	3191	3195	rVV	3742946	5387482	100.00%	10.580%
44	21.392	3195	3197	3203	rVB2	273880	324291	6.02%	0.637%
45	21.509	3214	3217	3222	rBV3	81868	115542	2.14%	0.227%
46	21.950	3289	3292	3294	rBV4	73664	105672	1.96%	0.208%
47	22.938	3455	3460	3465	rBV2	376985	786492	14.60%	1.544%
48	23.427	3539	3543	3546	rBV2	148587	259669	4.82%	0.510%
49	23.480	3546	3552	3567	rVV2	1876838	4183591	77.65%	8.215%
50	23.627	3569	3577	3592	rVB	2497954	5174957	96.06%	10.162%
51	24.168	3664	3669	3676	rVB	241845	501048	9.30%	0.984%


Sum of corrected areas: 50923324

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007211.D
Acq On : 18 Aug 2016 19:27
Operator : UM/SJ
Sample : H4445-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N23

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

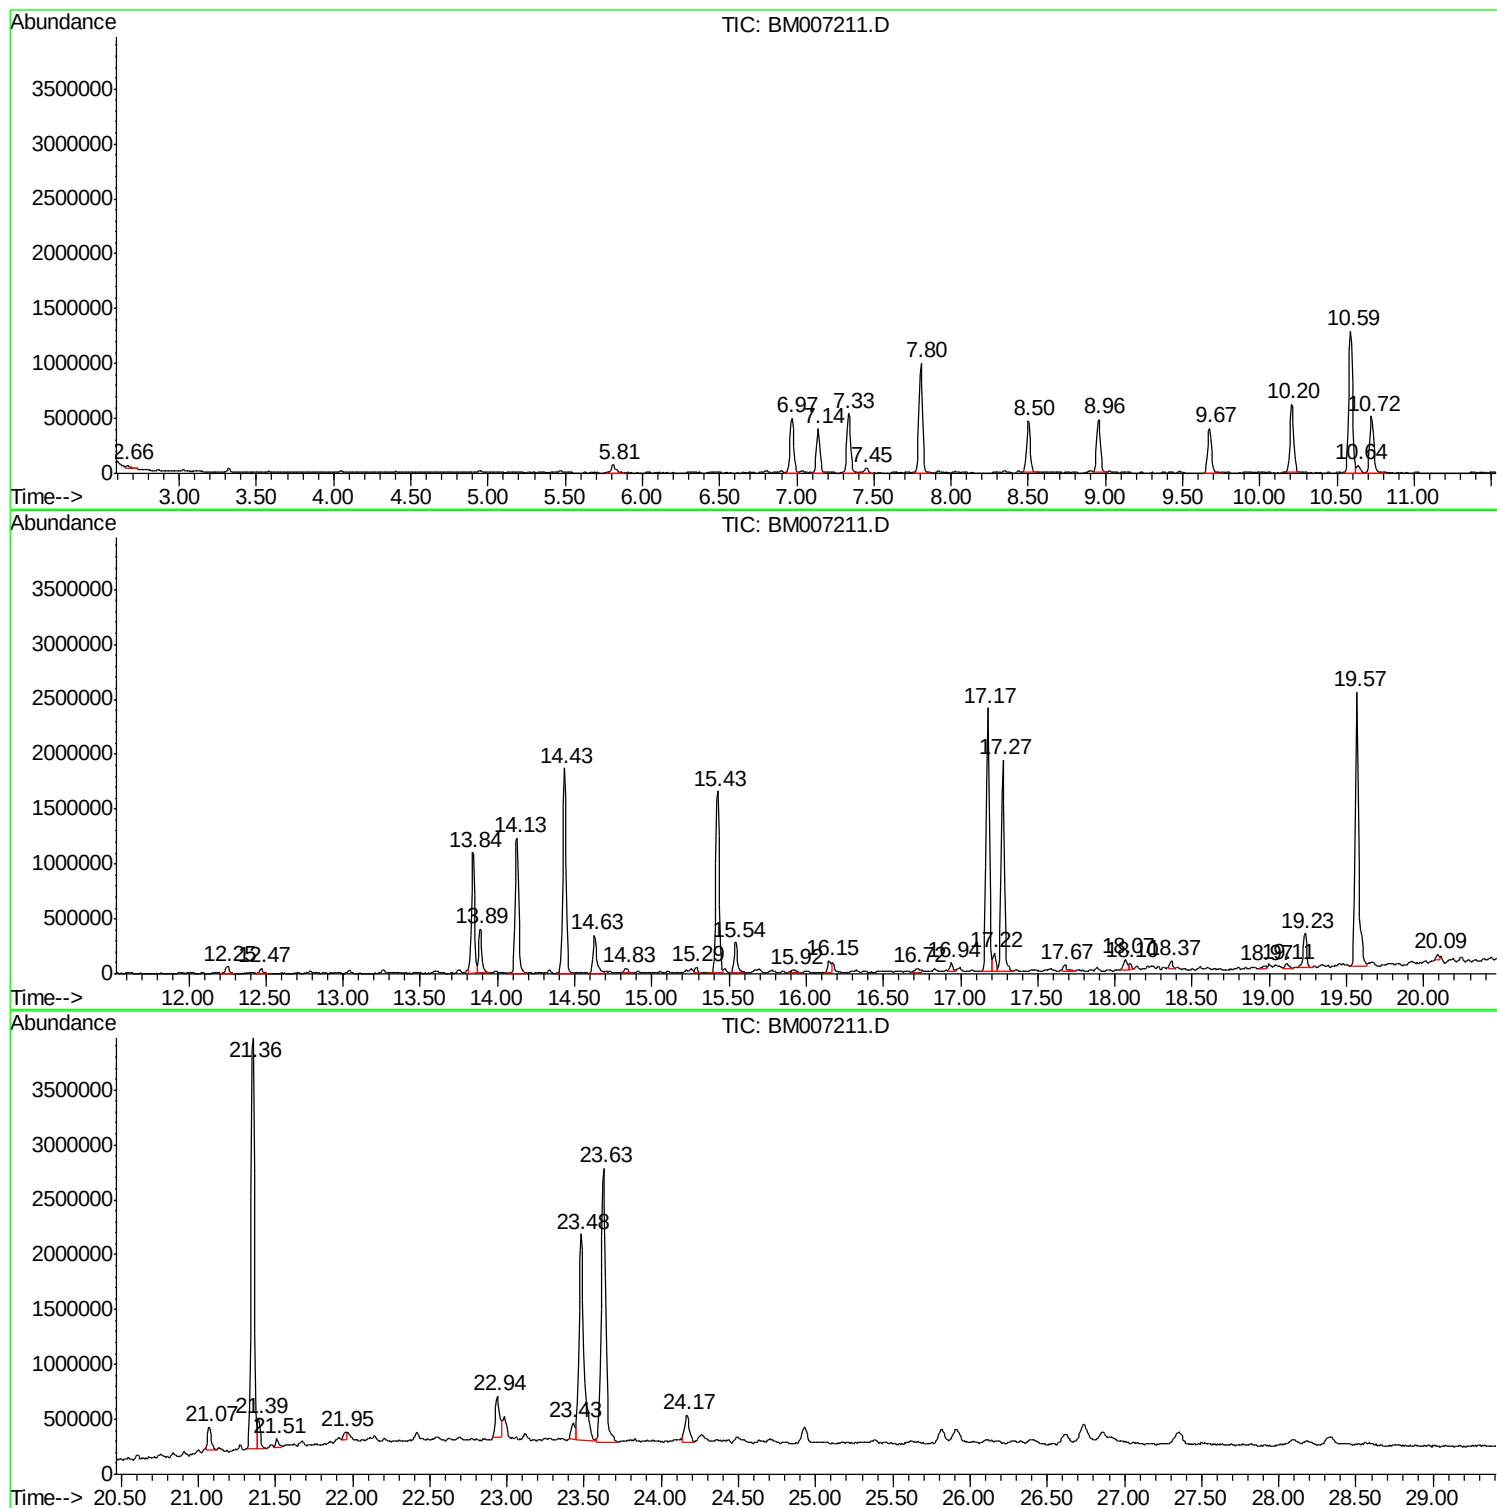

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007211.D
Acq On : 18 Aug 2016 19:27
Operator : UM/SJ
Sample : H4445-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N23

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007211.D
Acq On : 18 Aug 2016 19:27
Operator : UM/SJ
Sample : H4445-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N23

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc