

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007212.D
 Acq On : 18 Aug 2016 20:03
 Operator : UM/SJ
 Sample : H4445-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E5N25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.663	10	13	25	rVB4	36425	80998	1.32%	0.125%
2	6.969	737	745	755	rBV	657676	1063526	17.33%	1.648%
3	7.140	767	774	785	rBV	528610	834303	13.60%	1.293%
4	7.334	801	807	818	rBV	714259	1173589	19.13%	1.818%
5	7.804	879	887	894	rBV	939473	1511302	24.63%	2.342%
6	8.498	997	1005	1020	rBV	691737	1134431	18.49%	1.758%
7	8.957	1075	1083	1091	rBV	665552	1127584	18.38%	1.747%
8	9.675	1197	1205	1218	rVB	556083	945724	15.41%	1.465%
9	10.204	1288	1295	1305	rBV	860451	1486461	24.22%	2.303%
10	10.586	1352	1360	1367	rBV	1233049	2087626	34.02%	3.235%
11	10.722	1376	1383	1398	rBV	765752	1325210	21.60%	2.053%
12	13.839	1903	1913	1918	rBV	1528927	2236771	36.45%	3.466%
13	13.886	1918	1921	1930	rVB	520904	710978	11.59%	1.102%
14	14.121	1955	1961	1972	rVB	1721096	2653930	43.25%	4.112%
15	14.433	2007	2014	2021	rBV2	1819827	2775519	45.23%	4.300%
16	14.627	2041	2047	2061	rBV	530270	894034	14.57%	1.385%
17	15.427	2176	2183	2189	rBV	2373457	3390226	55.25%	5.253%
18	15.545	2197	2203	2211	rBV	453962	677775	11.05%	1.050%
19	16.145	2300	2305	2308	rBV	58207	83344	1.36%	0.129%
20	17.174	2474	2480	2485	rBV2	2413853	3564644	58.09%	5.523%
21	17.215	2485	2487	2492	rVV	496674	624574	10.18%	0.968%
22	17.274	2492	2497	2509	rVB	2661084	3911879	63.75%	6.061%
23	17.580	2539	2549	2556	rBV	71209	138499	2.26%	0.215%
24	18.062	2624	2631	2634	rBV2	94818	192151	3.13%	0.298%
25	18.098	2634	2637	2642	rVV	99256	147596	2.41%	0.229%
26	18.145	2642	2645	2648	rVV	49179	61728	1.01%	0.096%
27	18.245	2657	2662	2666	rVV2	90922	169011	2.75%	0.262%
28	18.280	2666	2668	2673	rVB	49980	62586	1.02%	0.097%
29	18.551	2710	2714	2718	rBV	47186	63979	1.04%	0.099%
30	18.974	2779	2786	2789	rBV2	43489	80747	1.32%	0.125%
31	19.233	2820	2830	2835	rBV	848673	1205260	19.64%	1.867%
32	19.456	2859	2868	2870	rBV2	44137	91969	1.50%	0.142%
33	19.568	2881	2887	2900	rBV2	3579290	6136280	100.00%	9.508%
34	19.668	2900	2904	2910	rVB2	75431	148397	2.42%	0.230%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007212.D
Acq On : 18 Aug 2016 20:03
Operator : UM/SJ
Sample : H4445-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N25

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Title : SVOA CALIBRATION

35	19.774	2919	2922	2928	rVB2	55484	79581	1.30%	0.123%
36	19.921	2941	2947	2953	rBV3	59224	148086	2.41%	0.229%
37	20.092	2972	2976	2982	rVB2	118135	188757	3.08%	0.292%
38	20.192	2989	2993	2996	rBV3	57572	72238	1.18%	0.112%
39	20.250	2996	3003	3007	rBV3	94285	173003	2.82%	0.268%
40	20.433	3031	3034	3038	rVB2	49446	65209	1.06%	0.101%
41	20.833	3099	3102	3107	rVB	75757	103878	1.69%	0.161%
42	20.909	3112	3115	3123	rBV6	49496	82797	1.35%	0.128%
43	21.003	3128	3131	3134	rVV	101068	146037	2.38%	0.226%
44	21.039	3134	3137	3139	rVV	93605	122948	2.00%	0.190%
45	21.074	3139	3143	3149	rVV3	232783	452176	7.37%	0.701%
46	21.133	3150	3153	3162	rVB2	99528	170078	2.77%	0.264%
47	21.356	3184	3191	3195	rVV2	3972198	5853022	95.38%	9.069%
48	21.392	3195	3197	3205	rVB	528683	619455	10.09%	0.960%
49	21.509	3214	3217	3223	rBV3	86674	126691	2.06%	0.196%
50	21.668	3242	3244	3248	rVB2	71382	87618	1.43%	0.136%
51	22.939	3454	3460	3466	rBV2	477785	1165110	18.99%	1.805%
52	23.433	3539	3544	3546	rBV	204477	352837	5.75%	0.547%
53	23.480	3546	3552	3567	rVB2	2644455	5915004	96.39%	9.165%
54	23.627	3570	3577	3584	rBV	2451500	4752234	77.44%	7.363%
55	24.168	3665	3669	3676	rVB3	174043	340901	5.56%	0.528%
56	24.927	3794	3798	3805	rVB2	135019	276891	4.51%	0.429%
57	25.909	3960	3965	3976	rVB2	168485	453273	7.39%	0.702%


Sum of corrected areas: 64540455

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007212.D
Acq On : 18 Aug 2016 20:03
Operator : UM/SJ
Sample : H4445-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

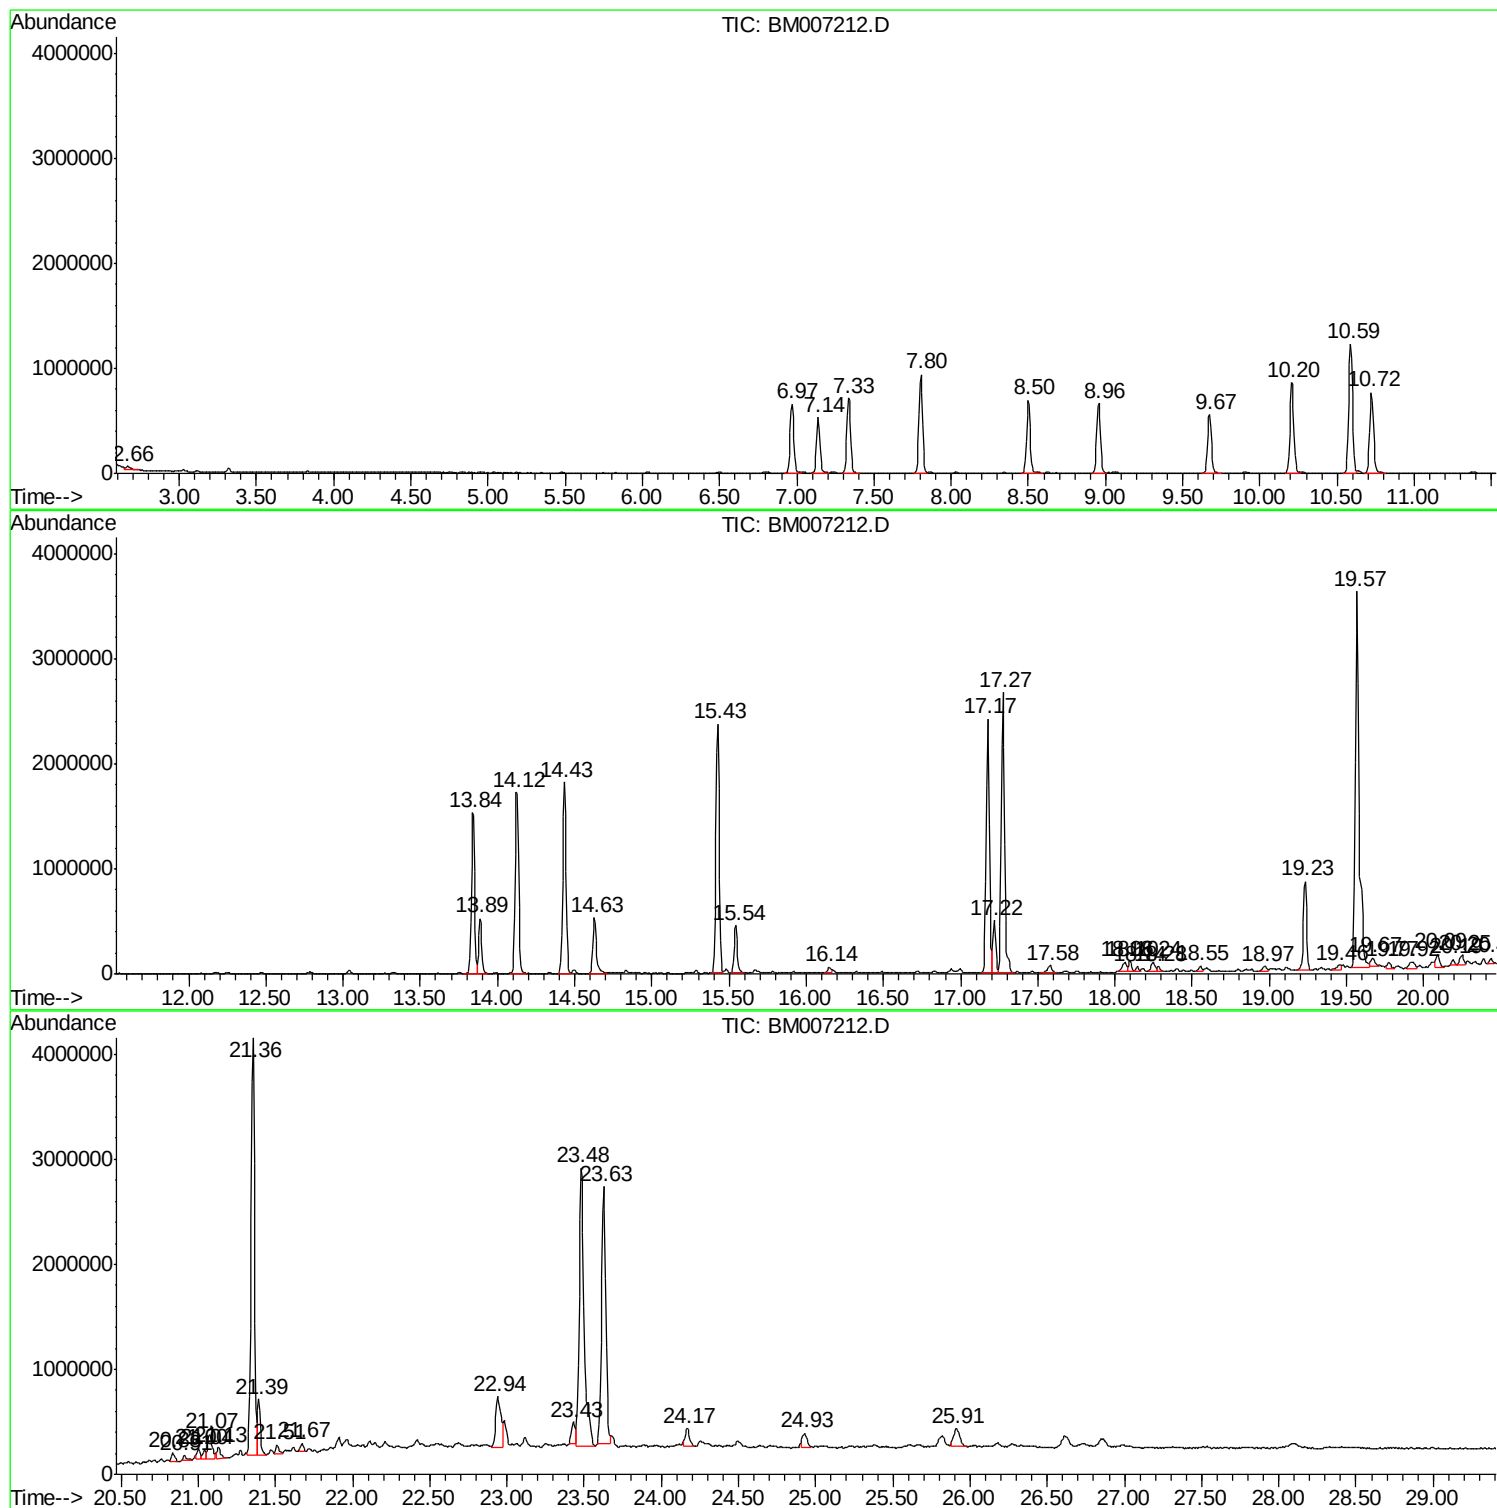

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007212.D
Acq On : 18 Aug 2016 20:03
Operator : UM/SJ
Sample : H4445-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007212.D
Acq On : 18 Aug 2016 20:03
Operator : UM/SJ
Sample : H4445-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E5N25

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc