

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
 Data File : BM007219.D
 Acq On : 19 Aug 2016 00:15
 Operator : UM/SJ
 Sample : PB92919BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	121	125	131	rVB	71361	97404	1.31%	0.133%
2	6.969	734	745	759	rBV	1215204	1927301	25.98%	2.628%
3	7.139	765	774	783	rVB	887207	1377945	18.58%	1.879%
4	7.334	801	807	818	rBV	1204464	2009933	27.10%	2.741%
5	7.804	880	887	896	rVB	1087413	1737845	23.43%	2.370%
6	8.498	998	1005	1017	rBV	1472669	2409103	32.48%	3.286%
7	8.957	1074	1083	1092	rBV	1123152	1859095	25.06%	2.535%
8	9.675	1197	1205	1214	rBV	932091	1585771	21.38%	2.163%
9	10.204	1288	1295	1308	rBV	1414837	2486062	33.52%	3.391%
10	10.586	1353	1360	1368	rVB	1401631	2387920	32.19%	3.257%
11	10.722	1375	1383	1396	rBV	1374704	2392386	32.25%	3.263%
12	13.845	1907	1914	1923	rVB	2382472	3493668	47.10%	4.765%
13	14.127	1954	1962	1974	rBV	2679834	4141537	55.84%	5.648%
14	14.433	2007	2014	2026	rBV2	2048148	3153238	42.51%	4.300%
15	14.627	2040	2047	2064	rBV	1021664	1660380	22.39%	2.264%
16	15.427	2176	2183	2191	rBV	3555620	5117173	68.99%	6.979%
17	15.545	2197	2203	2214	rBV	803347	1164515	15.70%	1.588%
18	17.174	2474	2480	2488	rVB2	2645154	3854714	51.97%	5.257%
19	17.274	2490	2497	2509	rBV2	3818922	5630267	75.91%	7.679%
20	19.203	2818	2825	2832	rBV	49099	76015	1.02%	0.104%
21	19.568	2880	2887	2894	rBV	4876539	6809324	91.80%	9.287%
22	21.356	3186	3191	3200	rBV	4176342	5278677	71.17%	7.199%
23	23.485	3545	3553	3566	rVV2	3800116	7417300	100.00%	10.116%
24	23.632	3570	3578	3592	rVB	2694170	5255748	70.86%	7.168%


Sum of corrected areas: 73323321

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007219.D
Acq On : 19 Aug 2016 00:15
Operator : UM/SJ
Sample : PB92919BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK19

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

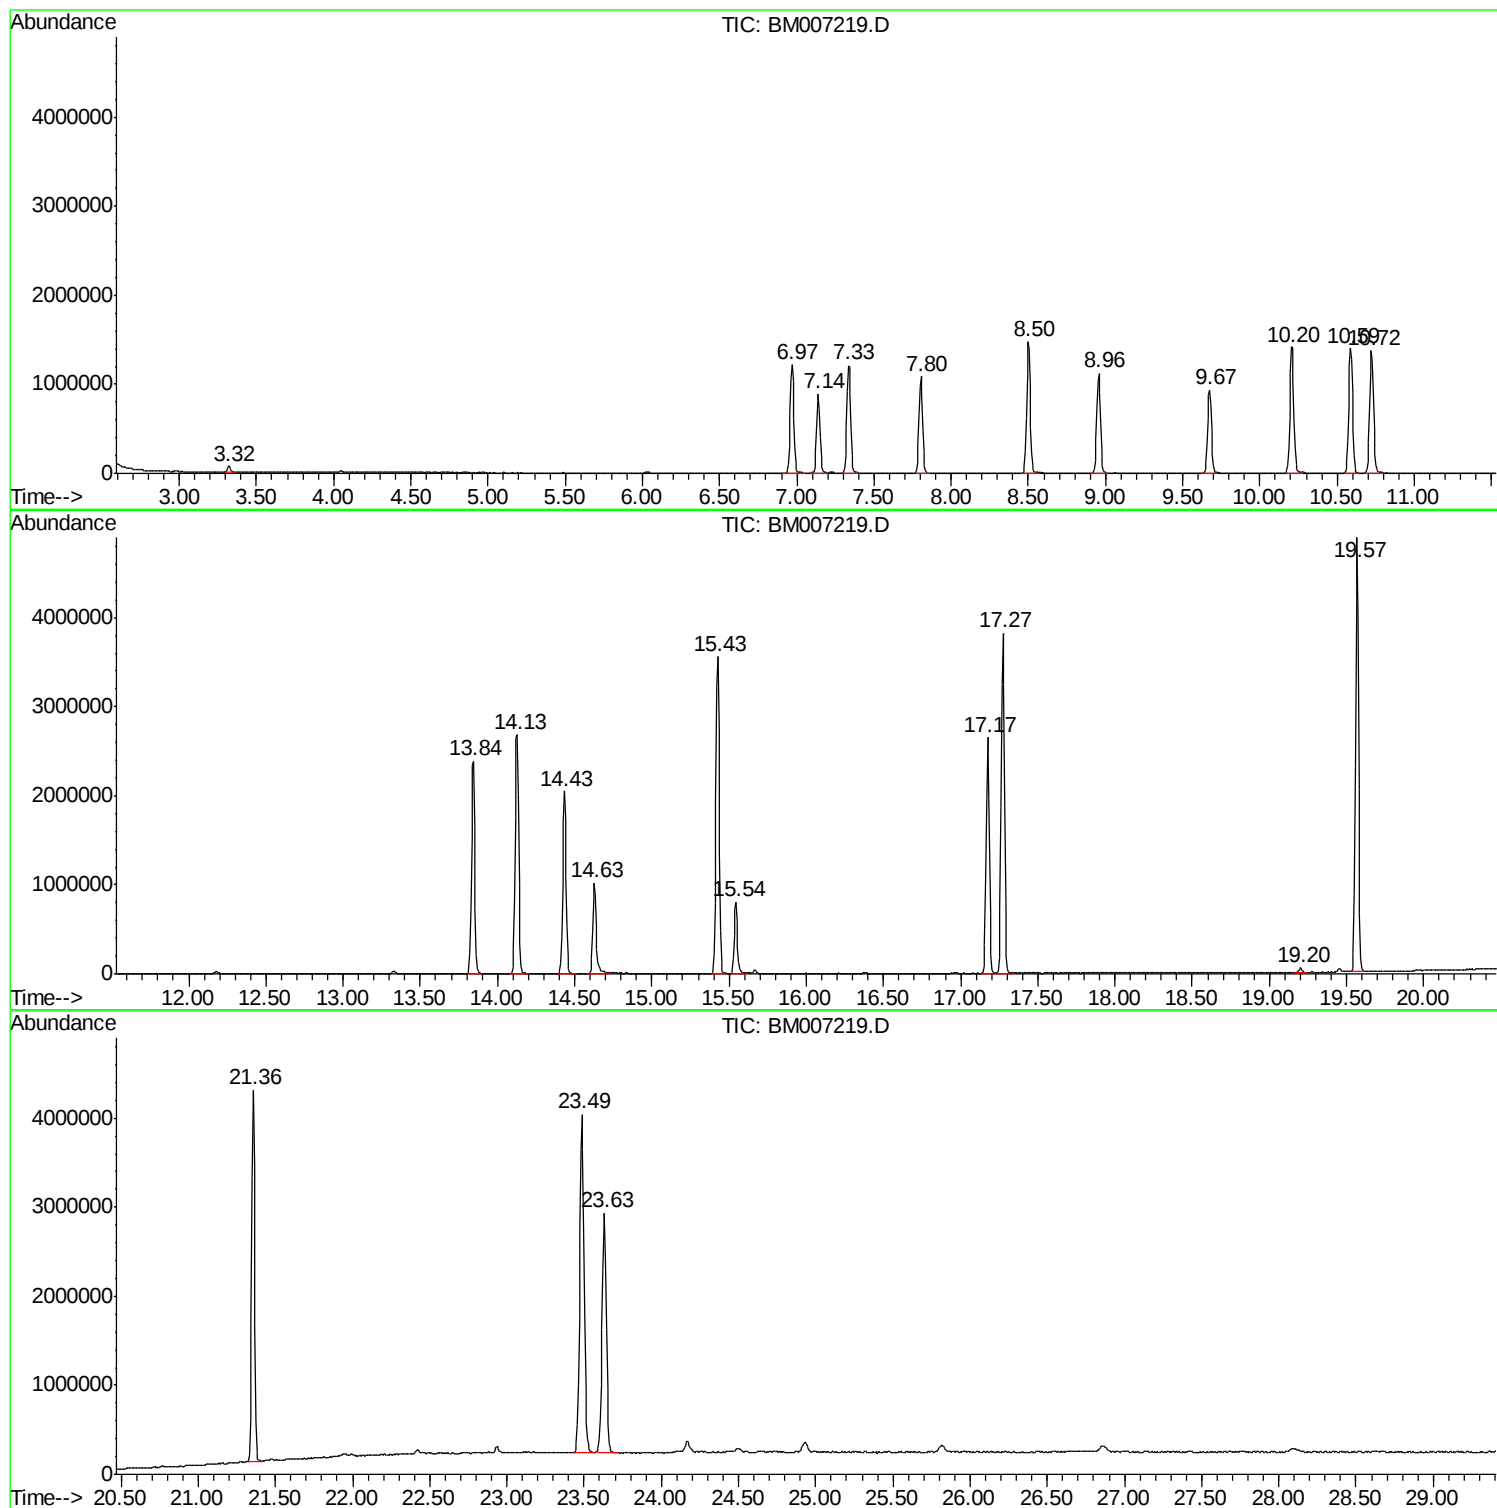

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007219.D
Acq On : 19 Aug 2016 00:15
Operator : UM/SJ
Sample : PB92919BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK19

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081916\
Data File : BM007219.D
Acq On : 19 Aug 2016 00:15
Operator : UM/SJ
Sample : PB92919BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK19

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc