
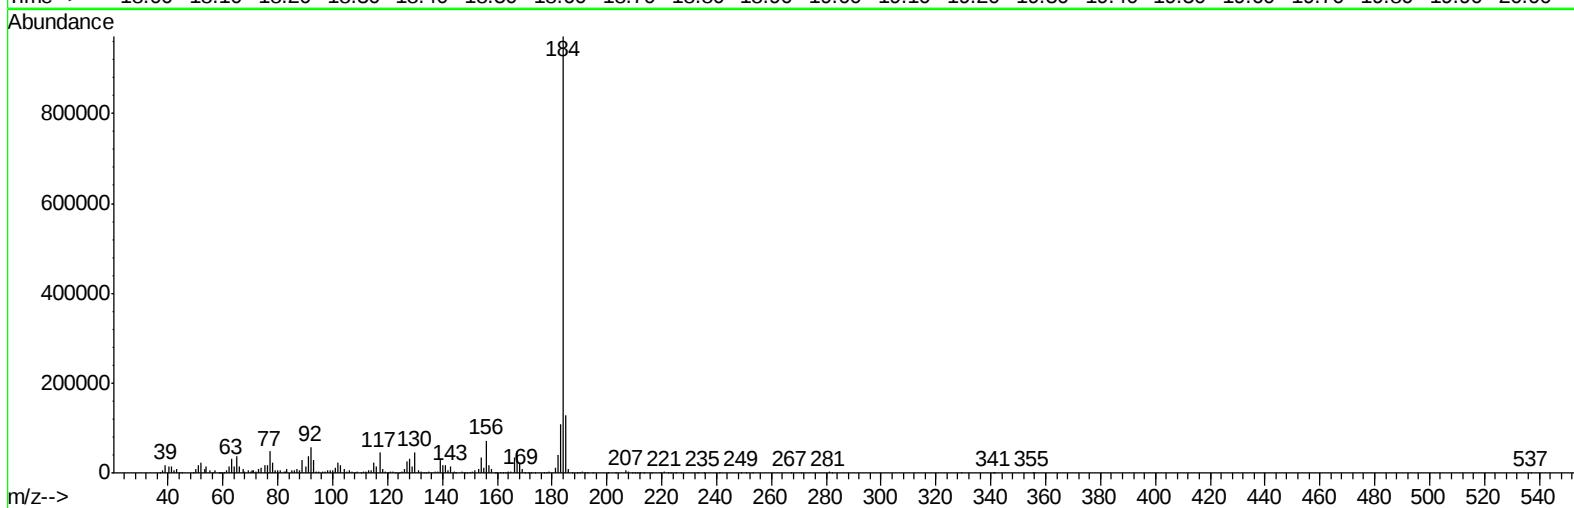


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081917\
Data File : BM011309.D
Acq On : 19 Aug 2017 09:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 02:23:16 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

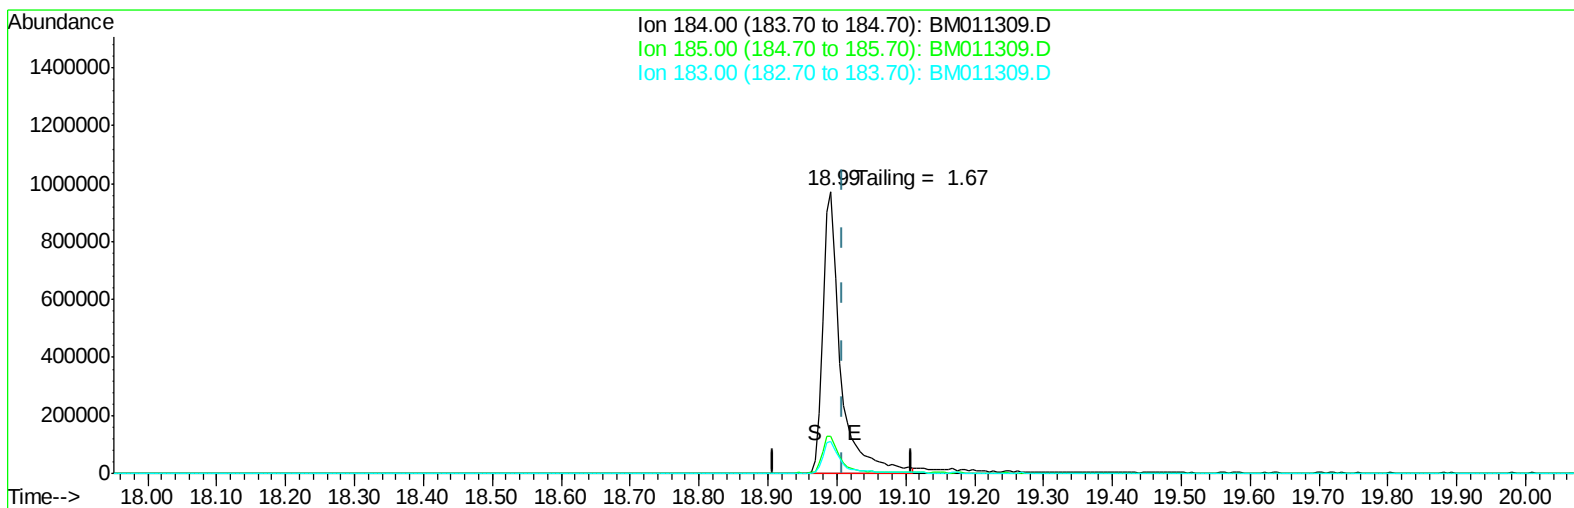

TIC: BM011309.D

(76) Benzidine



18.992min (-0.017) 1869.66ng

response 1673028

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.09
183.00	11.10	11.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081917\
Data File : BM011309.D
Acq On : 19 Aug 2017 09:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 02:23:16 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

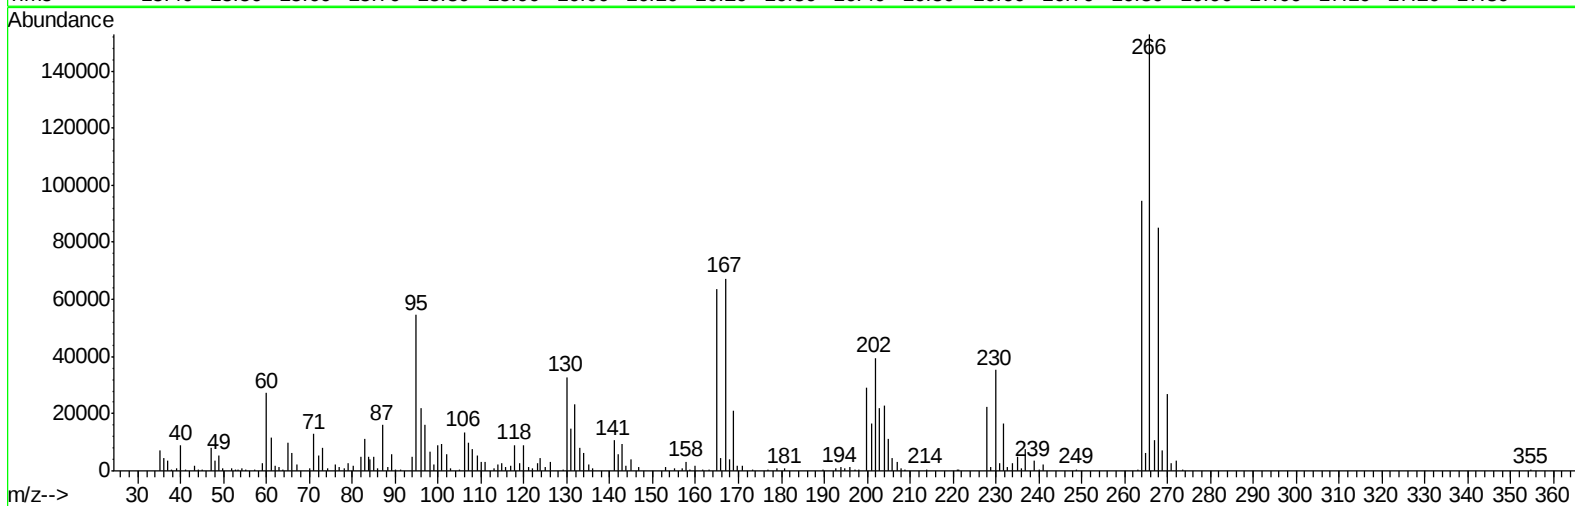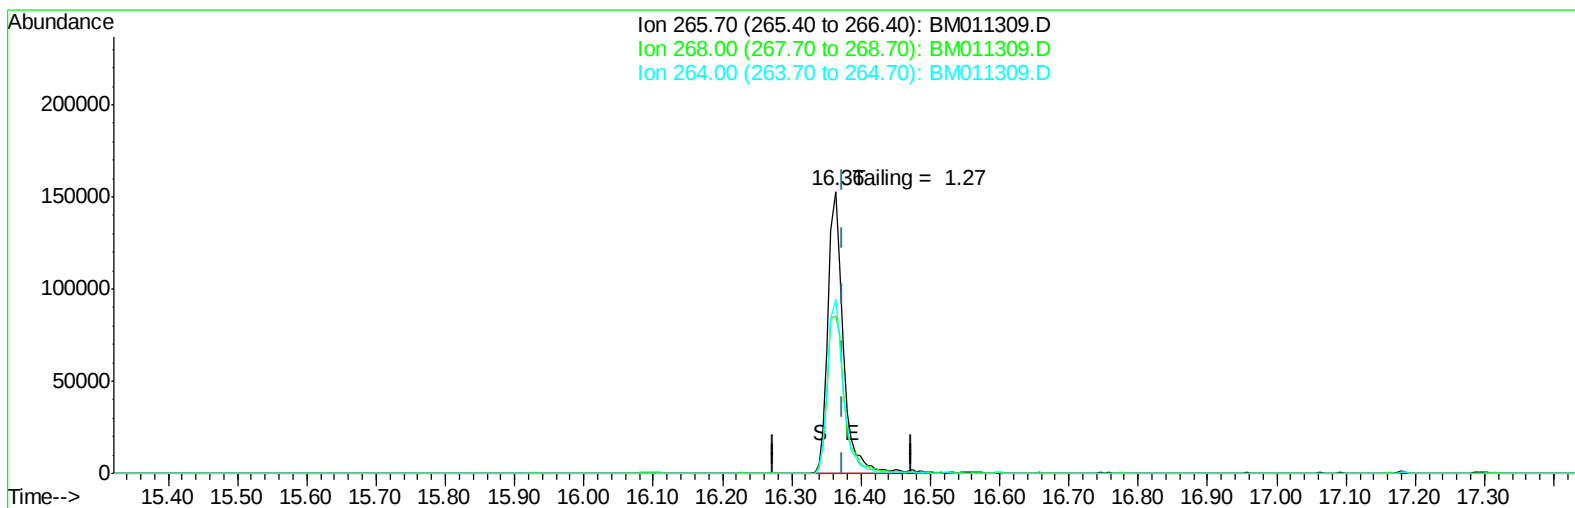

TIC: BM011309.D

(69) Pentachlorophenol (C)

16.363min (-0.012) 1426.25ng

response 230386

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	55.70
264.00	61.20	61.82
0.00	0.00	0.00