

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011311.D
 Acq On : 19 Aug 2017 10:48
 Operator : SJ/JU
 Sample : PB101645BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB101645BL

Quant Time: Aug 21 01:55:11 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	144158	20.00	ng	-0.02
21) Naphthalene-d8	10.02	136	534823	20.00	ng	-0.02
38) Acenaphthene-d10	13.94	164	328273	20.00	ng	-0.02
63) Phenanthrene-d10	16.70	188	746234	20.00	ng	-0.02
75) Chrysene-d12	20.93	240	871816	20.00	ng	-0.02
86) Perylene-d12	23.00	264	847259	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	1202878	141.05	ng	-0.02
7) Phenol-d6	6.47	99	1712145	141.31	ng	-0.02
23) Nitrobenzene-d5	8.42	82	1429993	100.35	ng	-0.02
41) 2,4,6-Tribromophenol	15.44	330	603881	114.77	ng	-0.02
44) 2-Fluorobiphenyl	12.55	172	2381383	90.98	ng	-0.02
78) Terphenyl-d14	19.37	244	3570761	81.13	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011311.D
Acq On : 19 Aug 2017 10:48
Operator : SJ/JU
Sample : PB101645BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB101645BL

Quant Time: Aug 21 01:55:11 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration




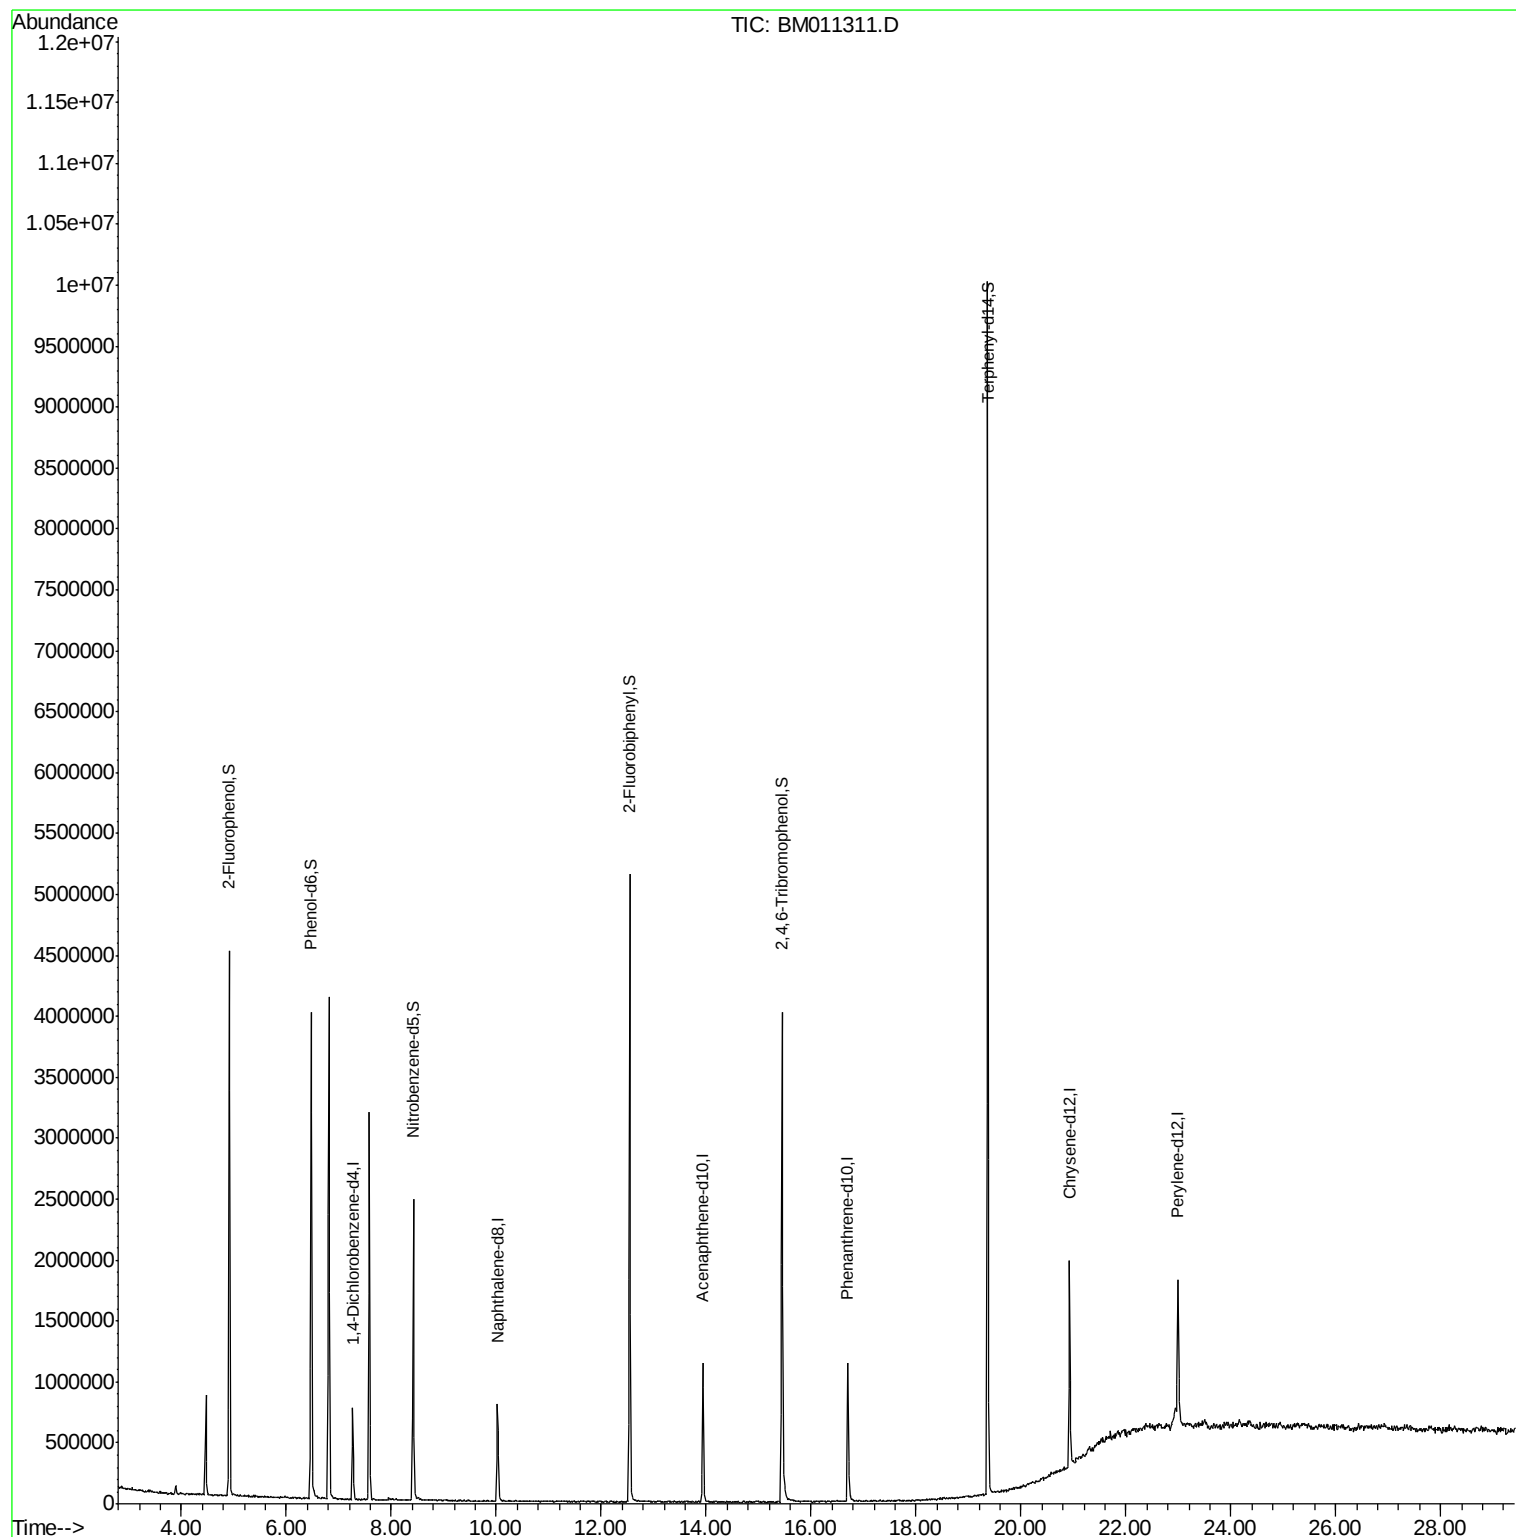


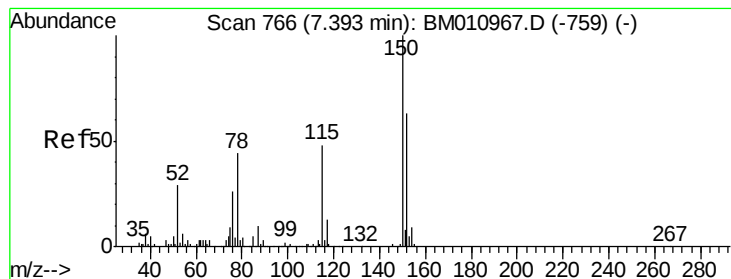

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.27 min Scan# 762
 Delta R.T. -0.02 min
 Lab File: BM011311.D
 Acq: 19 Aug 2017 10:48




Instrument :
 BNA_M
 ClientSampleId :
 PB101645BL


Tgt Ion:152 Resp: 144158
 Ion Ratio Lower Upper
 152 100
 150 145.1 119.5 179.3
 115 69.6 43.0 64.4#

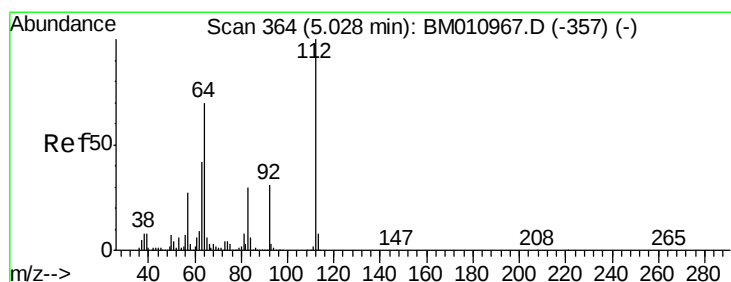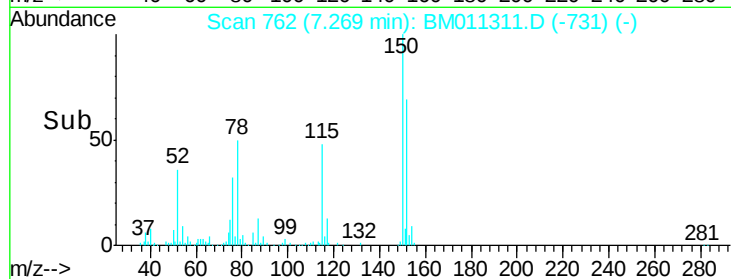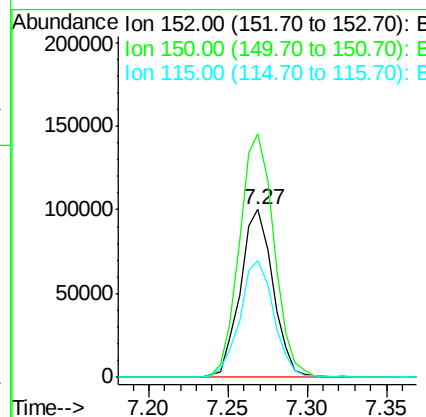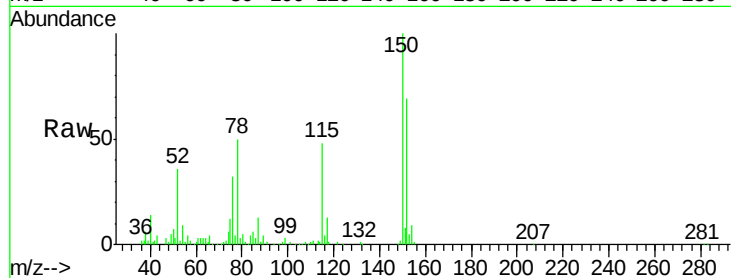

#5
 2-Fluorophenol
 Concen: 141.053 ng
 RT: 4.91 min Scan# 361
 Delta R.T. -0.02 min
 Lab File: BM011311.D
 Acq: 19 Aug 2017 10:48

Tgt Ion:112 Resp: 1202878
 Ion Ratio Lower Upper
 112 100
 64 81.5 38.6 57.8#
 63 49.3 19.3 28.9#

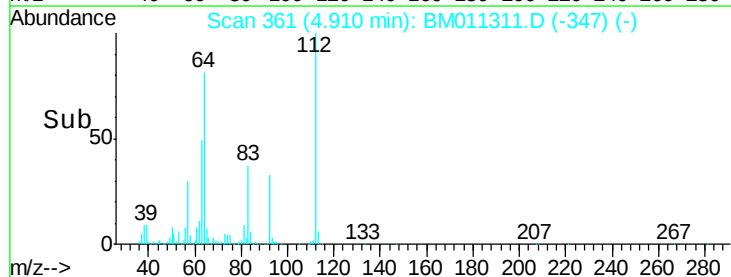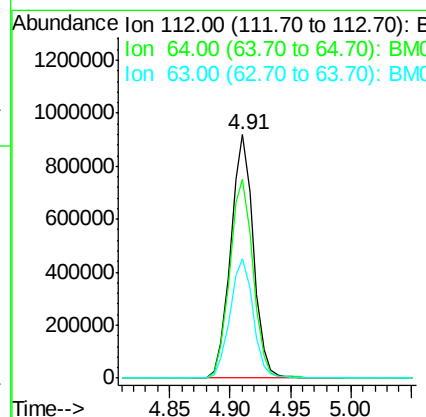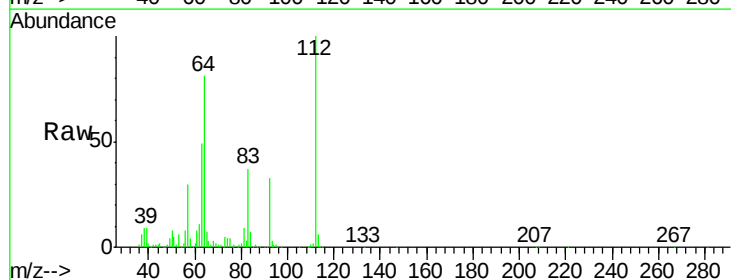

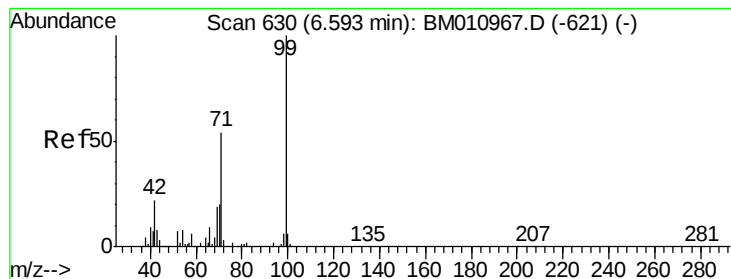

#7

Phenol-d6

Concen: 141.307 ng

RT: 6.47 min Scan# 627

Delta R.T. -0.02 min

Lab File: BM011311.D

Acq: 19 Aug 2017 10:48

Instrument :

BNA_M

ClientSampleId :

PB101645BL


Tgt Ion: 99 Resp: 1712145

Ion Ratio Lower Upper




99 100

42 23.2 11.0 16.4#

71 57.4 23.4 35.2#

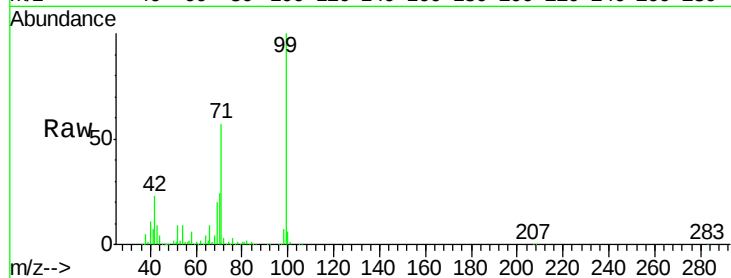

Abundance Ion 99.00 (98.70 to 99.70): BM011311.D (-613) (-)

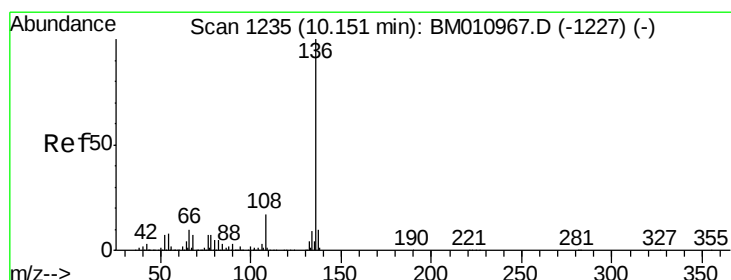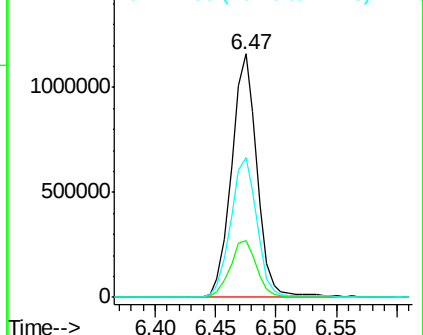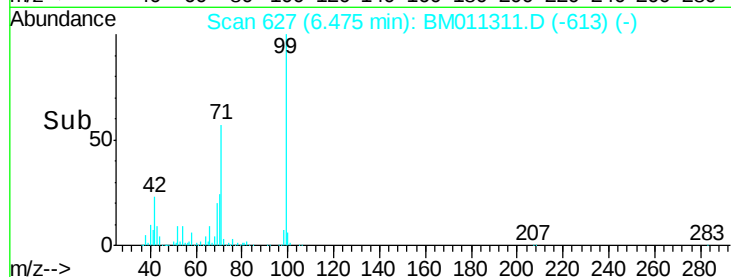

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.02 min Scan# 1230

Delta R.T. -0.02 min

Lab File: BM011311.D

Acq: 19 Aug 2017 10:48

Tgt Ion: 136 Resp: 534823


Ion Ratio Lower Upper

136 100



137 10.1 8.7 13.1


54 9.2 4.6 6.8#

68 8.6 3.7 5.5#

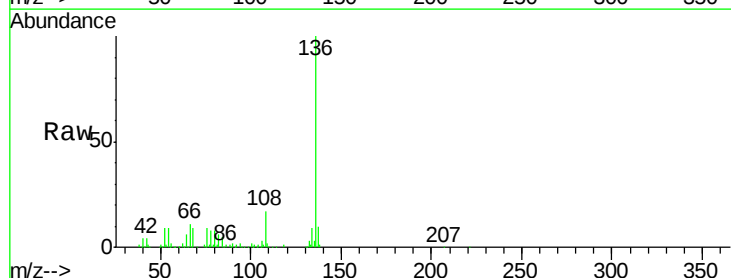

Abundance Ion 136.00 (135.70 to 136.70): BM011311.D (-1217) (-)



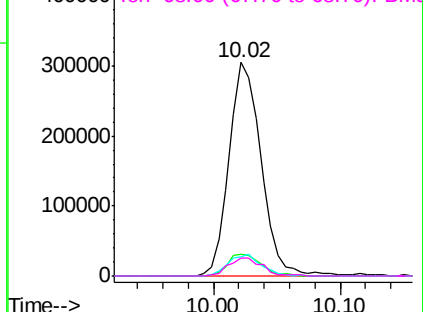
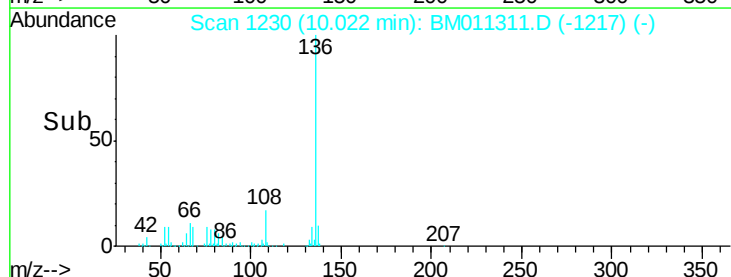


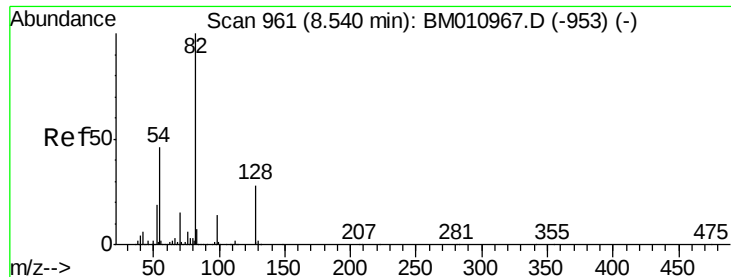

#23
Nitrobenzene-d5
Concen: 100.351 ng
RT: 8.42 min Scan# 957
Delta R.T. -0.02 min
Lab File: BM011311.D
Acq: 19 Aug 2017 10:48




Instrument :
BNA_M
ClientSampleId :
PB101645BL


Tgt Ion: 82 Resp: 1429993
Ion Ratio Lower Upper
82 100
128 24.7 32.8 49.2#
54 47.2 40.6 60.8

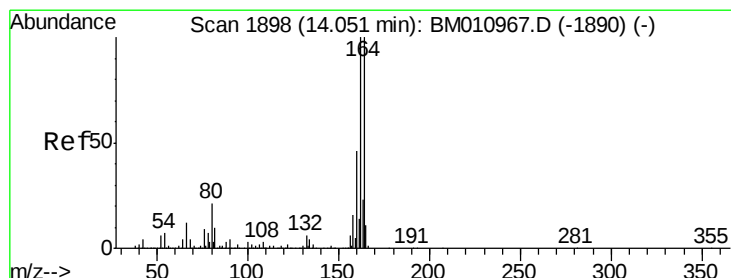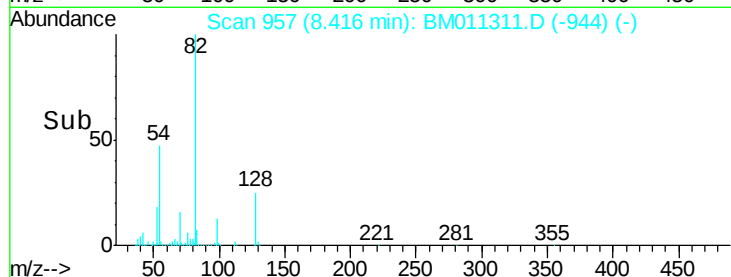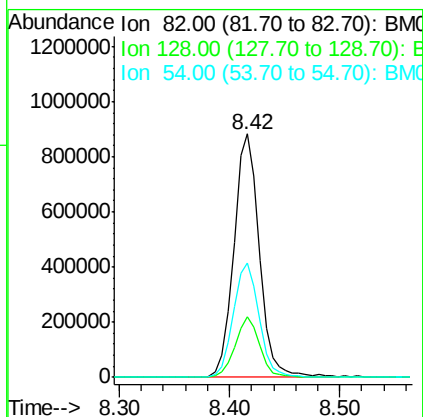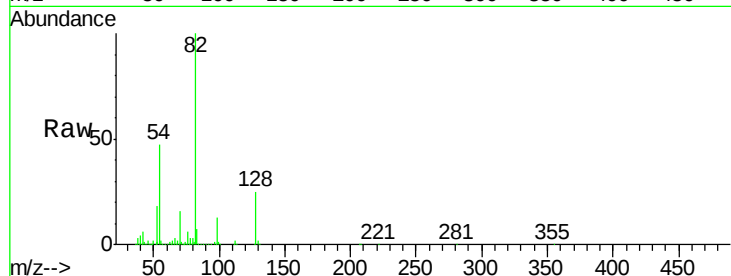

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 13.94 min Scan# 1896
Delta R.T. -0.02 min
Lab File: BM011311.D
Acq: 19 Aug 2017 10:48

Tgt Ion: 164 Resp: 328273
Ion Ratio Lower Upper
164 100
162 94.2 82.4 123.6
160 44.0 35.8 53.6

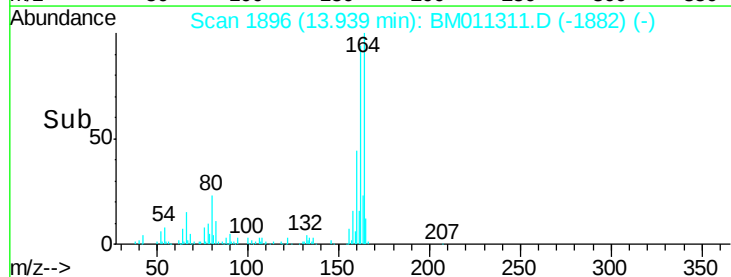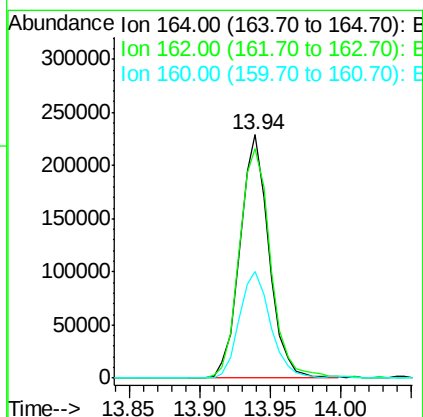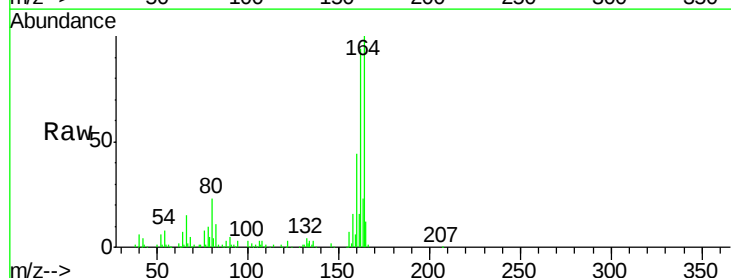


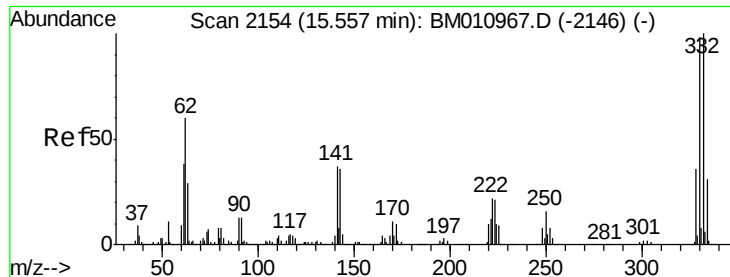




#41
 2,4,6-Tribromophenol
 Concen: 114.773 ng
 RT: 15.44 min Scan# 2152
 Delta R.T. -0.02 min
 Lab File: BM011311.D
 Acq: 19 Aug 2017 10:48

Instrument :
 BNA_M
 ClientSampleId :
 PB101645BL

Tgt Ion	Ratio	Resp	Lower	Upper
330	100			
332	97.9	603881	0.0	0.0#
141	45.1		0.0	0.0#

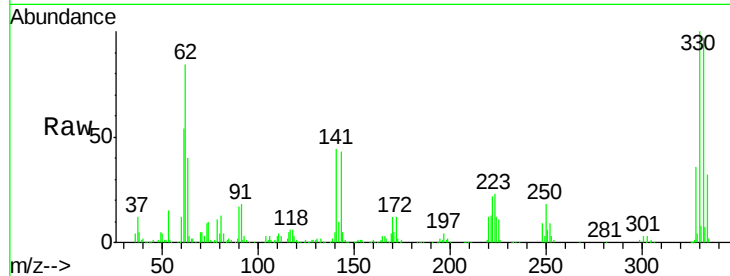


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

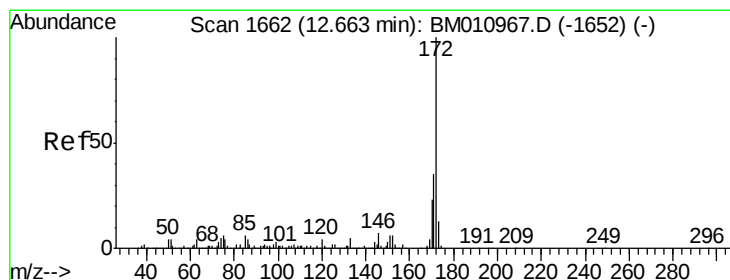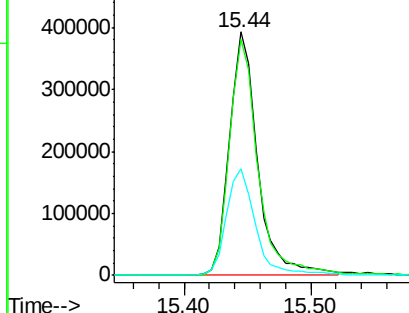
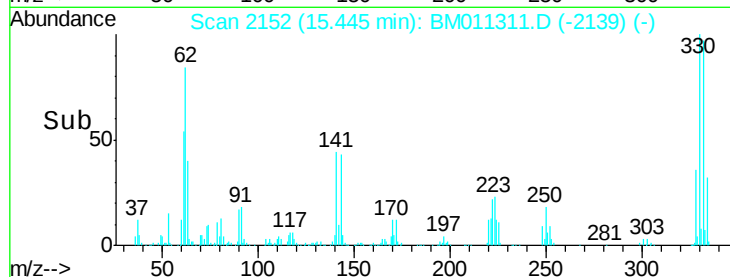



#44
 2-Fluorobiphenyl
 Concen: 90.978 ng
 RT: 12.55 min Scan# 1659
 Delta R.T. -0.02 min
 Lab File: BM011311.D
 Acq: 19 Aug 2017 10:48

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	2381383		
171	34.9		28.5	42.7
170	23.3		18.8	28.2

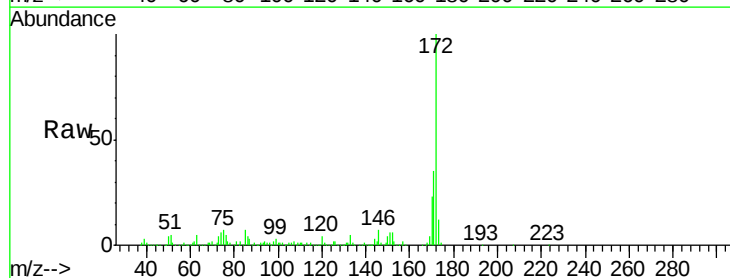

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



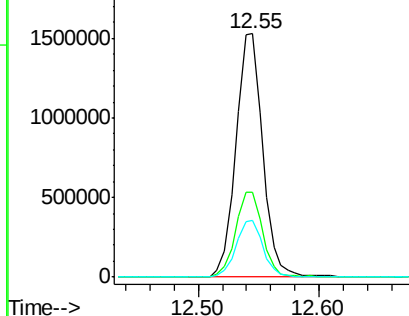
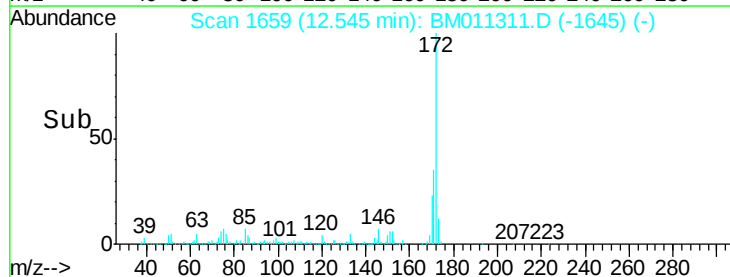


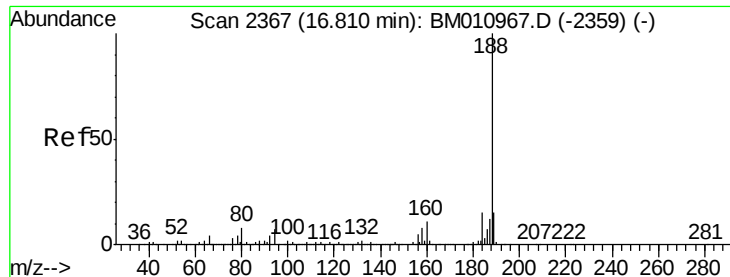

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.70 min Scan# 2365
Delta R.T. -0.02 min
Lab File: BM011311.D
Acq: 19 Aug 2017 10:48




Instrument :
BNA_M
ClientSampleId :
PB101645BL


Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.1	8.7	13.1#
80	10.2	9.3	13.9

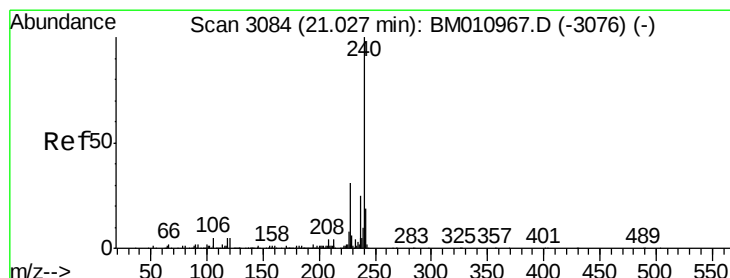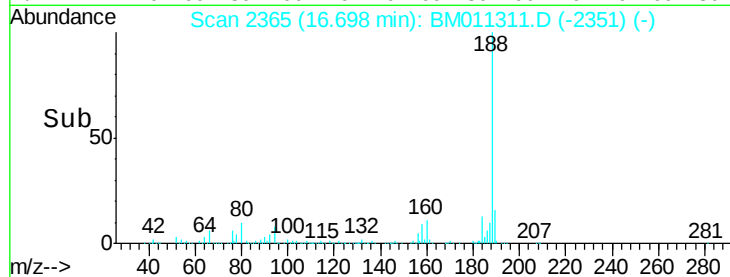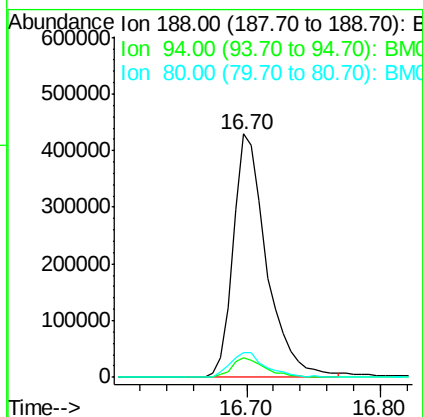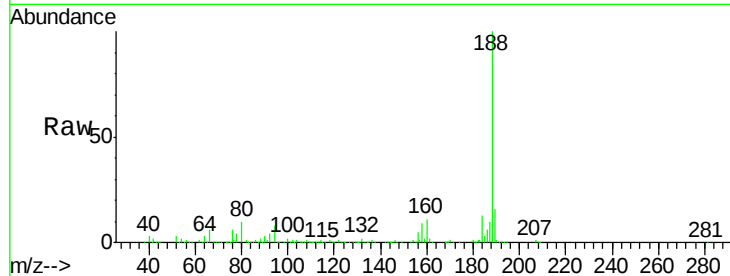

#75
Chrysene-d12
Concen: 20.000 ng
RT: 20.93 min Scan# 3084
Delta R.T. -0.02 min
Lab File: BM011311.D
Acq: 19 Aug 2017 10:48

Tgt Ion	Ratio	Lower	Upper
240	100		
120	4.4	8.2	12.2#
236	26.6	20.0	30.0

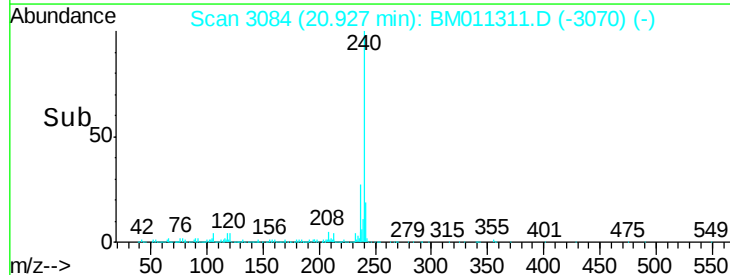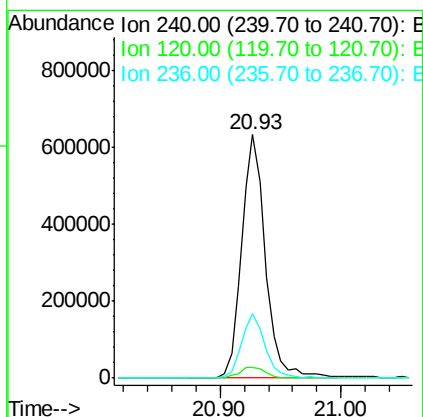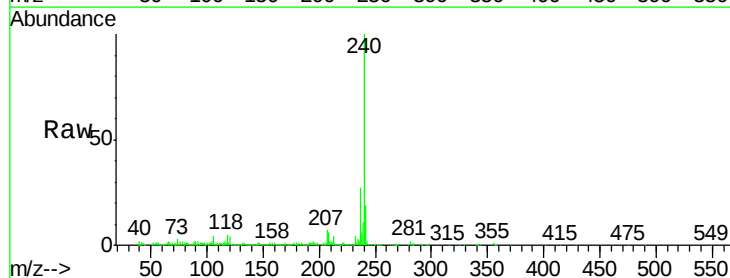

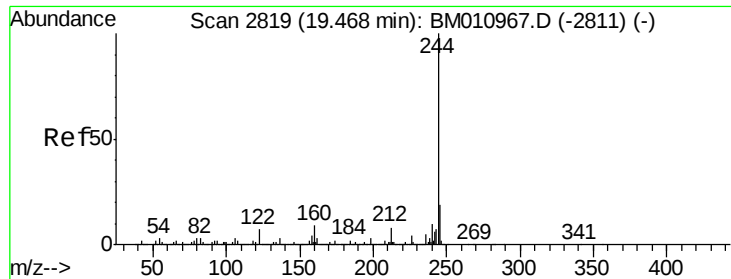

#78

Terphenyl-d14

Concen: 81.132 ng

RT: 19.37 min Scan# 2819

Delta R.T. -0.02 min

Lab File: BM011311.D

Acq: 19 Aug 2017 10:48

Instrument :

BNA_M

ClientSampleId :

PB101645BL


Tgt Ion:244 Resp: 3570761

Ion Ratio Lower Upper




244 100

212 8.1 4.9 7.3#

122 6.3 6.2 9.4

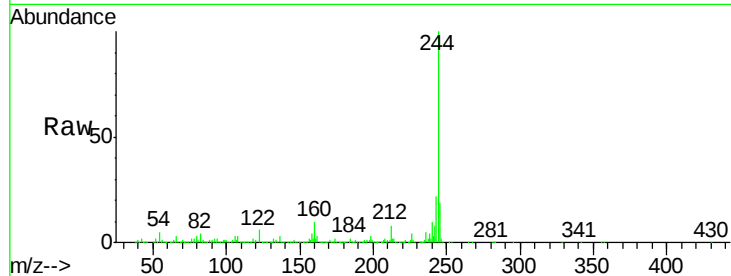

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

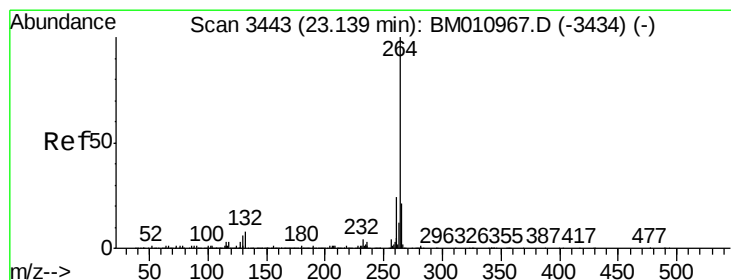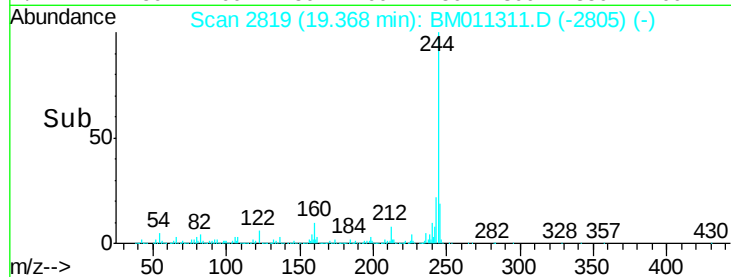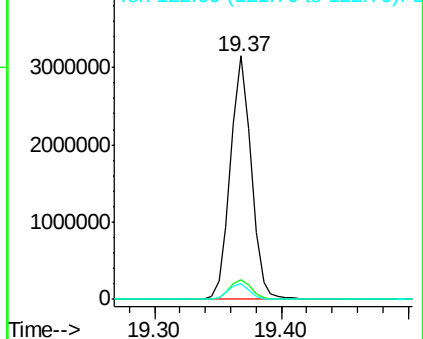

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.00 min Scan# 3436

Delta R.T. -0.02 min

Lab File: BM011311.D

Acq: 19 Aug 2017 10:48


Tgt Ion:264 Resp: 847259

Ion Ratio Lower Upper

264 100

260 24.7 18.6 27.8

265 23.4 17.3 25.9

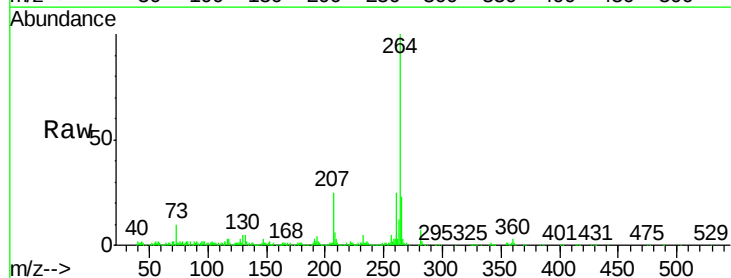

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

