

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011315.D
 Acq On : 19 Aug 2017 13:13
 Operator : SJ/JU
 Sample : I4875-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-B

Quant Time: Aug 21 02:01:01 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	149333	20.00	ng	-0.02
21) Naphthalene-d8	10.03	136	528089	20.00	ng	-0.02
38) Acenaphthene-d10	13.94	164	329952	20.00	ng	-0.02
63) Phenanthrene-d10	16.70	188	812279	20.00	ng	-0.02
75) Chrysene-d12	20.93	240	1117122	20.00	ng	-0.02
86) Perylene-d12	22.99	264	1061740	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	989087	111.96	ng	-0.02
7) Phenol-d6	6.47	99	1300368	103.60	ng	-0.02
23) Nitrobenzene-d5	8.42	82	1326465	94.27	ng	-0.02
41) 2,4,6-Tribromophenol	15.44	330	569200	107.63	ng	-0.02
44) 2-Fluorobiphenyl	12.55	172	2092853	79.55	ng	-0.02
78) Terphenyl-d14	19.37	244	3824676	67.82	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011315.D
Acq On : 19 Aug 2017 13:13
Operator : SJ/JU
Sample : I4875-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-081717-B

Quant Time: Aug 21 02:01:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

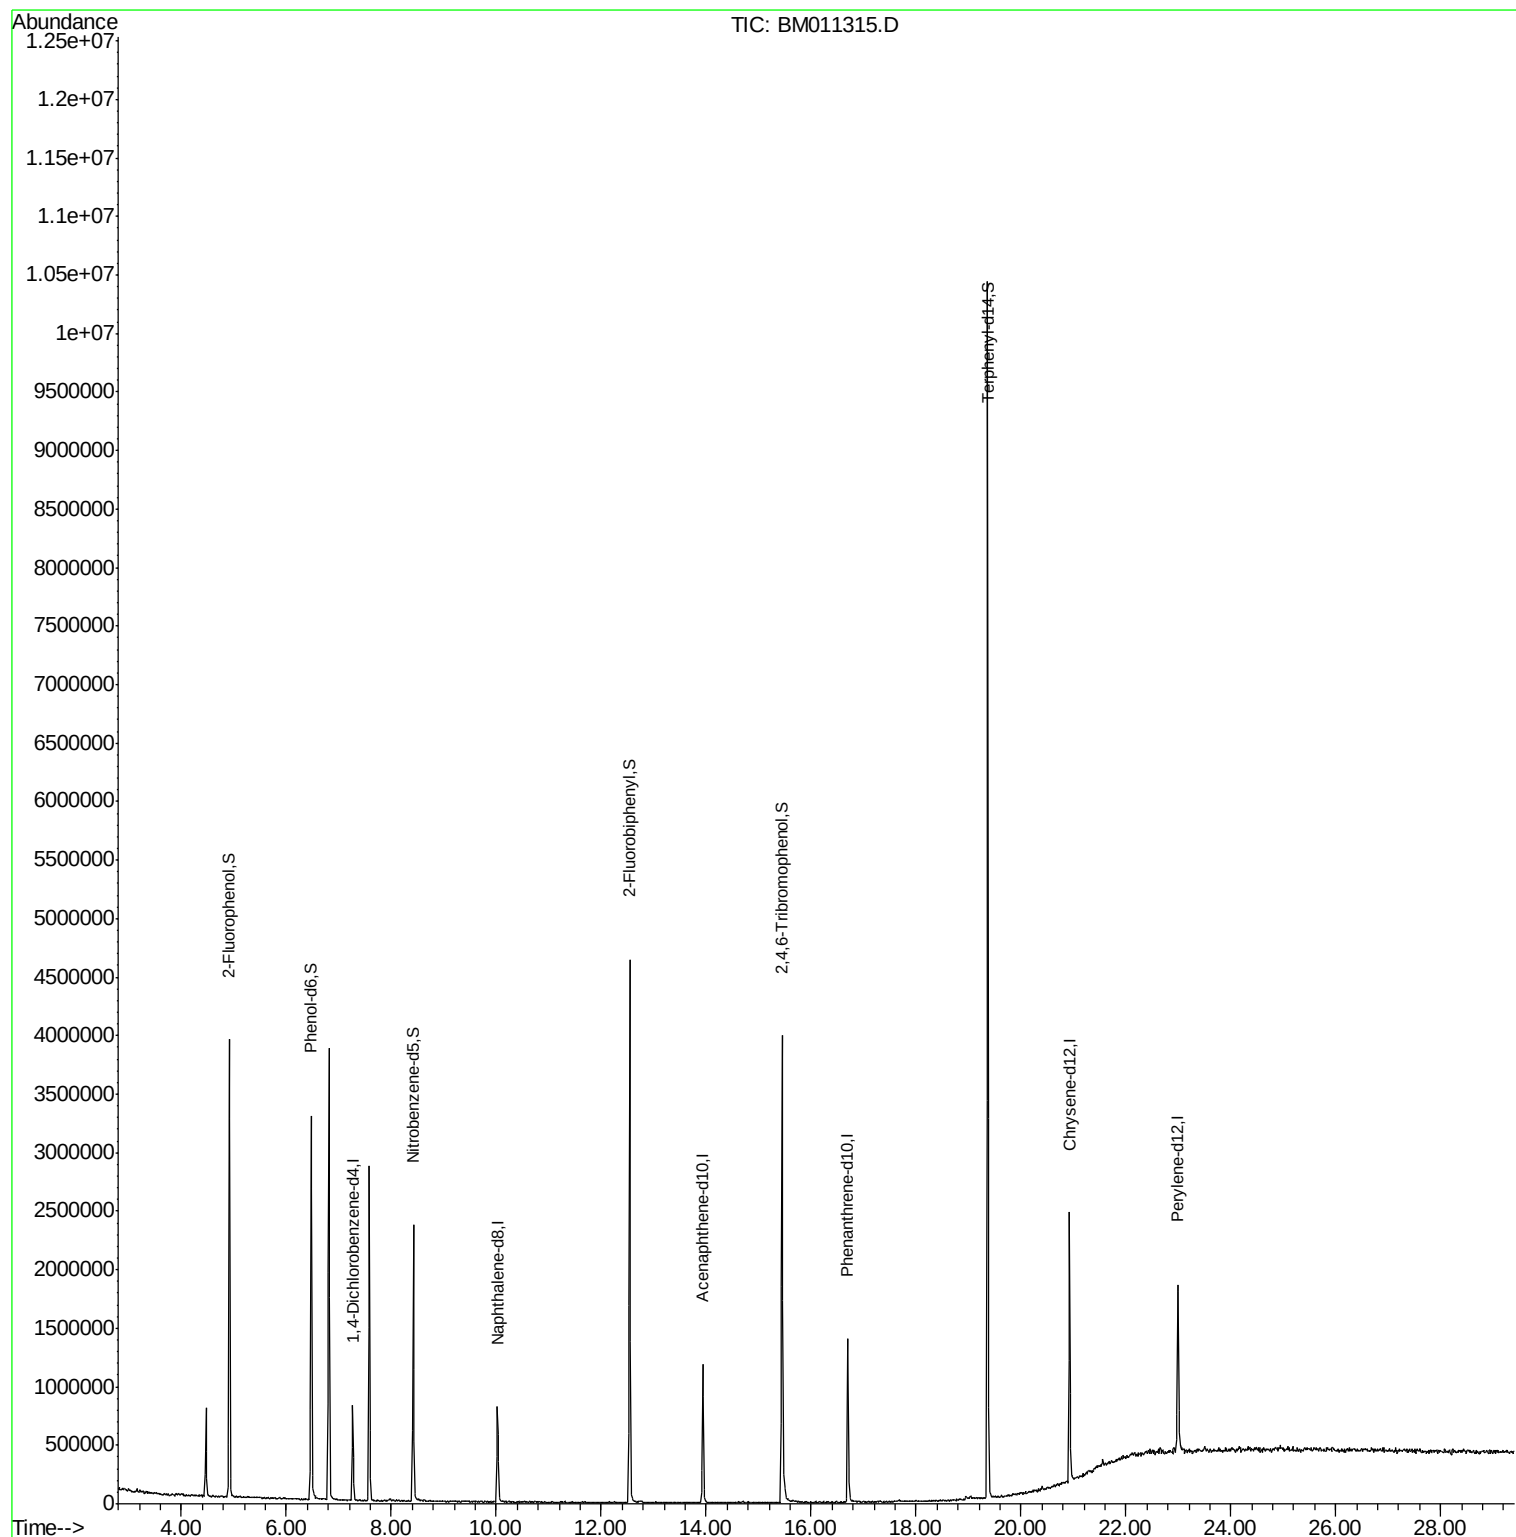

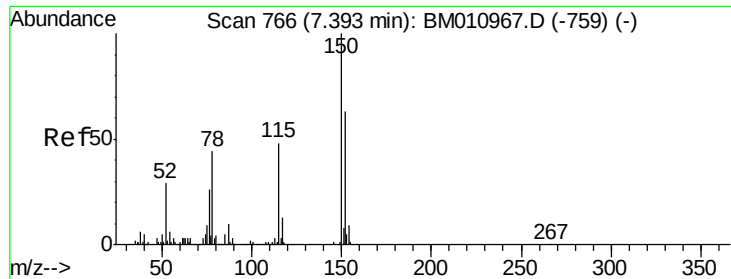


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.27 min Scan# 762
Delta R.T. -0.02 min
Lab File: BM011315.D
Acq: 19 Aug 2017 13:13

Instrument :
BNA_M
ClientSampleId :
CL-02-081717-B

Tgt Ion	Ratio	Lower	Upper
152	100		
150	159.5	119.5	179.3
115	76.2	43.0	64.4

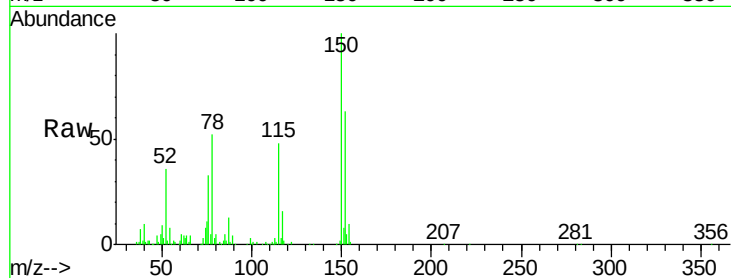


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

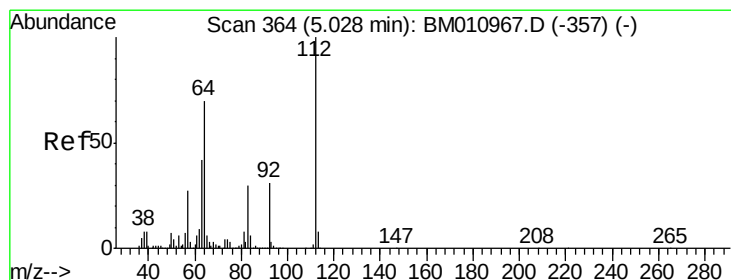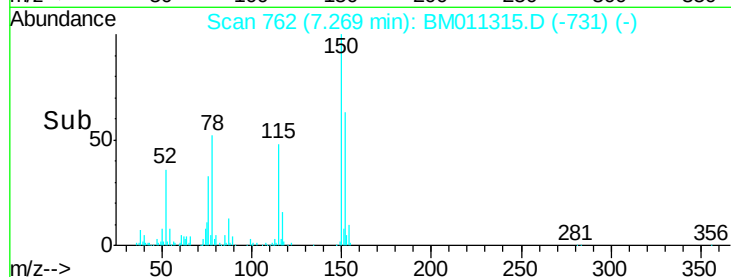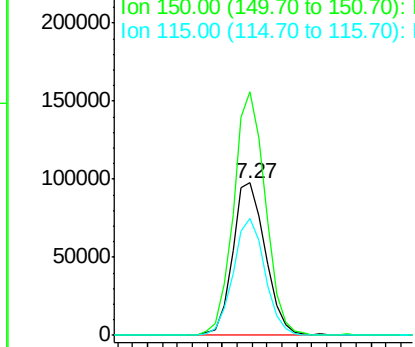



#5


2-Fluorophenol
Concen: 111.964 ng
RT: 4.91 min Scan# 361
Delta R.T. -0.02 min
Lab File: BM011315.D
Acq: 19 Aug 2017 13:13

Tgt Ion	Ratio	Lower	Upper
112	100		
64	87.4	38.6	57.8
63	54.1	19.3	28.9

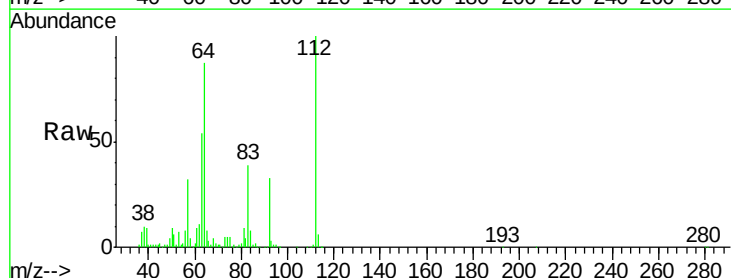

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

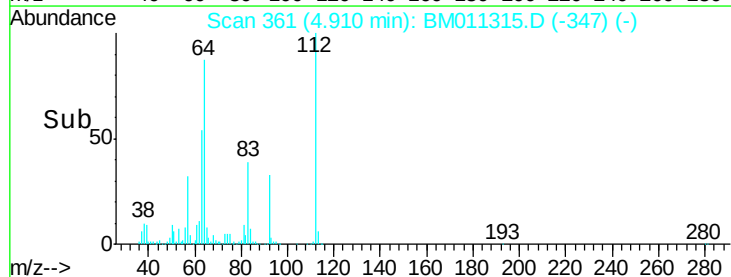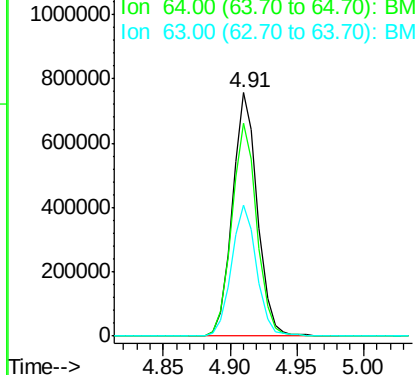

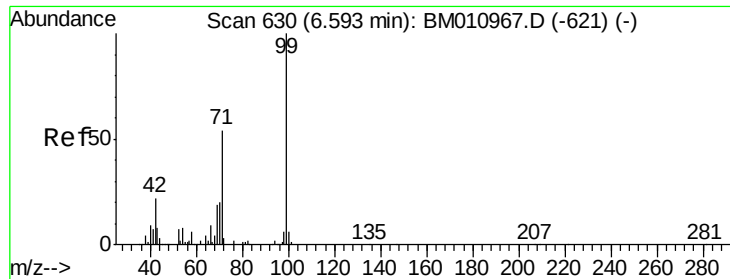

#7

Phenol-d6

Concen: 103.603 ng

RT: 6.47 min Scan# 627

Delta R.T. -0.02 min

Lab File: BM011315.D

Acq: 19 Aug 2017 13:13

Instrument :

BNA_M

ClientSampleId :

CL-02-081717-B


Tgt Ion: 99 Resp: 1300368

Ion Ratio Lower Upper

99 100

42 27.5 11.0 16.4#




71 63.5 23.4 35.2#

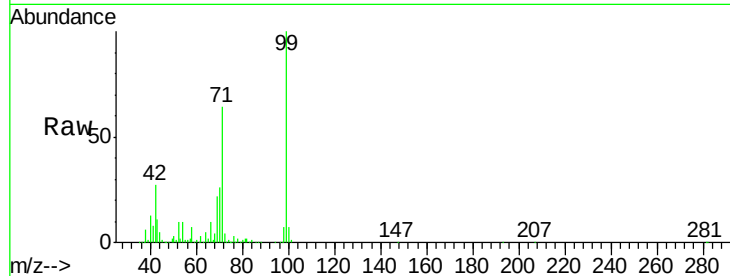

Abundance Ion 99.00 (98.70 to 99.70): BM011315.D (-613) (-)

Ion 42.00 (41.70 to 42.70): BM011315.D (-613) (-)

Ion 71.00 (70.70 to 71.70): BM011315.D (-613) (-)

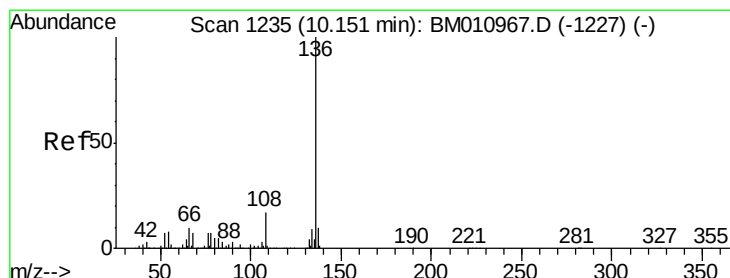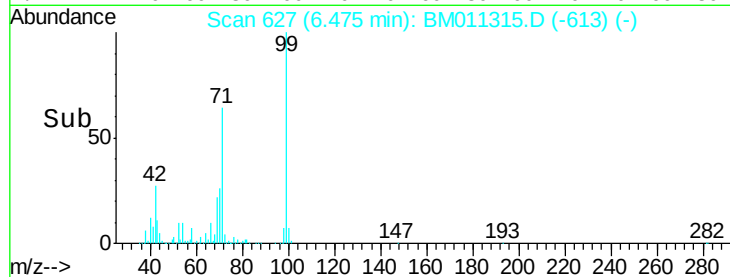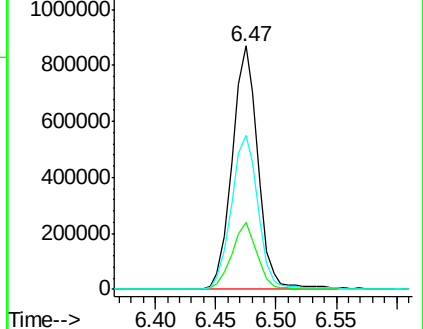

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.03 min Scan# 1231

Delta R.T. -0.02 min

Lab File: BM011315.D

Acq: 19 Aug 2017 13:13

Tgt Ion: 136 Resp: 528089


Ion Ratio Lower Upper

136 100

137 9.1 8.7 13.1

54 10.7 4.6 6.8#

68 7.7 3.7 5.5#


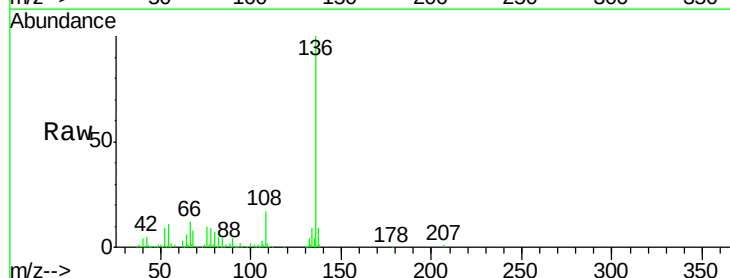



Abundance Ion 136.00 (135.70 to 136.70): BM011315.D (-1217) (-)

Ion 137.00 (136.70 to 137.70): BM011315.D (-1217) (-)

Ion 54.00 (53.70 to 54.70): BM011315.D (-1217) (-)

Ion 68.00 (67.70 to 68.70): BM011315.D (-1217) (-)



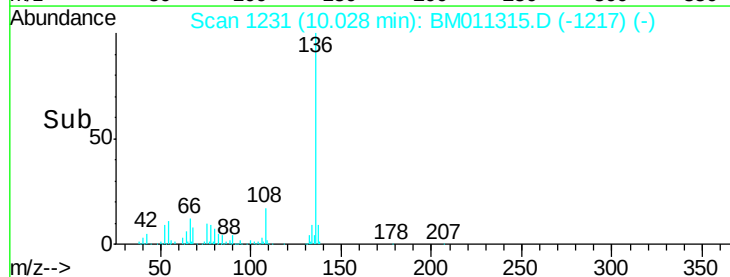
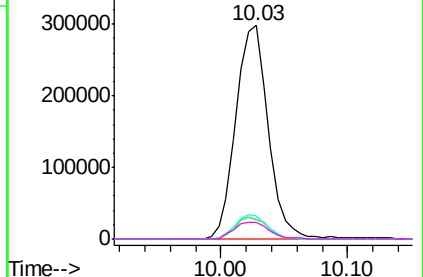


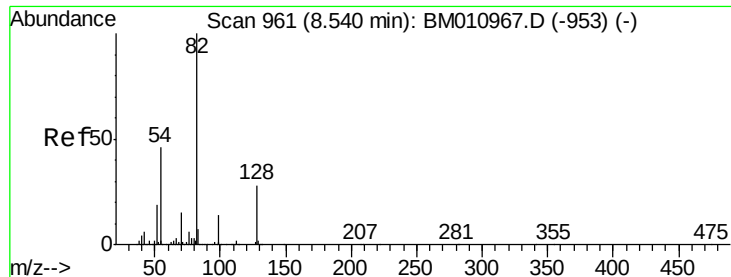

#23
 Nitrobenzene-d5
 Concen: 94.273 ng
 RT: 8.42 min Scan# 957
 Delta R.T. -0.02 min
 Lab File: BM011315.D
 Acq: 19 Aug 2017 13:13




Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-B


Tgt Ion: 82 Resp: 1326465
 Ion Ratio Lower Upper
 82 100
 128 22.1 32.8 49.2#
 54 49.5 40.6 60.8

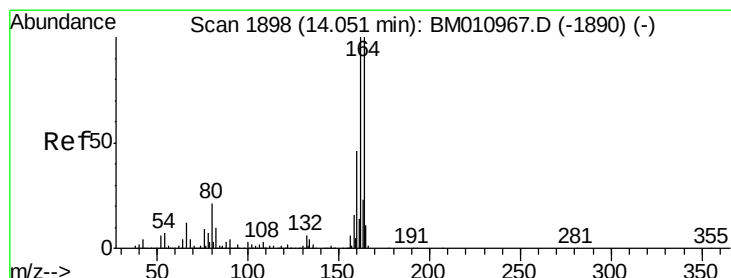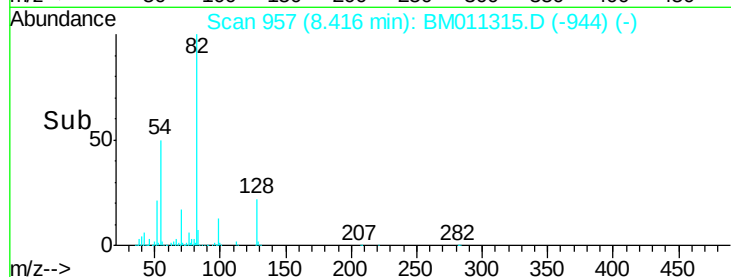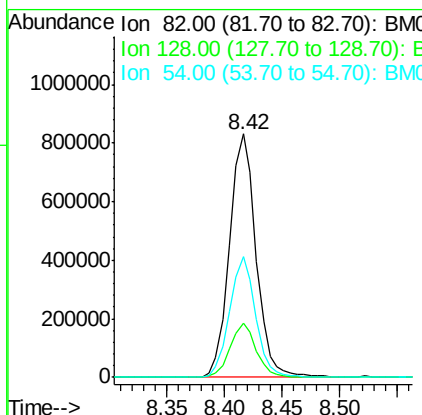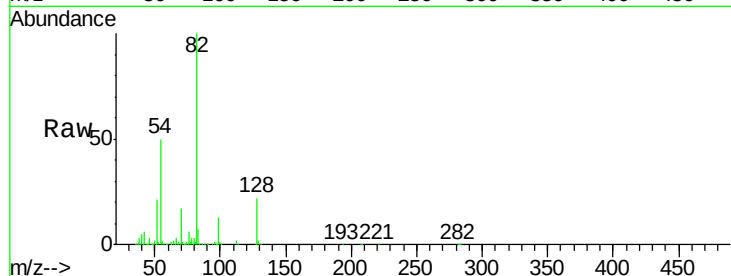

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.94 min Scan# 1896
 Delta R.T. -0.02 min
 Lab File: BM011315.D
 Acq: 19 Aug 2017 13:13

Tgt Ion: 164 Resp: 329952
 Ion Ratio Lower Upper
 164 100
 162 104.9 82.4 123.6
 160 45.2 35.8 53.6

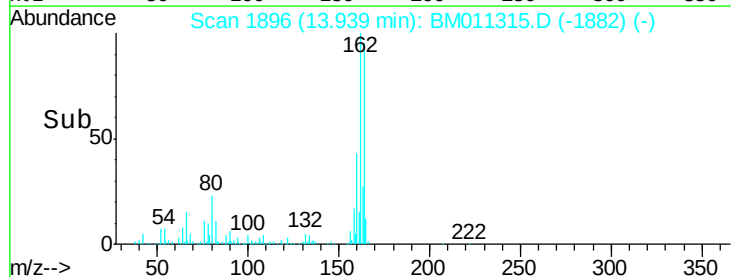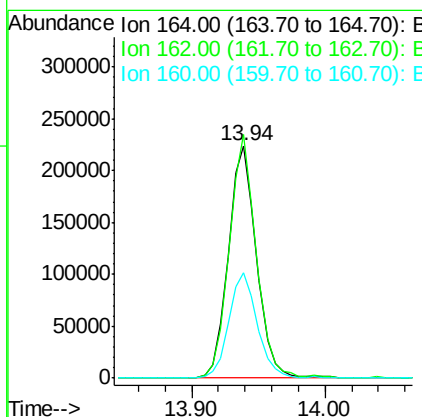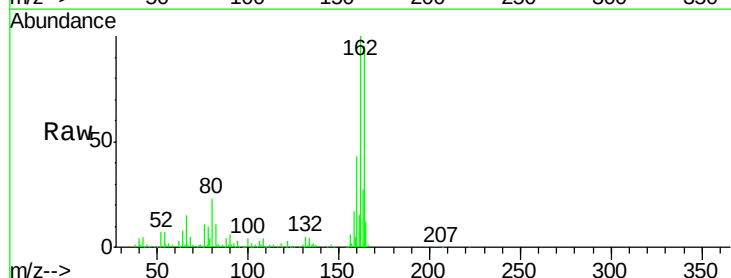


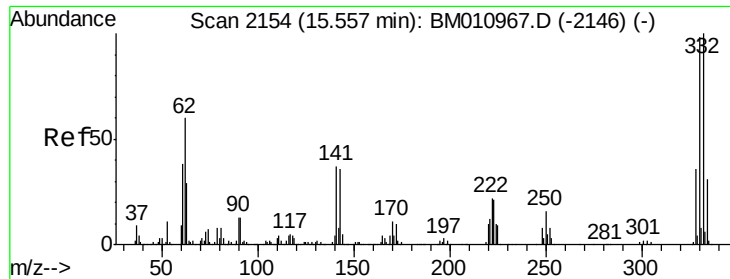




#41
 2,4,6-Tribromophenol
 Concen: 107.631 ng
 RT: 15.44 min Scan# 2152
 Delta R.T. -0.02 min
 Lab File: BM011315.D
 Acq: 19 Aug 2017 13:13

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-B

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	569200		
332	97.1	0.0	0.0	0.0
141	47.1	0.0	0.0	0.0

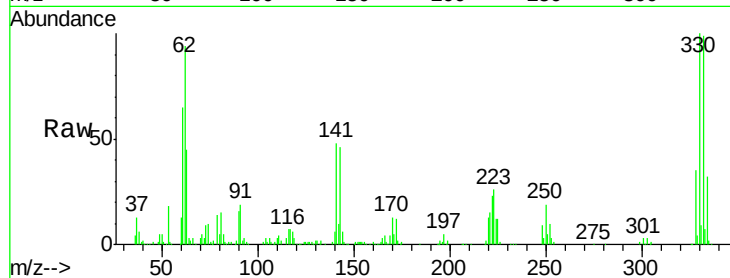


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

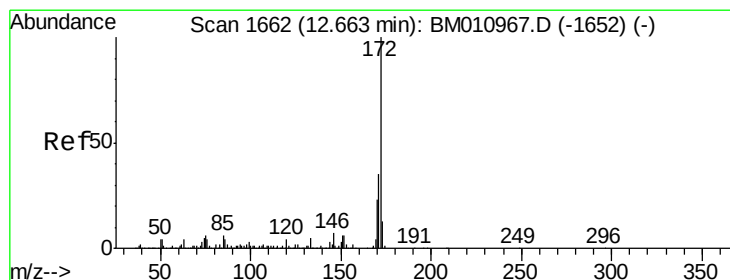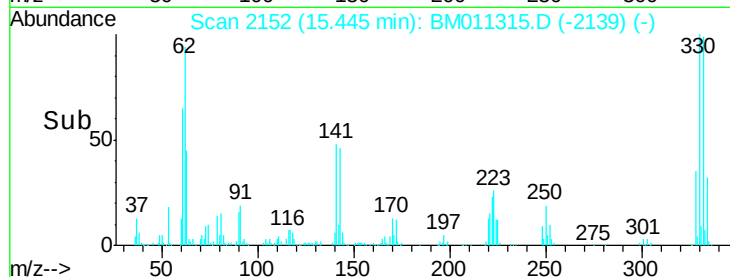
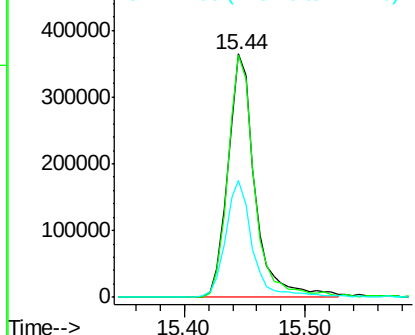



#44
 2-Fluorobiphenyl
 Concen: 79.549 ng
 RT: 12.55 min Scan# 1659
 Delta R.T. -0.02 min
 Lab File: BM011315.D
 Acq: 19 Aug 2017 13:13

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	2092853		
171	34.9	28.5	42.7	
170	23.6	18.8	28.2	

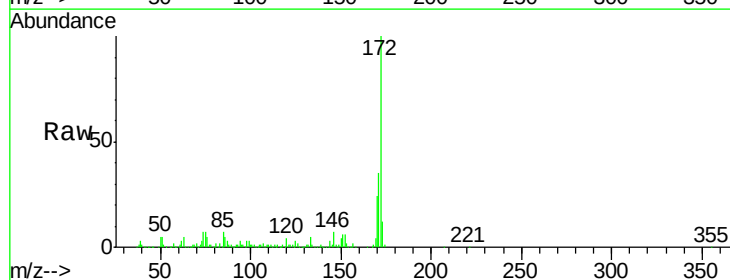

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



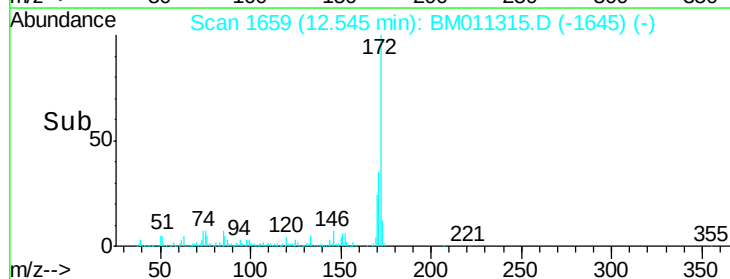
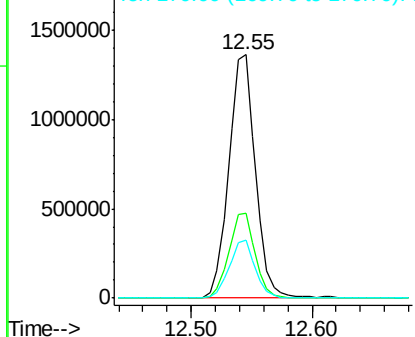


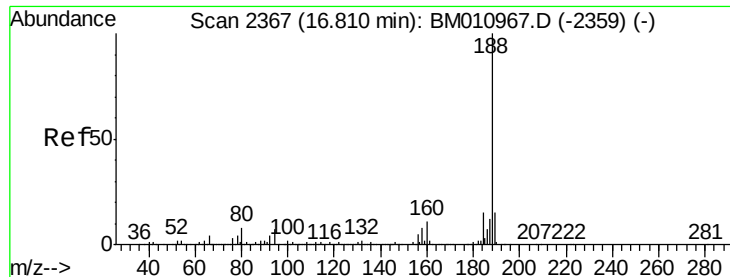

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.70 min Scan# 2365
Delta R.T. -0.02 min
Lab File: BM011315.D
Acq: 19 Aug 2017 13:13




Instrument :
BNA_M
ClientSampleId :
CL-02-081717-B


Tgt Ion:188 Resp: 812279
Ion Ratio Lower Upper
188 100
94 7.7 8.7 13.1#
80 10.5 9.3 13.9

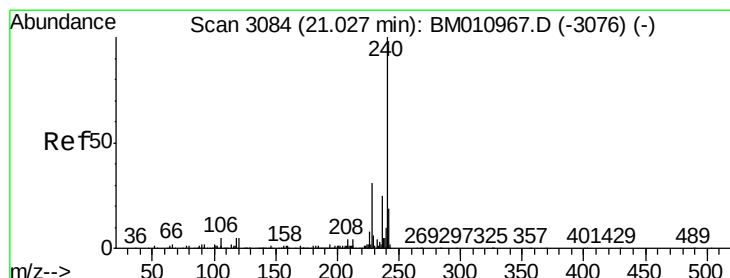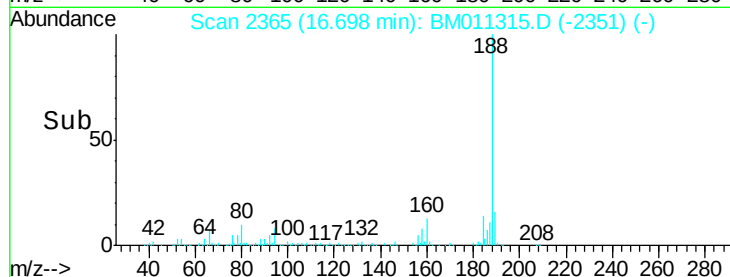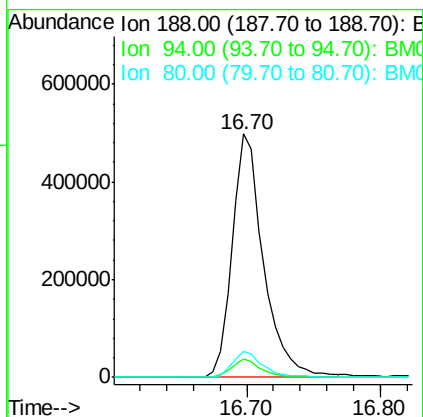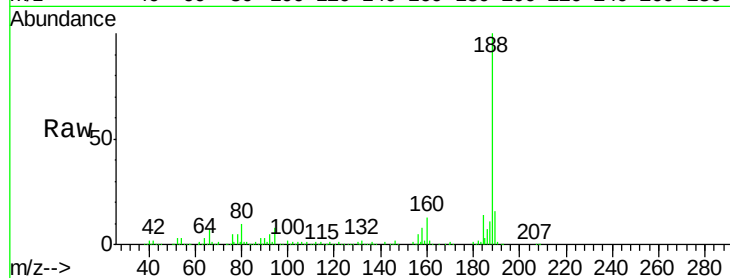

#75
Chrysene-d12
Concen: 20.000 ng
RT: 20.93 min Scan# 3084
Delta R.T. -0.02 min
Lab File: BM011315.D
Acq: 19 Aug 2017 13:13

Tgt Ion:240 Resp: 1117122
Ion Ratio Lower Upper
240 100
120 5.0 8.2 12.2#
236 27.0 20.0 30.0

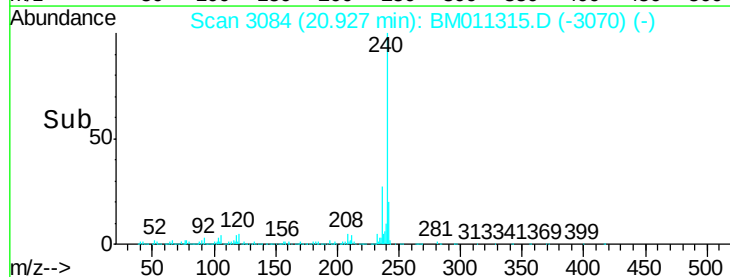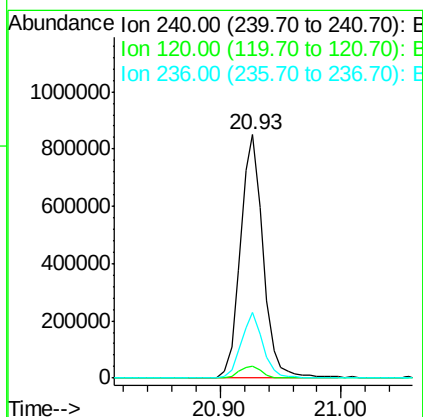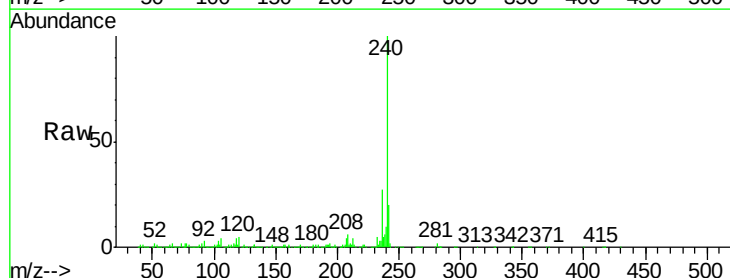

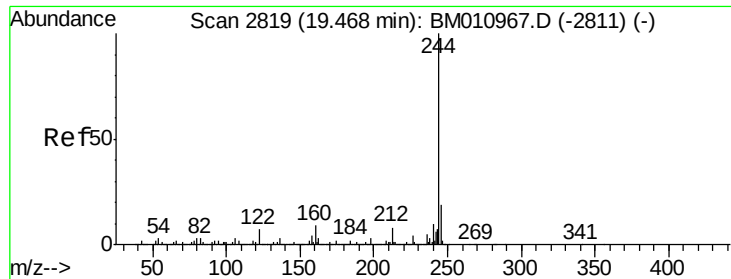

#78

Terphenyl-d14

Concen: 67.819 ng

RT: 19.37 min Scan# 2819

Delta R.T. -0.02 min

Lab File: BM011315.D

Acq: 19 Aug 2017 13:13

Instrument :

BNA_M

ClientSampleId :

CL-02-081717-B


Tgt Ion:244 Resp: 3824676

Ion Ratio Lower Upper

244 100

212 8.6 4.9 7.3#




122 6.4 6.2 9.4

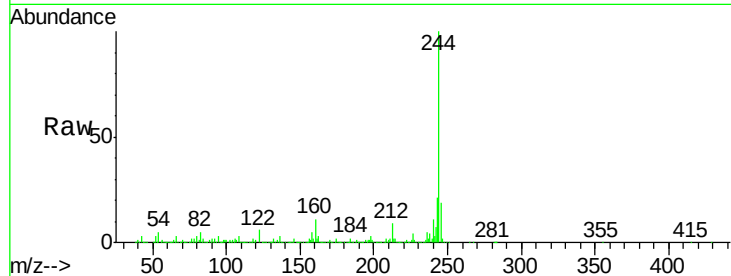

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

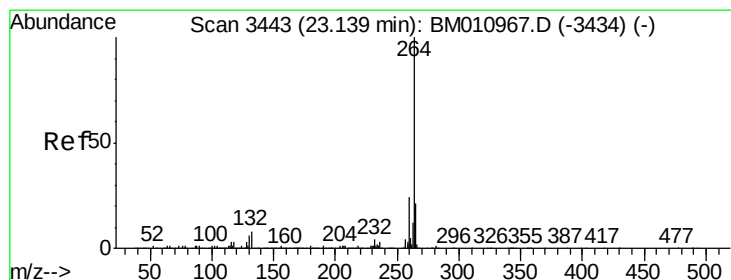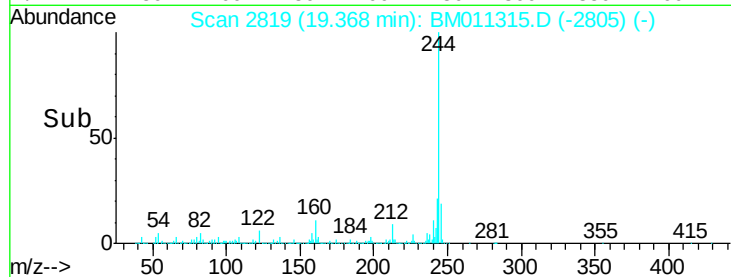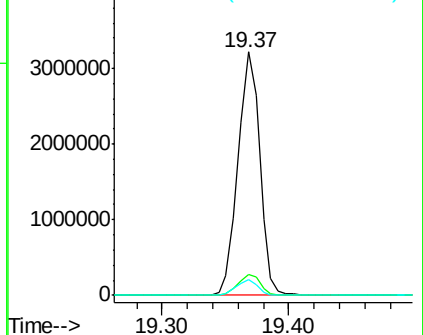

#86

Perylene-d12

Concen: 20.000 ng

RT: 22.99 min Scan# 3435

Delta R.T. -0.03 min

Lab File: BM011315.D

Acq: 19 Aug 2017 13:13


Tgt Ion:264 Resp: 1061740

Ion Ratio Lower Upper

264 100

260 24.2 18.6 27.8

265 21.9 17.3 25.9

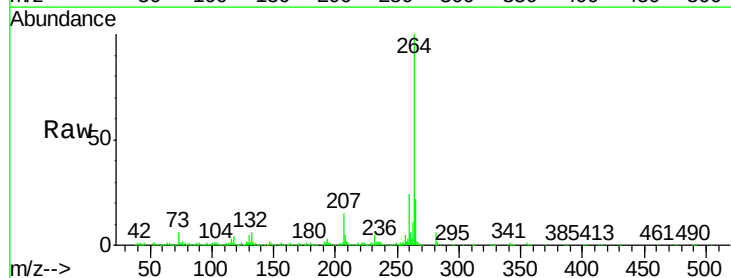

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

