

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011317.D
 Acq On : 19 Aug 2017 14:26
 Operator : SJ/JU
 Sample : I4875-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-D

Quant Time: Aug 21 02:04:44 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	130973	20.00	ng	-0.02
21) Naphthalene-d8	10.02	136	441113	20.00	ng	-0.02
38) Acenaphthene-d10	13.93	164	276025	20.00	ng	-0.02
63) Phenanthrene-d10	16.70	188	686275	20.00	ng	-0.02
75) Chrysene-d12	20.93	240	957598	20.00	ng	-0.02
86) Perylene-d12	22.99	264	935130	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	883442	114.02	ng	-0.02
7) Phenol-d6	6.47	99	1147681	104.26	ng	-0.02
23) Nitrobenzene-d5	8.42	82	1210281	102.98	ng	-0.02
41) 2,4,6-Tribromophenol	15.44	330	484481	109.51	ng	-0.02
44) 2-Fluorobiphenyl	12.54	172	1859011	84.47	ng	-0.02
78) Terphenyl-d14	19.37	244	3335828	69.00	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011317.D
Acq On : 19 Aug 2017 14:26
Operator : SJ/JU
Sample : I4875-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-081717-D

Quant Time: Aug 21 02:04:44 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

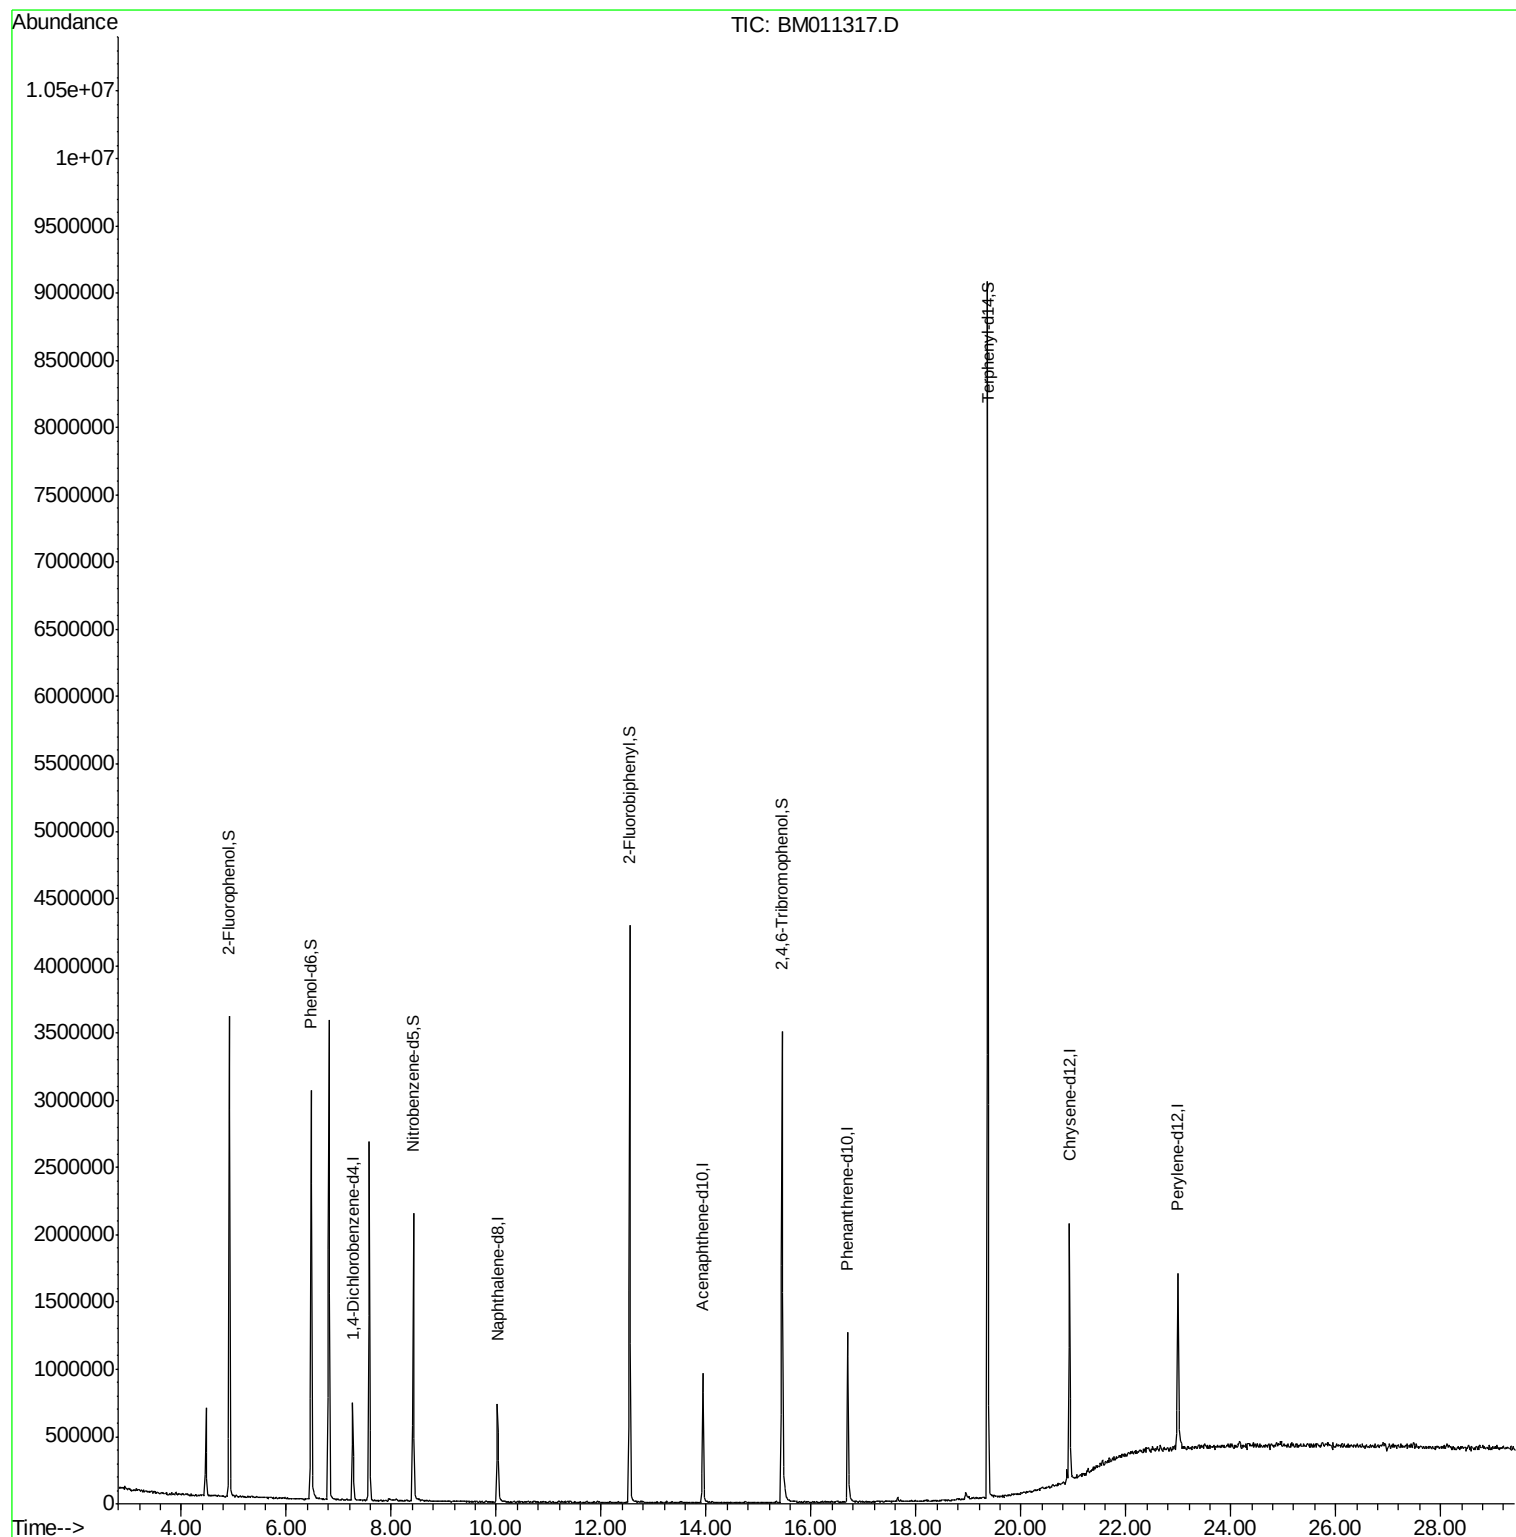




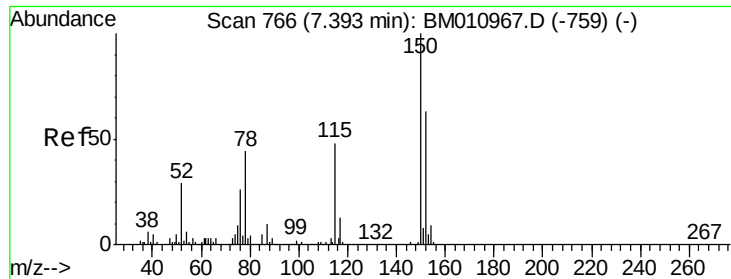


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.27 min Scan# 762
Delta R.T. -0.02 min
Lab File: BM011317.D
Acq: 19 Aug 2017 14:26

Instrument :
BNA_M
ClientSampleId :
CL-02-081717-D




Tgt Ion:152 Resp: 130973
Ion Ratio Lower Upper
152 100
150 154.3 119.5 179.3
115 73.7 43.0 64.4#

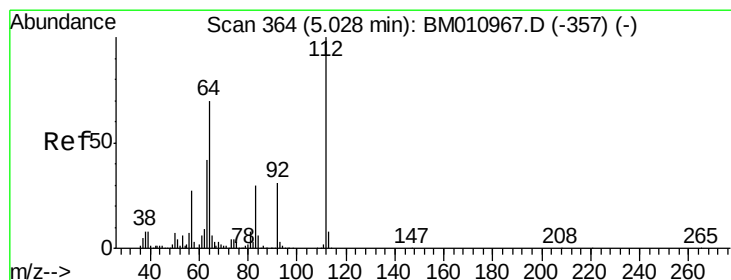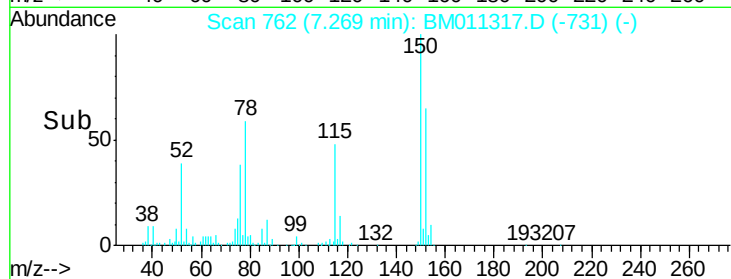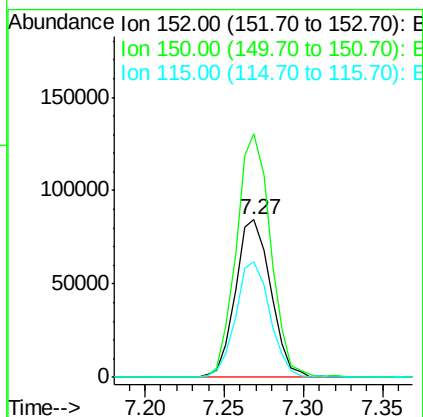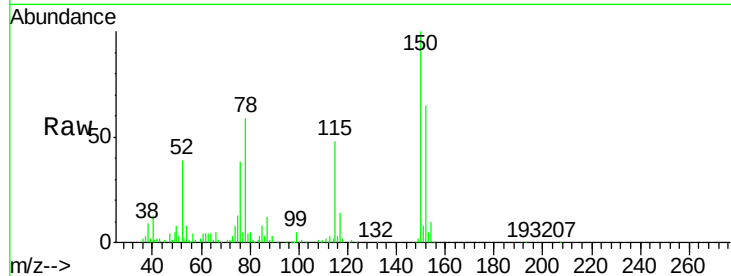


#5

2-Fluorophenol
Concen: 114.024 ng
RT: 4.91 min Scan# 361
Delta R.T. -0.02 min
Lab File: BM011317.D
Acq: 19 Aug 2017 14:26

Tgt Ion:112 Resp: 883442
Ion Ratio Lower Upper
112 100
64 89.8 38.6 57.8#
63 55.4 19.3 28.9#

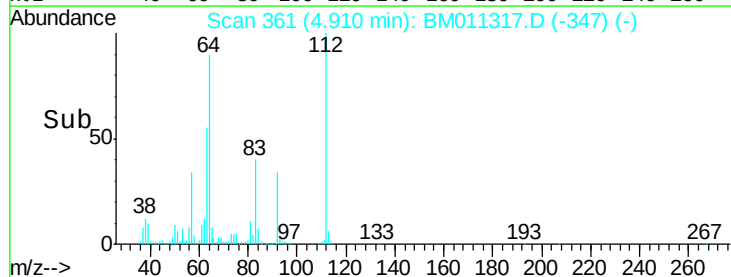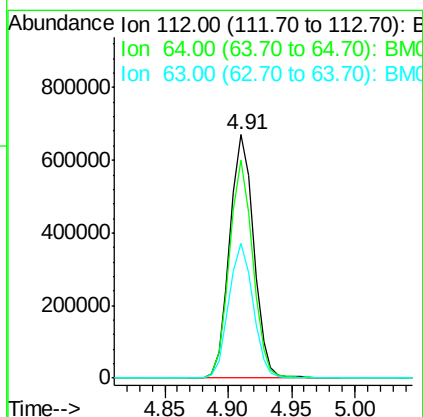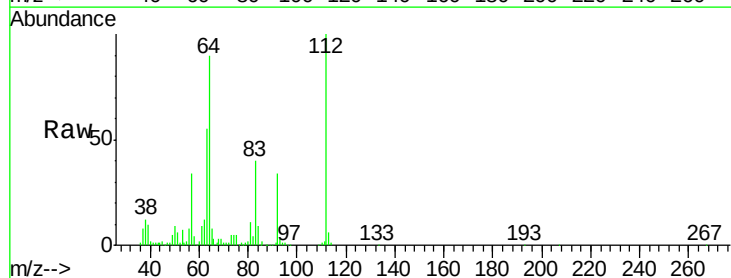

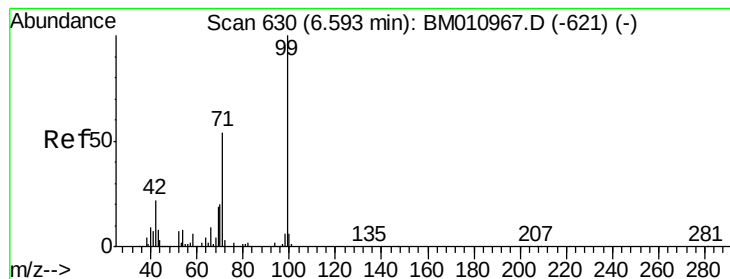

#7

Phenol-d6

Concen: 104.256 ng

RT: 6.47 min Scan# 627

Delta R.T. -0.02 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26

Instrument :

BNA_M

ClientSampleId :

CL-02-081717-D





Tgt Ion: 99 Resp: 1147681

Ion Ratio Lower Upper

99 100

42 27.7 11.0 16.4#

71 70.4 23.4 35.2#

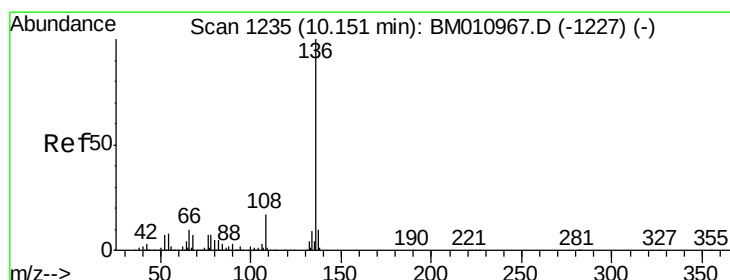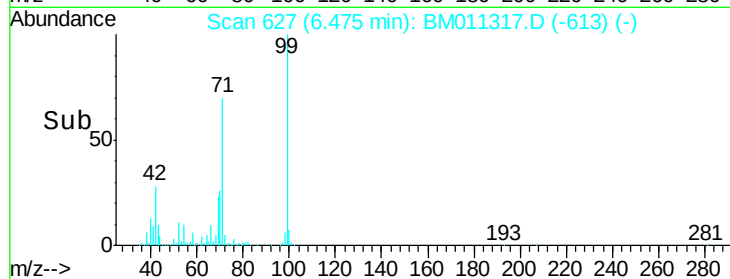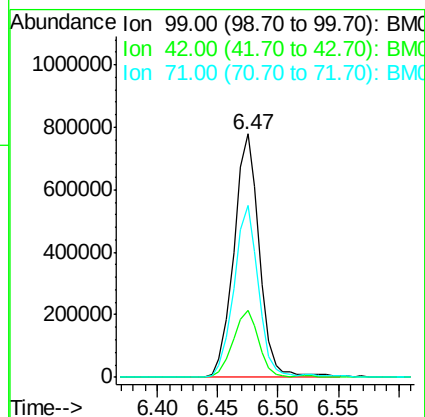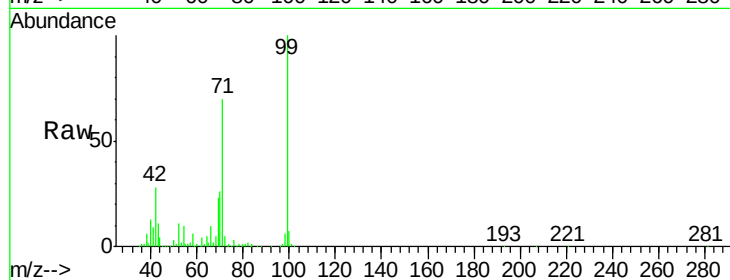

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.02 min Scan# 1230

Delta R.T. -0.02 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26

Tgt Ion: 136 Resp: 441113




Ion Ratio Lower Upper


136 100

137 9.7 8.7 13.1

54 11.2 4.6 6.8#

68 8.8 3.7 5.5#


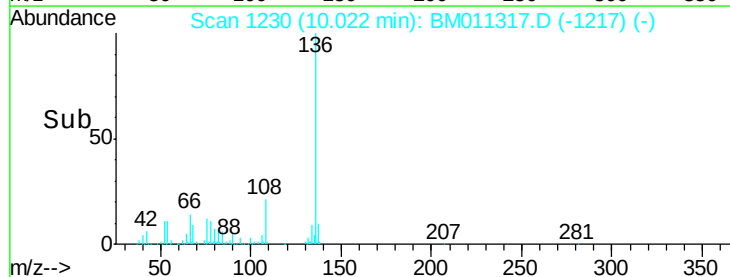
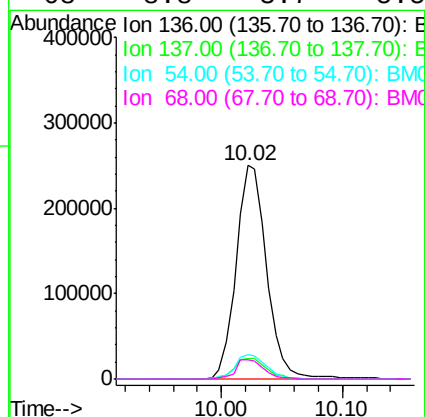
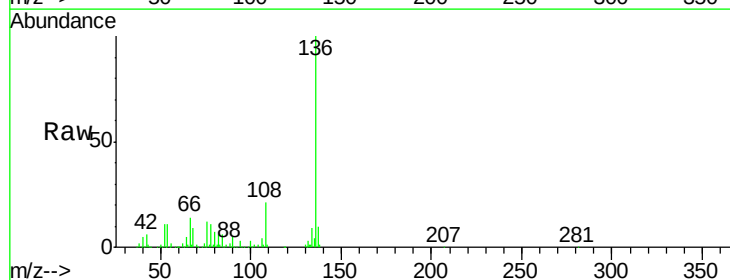


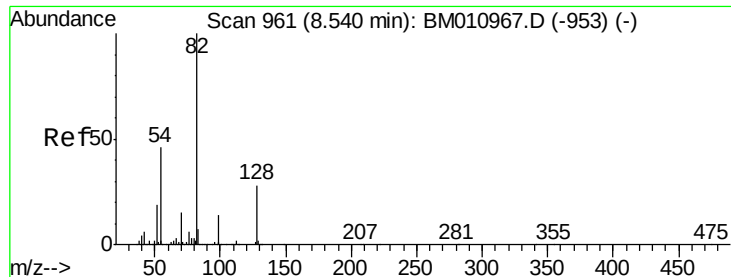

#23
 Nitrobenzene-d5
 Concen: 102.975 ng
 RT: 8.42 min Scan# 957
 Delta R.T. -0.02 min
 Lab File: BM011317.D
 Acq: 19 Aug 2017 14:26




Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-D


Tgt Ion: 82 Resp: 1210281
 Ion Ratio Lower Upper
 82 100
 128 21.4 32.8 49.2#
 54 51.1 40.6 60.8

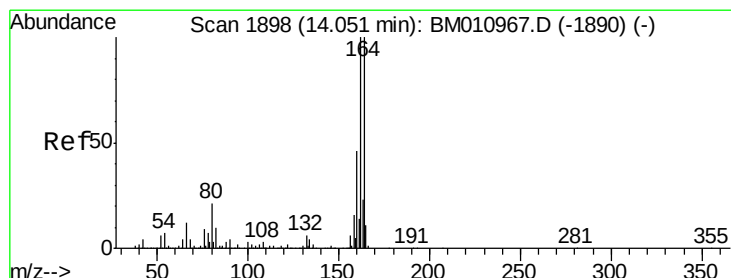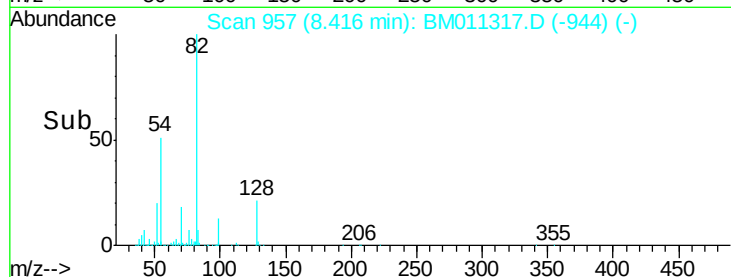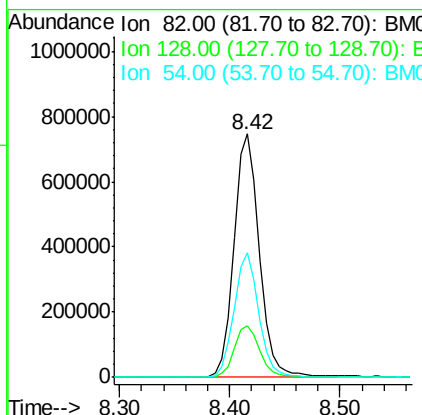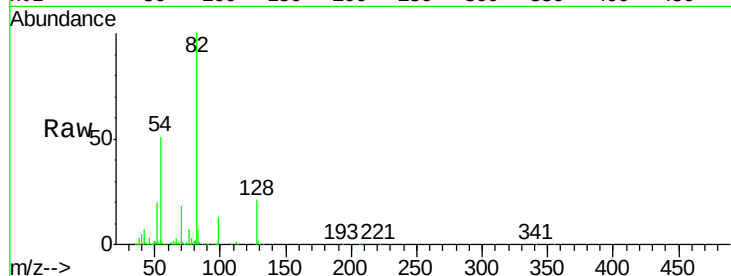

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 13.93 min Scan# 1895
 Delta R.T. -0.02 min
 Lab File: BM011317.D
 Acq: 19 Aug 2017 14:26

Tgt Ion: 164 Resp: 276025
 Ion Ratio Lower Upper
 164 100
 162 95.3 82.4 123.6
 160 41.7 35.8 53.6

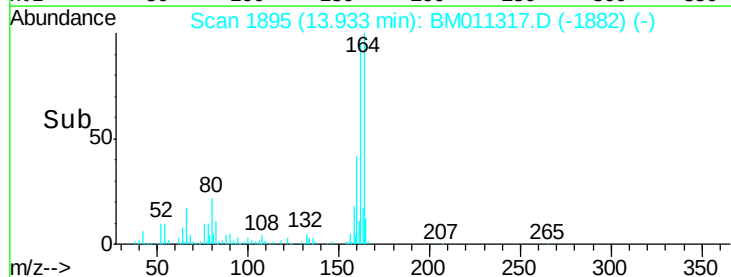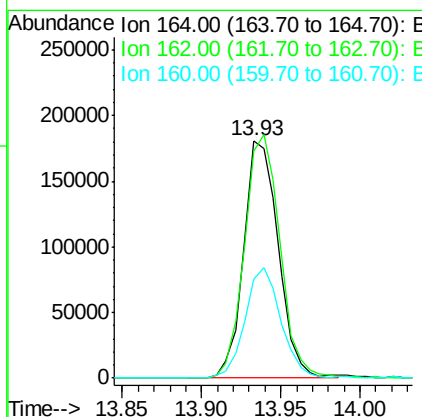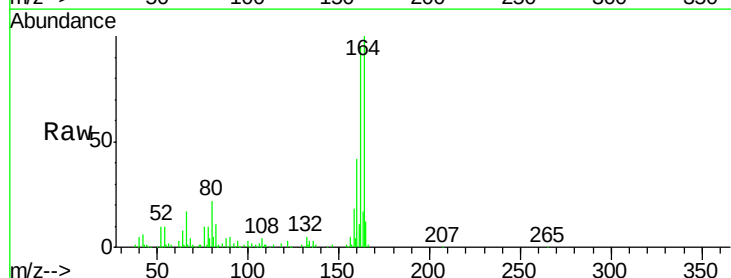


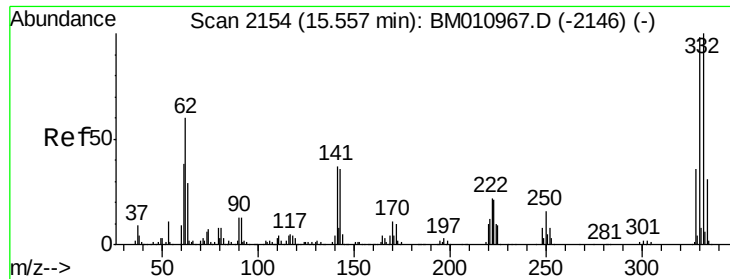




#41
 2,4,6-Tribromophenol
 Concen: 109.509 ng
 RT: 15.44 min Scan# 2152
 Delta R.T. -0.02 min
 Lab File: BM011317.D
 Acq: 19 Aug 2017 14:26

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-081717-D

Tgt Ion	Ratio	Resp	Lower	Upper
330	100			
332	98.9	0.0	0.0	0.0
141	49.4	0.0	0.0	0.0

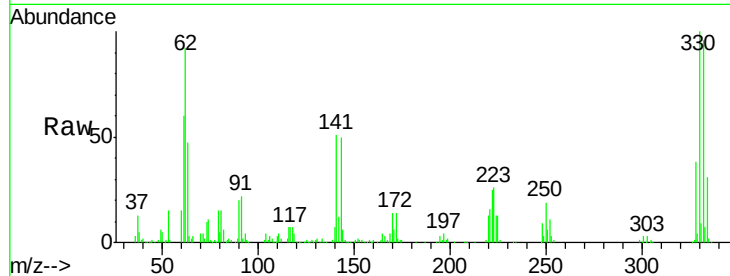


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

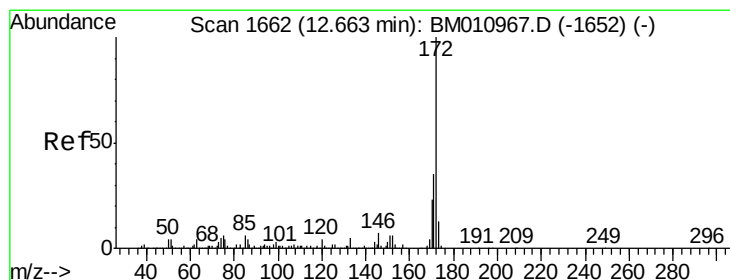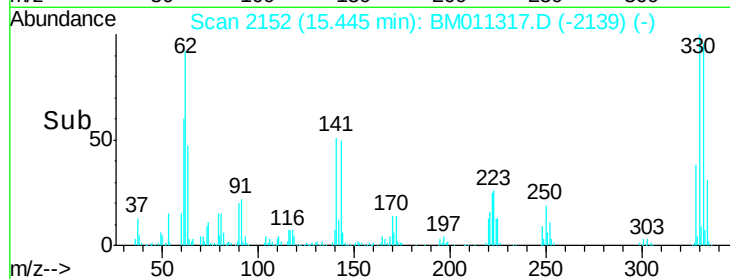
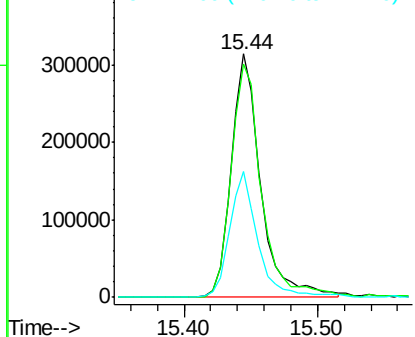



#44
 2-Fluorobiphenyl
 Concen: 84.465 ng
 RT: 12.54 min Scan# 1659
 Delta R.T. -0.02 min
 Lab File: BM011317.D
 Acq: 19 Aug 2017 14:26

Tgt Ion	Ratio	Resp	Lower	Upper
172	100			
171	35.0	28.5	42.7	
170	23.3	18.8	28.2	

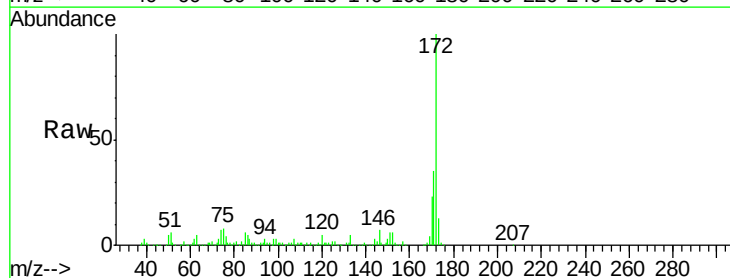

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

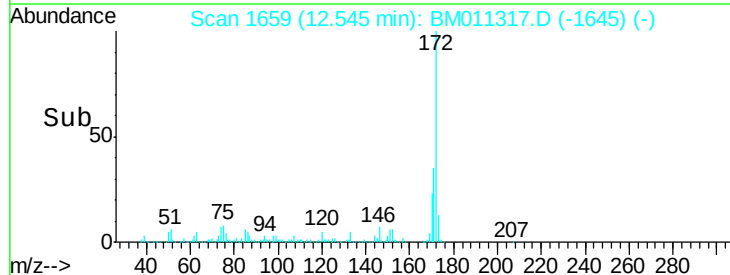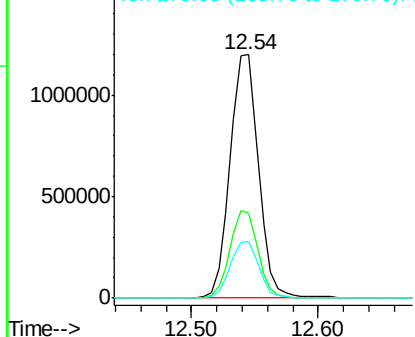

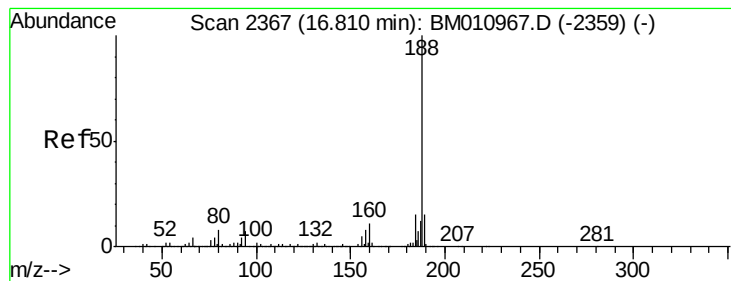

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.70 min Scan# 2365

Delta R.T. -0.02 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26

Instrument :

BNA_M

ClientSampleId :

CL-02-081717-D


Tgt Ion:188 Resp: 686275

Ion Ratio Lower Upper

188 100

94 7.3 8.7 13.1#




80 11.7 9.3 13.9

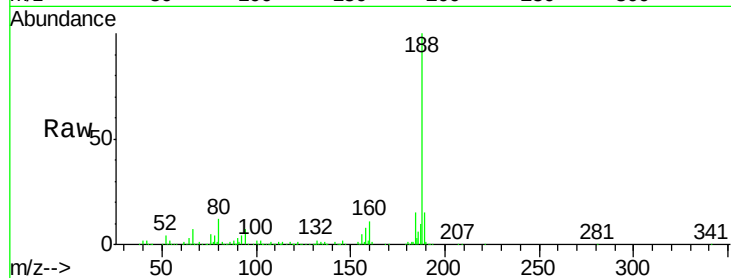

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

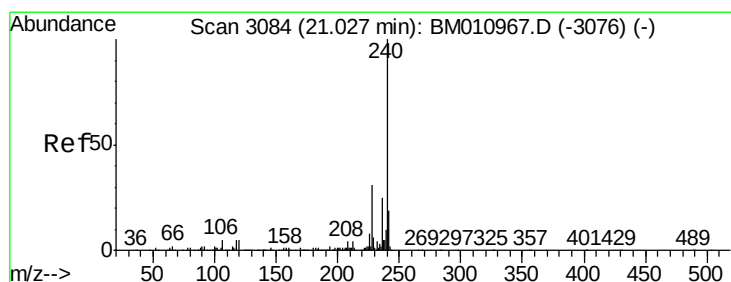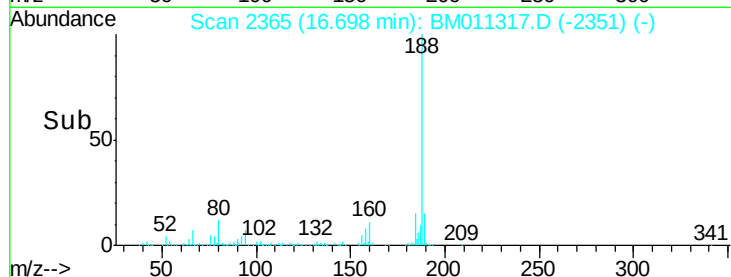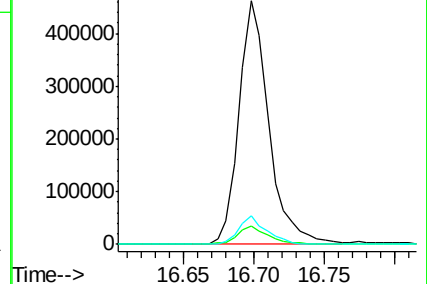

#75

Chrysene-d12

Concen: 20.000 ng

RT: 20.93 min Scan# 3084

Delta R.T. -0.02 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26


Tgt Ion:240 Resp: 957598

Ion Ratio Lower Upper

240 100

120 4.5 8.2 12.2#



236 26.2 20.0 30.0

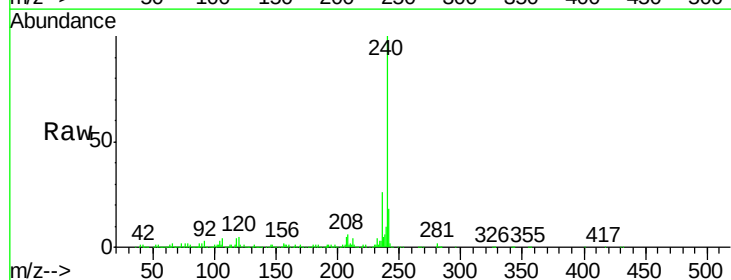


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

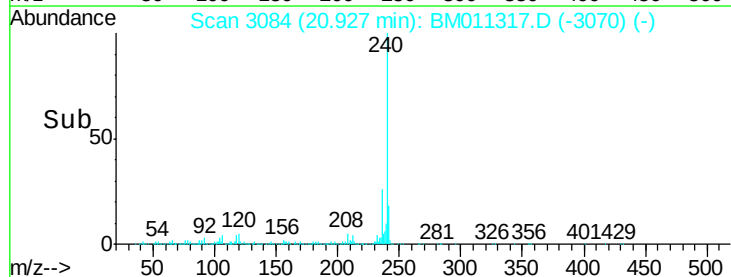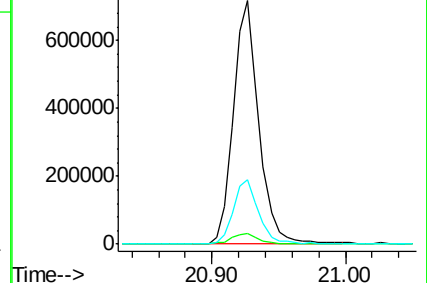

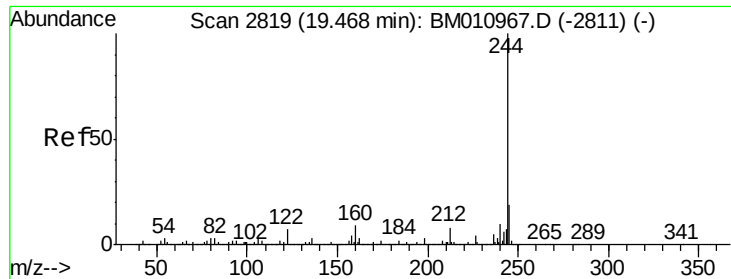

#78

Terphenyl-d14

Concen: 69.004 ng

RT: 19.37 min Scan# 2819

Delta R.T. -0.02 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26

Instrument :

BNA_M

ClientSampleId :

CL-02-081717-D


Tgt Ion:244 Resp: 3335828

Ion Ratio Lower Upper

244 100

212 8.8 4.9 7.3#




122 6.5 6.2 9.4

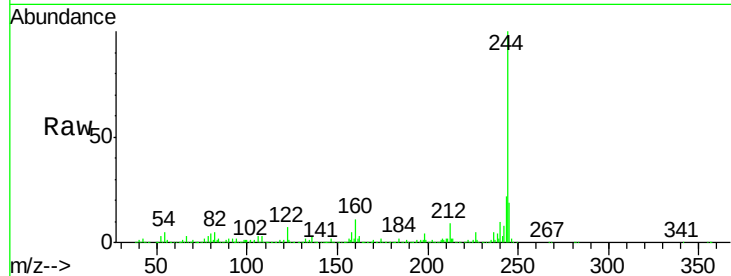

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

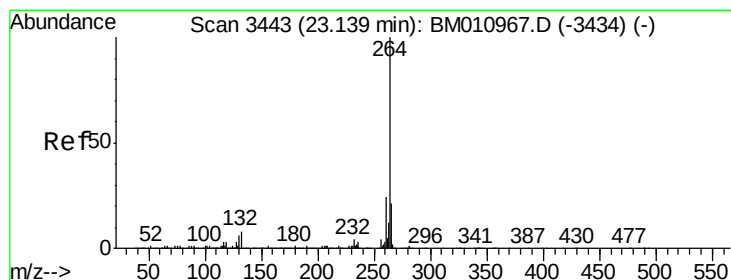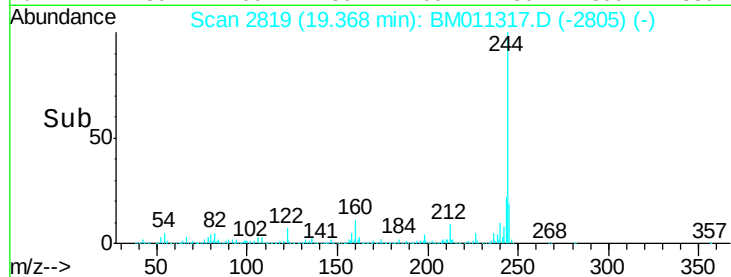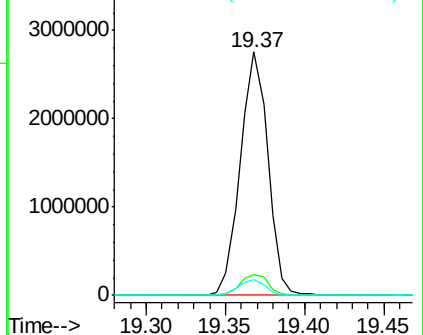

#86

Perylene-d12

Concen: 20.000 ng

RT: 22.99 min Scan# 3435

Delta R.T. -0.03 min

Lab File: BM011317.D

Acq: 19 Aug 2017 14:26


Tgt Ion:264 Resp: 935130

Ion Ratio Lower Upper

264 100

260 22.8 18.6 27.8

265 20.6 17.3 25.9

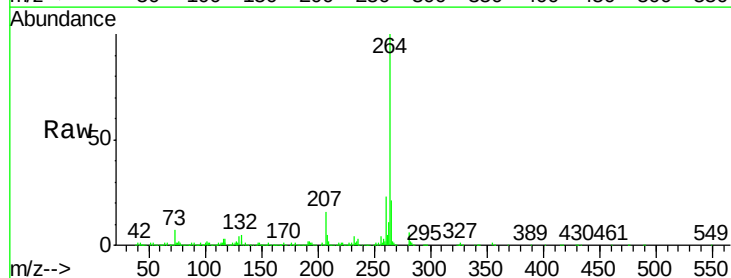

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

