

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011324.D
 Acq On : 19 Aug 2017 18:41
 Operator : SJ/JU
 Sample : I4848-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A2882RE

Quant Time: Aug 21 12:29:03 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 16 02:25:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.27	152	139697	20.00	ng	-0.02
21) Naphthalene-d8	10.02	136	533853	20.00	ng	-0.02
38) Acenaphthene-d10	13.93	164	458187	20.00	ng	-0.02
63) Phenanthrene-d10	16.70	188	1244580	20.00	ng	-0.02
75) Chrysene-d12	20.94	240	2190440	20.00	ng	0.00
86) Perylene-d12	23.04	264	1905943	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	4.91	112	92812	11.23	ng	-0.02
7) Phenol-d6	6.47	99	93712	7.98	ng	-0.02
23) Nitrobenzene-d5	8.42	82	568923	40.00	ng	-0.02
41) 2,4,6-Tribromophenol	15.44	330	195564	26.63	ng	-0.02
44) 2-Fluorobiphenyl	12.54	172	1224041	33.50	ng	-0.02
78) Terphenyl-d14	19.37	244	2504856	22.65	ng	-0.01
Target Compounds						
10) Phenol	6.50	94	34879	2.735	ng	Qvalue 88
20) 3+4-Methylphenols	8.05	107	29212	2.578	ng	# 81
37) 2-Methylnaphthalene	11.70	142	54406	2.758	ng	# 72
49) Dimethylphthalate	13.41	163	329726	8.412	ng	98
70) Phenanthrene	16.74	178	214004	3.284	ng	# 89
83) Bis(2-ethylhexyl)phthalate	20.90	149	996027	14.629	ng	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011324.D
Acq On : 19 Aug 2017 18:41
Operator : SJ/JU
Sample : I4848-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A2882RE

Quant Time: Aug 21 12:29:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 16 02:25:04 2017
Response via : Initial Calibration

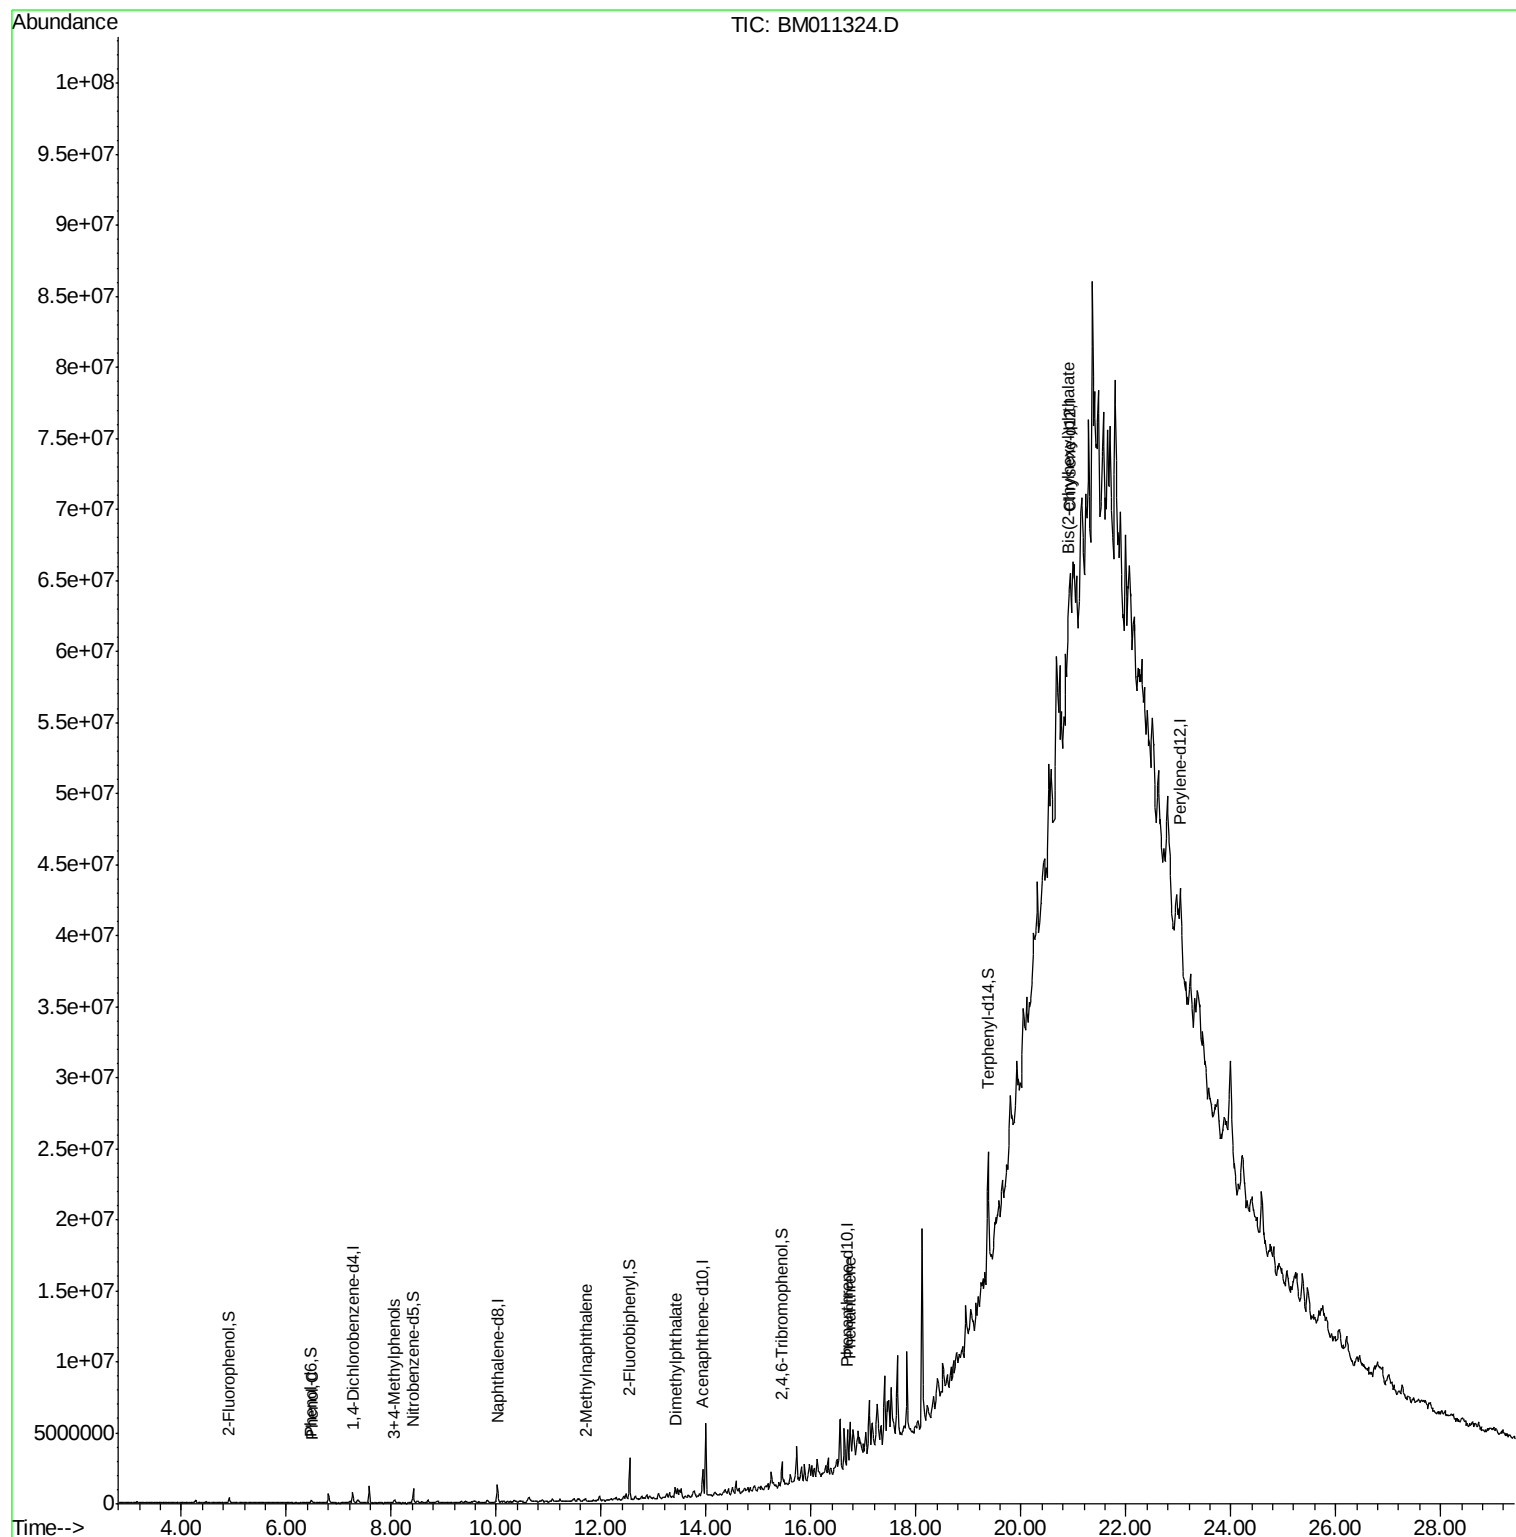




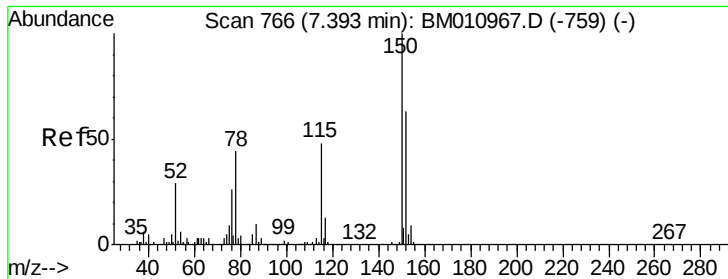


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.27 min Scan# 762
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41

Instrument :
BNA_M
ClientSampleId :
A2882RE




Tgt Ion	Resp	Lower	Upper
152	139697		
150	163.6	119.5	179.3
115	71.9	43.0	64.4#

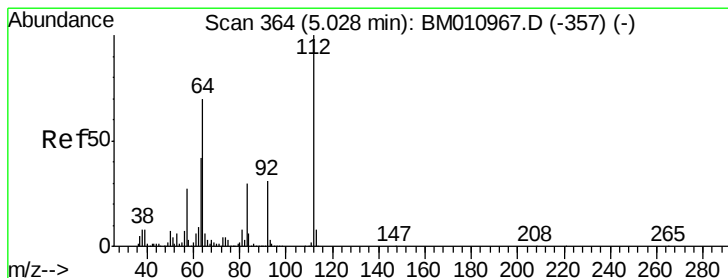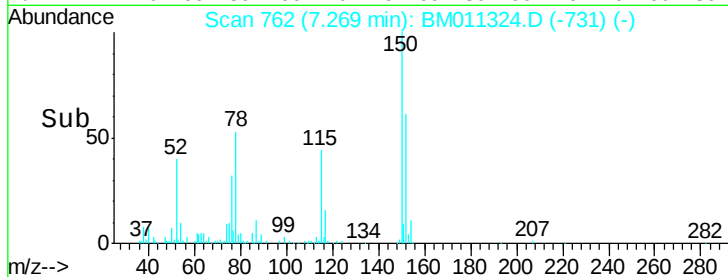
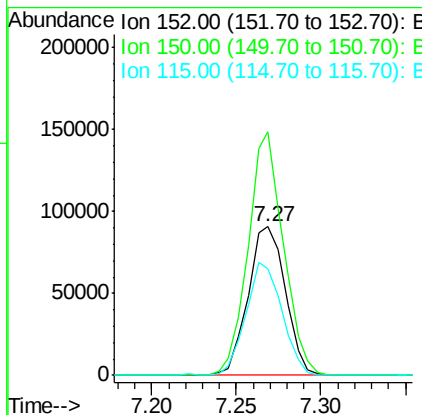
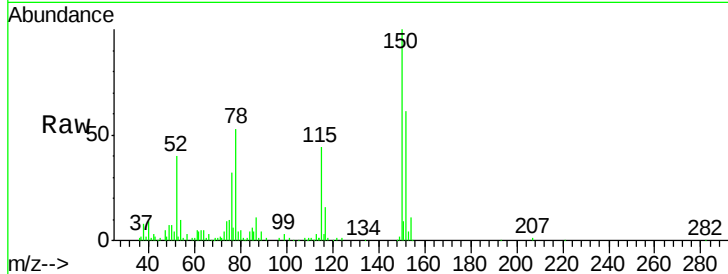


#5

2-Fluorophenol
Concen: 11.231 ng
RT: 4.91 min Scan# 361
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41

Tgt Ion	Resp	Lower	Upper
112	92812		
112	100		
64	96.3	38.6	57.8#
63	57.3	19.3	28.9#

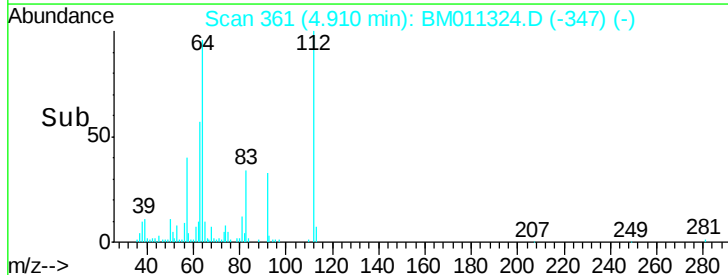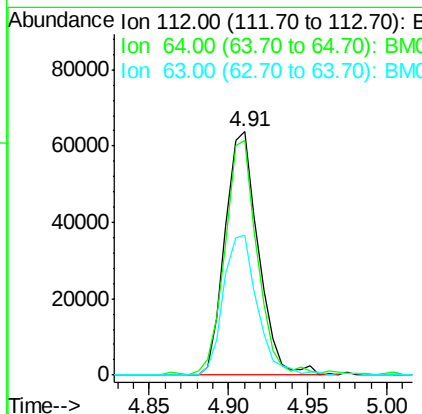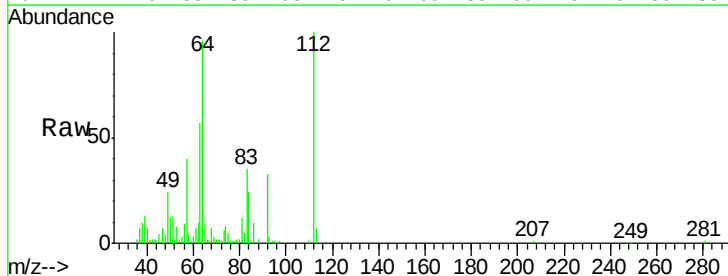

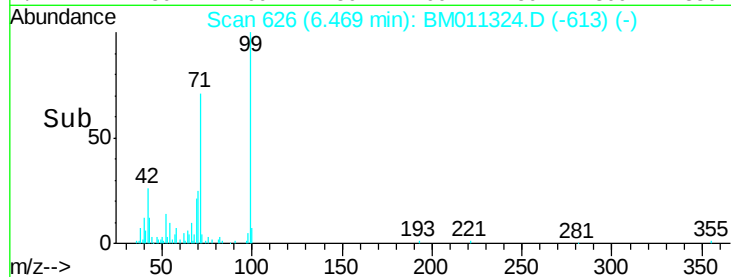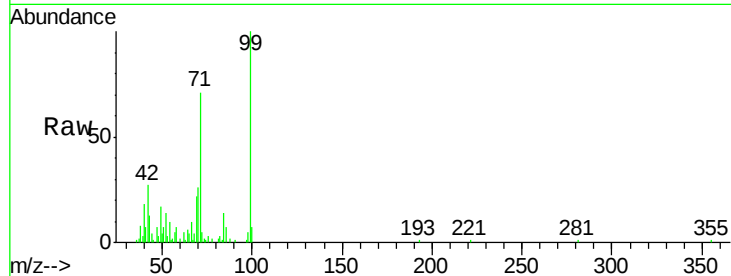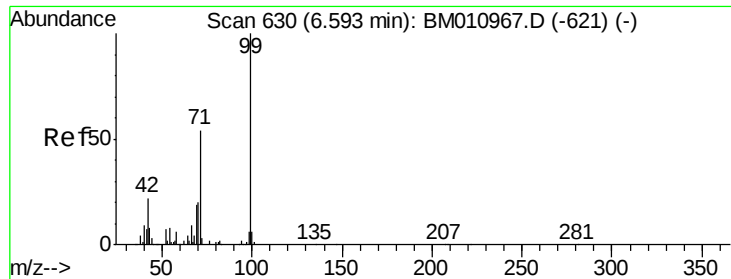

#7

Phenol-d6

Concen: 7.981 ng

RT: 6.47 min Scan# 626

Delta R.T. -0.02 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41

Instrument :

BNA_M

ClientSampleId :

A2882RE





Tgt Ion: 99 Resp: 93712

Ion Ratio Lower Upper

99 100

42 26.8 11.0 16.4#

71 71.2 23.4 35.2#

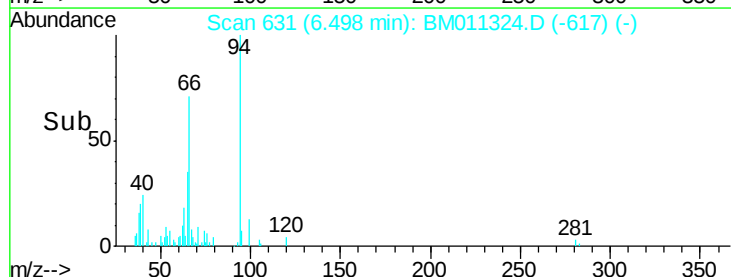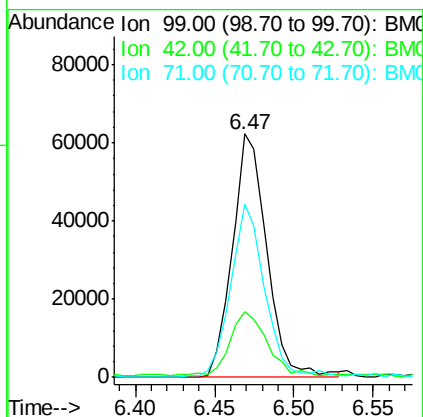

#10

Phenol

Concen: 2.735 ng

RT: 6.50 min Scan# 631

Delta R.T. -0.02 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41


Tgt Ion: 94 Resp: 34879


Ion Ratio Lower Upper

94 100

65 34.6 18.8 58.8

66 71.4 39.9 79.9




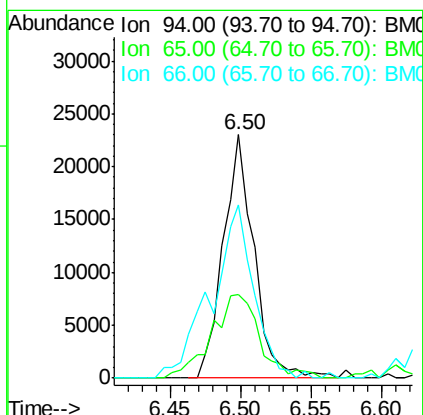


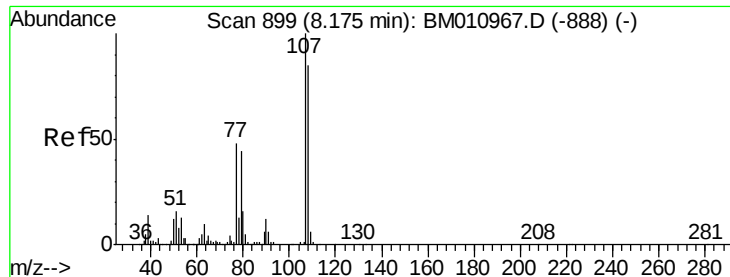

#20
3+4-Methylphenols
Concen: 2.578 ng
RT: 8.05 min Scan# 895
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41




Instrument :
BNA_M
ClientSampleId :
A2882RE


Tgt Ion:	107	Resp:	29212
Ion	Ratio	Lower	Upper
107	100		
108	83.2	73.2	113.2
77	55.2	10.7	50.7#
79	38.9	9.6	49.6

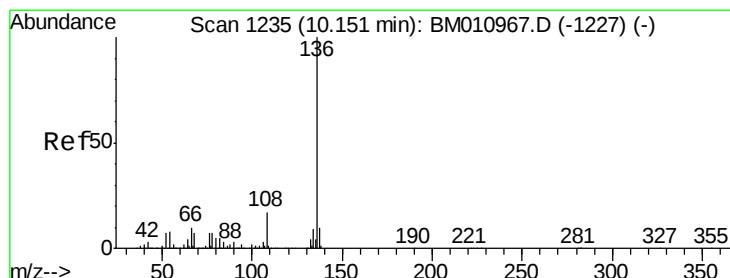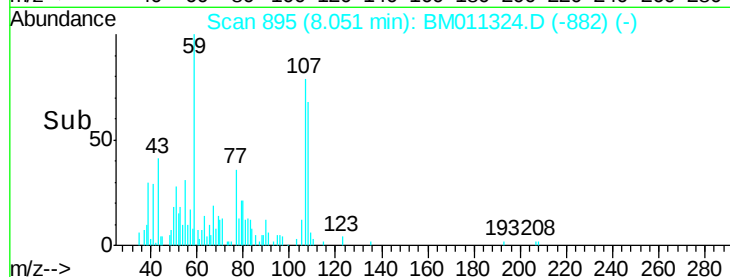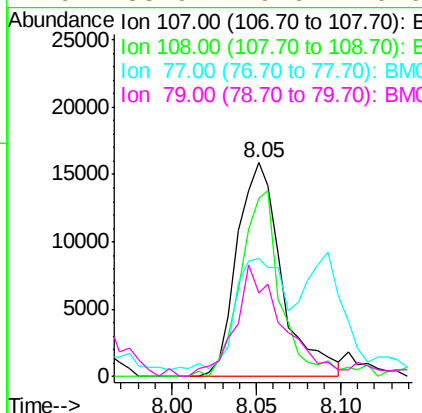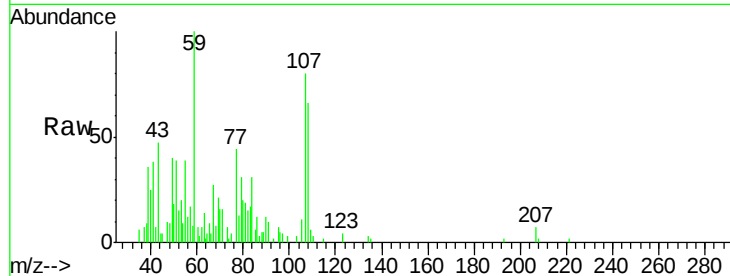

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.02 min Scan# 1230
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41

Tgt Ion:	136	Resp:	533853
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.7	13.1
54	14.1	4.6	6.8#
68	10.5	3.7	5.5#


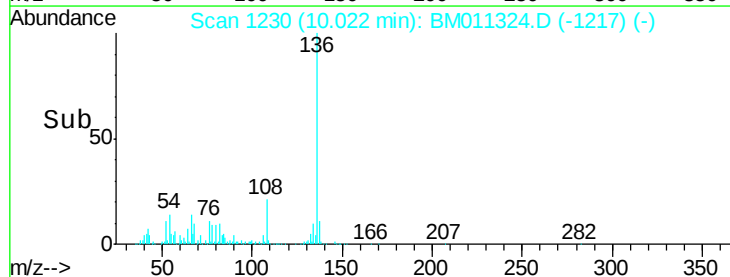
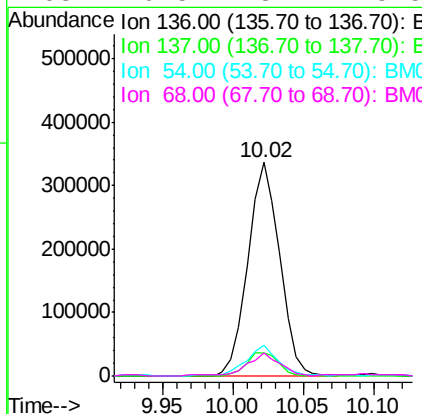
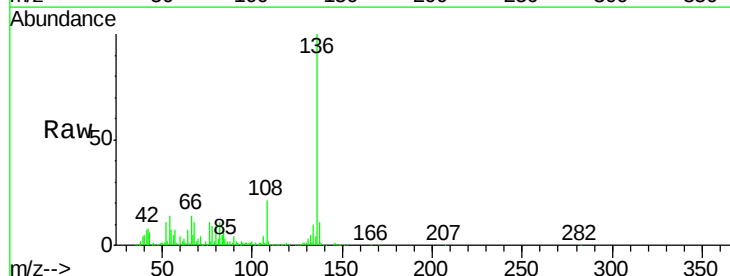


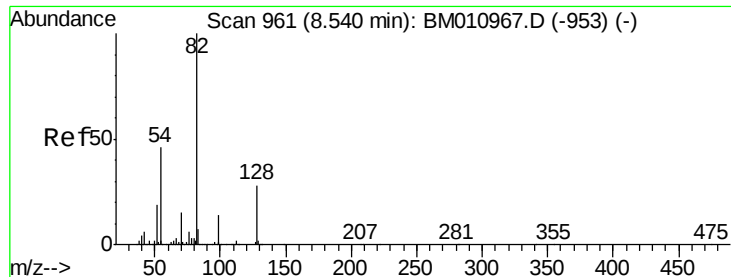

#23
 Nitrobenzene-d5
 Concen: 39.997 ng
 RT: 8.42 min Scan# 957
 Delta R.T. -0.02 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41




Instrument :
 BNA_M
 ClientSampleId :
 A2882RE


Tgt Ion	Ratio	Lower	Upper
82	100		
128	20.0	32.8	49.2#
54	49.6	40.6	60.8

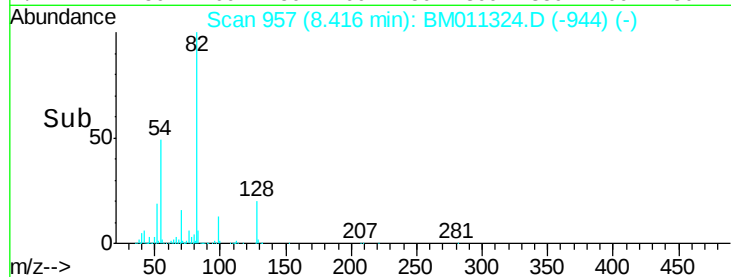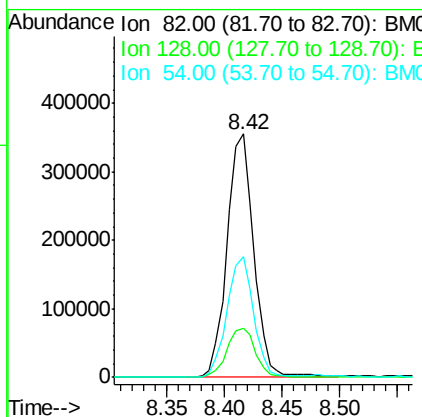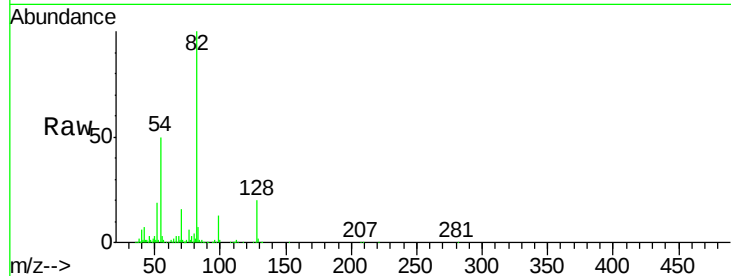

#37
 2-Methylnaphthalene
 Concen: 2.758 ng
 RT: 11.70 min Scan# 1515
 Delta R.T. -0.02 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41

Tgt Ion	Ratio	Lower	Upper
142	100		
141	79.1	71.9	107.9
115	74.2	25.4	38.0#

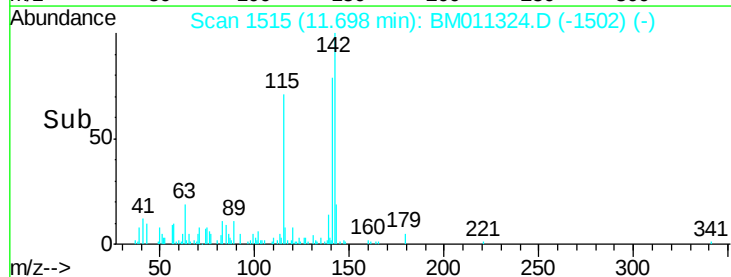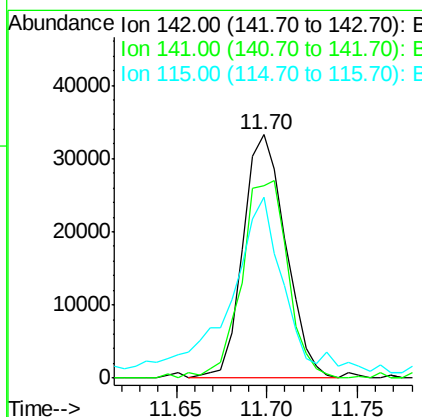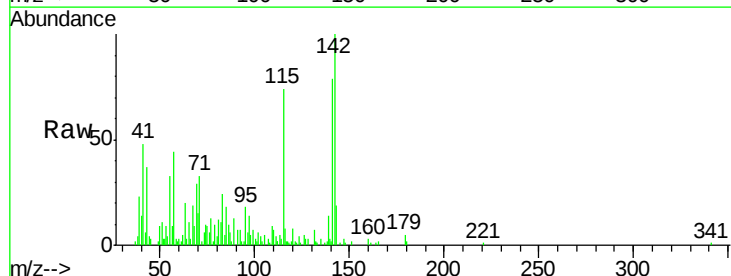

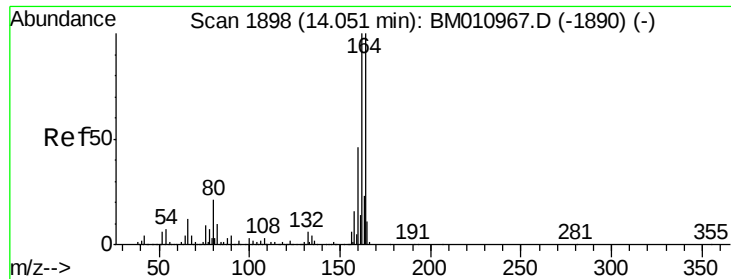

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 13.93 min Scan# 1895

Delta R.T. -0.02 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41

Instrument :


BNA_M

ClientSampleId :

A2882RE

Tgt Ion:164 Resp: 458187




Ion	Ratio	Lower	Upper
164	100		
162	102.9	82.4	123.6
160	45.7	35.8	53.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

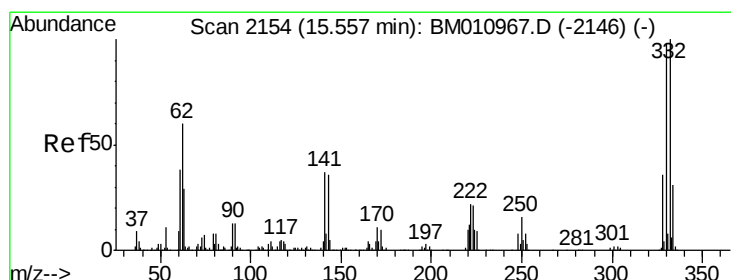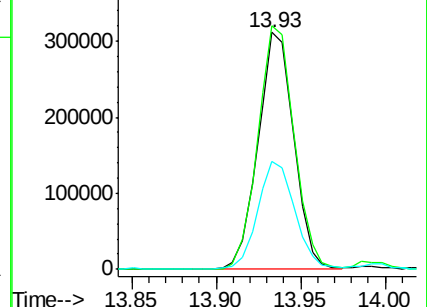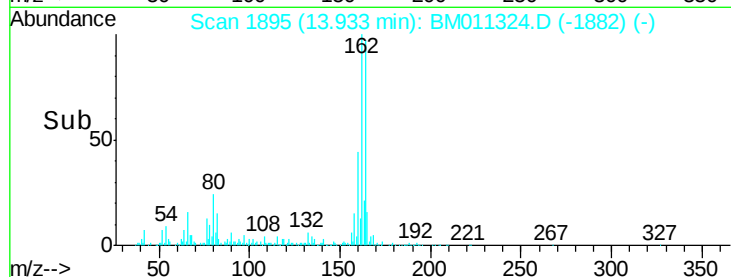

#41

2,4,6-Tribromophenol

Concen: 26.630 ng

RT: 15.44 min Scan# 2152


Delta R.T. -0.02 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41

Tgt Ion:330 Resp: 195564



Ion	Ratio	Lower	Upper
330	100		
332	93.1	0.0	0.0#
141	50.8	0.0	0.0#

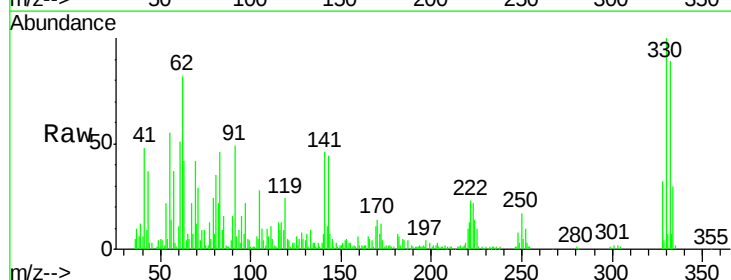


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

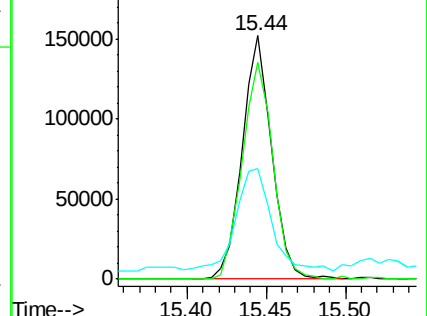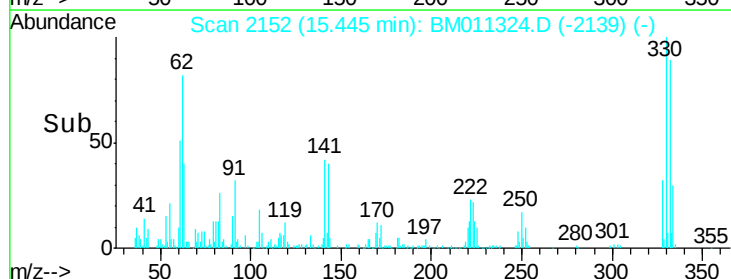

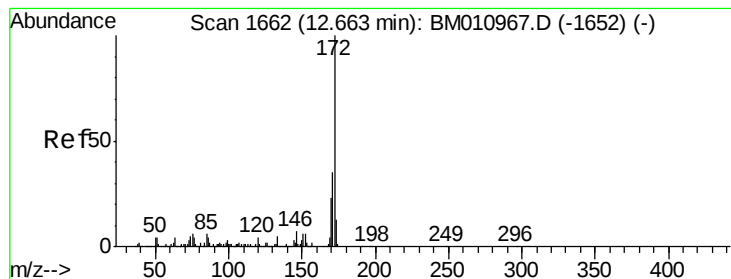

#44

2-Fluorobiphenyl

Concen: 33.504 ng

RT: 12.54 min Scan# 1658

Delta R.T. -0.02 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41

Instrument :


BNA_M

ClientSampleId :

A2882RE

Tgt Ion:172 Resp: 1224041




Ion	Ratio	Lower	Upper
172	100		
171	35.7	28.5	42.7
170	23.3	18.8	28.2



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

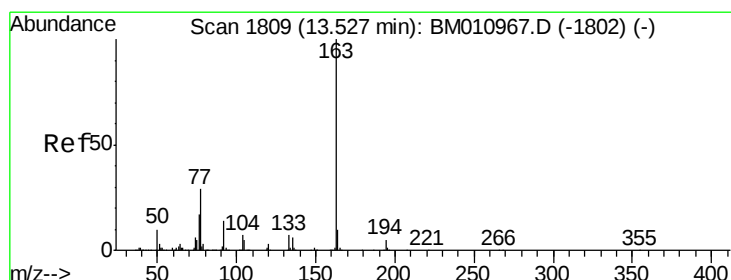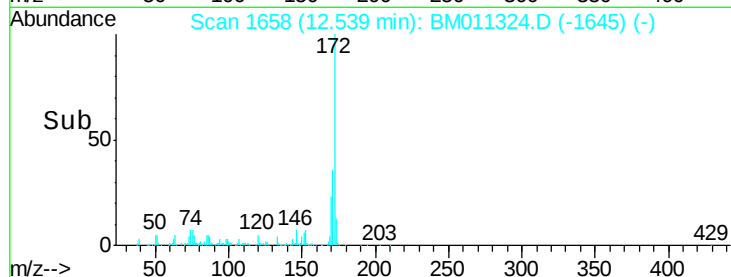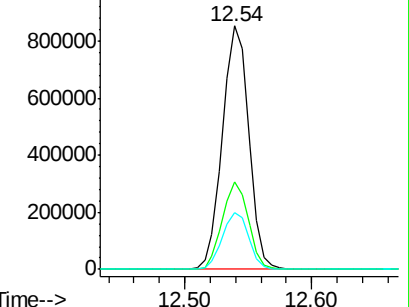

#49

Dimethylphthalate

Concen: 8.412 ng

RT: 13.41 min Scan# 1806


Delta R.T. -0.03 min

Lab File: BM011324.D

Acq: 19 Aug 2017 18:41

Tgt Ion:163 Resp: 329726



Ion	Ratio	Lower	Upper
163	100		
194	4.0	2.7	4.1
164	10.9	8.2	12.2




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



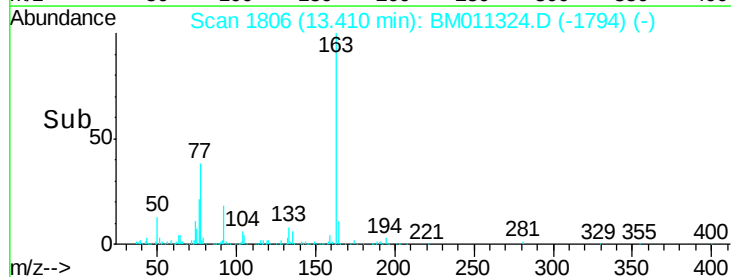
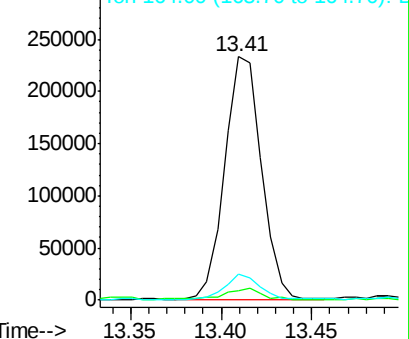


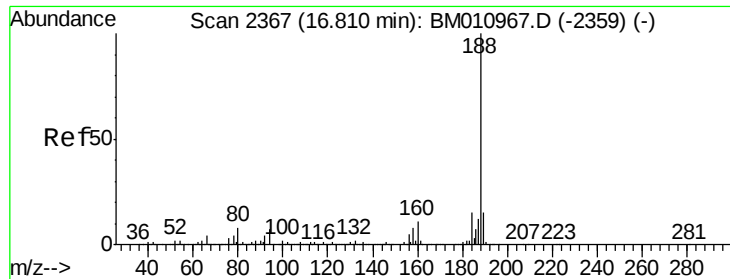

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 16.70 min Scan# 2365
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41




Instrument :
BNA_M
ClientSampleId :
A2882RE


Tgt Ion:188 Resp: 1244580
Ion Ratio Lower Upper
188 100
94 8.5 8.7 13.1#
80 11.1 9.3 13.9

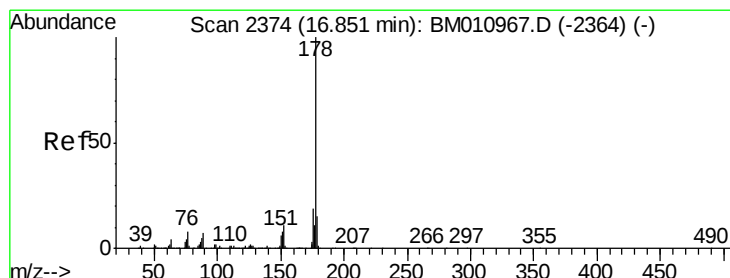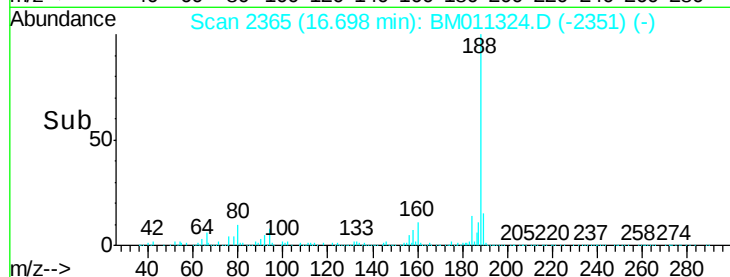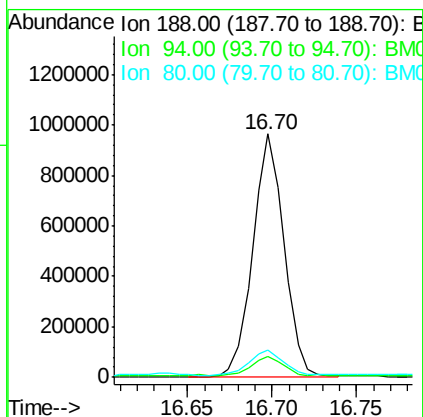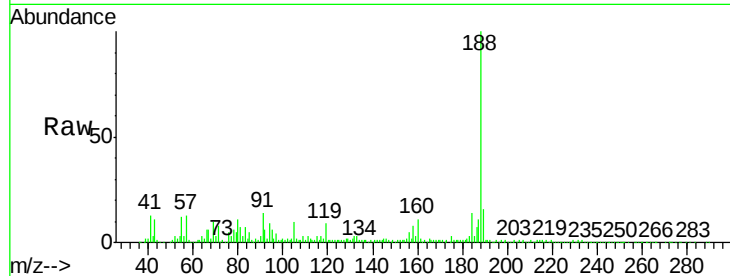

#70
Phenanthrene
Concen: 3.284 ng
RT: 16.74 min Scan# 2372
Delta R.T. -0.02 min
Lab File: BM011324.D
Acq: 19 Aug 2017 18:41

Tgt Ion:178 Resp: 214004
Ion Ratio Lower Upper
178 100
176 23.2 15.2 22.8#
179 20.7 12.1 18.1#


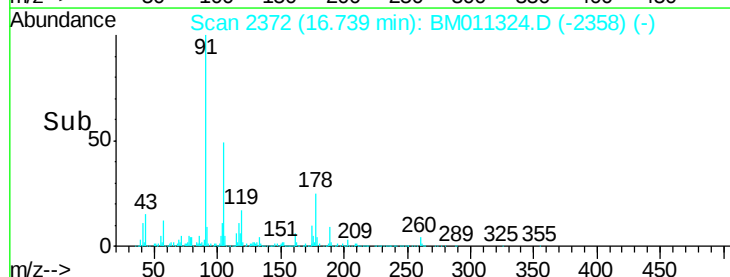
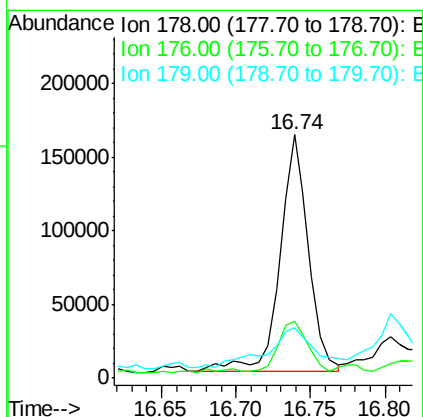
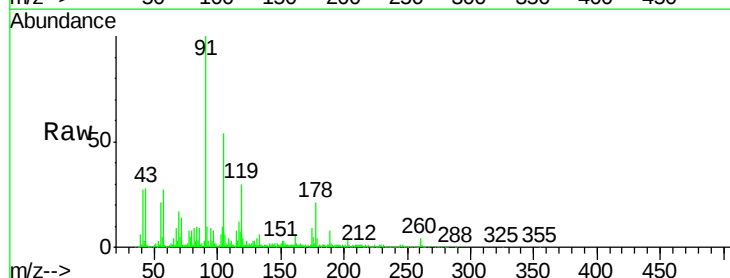


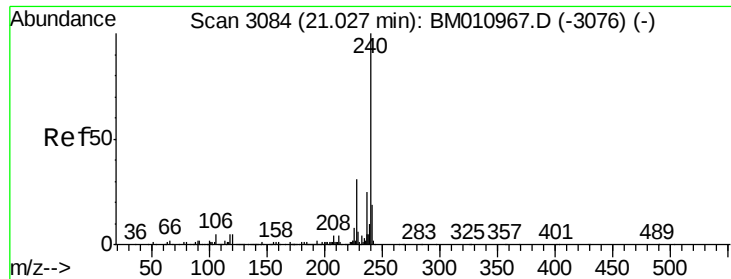

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 20.94 min Scan# 3087
 Delta R.T. 0.00 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41




Instrument :
 BNA_M
 ClientSampleId :
 A2882RE


Tgt Ion:240 Resp: 2190440
 Ion Ratio Lower Upper
 240 100
 120 16.1 8.2 12.2#
 236 28.7 20.0 30.0

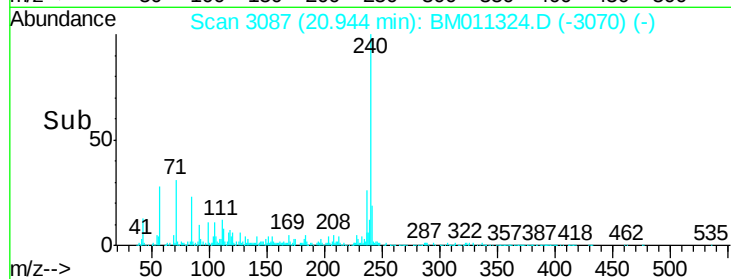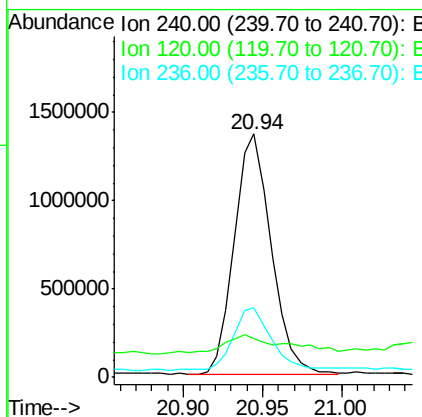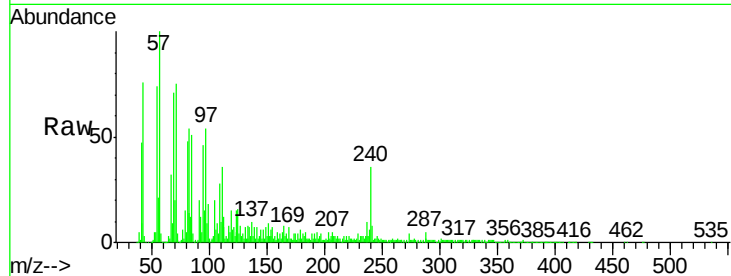

#78
 Terphenyl-d14
 Concen: 22.652 ng
 RT: 19.37 min Scan# 2820
 Delta R.T. -0.01 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41

Tgt Ion:244 Resp: 2504856
 Ion Ratio Lower Upper
 244 100
 212 9.3 4.9 7.3#
 122 9.1 6.2 9.4


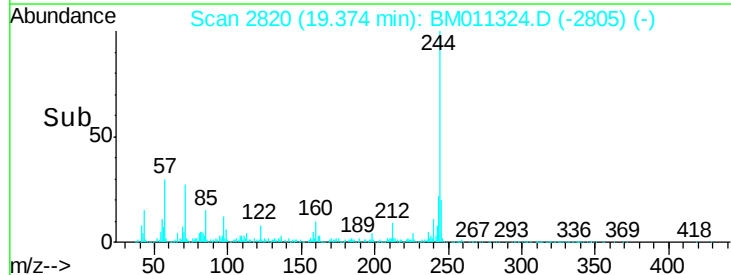
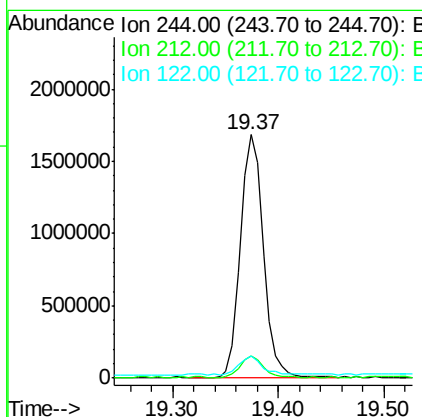



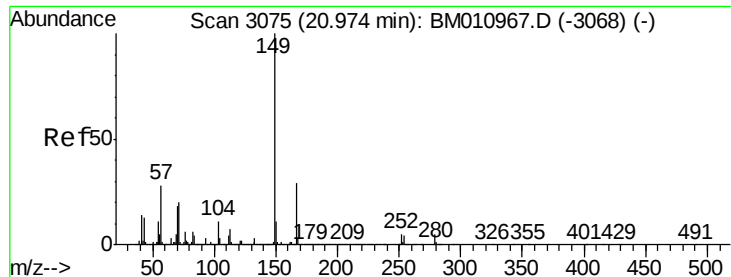

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 14.629 ng
 RT: 20.90 min Scan# 3079
 Delta R.T. 0.00 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41

Instrument :
 BNA_M
 ClientSampleId :
 A2882RE

Tgt Ion:149 Resp: 996027
 Ion Ratio Lower Upper
 149 100
 167 40.4 22.4 33.6#
 279 6.6 3.4 5.0#

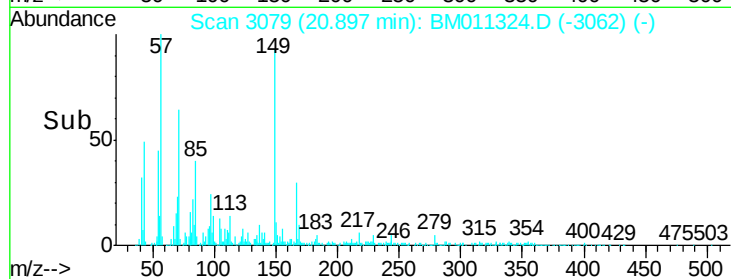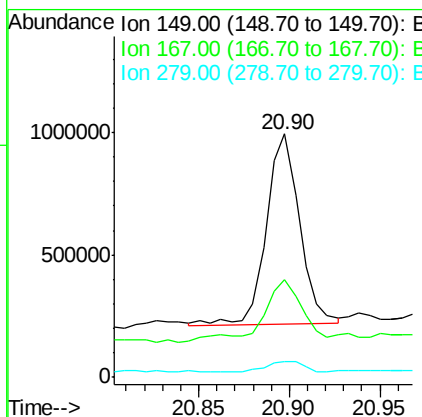

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.04 min Scan# 3443
 Delta R.T. 0.02 min
 Lab File: BM011324.D
 Acq: 19 Aug 2017 18:41

Tgt Ion:264 Resp: 1905943
 Ion Ratio Lower Upper
 264 100
 260 25.7 18.6 27.8
 265 22.4 17.3 25.9

