

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011324.D
 Acq On : 19 Aug 2017 18:41
 Operator : SJ/JU
 Sample : I4848-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A2882RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.804	678	683	693	rBV	630627	1002653	4.58%	0.667%
2	7.269	756	762	768	rVB	783440	1224161	5.59%	0.814%
3	7.581	809	815	822	rVB	1235954	1947792	8.90%	1.295%
4	8.416	951	957	964	rBV	995065	1594060	7.28%	1.060%
5	10.022	1221	1230	1236	rBV	1232164	2083431	9.52%	1.385%
6	10.622	1322	1332	1341	rBV2	400386	1185179	5.42%	0.788%
7	12.539	1653	1658	1664	rVB	2932715	4114359	18.80%	2.736%
8	13.086	1746	1751	1761	rBV7	397062	1004433	4.59%	0.668%
9	13.410	1801	1806	1810	rBV	737649	1198214	5.47%	0.797%
10	13.521	1822	1825	1829	rVB2	689626	907858	4.15%	0.604%
11	13.774	1860	1868	1875	rVB3	413822	1205654	5.51%	0.802%
12	13.933	1890	1895	1900	rBV2	1795454	2815804	12.87%	1.872%
13	13.992	1900	1905	1910	rVB	4990380	6188943	28.28%	4.115%
14	14.568	1999	2003	2009	rBV2	896196	1368185	6.25%	0.910%
15	15.245	2111	2118	2121	rBV2	1234404	2344049	10.71%	1.559%
16	15.445	2147	2152	2156	rBV3	1703110	2543571	11.62%	1.691%
17	15.604	2176	2179	2184	rBV	631428	922448	4.21%	0.613%
18	15.727	2196	2200	2204	rVB	2340661	3076893	14.06%	2.046%
19	15.815	2209	2215	2219	rVB3	1055549	1844369	8.43%	1.226%
20	15.880	2222	2226	2232	rVB	1152534	1609342	7.35%	1.070%
21	16.010	2245	2248	2252	rVB	794735	895161	4.09%	0.595%
22	16.062	2252	2257	2261	rVB4	609897	1079798	4.93%	0.718%
23	16.115	2262	2266	2270	rBV2	1160148	1950756	8.91%	1.297%
24	16.321	2297	2301	2305	rVB	1139194	1431043	6.54%	0.952%
25	16.551	2336	2340	2349	rVB	3566940	5848794	26.72%	3.889%
26	16.633	2350	2354	2359	rBV	2912351	4101223	18.74%	2.727%
27	16.698	2361	2365	2369	rVV	2395800	3213743	14.68%	2.137%
28	16.745	2369	2373	2376	rVV2	2738114	3955273	18.07%	2.630%
29	16.798	2379	2382	2390	rVB3	1903956	4019540	18.37%	2.673%
30	16.998	2413	2416	2419	rBV	688443	846532	3.87%	0.563%
31	17.104	2430	2434	2440	rBV2	3749919	7062195	32.27%	4.696%
32	17.157	2440	2443	2452	rVV2	1781952	4188434	19.14%	2.785%
33	17.262	2455	2461	2467	rVV2	2635412	6170330	28.19%	4.103%
34	17.398	2479	2484	2490	rBV2	4852244	9419612	43.04%	6.264%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011324.D
Acq On : 19 Aug 2017 18:41
Operator : SJ/JU
Sample : I4848-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A2882RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.456	2490	2494	2495	rBV	2152312	2614152	11.94%	1.738%
36	17.527	2503	2506	2510	rBV	2730764	3480504	15.90%	2.314%
37	17.639	2521	2525	2534	rVB2	5562478	8837469	40.38%	5.877%
38	17.827	2553	2557	2567	rVB	5438556	7655406	34.98%	5.091%
39	18.115	2601	2606	2614	rBV	13969751	21885280	100.00%	14.553%
40	19.374	2817	2820	2829	rVB2	7399154	11548823	52.77%	7.679%


Sum of corrected areas: 150385466

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
Data File : BM011324.D
Acq On : 19 Aug 2017 18:41
Operator : SJ/JU
Sample : I4848-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A2882RE

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

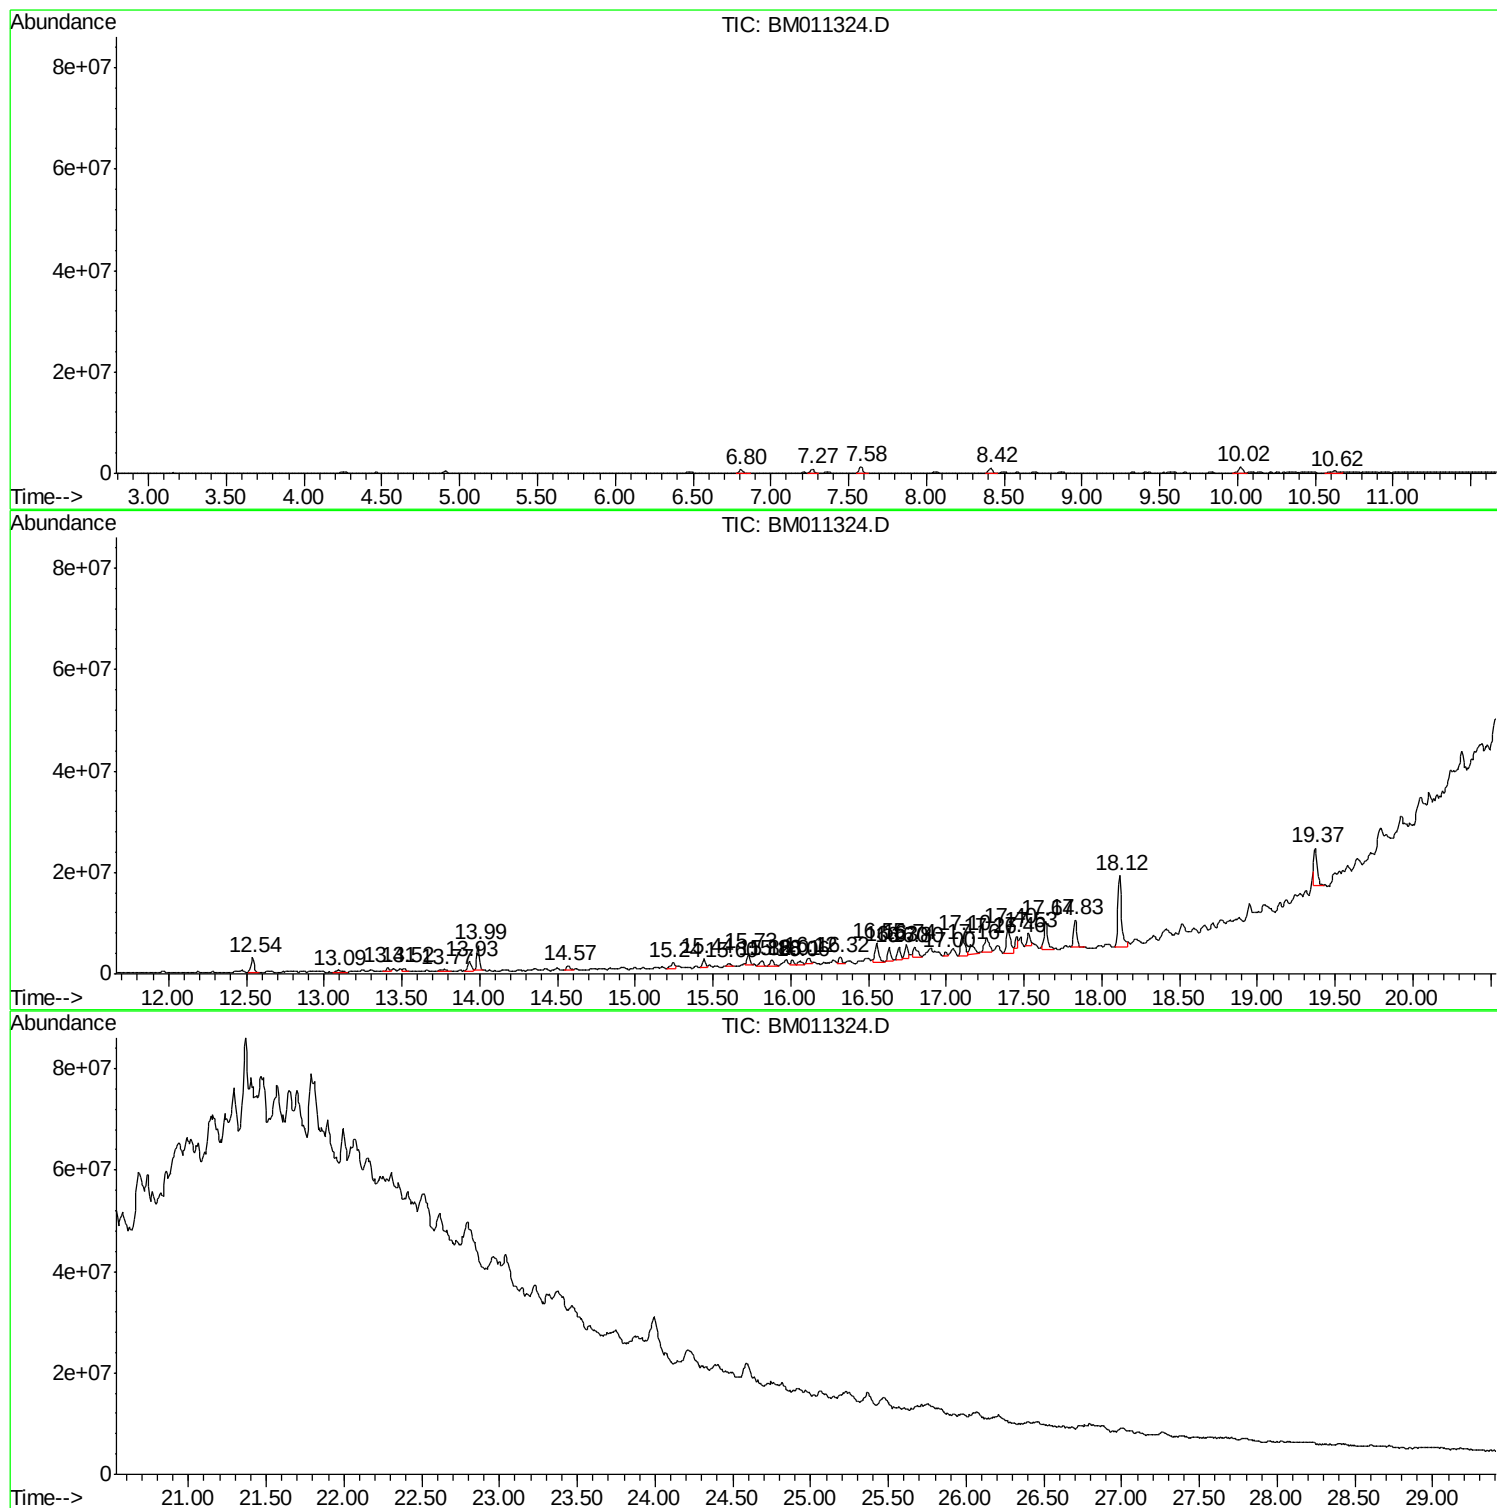

DbaaaPbath::ZZ\NRPBEMM\BBAAMMDAA\BBO0899IX\
 DbaaaFfile::BBO013224DD
 Aeqq00n ::199Aagg2007 188441
 Opeaaor ::SSJUU
 Samplee ::I488800RE
 Misc ::
 AASSVaal ::166 SampleeMMultiplier:11

Instrument :
 BNA_M
 ClientSampleId :
 A2882RE

QqaabMebbdd::ZZ\NRPBEMM\BBAAMMMEH00S88200BBO020617MM
 QqaabTitee ::ASBPBNASSAN000BSF00R55P000NTC0AIBBATION

TICCLibbaay ::CC\DATA\BBSSEN0\$S002LL
 TICInteggaionPaaameess:L66CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
