


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081917\
 Data File : BM011309.D
 Acq On : 19 Aug 2017 09:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 16 02:25:04 2017

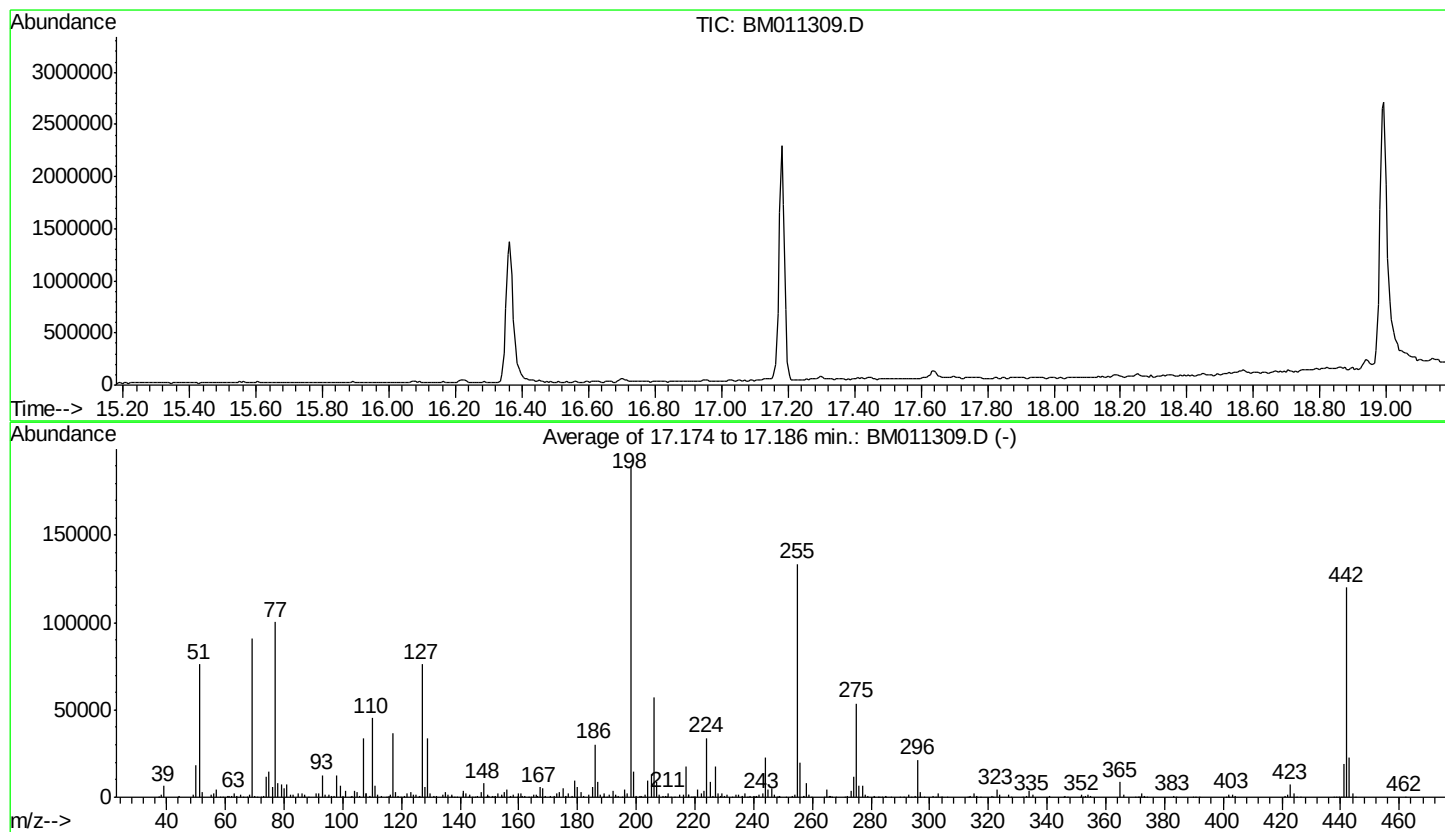

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	76026	PASS
68	69	0.00	2	1.4	1248	PASS
69	198	0.00	100	48.0	91156	PASS
70	69	0.00	2	1.1	959	PASS
127	198	10	80	40.0	76018	PASS
197	198	0.00	2	1.1	2162	PASS
198	198	100	100	100.0	189930	PASS
199	198	5	9	7.6	14466	PASS
275	198	10	60	28.3	53789	PASS
365	198	1	100	4.6	8756	PASS
441	442	0.01	24	15.8	19021	PASS
442	198	50	100	63.2	120026	PASS
443	442	15	24	19.0	22799	PASS