

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
 Data File : BM031822.D
 Acq On : 19 Aug 2021 11:05
 Operator : CG/JU
 Sample : PB138384BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138384BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM031822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	349	355	370	rVB	845297	1203463	38.14%	10.083%
2	6.734	613	620	634	rBV	834362	1273922	40.37%	10.673%
3	7.540	750	757	764	rBV	127362	203921	6.46%	1.709%
4	8.687	944	952	971	rBV	460227	779092	24.69%	6.527%
5	10.298	1219	1226	1234	rBV	161815	270188	8.56%	2.264%
6	12.786	1642	1649	1659	rBV	1121687	1654932	52.45%	13.865%
7	14.174	1879	1885	1894	rBV	240693	359544	11.39%	3.012%
8	15.674	2134	2140	2154	rBV	981176	1412620	44.77%	11.835%
9	16.927	2347	2353	2363	rBV	315102	456552	14.47%	3.825%
10	19.580	2798	2804	2809	rBV	2681504	3155530	100.00%	26.438%
11	21.133	3062	3068	3076	rBV	448792	562130	17.81%	4.710%
12	23.280	3427	3433	3440	rVB2	342628	603739	19.13%	5.058%


Sum of corrected areas: 11935633

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031822.D
Acq On : 19 Aug 2021 11:05
Operator : CG/JU
Sample : PB138384BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

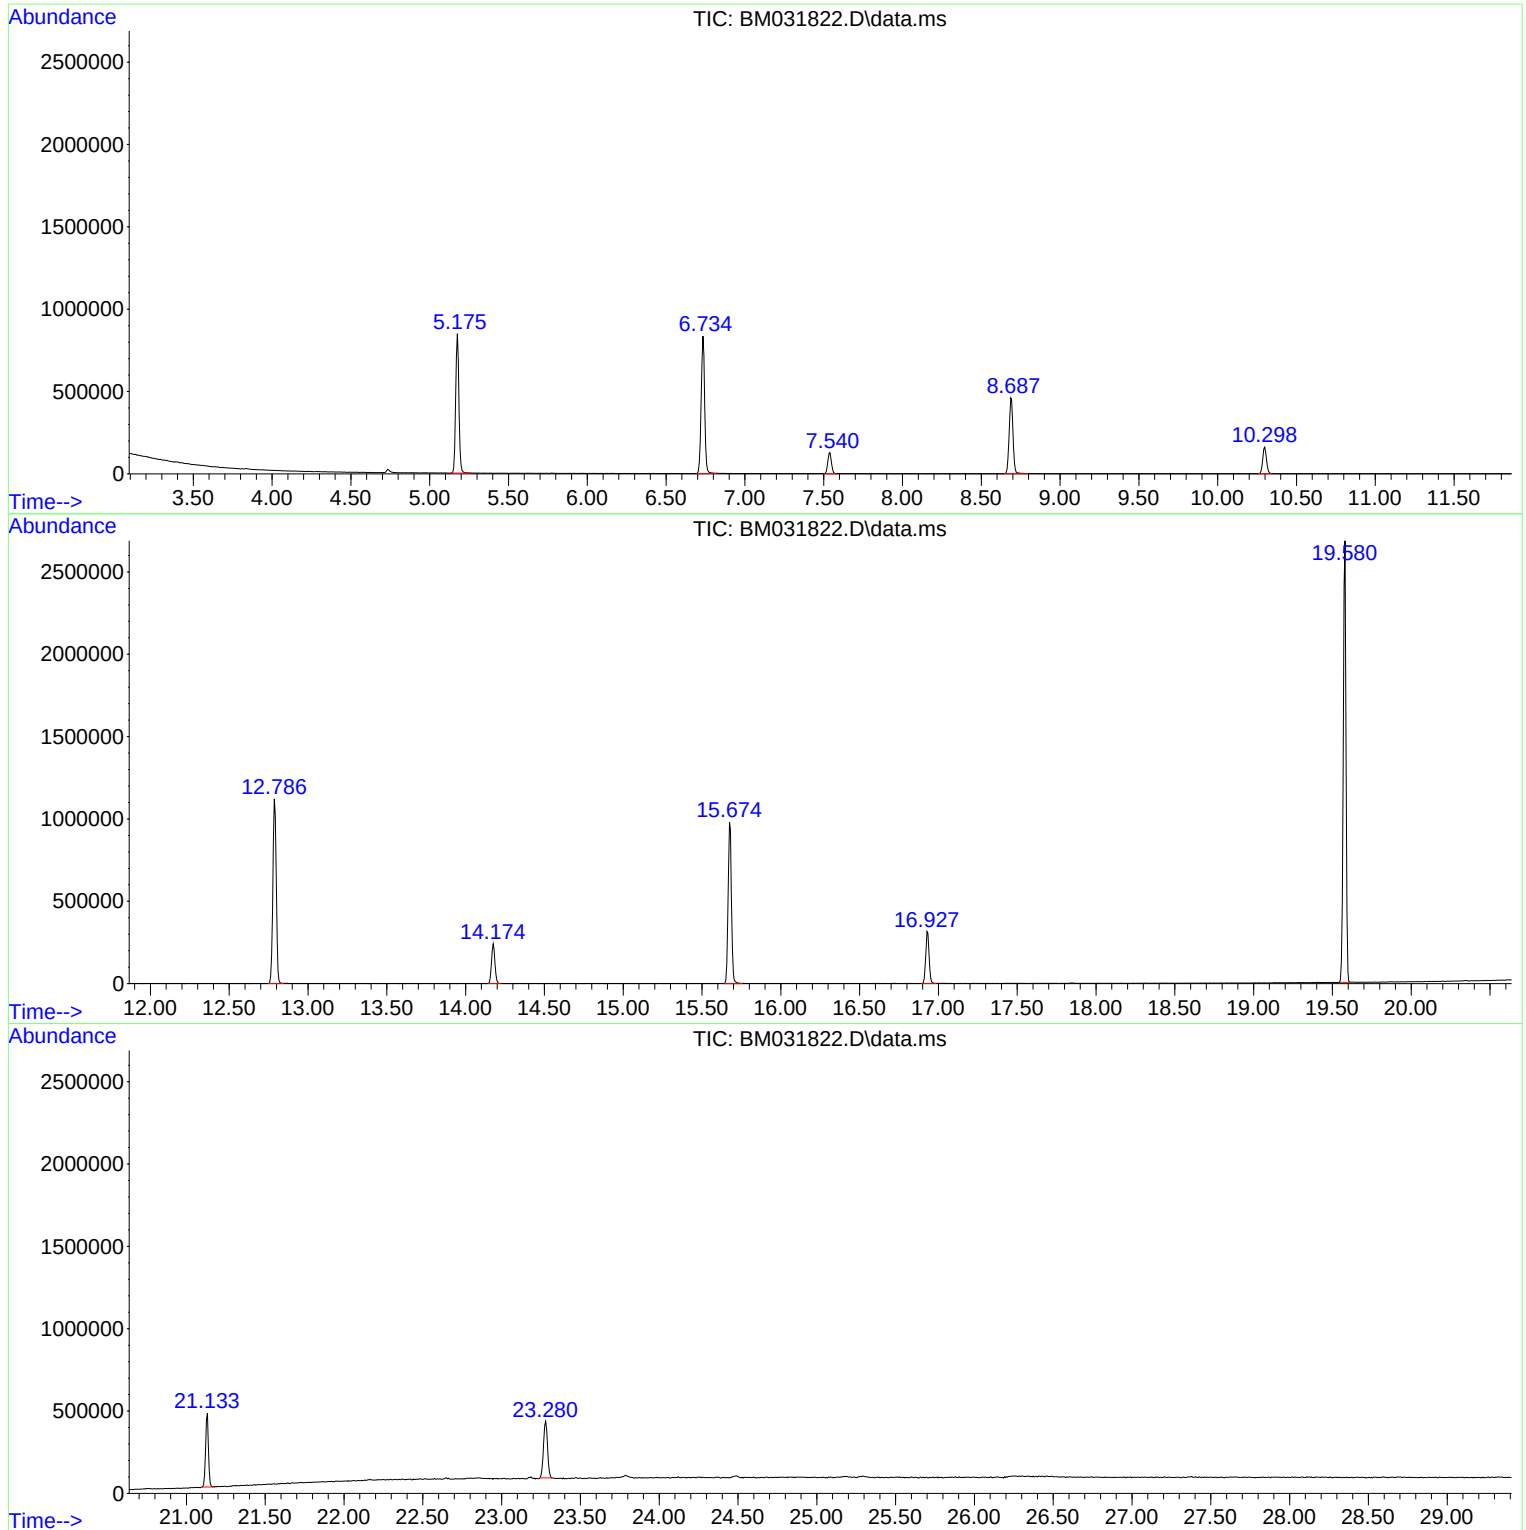

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031822.D
Acq On : 19 Aug 2021 11:05
Operator : CG/JU
Sample : PB138384BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081921\
Data File : BM031822.D
Acq On : 19 Aug 2021 11:05
Operator : CG/JU
Sample : PB138384BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138384BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------